

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029415.D
 Acq On : 13 Jun 2022 16:13
 Operator : JC/MD
 Sample : N3291-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M

Title : VOC Analysis

Signal : TIC: VX029415.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	54	rVB	191965	194987	13.91%	1.794%
2	1.666	91	95	102	rVB	144656	171909	12.26%	1.582%
3	2.306	194	200	210	rBV	304413	483881	34.51%	4.452%
4	2.770	272	276	277	rBV2	370	493	0.04%	0.005%
5	2.788	277	279	284	rVV2	1113	1617	0.12%	0.015%
6	2.946	302	305	306	rBV2	446	486	0.03%	0.004%
7	3.093	327	329	330	rBV2	396	383	0.03%	0.004%
8	3.123	332	334	339	rVB3	616	611	0.04%	0.006%
9	3.245	352	354	356	rBV2	265	281	0.02%	0.003%
10	3.459	385	389	392	rBV3	265	286	0.02%	0.003%
11	3.483	392	393	396	rVB2	351	307	0.02%	0.003%
12	3.513	396	398	399	rBV2	352	302	0.02%	0.003%
13	3.623	413	416	417	rBV	505	378	0.03%	0.003%
14	3.739	433	435	438	rVV2	264	292	0.02%	0.003%
15	3.776	440	441	446	rVB2	328	383	0.03%	0.004%
16	3.940	466	468	470	rBV	323	384	0.03%	0.004%
17	4.013	478	480	483	rBV2	308	355	0.03%	0.003%
18	4.086	489	492	493	rBV	234	246	0.02%	0.002%
19	4.464	545	554	573	rBV	121189	351053	25.03%	3.230%
20	5.062	640	652	672	rVV	181649	565067	40.30%	5.199%
21	5.391	701	706	713	rVB4	1650	3445	0.25%	0.032%
22	5.476	718	720	722	rBV2	717	608	0.04%	0.006%
23	5.562	725	734	742	rBV4	2560	7275	0.52%	0.067%
24	5.976	789	802	820	rBV2	481838	1402273	100.00%	12.901%
25	6.299	851	855	856	rBV2	388	292	0.02%	0.003%
26	6.318	856	858	861	rVV3	287	314	0.02%	0.003%
27	6.495	885	887	889	rVB2	392	288	0.02%	0.003%
28	6.556	893	897	898	rBV3	417	593	0.04%	0.005%
29	6.610	904	906	910	rVB	272	322	0.02%	0.003%
30	6.769	922	932	945	rBV	346758	833226	59.42%	7.666%
31	7.129	983	991	1002	rVB3	38644	89667	6.39%	0.825%
32	7.311	1012	1021	1039	rVV	281795	618203	44.09%	5.687%
33	7.482	1046	1049	1052	rBV3	1029	1172	0.08%	0.011%
34	7.610	1067	1070	1073	rVB3	314	429	0.03%	0.004%
35	7.635	1073	1074	1078	rBV3	340	284	0.02%	0.003%
36	7.824	1103	1105	1108	rVB3	521	521	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029415.D
 Acq On : 13 Jun 2022 16:13
 Operator : JC/MD
 Sample : N3291-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.939	1116	1124	1132	rVB4	1005	2703	0.19%	0.025%
38	8.006	1132	1135	1137	rBV2	285	330	0.02%	0.003%
39	8.055	1141	1143	1145	rBV2	302	323	0.02%	0.003%
40	8.275	1175	1179	1180	rBV3	311	335	0.02%	0.003%
41	8.330	1181	1188	1202	rVV	190671	312875	22.31%	2.878%
42	8.543	1221	1223	1225	rBV3	315	330	0.02%	0.003%
43	8.653	1234	1241	1249	rBV	750434	1145879	81.72%	10.542%
44	8.726	1249	1253	1259	rVB	10814	17422	1.24%	0.160%
45	8.951	1284	1290	1302	rVV	128804	195016	13.91%	1.794%
46	9.092	1311	1313	1315	rBV	400	410	0.03%	0.004%
47	9.165	1323	1325	1328	rBV3	264	240	0.02%	0.002%
48	9.244	1336	1338	1340	rVV2	314	232	0.02%	0.002%
49	9.281	1340	1344	1348	rVV3	3678	5152	0.37%	0.047%
50	9.390	1356	1362	1378	rBV	527336	783289	55.86%	7.206%
51	9.616	1397	1399	1401	rVB2	516	399	0.03%	0.004%
52	10.055	1466	1471	1481	rVV	718426	967701	69.01%	8.903%
53	10.311	1507	1513	1518	rBV4	1811	3041	0.22%	0.028%
54	10.500	1543	1544	1547	rBV2	312	381	0.03%	0.004%
55	10.579	1554	1557	1558	rBV2	327	301	0.02%	0.003%
56	10.646	1564	1568	1573	rBV3	948	1850	0.13%	0.017%
57	10.817	1595	1596	1600	rVB2	268	252	0.02%	0.002%
58	10.860	1600	1603	1604	rBV2	351	376	0.03%	0.003%
59	10.957	1617	1619	1624	rVV2	512	644	0.05%	0.006%
60	11.091	1638	1641	1643	rBV2	1010	1059	0.08%	0.010%
61	11.122	1643	1646	1651	rVB3	3484	4621	0.33%	0.043%
62	11.195	1652	1658	1666	rBV	565946	712183	50.79%	6.552%
63	11.384	1687	1689	1692	rBV2	373	450	0.03%	0.004%
64	11.463	1698	1702	1704	rBV4	699	1093	0.08%	0.010%
65	11.549	1714	1716	1721	rVB2	573	599	0.04%	0.006%
66	11.634	1728	1730	1734	rVB3	544	512	0.04%	0.005%
67	11.677	1734	1737	1740	rBV2	526	635	0.05%	0.006%
68	11.713	1740	1743	1745	rVB3	611	545	0.04%	0.005%
69	11.750	1745	1749	1755	rVB4	4545	5953	0.42%	0.055%
70	11.811	1758	1759	1761	rBV2	299	245	0.02%	0.002%
71	11.847	1761	1765	1768	rVB2	724	888	0.06%	0.008%
72	11.933	1774	1779	1784	rBV4	1548	2766	0.20%	0.025%
73	11.975	1784	1786	1789	rVB	1030	876	0.06%	0.008%
74	12.024	1789	1794	1806	rBV	809033	964767	68.80%	8.876%
75	12.122	1808	1810	1813	rBV3	1060	1523	0.11%	0.014%
76	12.262	1831	1833	1836	rBV3	405	435	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029415.D
 Acq On : 13 Jun 2022 16:13
 Operator : JC/MD
 Sample : N3291-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.323	1836	1843	1851	rBV	794384	982935	70.10%	9.043%
78	12.426	1857	1860	1864	rVB4	997	1597	0.11%	0.015%
79	12.481	1866	1869	1874	rVB4	515	877	0.06%	0.008%
80	12.652	1895	1897	1898	rBV2	432	364	0.03%	0.003%
81	12.731	1906	1910	1911	rBV3	268	376	0.03%	0.003%
82	12.762	1913	1915	1916	rVB2	511	337	0.02%	0.003%
83	12.853	1928	1930	1933	rVV3	447	530	0.04%	0.005%
84	13.115	1971	1973	1977	rVB4	1028	1282	0.09%	0.012%
85	13.432	2021	2025	2026	rBV	368	290	0.02%	0.003%
86	13.530	2039	2041	2042	rBV	483	314	0.02%	0.003%
87	13.591	2048	2051	2056	rVB3	1447	1915	0.14%	0.018%
88	13.640	2058	2059	2062	rBV2	418	388	0.03%	0.004%
89	13.670	2062	2064	2066	rBV2	233	255	0.02%	0.002%
90	13.786	2078	2083	2087	rBV2	1270	1920	0.14%	0.018%
91	13.853	2091	2094	2096	rBV2	310	435	0.03%	0.004%
92	13.963	2107	2112	2118	rBV3	1167	1611	0.11%	0.015%
93	14.042	2123	2125	2128	rBV3	276	254	0.02%	0.002%
94	14.200	2149	2151	2153	rBV2	375	385	0.03%	0.004%
95	14.389	2180	2182	2184	rBV2	412	432	0.03%	0.004%
96	14.493	2197	2199	2202	rBV2	336	295	0.02%	0.003%
97	14.908	2264	2267	2272	rVB4	420	605	0.04%	0.006%
98	14.993	2279	2281	2282	rBV	484	328	0.02%	0.003%
99	15.249	2321	2323	2324	rBV	752	378	0.03%	0.003%
100	16.712	2561	2563	2566	rBV2	593	424	0.03%	0.004%




Sum of corrected areas: 10869771

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029415.D
Acq On : 13 Jun 2022 16:13
Operator : JC/MD
Sample : N3291-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

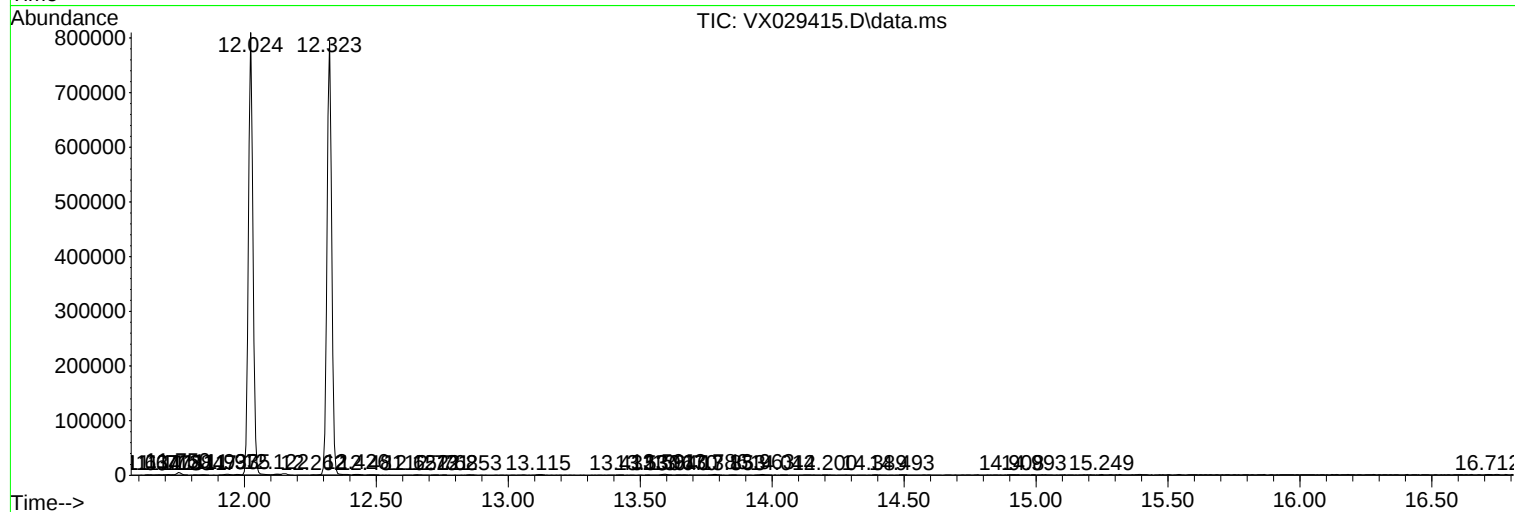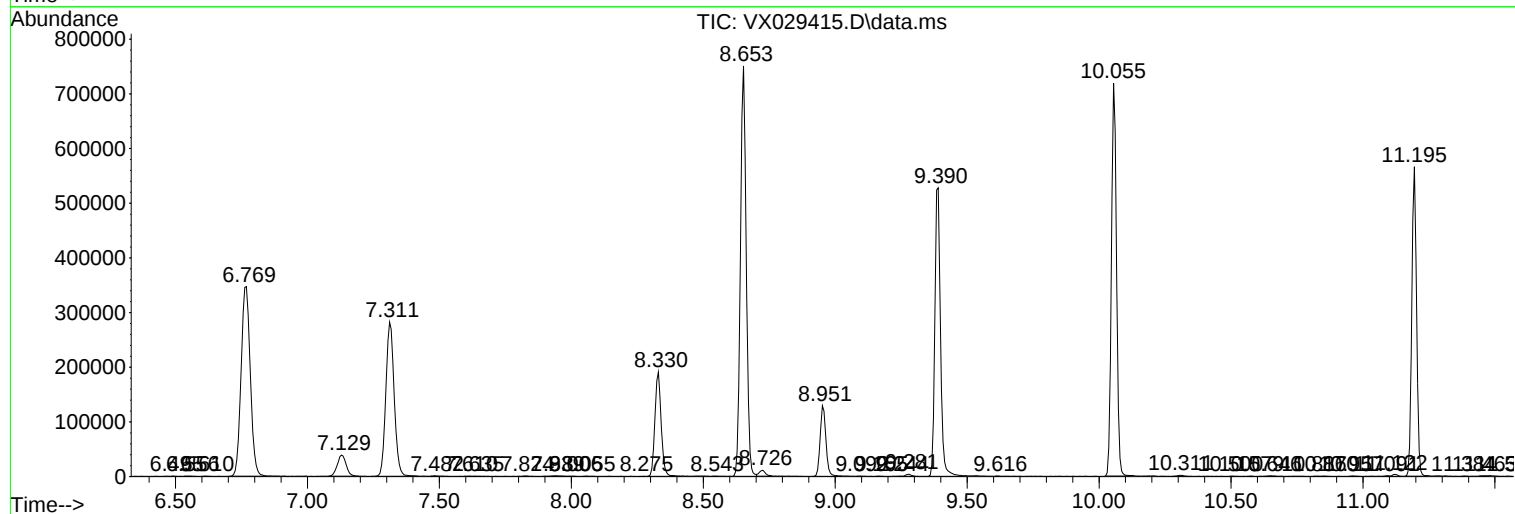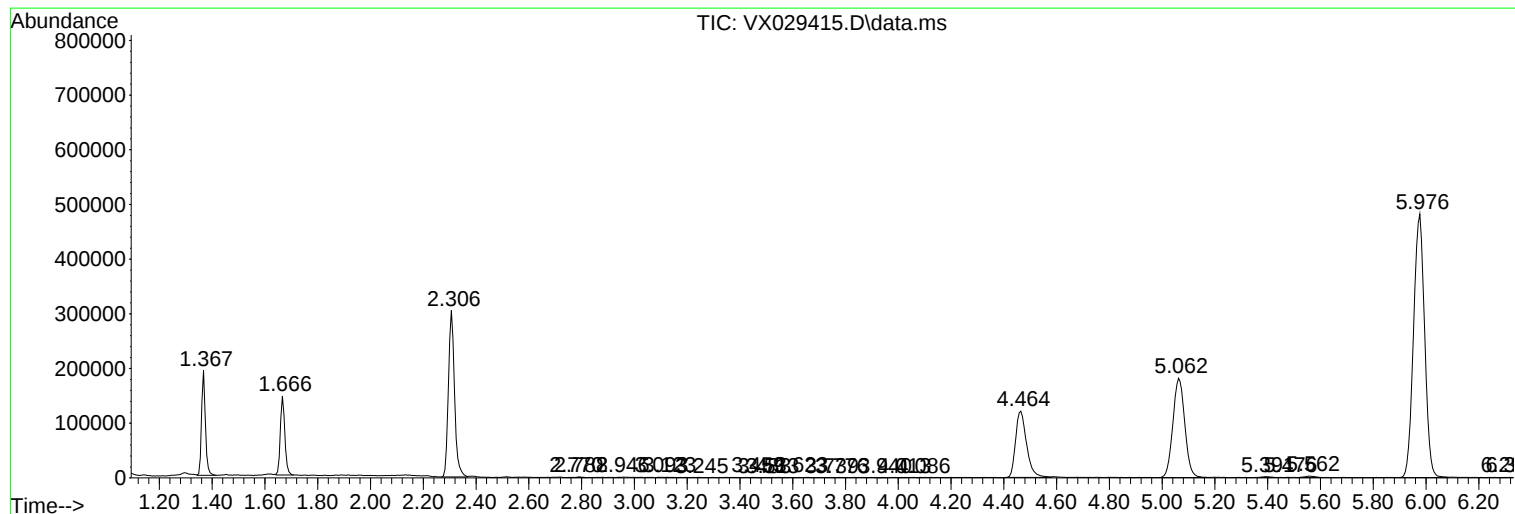

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029415.D
Acq On : 13 Jun 2022 16:13
Operator : JC/MD
Sample : N3291-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029415.D
Acq On : 13 Jun 2022 16:13
Operator : JC/MD
Sample : N3291-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc