

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029416.D
 Acq On : 13 Jun 2022 16:36
 Operator : JC/MD
 Sample : N3291-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029416.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.295	30	34	38	rBV3	6696	11540	0.82%	0.105%
2	1.368	42	46	54	rVB	190271	197741	14.01%	1.795%
3	1.666	91	95	104	rVB	143732	170075	12.05%	1.544%
4	2.307	194	200	212	rBV	305304	488828	34.63%	4.439%
5	2.794	276	280	284	rVB5	1064	1776	0.13%	0.016%
6	2.947	298	305	309	rBV4	585	1356	0.10%	0.012%
7	3.002	313	314	319	rVB2	462	492	0.03%	0.004%
8	3.099	328	330	332	rBV2	327	339	0.02%	0.003%
9	3.361	371	373	375	rBV2	329	302	0.02%	0.003%
10	3.398	376	379	381	rVB	352	298	0.02%	0.003%
11	3.617	410	415	416	rBV3	427	443	0.03%	0.004%
12	3.904	460	462	464	rBV2	300	299	0.02%	0.003%
13	4.148	500	502	503	rBV2	318	336	0.02%	0.003%
14	4.392	540	542	545	rBV2	216	333	0.02%	0.003%
15	4.465	545	554	572	rBV	123666	355066	25.15%	3.224%
16	4.654	583	585	587	rBV2	427	387	0.03%	0.004%
17	4.959	633	635	636	rBV	526	393	0.03%	0.004%
18	5.062	639	652	671	rBV2	184647	572675	40.57%	5.200%
19	5.288	687	689	692	rVB3	267	299	0.02%	0.003%
20	5.519	725	727	728	rBV	400	278	0.02%	0.003%
21	5.562	728	734	742	rVB2	2310	5745	0.41%	0.052%
22	5.769	765	768	772	rVB2	255	324	0.02%	0.003%
23	5.977	790	802	817	rBV2	473967	1411521	100.00%	12.817%
24	6.239	844	845	848	rVB2	446	299	0.02%	0.003%
25	6.294	851	854	857	rBV3	299	423	0.03%	0.004%
26	6.336	860	861	864	rBV2	378	392	0.03%	0.004%
27	6.403	870	872	875	rVB	404	327	0.02%	0.003%
28	6.464	880	882	887	rVB2	297	305	0.02%	0.003%
29	6.550	893	896	899	rBV3	368	555	0.04%	0.005%
30	6.763	921	931	946	rBV	355658	847055	60.01%	7.691%
31	6.976	964	966	969	rBV2	339	422	0.03%	0.004%
32	7.129	980	991	1002	rBV2	74007	166894	11.82%	1.515%
33	7.312	1011	1021	1039	rBV	287126	625079	44.28%	5.676%
34	7.489	1048	1050	1053	rVB4	913	752	0.05%	0.007%
35	7.568	1061	1063	1066	rBV2	322	369	0.03%	0.003%
36	7.659	1076	1078	1081	rVB2	253	276	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029416.D
 Acq On : 13 Jun 2022 16:36
 Operator : JC/MD
 Sample : N3291-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.800	1098	1101	1102	rBV2	347	396	0.03%	0.004%
38	7.812	1102	1103	1111	rVV5	576	1055	0.07%	0.010%
39	7.934	1119	1123	1125	rBV4	1163	1568	0.11%	0.014%
40	8.330	1181	1188	1197	rBV	190150	310979	22.03%	2.824%
41	8.434	1202	1205	1207	rBV2	597	559	0.04%	0.005%
42	8.598	1230	1232	1234	rBV	552	471	0.03%	0.004%
43	8.653	1234	1241	1249	rVV	738753	1150716	81.52%	10.448%
44	8.726	1249	1253	1258	rVB	10408	16411	1.16%	0.149%
45	8.879	1275	1278	1279	rBV	357	300	0.02%	0.003%
46	8.952	1285	1290	1304	rVB	128558	194583	13.79%	1.767%
47	9.086	1310	1312	1315	rVB3	497	480	0.03%	0.004%
48	9.281	1339	1344	1348	rBV2	3959	5026	0.36%	0.046%
49	9.385	1356	1361	1378	rBV	537677	791318	56.06%	7.185%
50	10.055	1465	1471	1482	rBV	745614	984687	69.76%	8.941%
51	10.202	1492	1495	1500	rVB3	973	1466	0.10%	0.013%
52	10.238	1500	1501	1505	rBV	337	361	0.03%	0.003%
53	10.305	1508	1512	1517	rBV2	1935	2978	0.21%	0.027%
54	10.549	1548	1552	1555	rVB2	333	357	0.03%	0.003%
55	10.647	1565	1568	1570	rVV2	852	964	0.07%	0.009%
56	10.701	1574	1577	1578	rBV	280	284	0.02%	0.003%
57	10.939	1613	1616	1618	rBV2	421	516	0.04%	0.005%
58	10.970	1618	1621	1624	rVB3	548	687	0.05%	0.006%
59	11.067	1635	1637	1638	rBV2	324	307	0.02%	0.003%
60	11.086	1638	1640	1643	rVV3	498	580	0.04%	0.005%
61	11.122	1643	1646	1650	rVB3	3374	4198	0.30%	0.038%
62	11.195	1652	1658	1668	rBV	568690	711896	50.43%	6.464%
63	11.366	1683	1686	1687	rBV2	392	410	0.03%	0.004%
64	11.384	1687	1689	1691	rVV2	316	306	0.02%	0.003%
65	11.457	1698	1701	1702	rBV2	1067	1014	0.07%	0.009%
66	11.677	1735	1737	1739	rVB	583	434	0.03%	0.004%
67	11.713	1741	1743	1745	rVV2	722	627	0.04%	0.006%
68	11.750	1745	1749	1756	rVV4	3632	4976	0.35%	0.045%
69	11.841	1762	1764	1768	rVB3	649	809	0.06%	0.007%
70	11.927	1776	1778	1783	rBV4	1813	2542	0.18%	0.023%
71	11.976	1783	1786	1789	rVV3	1103	1185	0.08%	0.011%
72	12.024	1789	1794	1804	rVV	793786	958731	67.92%	8.705%
73	12.323	1837	1843	1851	rBV	784145	977431	69.25%	8.875%
74	12.427	1858	1860	1866	rVB4	1092	1529	0.11%	0.014%
75	12.475	1866	1868	1875	rVB4	587	1212	0.09%	0.011%
76	12.616	1885	1891	1892	rBV2	337	436	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029416.D
 Acq On : 13 Jun 2022 16:36
 Operator : JC/MD
 Sample : N3291-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.664	1897	1899	1903	rVB3	650	903	0.06%	0.008%
78	12.695	1903	1904	1907	rBV	345	312	0.02%	0.003%
79	12.969	1947	1949	1952	rVB2	409	423	0.03%	0.004%
80	13.000	1952	1954	1955	rBV	481	373	0.03%	0.003%
81	13.116	1970	1973	1978	rVB3	754	1081	0.08%	0.010%
82	13.256	1995	1996	1999	rBV	370	309	0.02%	0.003%
83	13.463	2028	2030	2031	rBV	323	326	0.02%	0.003%
84	13.591	2048	2051	2057	rVB3	1049	1636	0.12%	0.015%
85	13.640	2057	2059	2061	rBV2	467	412	0.03%	0.004%
86	13.664	2061	2063	2066	rVB2	275	292	0.02%	0.003%
87	13.744	2073	2076	2078	rBV	310	455	0.03%	0.004%
88	13.786	2079	2083	2088	rVB4	1119	1847	0.13%	0.017%
89	13.829	2088	2090	2093	rBV3	357	457	0.03%	0.004%
90	14.024	2120	2122	2126	rVB3	419	365	0.03%	0.003%
91	14.109	2134	2136	2137	rVB	615	320	0.02%	0.003%
92	14.134	2137	2140	2146	rBV3	512	976	0.07%	0.009%
93	14.176	2146	2147	2149	rBV	483	427	0.03%	0.004%
94	14.225	2152	2155	2156	rBV	461	483	0.03%	0.004%
95	14.298	2164	2167	2169	rBV3	368	315	0.02%	0.003%
96	14.597	2213	2216	2220	rBV3	346	550	0.04%	0.005%
97	14.737	2236	2239	2241	rVB3	464	433	0.03%	0.004%
98	14.859	2257	2259	2261	rBV2	477	430	0.03%	0.004%
99	15.572	2374	2376	2377	rBV2	540	342	0.02%	0.003%
100	16.542	2532	2535	2538	rBV3	772	1019	0.07%	0.009%




Sum of corrected areas: 11013265

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029416.D
Acq On : 13 Jun 2022 16:36
Operator : JC/MD
Sample : N3291-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

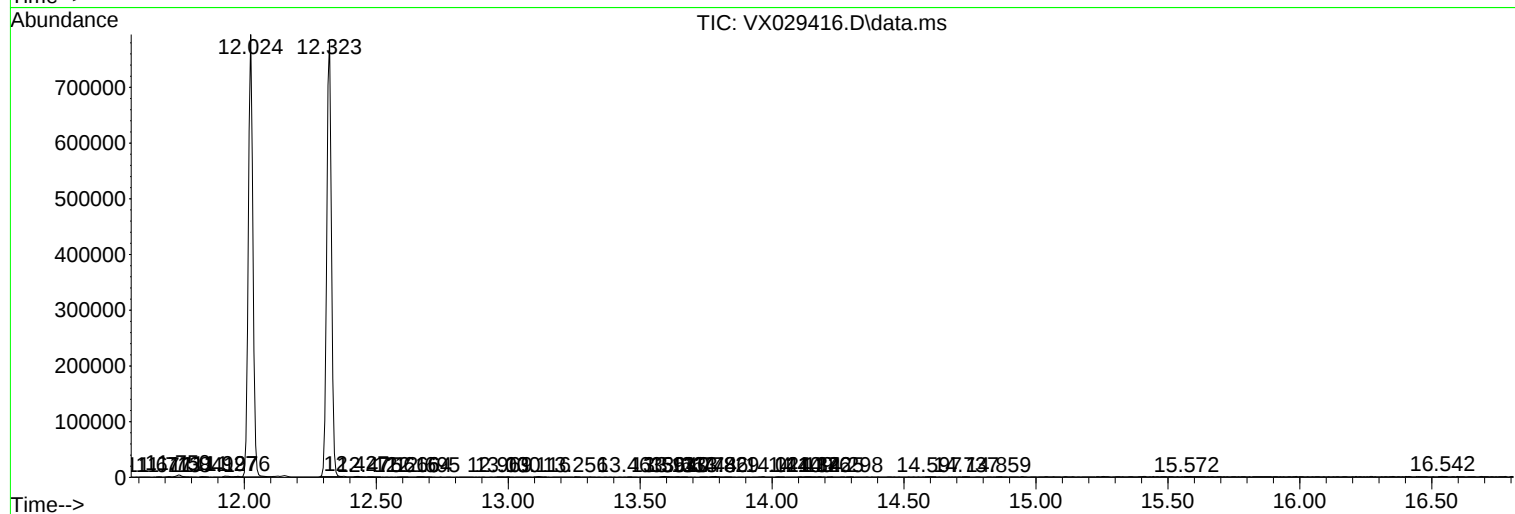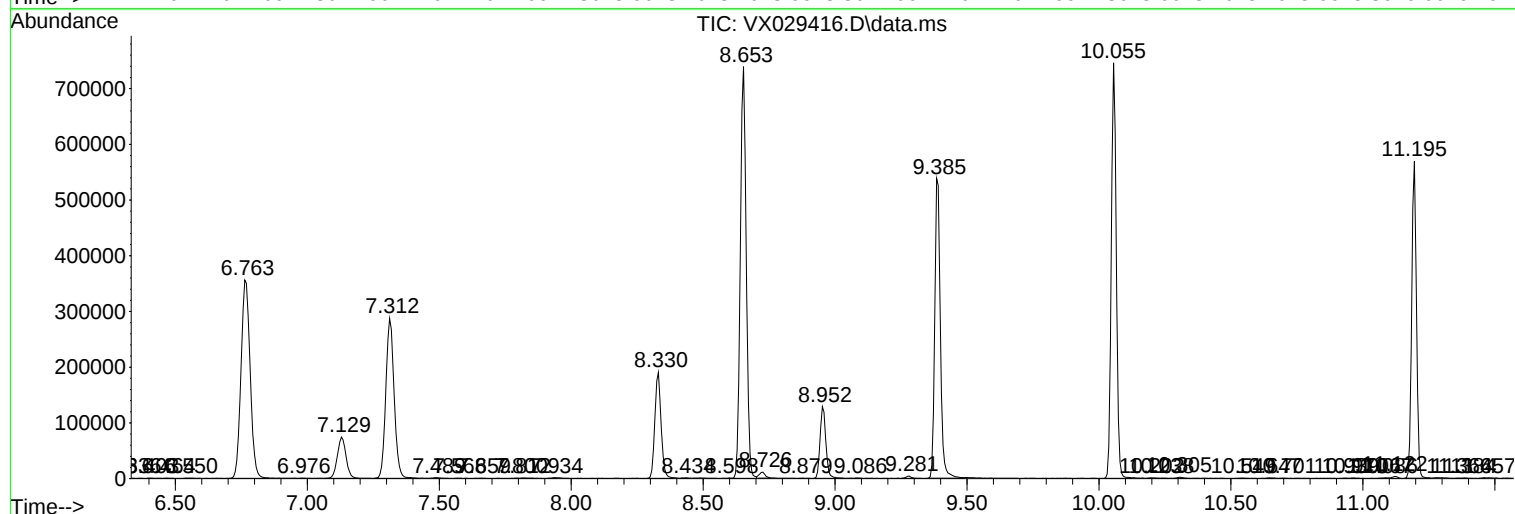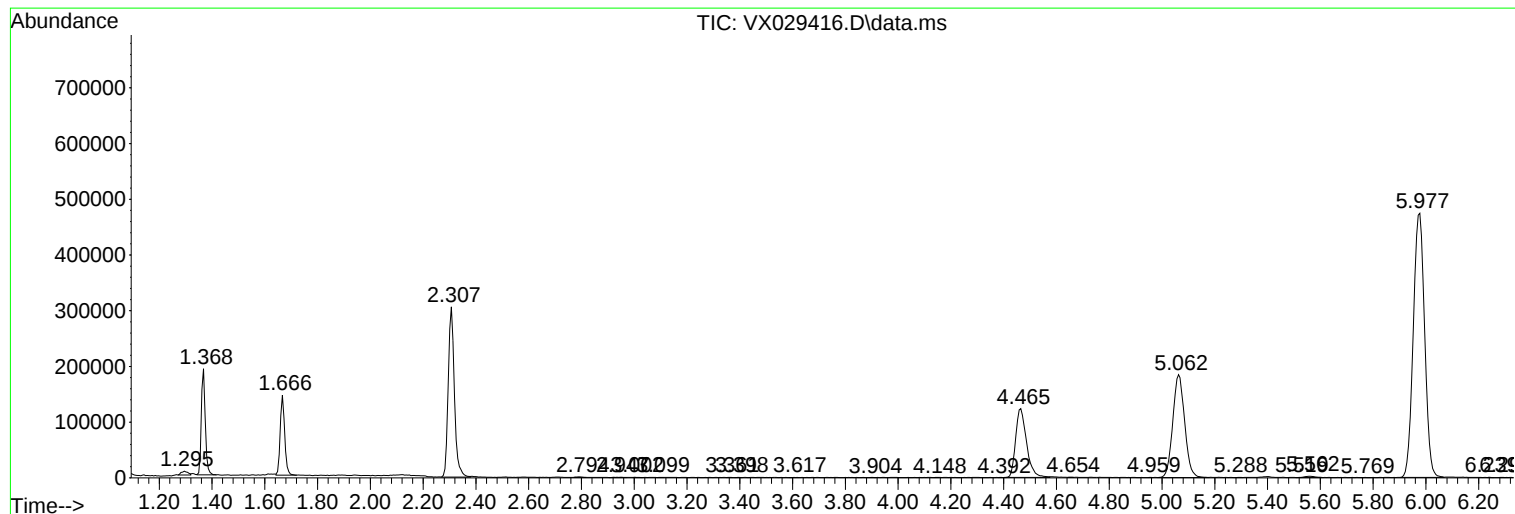

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029416.D
Acq On : 13 Jun 2022 16:36
Operator : JC/MD
Sample : N3291-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029416.D
Acq On : 13 Jun 2022 16:36
Operator : JC/MD
Sample : N3291-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------