

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029417.D
 Acq On : 13 Jun 2022 16:59
 Operator : JC/MD
 Sample : N3291-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	56	rVB	188593	191761	13.81%	1.766%
2	1.666	91	95	103	rVB	144581	170575	12.29%	1.571%
3	2.306	194	200	212	rBV	306766	490621	35.34%	4.519%
4	2.501	230	232	237	rVB3	745	1046	0.08%	0.010%
5	2.788	275	279	284	rVB2	1369	2339	0.17%	0.022%
6	2.940	302	304	305	rVB	540	284	0.02%	0.003%
7	3.129	333	335	336	rVB	519	300	0.02%	0.003%
8	3.263	353	357	358	rVV	310	288	0.02%	0.003%
9	3.367	370	374	377	rBV3	279	439	0.03%	0.004%
10	3.483	390	393	394	rBV2	300	240	0.02%	0.002%
11	3.611	410	414	418	rVB2	394	582	0.04%	0.005%
12	4.080	490	491	494	rBV2	245	245	0.02%	0.002%
13	4.141	498	501	502	rBV2	253	256	0.02%	0.002%
14	4.464	545	554	571	rBV	123438	359653	25.91%	3.312%
15	5.062	639	652	673	rBV	183817	570024	41.06%	5.250%
16	5.397	699	707	708	rBV2	1220	2363	0.17%	0.022%
17	5.531	727	729	730	rBV2	495	494	0.04%	0.005%
18	5.550	730	732	733	rBV2	859	612	0.04%	0.006%
19	5.659	748	750	752	rVB2	420	335	0.02%	0.003%
20	5.696	754	756	761	rVV2	223	263	0.02%	0.002%
21	5.812	772	775	777	rVB	395	278	0.02%	0.003%
22	5.879	783	786	788	rBV	247	347	0.02%	0.003%
23	5.976	789	802	819	rBV2	470004	1388125	100.00%	12.784%
24	6.269	847	850	855	rVB2	363	556	0.04%	0.005%
25	6.312	855	857	858	rBV	470	284	0.02%	0.003%
26	6.367	864	866	867	rBV2	314	288	0.02%	0.003%
27	6.434	874	877	878	rBV2	374	317	0.02%	0.003%
28	6.458	880	881	883	rVV	434	278	0.02%	0.003%
29	6.482	883	885	887	rVB3	360	301	0.02%	0.003%
30	6.519	887	891	893	rBV3	340	418	0.03%	0.004%
31	6.543	893	895	898	rVV2	373	413	0.03%	0.004%
32	6.665	913	915	917	rBV	435	331	0.02%	0.003%
33	6.684	917	918	920	rBV2	418	310	0.02%	0.003%
34	6.769	922	932	945	rBV	355474	848423	61.12%	7.814%
35	6.927	956	958	959	rBV2	564	367	0.03%	0.003%
36	7.055	976	979	980	rBV2	386	334	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029417.D
 Acq On : 13 Jun 2022 16:59
 Operator : JC/MD
 Sample : N3291-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.129	983	991	1001	rVV4	37277	88459	6.37%	0.815%
38	7.312	1012	1021	1036	rBV	277825	611114	44.02%	5.628%
39	7.488	1046	1050	1054	rVB4	737	1013	0.07%	0.009%
40	7.604	1066	1069	1071	rBV3	253	367	0.03%	0.003%
41	7.665	1077	1079	1081	rVB2	286	252	0.02%	0.002%
42	7.824	1099	1105	1110	rVV4	559	1053	0.08%	0.010%
43	7.939	1119	1124	1129	rBV3	1035	1787	0.13%	0.016%
44	8.037	1137	1140	1144	rBV3	219	413	0.03%	0.004%
45	8.141	1155	1157	1158	rBV	322	258	0.02%	0.002%
46	8.189	1164	1165	1168	rBV2	312	311	0.02%	0.003%
47	8.220	1168	1170	1173	rVV2	226	251	0.02%	0.002%
48	8.330	1181	1188	1198	rBV	187601	306764	22.10%	2.825%
49	8.476	1211	1212	1215	rBV3	506	624	0.04%	0.006%
50	8.653	1234	1241	1249	rBV	729765	1132792	81.61%	10.433%
51	8.726	1249	1253	1260	rVB	10574	17126	1.23%	0.158%
52	8.951	1285	1290	1304	rBV	131292	191770	13.82%	1.766%
53	9.043	1304	1305	1309	rVV2	589	447	0.03%	0.004%
54	9.098	1311	1314	1315	rBV2	328	263	0.02%	0.002%
55	9.201	1329	1331	1333	rVV2	354	328	0.02%	0.003%
56	9.275	1337	1343	1350	rVV6	3386	5346	0.39%	0.049%
57	9.390	1356	1362	1377	rBV	541794	786992	56.69%	7.248%
58	9.646	1402	1404	1407	rBV2	387	388	0.03%	0.004%
59	10.055	1465	1471	1483	rBV	741183	988960	71.24%	9.108%
60	10.159	1487	1488	1491	rVB2	689	417	0.03%	0.004%
61	10.195	1492	1494	1496	rVB3	574	354	0.03%	0.003%
62	10.305	1508	1512	1516	rBV2	2070	2428	0.17%	0.022%
63	10.646	1564	1568	1571	rBV2	789	1245	0.09%	0.011%
64	10.756	1584	1586	1589	rBV2	353	373	0.03%	0.003%
65	10.957	1616	1619	1622	rBV3	326	491	0.04%	0.005%
66	11.055	1633	1635	1637	rBV3	254	248	0.02%	0.002%
67	11.091	1637	1641	1642	rBV3	856	838	0.06%	0.008%
68	11.122	1642	1646	1650	rVB3	3006	4588	0.33%	0.042%
69	11.195	1652	1658	1666	rBV	566231	701933	50.57%	6.465%
70	11.451	1698	1700	1702	rBV2	729	666	0.05%	0.006%
71	11.542	1713	1715	1718	rVB2	589	598	0.04%	0.006%
72	11.573	1718	1720	1721	rBV	528	304	0.02%	0.003%
73	11.683	1733	1738	1740	rBV2	522	894	0.06%	0.008%
74	11.750	1745	1749	1757	rVV4	3427	5655	0.41%	0.052%
75	11.841	1762	1764	1767	rVV	988	936	0.07%	0.009%
76	11.933	1774	1779	1783	rBV4	1580	2183	0.16%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029417.D
 Acq On : 13 Jun 2022 16:59
 Operator : JC/MD
 Sample : N3291-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.975	1783	1786	1788	rVB3	999	1134	0.08%	0.010%
78	12.024	1789	1794	1805	rVV	786681	969739	69.86%	8.931%
79	12.122	1808	1810	1813	rVV4	1568	2365	0.17%	0.022%
80	12.152	1813	1815	1820	rVB3	2823	2933	0.21%	0.027%
81	12.323	1837	1843	1849	rBV	793784	971350	69.98%	8.946%
82	12.475	1866	1868	1869	rBV	493	339	0.02%	0.003%
83	12.622	1889	1892	1895	rBV2	422	801	0.06%	0.007%
84	13.048	1960	1962	1967	rBV4	470	750	0.05%	0.007%
85	13.115	1969	1973	1978	rVB2	714	1053	0.08%	0.010%
86	13.219	1988	1990	1991	rBV2	381	290	0.02%	0.003%
87	13.487	2033	2034	2037	rBV2	423	444	0.03%	0.004%
88	13.597	2046	2052	2054	rBV3	1426	1613	0.12%	0.015%
89	13.707	2068	2070	2074	rVB2	340	389	0.03%	0.004%
90	13.780	2079	2082	2087	rVV	3413	4253	0.31%	0.039%
91	13.835	2090	2091	2093	rBV	312	257	0.02%	0.002%
92	13.963	2111	2112	2115	rVB	806	477	0.03%	0.004%
93	14.091	2130	2133	2134	rBV	409	256	0.02%	0.002%
94	14.127	2137	2139	2141	rBV2	569	548	0.04%	0.005%
95	14.255	2158	2160	2164	rBV	363	346	0.02%	0.003%
96	14.566	2209	2211	2212	rBV2	329	280	0.02%	0.003%
97	15.036	2285	2288	2291	rBV3	549	729	0.05%	0.007%
98	15.365	2341	2342	2346	rBV2	637	629	0.05%	0.006%
99	15.560	2372	2374	2377	rBV4	715	1010	0.07%	0.009%
100	15.682	2392	2394	2396	rBV2	682	710	0.05%	0.007%




Sum of corrected areas: 10858014

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029417.D
Acq On : 13 Jun 2022 16:59
Operator : JC/MD
Sample : N3291-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

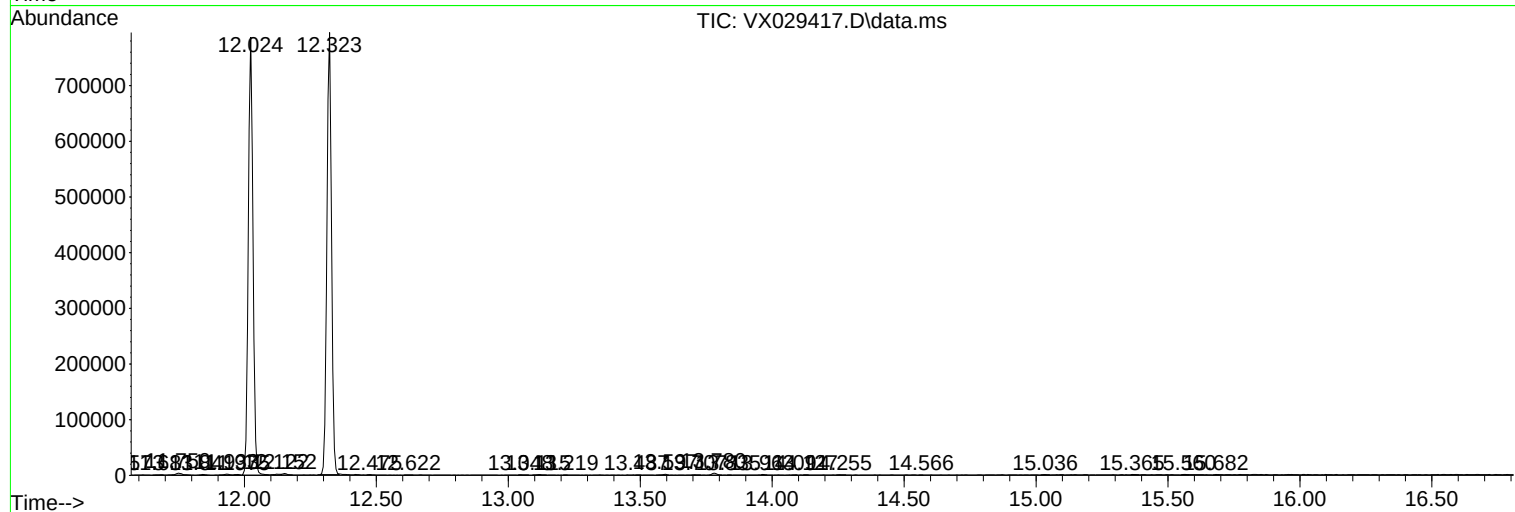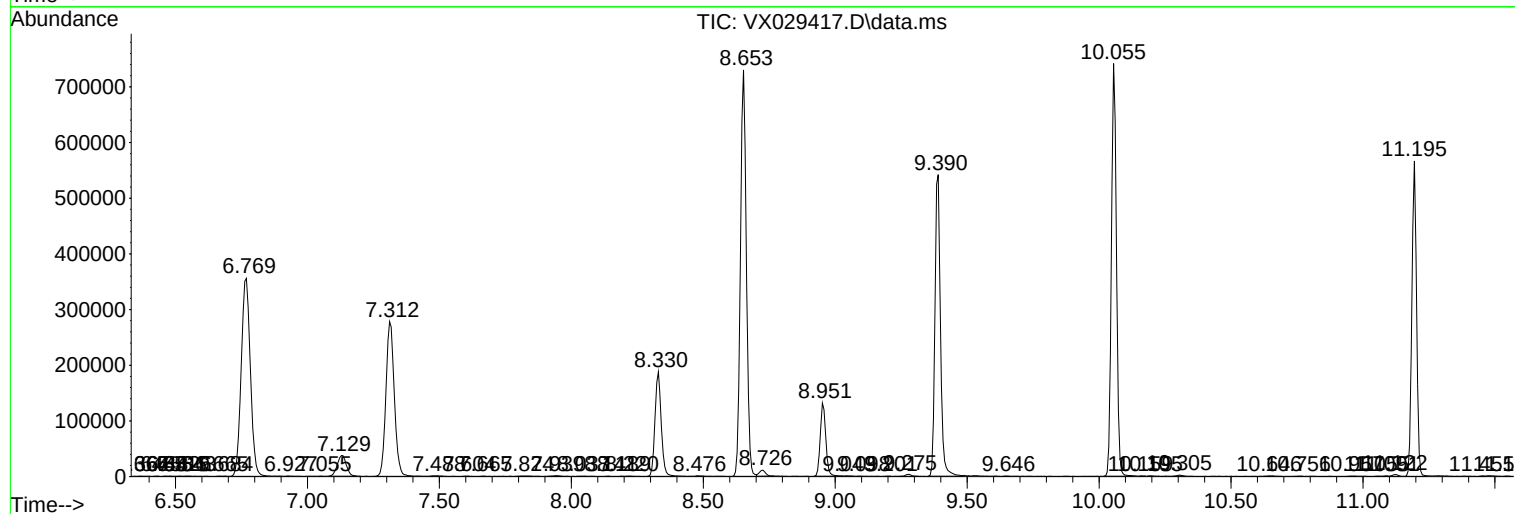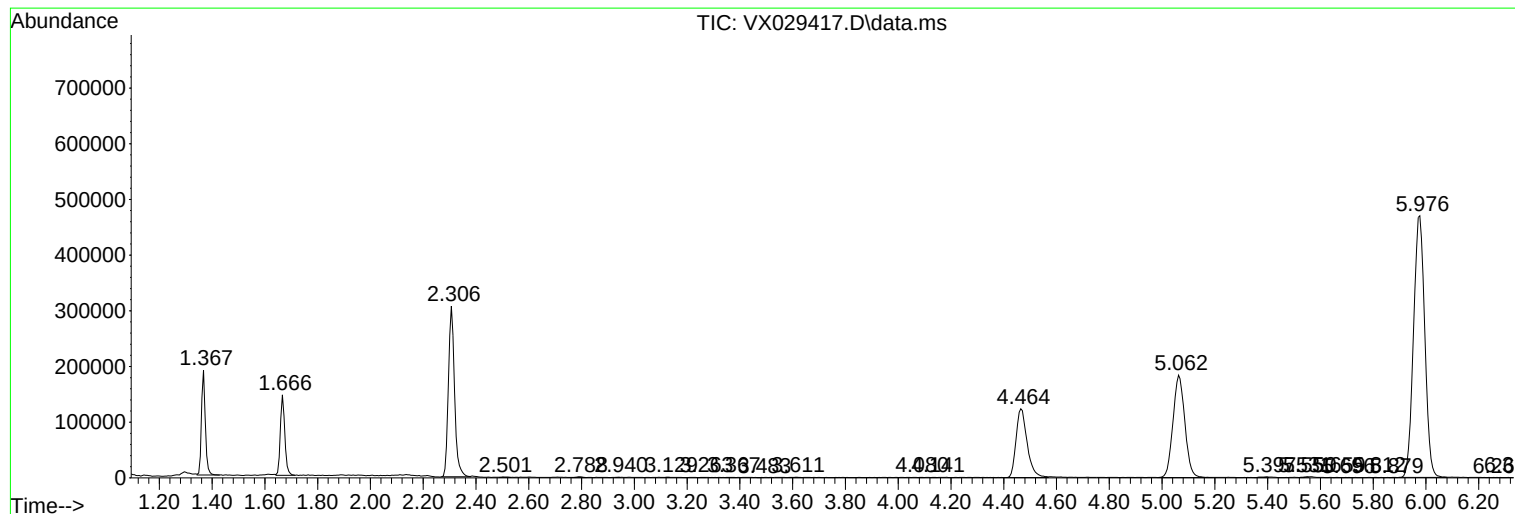

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029417.D
Acq On : 13 Jun 2022 16:59
Operator : JC/MD
Sample : N3291-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029417.D
Acq On : 13 Jun 2022 16:59
Operator : JC/MD
Sample : N3291-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc