

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029418.D
 Acq On : 13 Jun 2022 17:23
 Operator : JC/MD
 Sample : N3291-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029418.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB	182135	191358	13.91%	1.767%
2	1.666	91	95	105	rVB	135752	167280	12.16%	1.545%
3	2.307	194	200	210	rBV	298165	475717	34.58%	4.392%
4	2.788	275	279	283	rVB4	953	1700	0.12%	0.016%
5	2.837	283	287	288	rBV2	301	346	0.03%	0.003%
6	3.075	324	326	327	rBV	423	301	0.02%	0.003%
7	3.105	327	331	333	rBV2	383	614	0.04%	0.006%
8	3.325	363	367	368	rBV2	259	359	0.03%	0.003%
9	3.373	372	375	376	rBV2	246	271	0.02%	0.003%
10	3.404	376	380	381	rBV3	294	328	0.02%	0.003%
11	3.465	387	390	391	rBV	229	270	0.02%	0.002%
12	3.837	450	451	454	rBV2	283	279	0.02%	0.003%
13	4.068	487	489	491	rBV2	418	419	0.03%	0.004%
14	4.111	491	496	498	rBV3	223	412	0.03%	0.004%
15	4.245	516	518	521	rBV3	332	351	0.03%	0.003%
16	4.465	545	554	571	rBV	120478	350687	25.49%	3.238%
17	4.757	600	602	605	rVB2	404	367	0.03%	0.003%
18	4.971	635	637	638	rBV2	335	268	0.02%	0.002%
19	5.062	639	652	670	rVV	180380	564278	41.02%	5.210%
20	5.233	678	680	682	rBV2	328	321	0.02%	0.003%
21	5.397	700	707	714	rBV5	1811	5176	0.38%	0.048%
22	5.471	716	719	721	rBV2	282	335	0.02%	0.003%
23	5.550	727	732	733	rBV2	2422	3107	0.23%	0.029%
24	5.977	790	802	817	rBV2	465376	1375596	100.00%	12.701%
25	6.245	843	846	848	rBV2	442	455	0.03%	0.004%
26	6.275	848	851	853	rVV2	223	281	0.02%	0.003%
27	6.330	859	860	862	rBV	380	268	0.02%	0.002%
28	6.422	873	875	879	rVB2	233	290	0.02%	0.003%
29	6.550	892	896	898	rVV4	349	453	0.03%	0.004%
30	6.586	901	902	906	rBV	230	281	0.02%	0.003%
31	6.672	914	916	919	rBV	316	318	0.02%	0.003%
32	6.769	921	932	949	rBV	346104	830910	60.40%	7.672%
33	7.129	983	991	1006	rVB	99311	218025	15.85%	2.013%
34	7.312	1012	1021	1036	rBV	277396	611548	44.46%	5.646%
35	7.452	1041	1044	1045	rBV	460	488	0.04%	0.005%
36	7.482	1047	1049	1058	rVB5	921	1476	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029418.D
 Acq On : 13 Jun 2022 17:23
 Operator : JC/MD
 Sample : N3291-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.830	1101	1106	1107	rBV2	475	722	0.05%	0.007%
38	7.891	1113	1116	1117	rBV	340	287	0.02%	0.003%
39	7.940	1121	1124	1130	rVB3	1122	1985	0.14%	0.018%
40	8.330	1181	1188	1202	rVV	178732	301838	21.94%	2.787%
41	8.433	1204	1205	1207	rVB	431	282	0.02%	0.003%
42	8.531	1220	1221	1224	rBV2	366	379	0.03%	0.003%
43	8.653	1234	1241	1249	rBV	703716	1122547	81.60%	10.365%
44	8.726	1249	1253	1261	rVB	10424	17499	1.27%	0.162%
45	8.952	1283	1290	1303	rBV	127707	191212	13.90%	1.765%
46	9.098	1311	1314	1316	rVB2	516	607	0.04%	0.006%
47	9.128	1316	1319	1321	rBV2	364	393	0.03%	0.004%
48	9.275	1339	1343	1347	rBV3	3227	4578	0.33%	0.042%
49	9.385	1356	1361	1379	rBV	530789	776124	56.42%	7.166%
50	9.830	1432	1434	1437	rVB2	434	482	0.04%	0.004%
51	9.854	1437	1438	1440	rBV2	448	334	0.02%	0.003%
52	9.878	1440	1442	1445	rBV3	253	275	0.02%	0.003%
53	10.055	1465	1471	1482	rBV	728873	968095	70.38%	8.938%
54	10.201	1490	1495	1500	rBV6	783	1458	0.11%	0.013%
55	10.305	1508	1512	1518	rVB4	1723	2591	0.19%	0.024%
56	10.439	1531	1534	1535	rBV	365	339	0.02%	0.003%
57	10.646	1565	1568	1575	rVV4	950	1605	0.12%	0.015%
58	10.768	1584	1588	1591	rBV2	231	271	0.02%	0.003%
59	10.963	1615	1620	1622	rBV3	709	887	0.06%	0.008%
60	11.031	1629	1631	1634	rBV2	285	388	0.03%	0.004%
61	11.085	1636	1640	1641	rBV3	655	766	0.06%	0.007%
62	11.122	1643	1646	1650	rVB	2933	3761	0.27%	0.035%
63	11.195	1652	1658	1667	rBV	564629	698851	50.80%	6.453%
64	11.372	1686	1687	1690	rBV2	354	377	0.03%	0.003%
65	11.555	1713	1717	1719	rVB2	449	490	0.04%	0.005%
66	11.677	1732	1737	1741	rBV3	524	827	0.06%	0.008%
67	11.713	1741	1743	1745	rVV2	849	581	0.04%	0.005%
68	11.750	1745	1749	1754	rVB4	3684	5037	0.37%	0.047%
69	11.939	1774	1780	1783	rVV3	1672	2060	0.15%	0.019%
70	11.976	1783	1786	1789	rBV3	564	792	0.06%	0.007%
71	12.024	1789	1794	1807	rVV	788697	946154	68.78%	8.736%
72	12.152	1813	1815	1819	rVB4	1969	2325	0.17%	0.021%
73	12.238	1827	1829	1832	rVB2	268	330	0.02%	0.003%
74	12.323	1837	1843	1858	rVB	750140	953725	69.33%	8.806%
75	12.475	1866	1868	1869	rBV	529	269	0.02%	0.002%
76	12.652	1894	1897	1898	rVV2	335	321	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029418.D
 Acq On : 13 Jun 2022 17:23
 Operator : JC/MD
 Sample : N3291-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.664	1898	1899	1904	rVB3	518	510	0.04%	0.005%
78	13.055	1959	1963	1965	rBV2	537	669	0.05%	0.006%
79	13.122	1970	1974	1977	rVV3	717	1030	0.07%	0.010%
80	13.152	1977	1979	1981	rVV3	385	291	0.02%	0.003%
81	13.177	1981	1983	1986	rVV3	275	303	0.02%	0.003%
82	13.591	2047	2051	2056	rBV2	981	1480	0.11%	0.014%
83	13.676	2063	2065	2068	rVB2	604	557	0.04%	0.005%
84	13.707	2068	2070	2072	rBV2	438	437	0.03%	0.004%
85	13.780	2079	2082	2087	rBV2	1457	1691	0.12%	0.016%
86	13.908	2099	2103	2104	rBV3	417	420	0.03%	0.004%
87	13.932	2106	2107	2109	rVV	427	336	0.02%	0.003%
88	13.969	2111	2113	2116	rVV3	729	798	0.06%	0.007%
89	14.140	2138	2141	2143	rBV3	521	411	0.03%	0.004%
90	14.195	2147	2150	2151	rBV	342	301	0.02%	0.003%
91	14.249	2156	2159	2162	rBV	440	596	0.04%	0.006%
92	14.414	2184	2186	2189	rBV2	363	393	0.03%	0.004%
93	14.792	2247	2248	2251	rVB2	404	369	0.03%	0.003%
94	14.999	2280	2282	2284	rBV	365	360	0.03%	0.003%
95	15.213	2315	2317	2319	rBV2	531	390	0.03%	0.004%
96	15.292	2328	2330	2331	rVB	708	288	0.02%	0.003%
97	16.261	2486	2489	2491	rBV2	501	575	0.04%	0.005%
98	16.286	2491	2493	2496	rVB4	721	606	0.04%	0.006%
99	16.341	2501	2502	2503	rBV	582	282	0.02%	0.003%
100	16.670	2554	2556	2559	rBV4	784	765	0.06%	0.007%




Sum of corrected areas: 10830635

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029418.D
Acq On : 13 Jun 2022 17:23
Operator : JC/MD
Sample : N3291-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

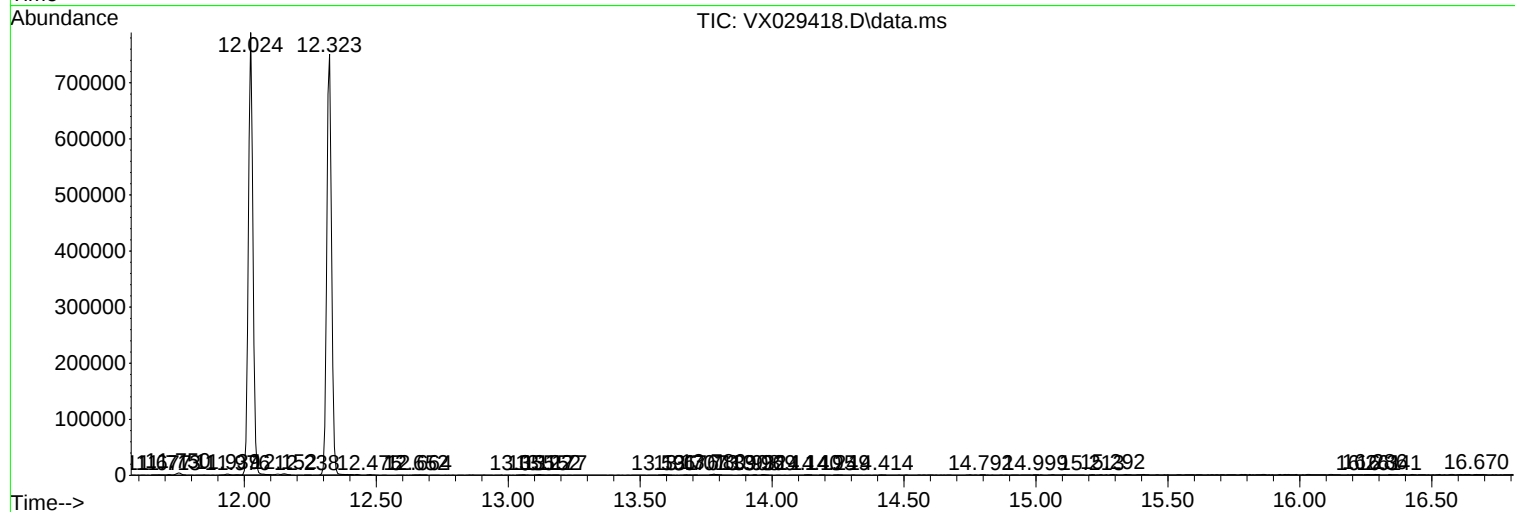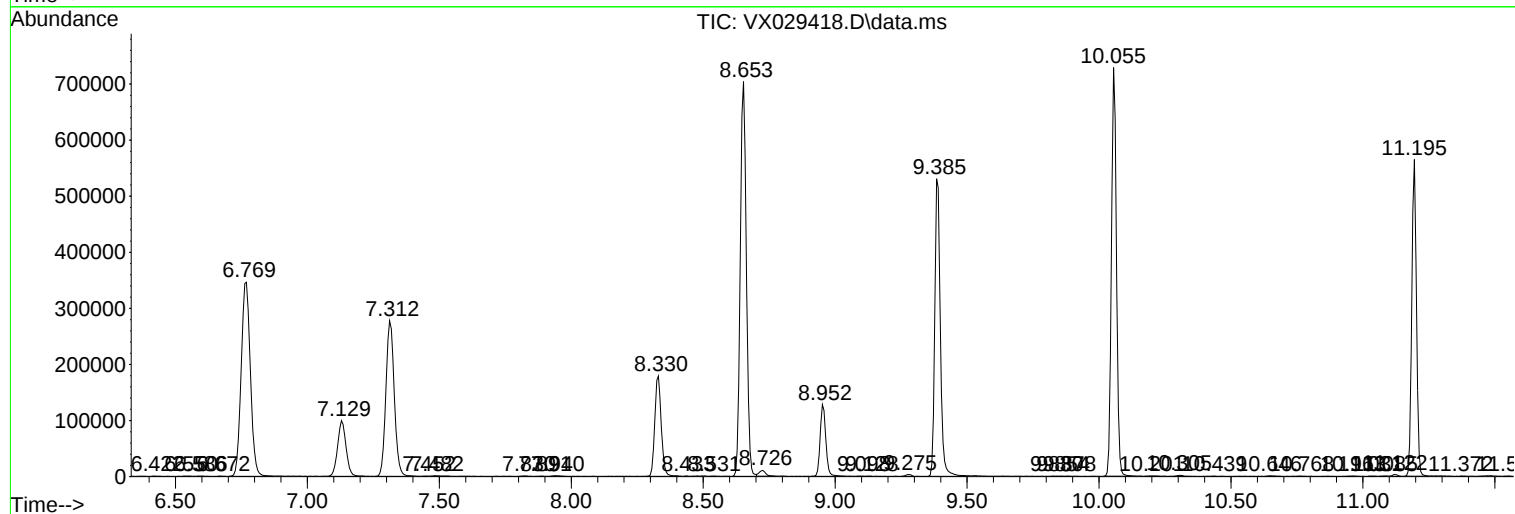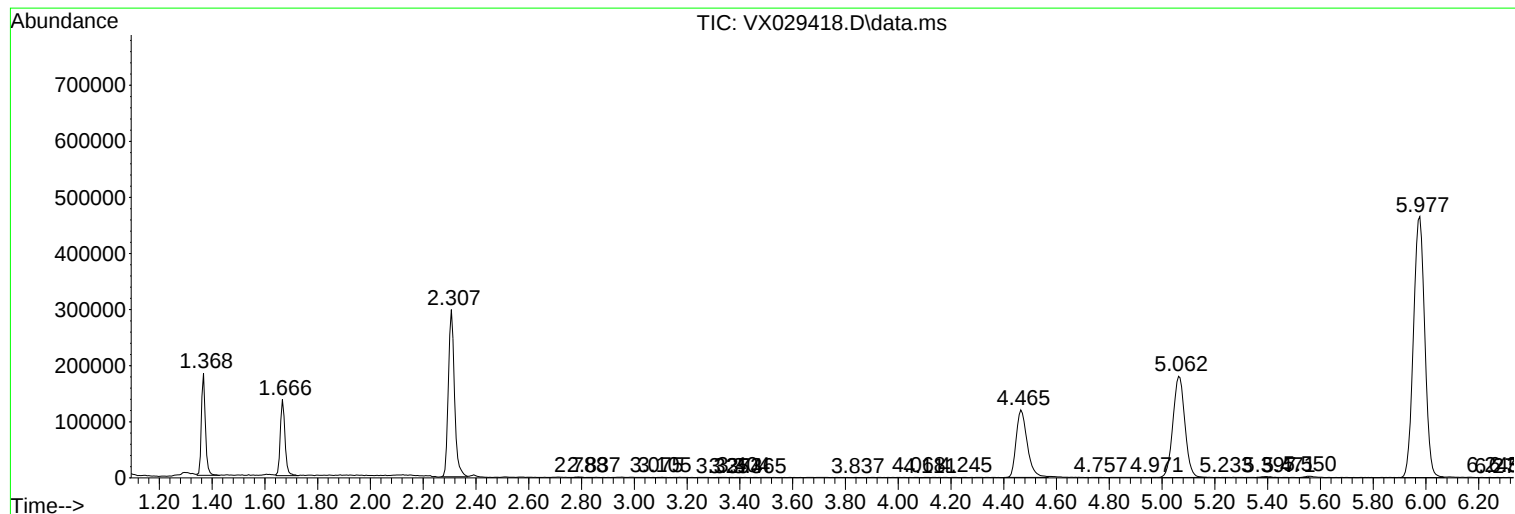

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029418.D
Acq On : 13 Jun 2022 17:23
Operator : JC/MD
Sample : N3291-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029418.D
Acq On : 13 Jun 2022 17:23
Operator : JC/MD
Sample : N3291-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------