

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029419.D
 Acq On : 13 Jun 2022 17:46
 Operator : JC/MD
 Sample : N3291-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029419.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	57	rVB	191497	195657	13.74%	1.791%
2	1.666	91	95	102	rVB	145046	172047	12.09%	1.575%
3	2.306	194	200	210	rBV	303634	481311	33.81%	4.407%
4	2.489	228	230	231	rBV	423	361	0.03%	0.003%
5	2.721	264	268	273	rVB4	665	988	0.07%	0.009%
6	2.794	275	280	284	rVB5	888	1545	0.11%	0.014%
7	2.916	298	300	301	rBV	341	309	0.02%	0.003%
8	2.989	308	312	314	rVB2	409	603	0.04%	0.006%
9	3.178	341	343	344	rBV2	369	255	0.02%	0.002%
10	3.270	357	358	360	rVB	474	267	0.02%	0.002%
11	3.312	362	365	366	rBV3	229	235	0.02%	0.002%
12	3.440	383	386	389	rBV2	229	298	0.02%	0.003%
13	3.471	389	391	396	rBV2	375	276	0.02%	0.003%
14	3.538	401	402	405	rBV2	271	254	0.02%	0.002%
15	3.580	408	409	411	rBV2	289	230	0.02%	0.002%
16	3.605	411	413	414	rBV	459	275	0.02%	0.003%
17	3.708	426	430	432	rVB2	326	393	0.03%	0.004%
18	3.739	432	435	438	rBV2	343	500	0.04%	0.005%
19	3.782	441	442	448	rVB2	460	675	0.05%	0.006%
20	3.843	448	452	453	rBV3	399	557	0.04%	0.005%
21	3.861	453	455	456	rVB	396	261	0.02%	0.002%
22	3.879	456	458	463	rBV2	411	622	0.04%	0.006%
23	3.946	468	469	472	rBV2	249	227	0.02%	0.002%
24	4.123	497	498	500	rVB2	440	260	0.02%	0.002%
25	4.208	510	512	516	rBV3	204	341	0.02%	0.003%
26	4.288	524	525	527	rVB	394	238	0.02%	0.002%
27	4.330	529	532	534	rBV2	360	438	0.03%	0.004%
28	4.385	540	541	545	rBV2	307	367	0.03%	0.003%
29	4.464	545	554	571	rBV	125868	360751	25.34%	3.303%
30	4.836	613	615	617	rBV3	272	242	0.02%	0.002%
31	5.062	639	652	672	rBV	186009	576724	40.51%	5.280%
32	5.397	701	707	714	rVB5	1247	3308	0.23%	0.030%
33	5.452	714	716	719	rBV2	263	318	0.02%	0.003%
34	5.550	726	732	733	rBV4	1602	2290	0.16%	0.021%
35	5.976	789	802	820	rBV2	481897	1423508	100.00%	13.033%
36	6.403	871	872	875	rBV3	279	268	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029419.D
 Acq On : 13 Jun 2022 17:46
 Operator : JC/MD
 Sample : N3291-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	6.525	887	892	893	rVV2	294	480	0.03%	0.004%
38	6.616	906	907	912	rVB	288	263	0.02%	0.002%
39	6.671	912	916	917	rVB2	311	271	0.02%	0.002%
40	6.763	922	931	945	rBV	343828	830478	58.34%	7.603%
41	6.988	966	968	969	rVB	398	230	0.02%	0.002%
42	7.129	982	991	1002	rVB4	37656	88993	6.25%	0.815%
43	7.311	1012	1021	1036	rBV	288539	625675	43.95%	5.728%
44	7.482	1047	1049	1054	rBV5	796	1012	0.07%	0.009%
45	7.738	1087	1091	1092	rBV2	346	406	0.03%	0.004%
46	7.817	1102	1104	1110	rVB3	541	891	0.06%	0.008%
47	7.933	1120	1123	1131	rVV4	1077	2227	0.16%	0.020%
48	8.037	1137	1140	1141	rBV	333	298	0.02%	0.003%
49	8.330	1181	1188	1199	rBV	190121	312488	21.95%	2.861%
50	8.653	1234	1241	1249	rBV	746108	1156205	81.22%	10.586%
51	8.726	1249	1253	1262	rVB	10357	17121	1.20%	0.157%
52	8.866	1274	1276	1278	rVB2	389	242	0.02%	0.002%
53	8.951	1285	1290	1302	rBV	129499	193830	13.62%	1.775%
54	9.134	1316	1320	1322	rBV2	362	477	0.03%	0.004%
55	9.177	1325	1327	1329	rBV	256	236	0.02%	0.002%
56	9.275	1339	1343	1348	rBV4	3251	4635	0.33%	0.042%
57	9.384	1356	1361	1377	rBV	539680	808502	56.80%	7.402%
58	9.841	1433	1436	1437	rBV2	243	227	0.02%	0.002%
59	9.878	1439	1442	1443	rBV	329	223	0.02%	0.002%
60	10.055	1466	1471	1486	rVB	737258	964423	67.75%	8.830%
61	10.238	1499	1501	1503	rBV2	328	222	0.02%	0.002%
62	10.305	1508	1512	1517	rBV3	1858	2553	0.18%	0.023%
63	10.427	1530	1532	1534	rVB3	410	396	0.03%	0.004%
64	10.451	1534	1536	1539	rBV2	331	400	0.03%	0.004%
65	10.494	1539	1543	1546	rBV3	221	431	0.03%	0.004%
66	10.652	1564	1569	1573	rBV4	785	1587	0.11%	0.015%
67	11.085	1638	1640	1643	rBV2	701	942	0.07%	0.009%
68	11.122	1643	1646	1650	rVB	3375	3940	0.28%	0.036%
69	11.195	1652	1658	1666	rBV	578712	719391	50.54%	6.586%
70	11.372	1685	1687	1689	rBV2	294	221	0.02%	0.002%
71	11.481	1699	1705	1707	rBV4	1009	1651	0.12%	0.015%
72	11.616	1723	1727	1729	rBV2	409	490	0.03%	0.004%
73	11.713	1741	1743	1745	rBV3	634	586	0.04%	0.005%
74	11.756	1745	1750	1753	rVV5	3113	4303	0.30%	0.039%
75	11.835	1760	1763	1764	rBV2	370	387	0.03%	0.004%
76	11.933	1776	1779	1783	rVB3	1455	1867	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029419.D
 Acq On : 13 Jun 2022 17:46
 Operator : JC/MD
 Sample : N3291-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.981	1783	1787	1789	rBV3	792	1057	0.07%	0.010%
78	12.024	1789	1794	1806	rVB	775043	945542	66.42%	8.657%
79	12.323	1837	1843	1850	rBV	801813	988555	69.44%	9.051%
80	12.426	1858	1860	1866	rVB5	1186	1062	0.07%	0.010%
81	12.481	1866	1869	1870	rBV2	694	609	0.04%	0.006%
82	12.579	1884	1885	1888	rBV2	348	306	0.02%	0.003%
83	12.658	1896	1898	1902	rBV3	498	676	0.05%	0.006%
84	12.859	1924	1931	1935	rVB3	367	852	0.06%	0.008%
85	12.908	1937	1939	1941	rBV2	265	230	0.02%	0.002%
86	12.969	1947	1949	1950	rBV	447	330	0.02%	0.003%
87	13.054	1960	1963	1967	rVV4	509	716	0.05%	0.007%
88	13.115	1971	1973	1975	rBV2	943	792	0.06%	0.007%
89	13.219	1987	1990	1993	rBV2	347	417	0.03%	0.004%
90	13.249	1993	1995	1997	rBV	217	227	0.02%	0.002%
91	13.420	2020	2023	2024	rBV3	294	346	0.02%	0.003%
92	13.530	2039	2041	2042	rBV2	347	294	0.02%	0.003%
93	13.591	2049	2051	2053	rVB2	649	442	0.03%	0.004%
94	13.701	2067	2069	2072	rVB2	412	292	0.02%	0.003%
95	13.780	2080	2082	2085	rVB3	746	678	0.05%	0.006%
96	13.810	2085	2087	2091	rVB3	383	489	0.03%	0.004%
97	13.963	2110	2112	2116	rVB2	518	519	0.04%	0.005%
98	14.548	2206	2208	2212	rVB3	345	471	0.03%	0.004%
99	14.828	2252	2254	2255	rVB2	491	304	0.02%	0.003%
100	15.755	2403	2406	2409	rBV3	515	872	0.06%	0.008%


Sum of corrected areas: 10922477

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029419.D
Acq On : 13 Jun 2022 17:46
Operator : JC/MD
Sample : N3291-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

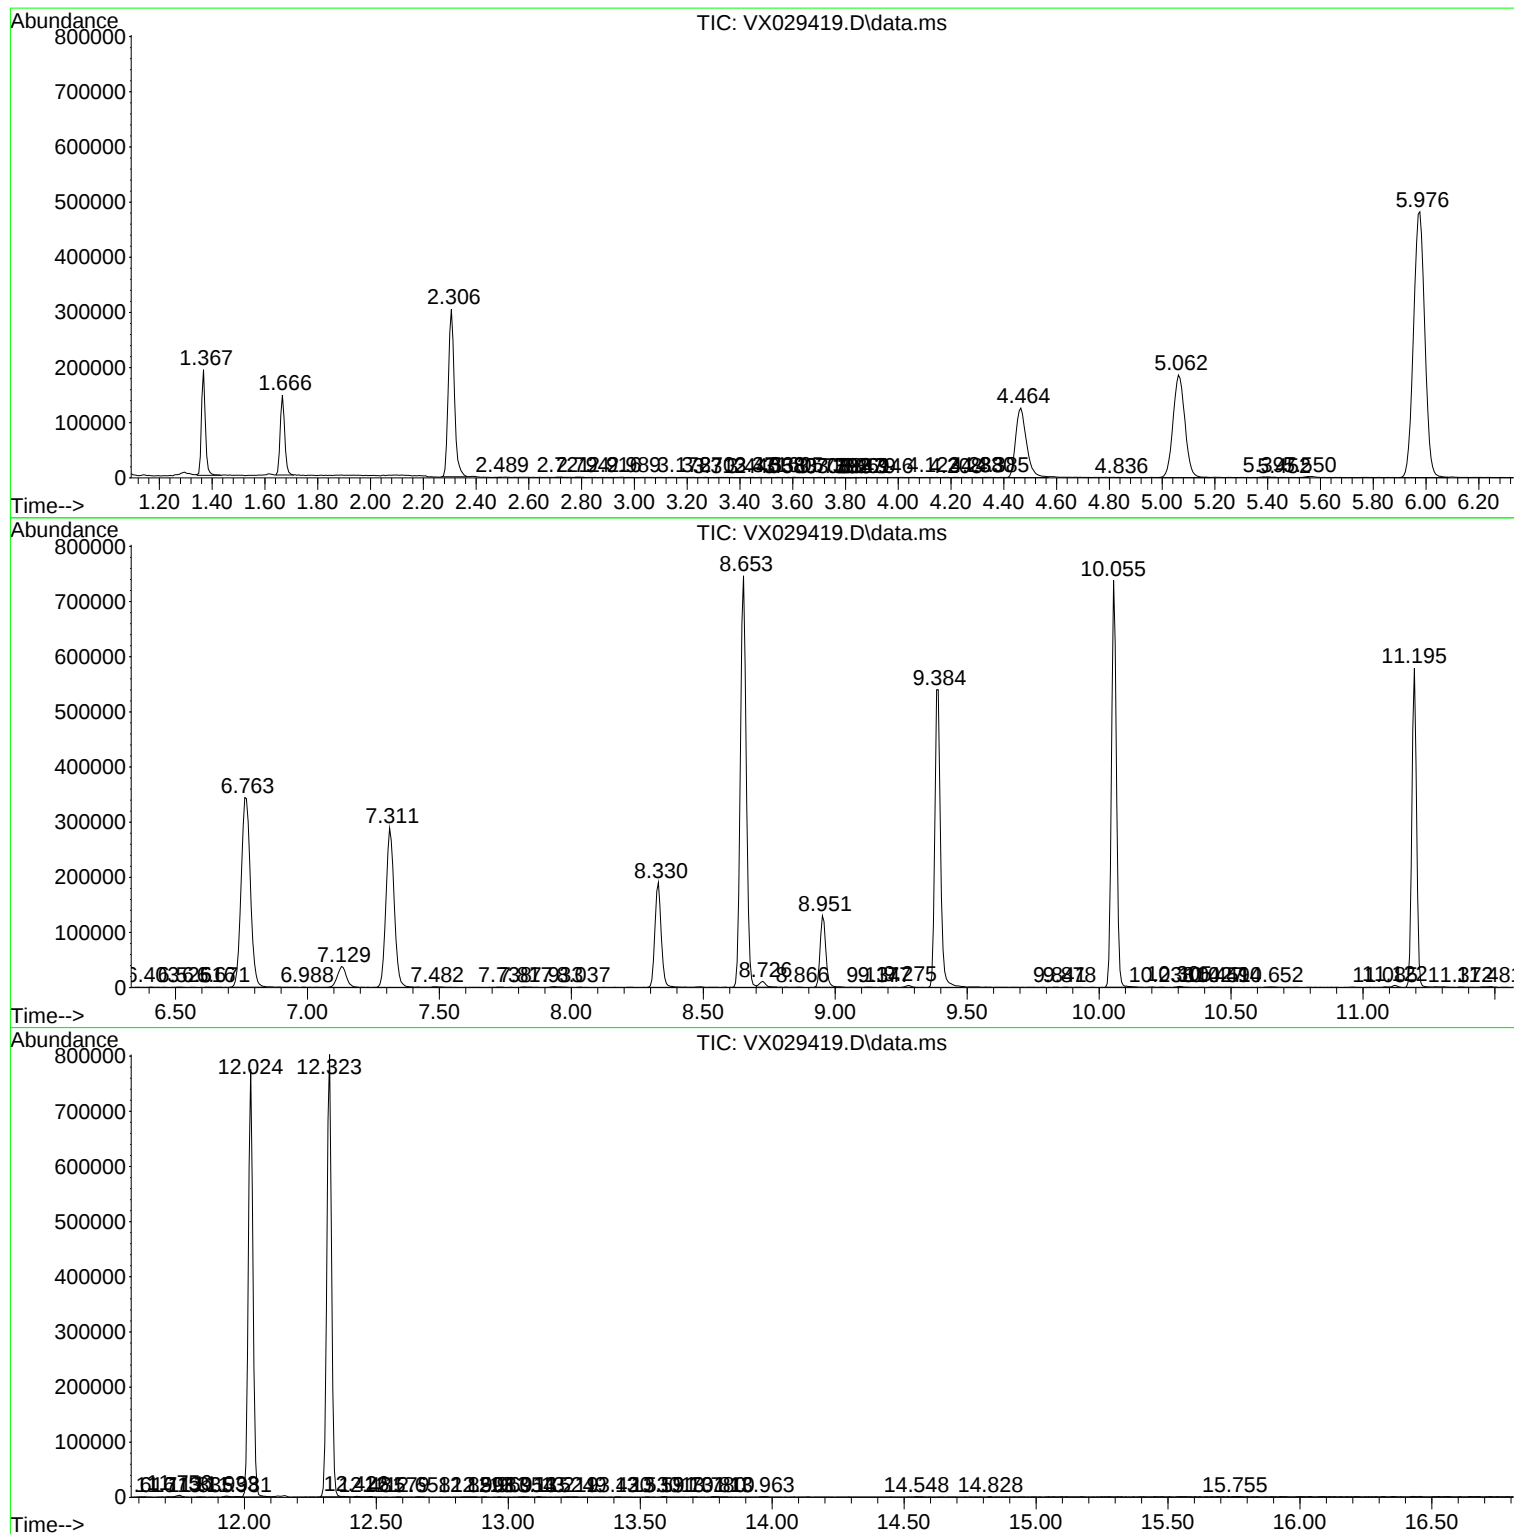

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029419.D
Acq On : 13 Jun 2022 17:46
Operator : JC/MD
Sample : N3291-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029419.D
Acq On : 13 Jun 2022 17:46
Operator : JC/MD
Sample : N3291-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
