

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029420.D
 Acq On : 13 Jun 2022 18:09
 Operator : JC/MD
 Sample : N3291-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CODY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029420.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	188390	192108	13.66%	1.613%
2	1.666	91	95	105	rVB	146320	174381	12.40%	1.464%
3	2.306	194	200	210	rBV2	315151	528113	37.55%	4.433%
4	2.569	239	243	244	rBV2	654	872	0.06%	0.007%
5	3.227	350	351	356	rVB3	381	305	0.02%	0.003%
6	3.270	356	358	361	rBV3	224	260	0.02%	0.002%
7	3.318	364	366	368	rBV	249	311	0.02%	0.003%
8	3.459	388	389	393	rBV2	252	421	0.03%	0.004%
9	3.617	411	415	420	rVB5	839	1604	0.11%	0.013%
10	3.703	428	429	431	rBV2	298	246	0.02%	0.002%
11	3.983	473	475	477	rBV	326	262	0.02%	0.002%
12	4.007	477	479	482	rVV2	319	301	0.02%	0.003%
13	4.062	486	488	490	rVB2	341	307	0.02%	0.003%
14	4.184	505	508	509	rBV3	248	269	0.02%	0.002%
15	4.294	520	526	528	rVB2	441	648	0.05%	0.005%
16	4.318	528	530	533	rBV2	272	366	0.03%	0.003%
17	4.465	545	554	571	rBV	128746	408970	29.08%	3.433%
18	4.788	605	607	608	rBV2	541	372	0.03%	0.003%
19	4.818	611	612	615	rBV	404	361	0.03%	0.003%
20	5.062	640	652	668	rBV	181632	574063	40.82%	4.819%
21	5.385	696	705	716	rVB4	5829	17976	1.28%	0.151%
22	5.464	716	718	723	rBV2	285	365	0.03%	0.003%
23	5.781	767	770	772	rVB2	334	383	0.03%	0.003%
24	5.873	784	785	788	rVB2	471	356	0.03%	0.003%
25	5.970	788	801	822	rBV2	473493	1406385	100.00%	11.805%
26	6.147	828	830	832	rVB2	425	386	0.03%	0.003%
27	6.184	832	836	837	rBV	448	393	0.03%	0.003%
28	6.379	864	868	873	rBV3	450	589	0.04%	0.005%
29	6.464	881	882	885	rBV2	293	259	0.02%	0.002%
30	6.489	885	886	889	rBV3	393	292	0.02%	0.002%
31	6.544	894	895	901	rVB2	515	552	0.04%	0.005%
32	6.763	922	931	945	rBV	345079	819869	58.30%	6.882%
33	7.129	982	991	1003	rBV	490210	1049065	74.59%	8.806%
34	7.312	1012	1021	1035	rBV	284430	620478	44.12%	5.208%
35	7.488	1046	1050	1053	rBV3	906	1255	0.09%	0.011%
36	7.556	1060	1061	1063	rVB	460	278	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029420.D
 Acq On : 13 Jun 2022 18:09
 Operator : JC/MD
 Sample : N3291-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CODY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.604	1068	1069	1074	rVB	310	341	0.02%	0.003%
38	7.818	1099	1104	1110	rBV3	696	1660	0.12%	0.014%
39	7.891	1113	1116	1117	rBV2	358	362	0.03%	0.003%
40	7.946	1120	1125	1129	rVV4	1050	2159	0.15%	0.018%
41	8.049	1140	1142	1147	rVB2	217	270	0.02%	0.002%
42	8.129	1149	1155	1156	rBV	313	453	0.03%	0.004%
43	8.214	1167	1169	1170	rBV	352	340	0.02%	0.003%
44	8.251	1174	1175	1178	rVV2	405	340	0.02%	0.003%
45	8.330	1181	1188	1202	rBV	191784	310603	22.09%	2.607%
46	8.494	1211	1215	1220	rVB5	790	1616	0.11%	0.014%
47	8.592	1230	1231	1234	rVB2	311	254	0.02%	0.002%
48	8.653	1234	1241	1249	rBV	733316	1136926	80.84%	9.543%
49	8.720	1249	1252	1261	rVB	10469	18317	1.30%	0.154%
50	8.952	1285	1290	1304	rBV	134046	191832	13.64%	1.610%
51	9.067	1307	1309	1310	rBV	323	249	0.02%	0.002%
52	9.202	1329	1331	1335	rBV2	270	400	0.03%	0.003%
53	9.281	1339	1344	1348	rVB3	3492	5039	0.36%	0.042%
54	9.330	1348	1352	1354	rBV2	205	274	0.02%	0.002%
55	9.391	1356	1362	1383	rBV	541082	800919	56.95%	6.723%
56	9.714	1414	1415	1418	rVB2	590	384	0.03%	0.003%
57	9.890	1442	1444	1447	rBV	318	388	0.03%	0.003%
58	10.055	1465	1471	1482	rBV	722323	960617	68.30%	8.063%
59	10.201	1492	1495	1499	rVB3	947	1037	0.07%	0.009%
60	10.305	1508	1512	1516	rBV2	2080	2215	0.16%	0.019%
61	10.445	1533	1535	1537	rBV2	253	289	0.02%	0.002%
62	10.494	1541	1543	1545	rBV2	421	409	0.03%	0.003%
63	10.640	1565	1567	1570	rBV4	622	859	0.06%	0.007%
64	10.805	1591	1594	1595	rBV	396	340	0.02%	0.003%
65	10.848	1598	1601	1603	rVB2	277	246	0.02%	0.002%
66	10.963	1617	1620	1623	rVB2	750	775	0.06%	0.007%
67	11.067	1633	1637	1638	rBV	374	355	0.03%	0.003%
68	11.085	1638	1640	1643	rVV3	982	1060	0.08%	0.009%
69	11.122	1643	1646	1650	rVB3	2859	4005	0.28%	0.034%
70	11.195	1652	1658	1670	rVV	569058	718283	51.07%	6.029%
71	11.274	1670	1671	1682	rVB4	946	2177	0.15%	0.018%
72	11.433	1695	1697	1698	rBV	294	283	0.02%	0.002%
73	11.591	1720	1723	1724	rBV	306	361	0.03%	0.003%
74	11.719	1741	1744	1745	rBV	474	590	0.04%	0.005%
75	11.750	1746	1749	1754	rVB4	3693	5049	0.36%	0.042%
76	11.841	1760	1764	1769	rBV4	611	1042	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029420.D
 Acq On : 13 Jun 2022 18:09
 Operator : JC/MD
 Sample : N3291-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CODY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.884	1769	1771	1774	rVB	515	330	0.02%	0.003%
78	11.933	1776	1779	1783	rBV3	1913	1710	0.12%	0.014%
79	11.975	1783	1786	1788	rVB3	649	618	0.04%	0.005%
80	12.024	1788	1794	1807	rBV	785206	945913	67.26%	7.940%
81	12.323	1835	1843	1853	rBV	799700	977825	69.53%	8.208%
82	12.427	1857	1860	1864	rVB4	1117	1185	0.08%	0.010%
83	12.652	1896	1897	1898	rBV	459	295	0.02%	0.002%
84	12.738	1909	1911	1914	rVB	323	297	0.02%	0.002%
85	12.811	1921	1923	1926	rVB2	389	328	0.02%	0.003%
86	13.116	1970	1973	1978	rBV4	546	724	0.05%	0.006%
87	13.347	2009	2011	2013	rBV	391	300	0.02%	0.003%
88	13.597	2049	2052	2058	rVB3	669	834	0.06%	0.007%
89	13.689	2065	2067	2070	rBV3	234	314	0.02%	0.003%
90	13.780	2080	2082	2087	rVB2	814	690	0.05%	0.006%
91	13.871	2096	2097	2099	rBV2	344	241	0.02%	0.002%
92	13.969	2111	2113	2117	rVB3	505	509	0.04%	0.004%
93	14.890	2261	2264	2266	rBV3	420	484	0.03%	0.004%
94	14.987	2278	2280	2282	rBV3	461	517	0.04%	0.004%
95	15.652	2387	2389	2390	rBV2	445	326	0.02%	0.003%
96	15.670	2390	2392	2394	rVV3	705	569	0.04%	0.005%
97	16.420	2514	2515	2517	rVB2	599	296	0.02%	0.002%
98	16.438	2517	2518	2520	rBV2	777	621	0.04%	0.005%
99	16.560	2535	2538	2540	rBV3	788	1197	0.09%	0.010%
100	16.694	2558	2560	2563	rBV3	545	505	0.04%	0.004%


Sum of corrected areas: 11913167

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029420.D
Acq On : 13 Jun 2022 18:09
Operator : JC/MD
Sample : N3291-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

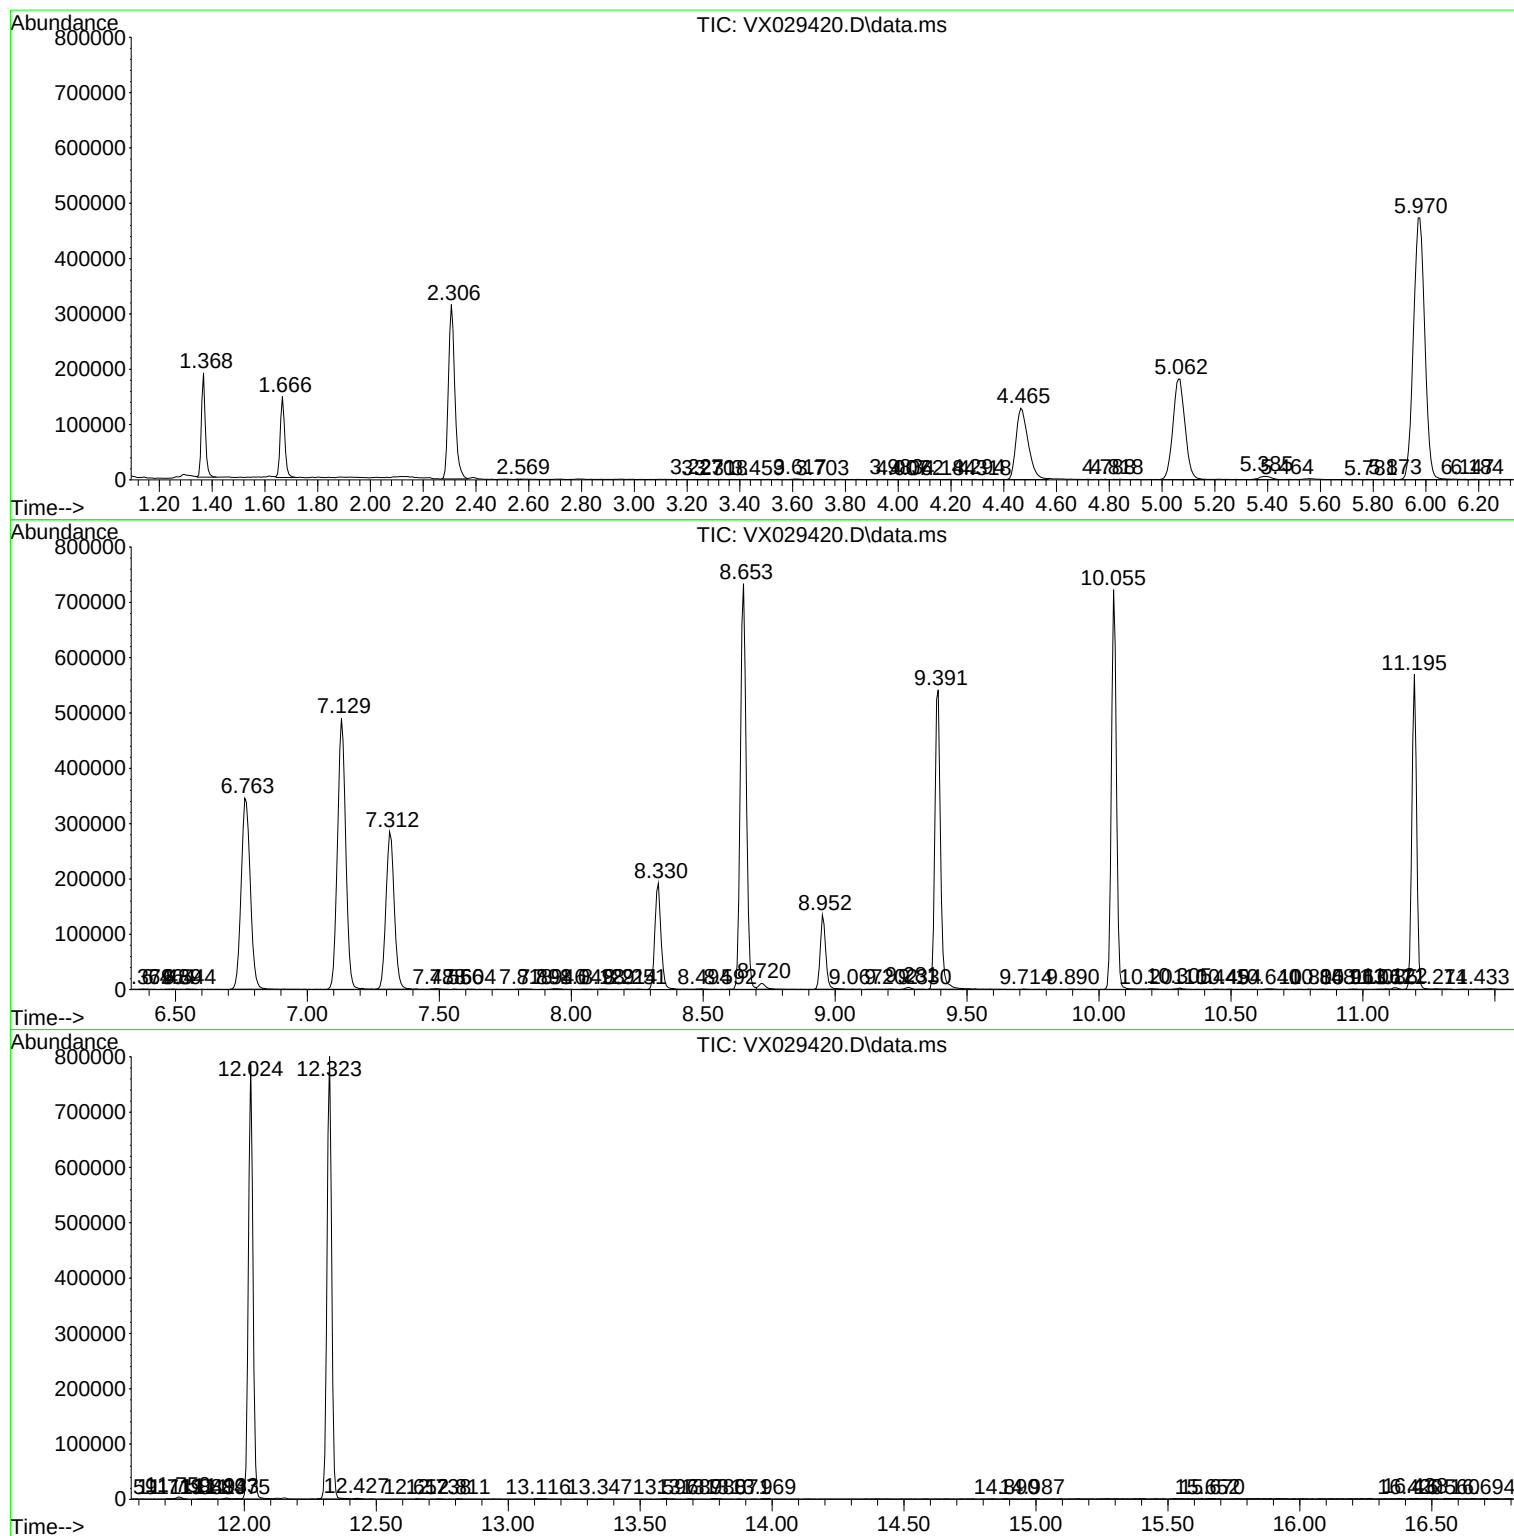

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029420.D
Acq On : 13 Jun 2022 18:09
Operator : JC/MD
Sample : N3291-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029420.D
Acq On : 13 Jun 2022 18:09
Operator : JC/MD
Sample : N3291-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc