

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029422.D
 Acq On : 13 Jun 2022 18:56
 Operator : JC/MD
 Sample : N3291-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CODY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rVB	188506	192295	13.57%	1.650%
2	1.666	91	95	104	rVB	143653	172950	12.20%	1.484%
3	2.306	194	200	210	rBV2	315709	518856	36.61%	4.451%
4	2.386	210	213	224	rVB	5565	10398	0.73%	0.089%
5	2.794	277	280	285	rVB3	801	1358	0.10%	0.012%
6	2.879	292	294	296	rBV2	373	299	0.02%	0.003%
7	2.947	300	305	310	rBV2	699	1172	0.08%	0.010%
8	3.568	404	407	408	rBV2	257	307	0.02%	0.003%
9	3.617	410	415	417	rBV4	1001	1595	0.11%	0.014%
10	3.928	462	466	468	rBV2	266	376	0.03%	0.003%
11	4.111	495	496	499	rBV2	350	324	0.02%	0.003%
12	4.215	511	513	517	rBV2	264	321	0.02%	0.003%
13	4.318	528	530	534	rVB3	233	314	0.02%	0.003%
14	4.361	534	537	541	rBV2	282	437	0.03%	0.004%
15	4.465	544	554	572	rBV	127692	405948	28.65%	3.482%
16	4.836	614	615	619	rVB3	337	418	0.03%	0.004%
17	4.879	619	622	625	rBV3	243	336	0.02%	0.003%
18	4.910	625	627	631	rVB2	359	306	0.02%	0.003%
19	4.958	631	635	637	rBV3	201	287	0.02%	0.002%
20	4.983	637	639	640	rBV	388	276	0.02%	0.002%
21	5.062	640	652	672	rVV	183897	573193	40.45%	4.917%
22	5.288	686	689	692	rBV3	279	329	0.02%	0.003%
23	5.397	698	707	716	rVB3	8227	24052	1.70%	0.206%
24	5.562	727	734	739	rBV4	1421	3487	0.25%	0.030%
25	5.751	760	765	766	rVB2	273	395	0.03%	0.003%
26	5.794	768	772	773	rBV2	291	352	0.02%	0.003%
27	5.976	788	802	818	rBV2	482317	1417125	100.00%	12.156%
28	6.208	838	840	843	rBV2	248	296	0.02%	0.003%
29	6.354	860	864	867	rBV2	519	755	0.05%	0.006%
30	6.409	870	873	874	rBV2	433	473	0.03%	0.004%
31	6.763	921	931	945	rBV	348923	836395	59.02%	7.175%
32	7.129	980	991	1004	rVV	339758	739819	52.21%	6.346%
33	7.312	1012	1021	1037	rBV	283440	623682	44.01%	5.350%
34	7.476	1046	1048	1049	rBV2	781	485	0.03%	0.004%
35	7.726	1086	1089	1092	rBV2	263	380	0.03%	0.003%
36	7.824	1098	1105	1107	rBV4	752	1439	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029422.D
 Acq On : 13 Jun 2022 18:56
 Operator : JC/MD
 Sample : N3291-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CODY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.848	1107	1109	1113	rVB2	462	527	0.04%	0.005%
38	7.885	1113	1115	1117	rBV2	451	472	0.03%	0.004%
39	7.933	1120	1123	1124	rBV3	815	729	0.05%	0.006%
40	8.043	1139	1141	1144	rVB2	415	395	0.03%	0.003%
41	8.153	1156	1159	1167	rVB3	298	544	0.04%	0.005%
42	8.330	1181	1188	1200	rVV	188734	306630	21.64%	2.630%
43	8.446	1205	1207	1209	rVB	551	429	0.03%	0.004%
44	8.482	1209	1213	1214	rBV2	863	1056	0.07%	0.009%
45	8.586	1228	1230	1233	rBV2	369	395	0.03%	0.003%
46	8.653	1233	1241	1249	rVV	745748	1147725	80.99%	9.845%
47	8.726	1249	1253	1261	rVB	10665	18545	1.31%	0.159%
48	8.885	1277	1279	1282	rVB2	333	261	0.02%	0.002%
49	8.952	1285	1290	1300	rVV	130893	192122	13.56%	1.648%
50	9.159	1319	1324	1326	rBV3	476	790	0.06%	0.007%
51	9.232	1334	1336	1339	rBV2	252	269	0.02%	0.002%
52	9.275	1339	1343	1349	rVV3	3218	4394	0.31%	0.038%
53	9.384	1356	1361	1376	rBV	540908	803359	56.69%	6.891%
54	9.531	1383	1385	1388	rVB2	714	585	0.04%	0.005%
55	9.634	1400	1402	1404	rBV3	344	323	0.02%	0.003%
56	9.677	1407	1409	1412	rBV3	307	385	0.03%	0.003%
57	9.836	1431	1435	1436	rBV2	468	418	0.03%	0.004%
58	9.890	1442	1444	1447	rBV2	452	460	0.03%	0.004%
59	9.976	1455	1458	1460	rBV	410	453	0.03%	0.004%
60	10.055	1465	1471	1482	rBV	730718	971560	68.56%	8.334%
61	10.305	1509	1512	1521	rVB4	1983	3420	0.24%	0.029%
62	10.403	1526	1528	1531	rVV2	325	287	0.02%	0.002%
63	10.463	1534	1538	1539	rBV2	309	323	0.02%	0.003%
64	10.555	1551	1553	1556	rBV3	313	395	0.03%	0.003%
65	10.652	1566	1569	1575	rBV4	595	1038	0.07%	0.009%
66	10.713	1577	1579	1582	rVB2	323	357	0.03%	0.003%
67	10.866	1602	1604	1607	rBV3	487	539	0.04%	0.005%
68	10.969	1619	1621	1623	rVB	722	325	0.02%	0.003%
69	11.024	1629	1630	1633	rBV2	329	383	0.03%	0.003%
70	11.091	1637	1641	1642	rBV3	623	719	0.05%	0.006%
71	11.122	1642	1646	1650	rVB2	2603	3284	0.23%	0.028%
72	11.195	1652	1658	1667	rBV	569878	712671	50.29%	6.113%
73	11.457	1697	1701	1702	rBV3	647	638	0.05%	0.005%
74	11.482	1702	1705	1708	rVV4	868	1035	0.07%	0.009%
75	11.573	1718	1720	1722	rVB2	423	336	0.02%	0.003%
76	11.610	1722	1726	1728	rBV3	563	776	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029422.D
 Acq On : 13 Jun 2022 18:56
 Operator : JC/MD
 Sample : N3291-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CODY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.750	1745	1749	1755	rVB3	4011	5412	0.38%	0.046%
78	11.841	1761	1764	1766	rVB2	454	493	0.03%	0.004%
79	11.939	1776	1780	1782	rBB3	1305	1539	0.11%	0.013%
80	11.969	1782	1785	1788	rVB3	489	595	0.04%	0.005%
81	12.024	1788	1794	1804	rBV	790278	952108	67.19%	8.167%
82	12.250	1830	1831	1832	rBV	456	288	0.02%	0.002%
83	12.323	1836	1843	1858	rVV	775701	979107	69.09%	8.399%
84	12.658	1896	1898	1902	rBV3	428	572	0.04%	0.005%
85	12.750	1911	1913	1914	rBV	279	257	0.02%	0.002%
86	12.866	1928	1932	1935	rVB4	320	443	0.03%	0.004%
87	12.975	1949	1950	1955	rVB	396	332	0.02%	0.003%
88	13.054	1960	1963	1966	rBV2	380	475	0.03%	0.004%
89	13.115	1972	1973	1978	rVB3	514	539	0.04%	0.005%
90	13.219	1988	1990	1993	rBV2	359	442	0.03%	0.004%
91	13.292	1999	2002	2003	rBV	245	260	0.02%	0.002%
92	13.524	2038	2040	2043	rVB	401	404	0.03%	0.003%
93	13.786	2082	2083	2085	rVB2	944	440	0.03%	0.004%
94	13.902	2101	2102	2103	rBV	414	277	0.02%	0.002%
95	13.938	2106	2108	2109	rBV	311	275	0.02%	0.002%
96	14.018	2119	2121	2123	rBV3	330	330	0.02%	0.003%
97	14.225	2154	2155	2157	rBV	456	498	0.04%	0.004%
98	14.298	2162	2167	2169	rBV3	450	744	0.05%	0.006%
99	15.463	2357	2358	2361	rBV3	478	442	0.03%	0.004%
100	16.005	2446	2447	2450	rBV3	670	706	0.05%	0.006%




Sum of corrected areas: 11657560

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029422.D
Acq On : 13 Jun 2022 18:56
Operator : JC/MD
Sample : N3291-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CODY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

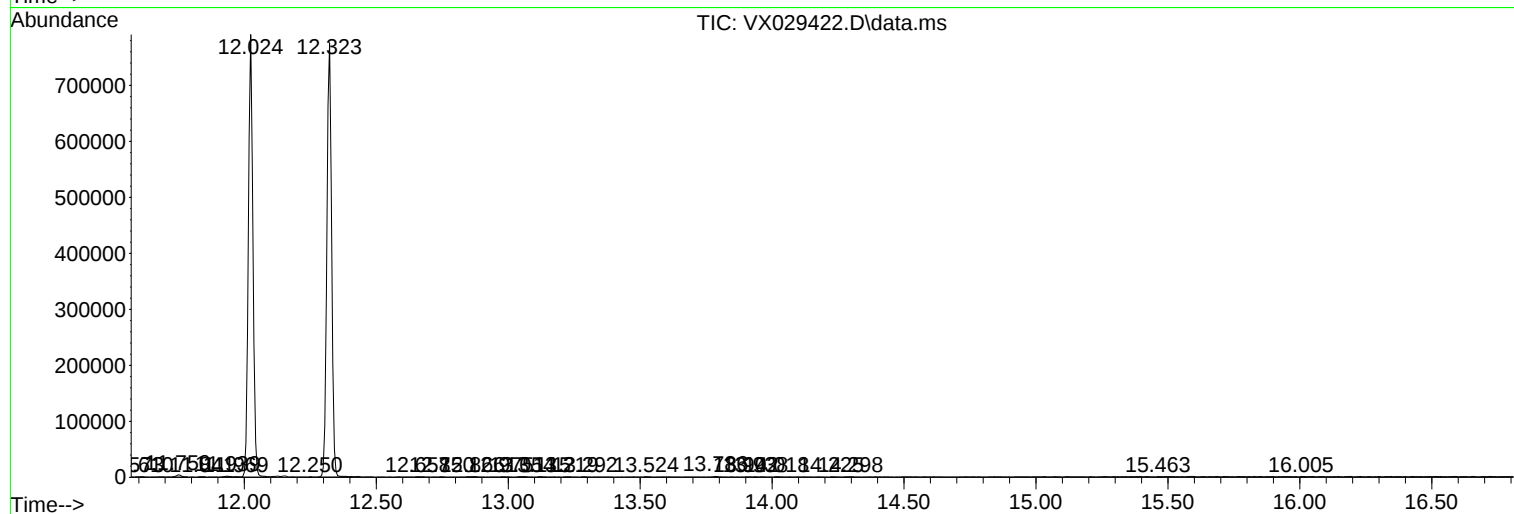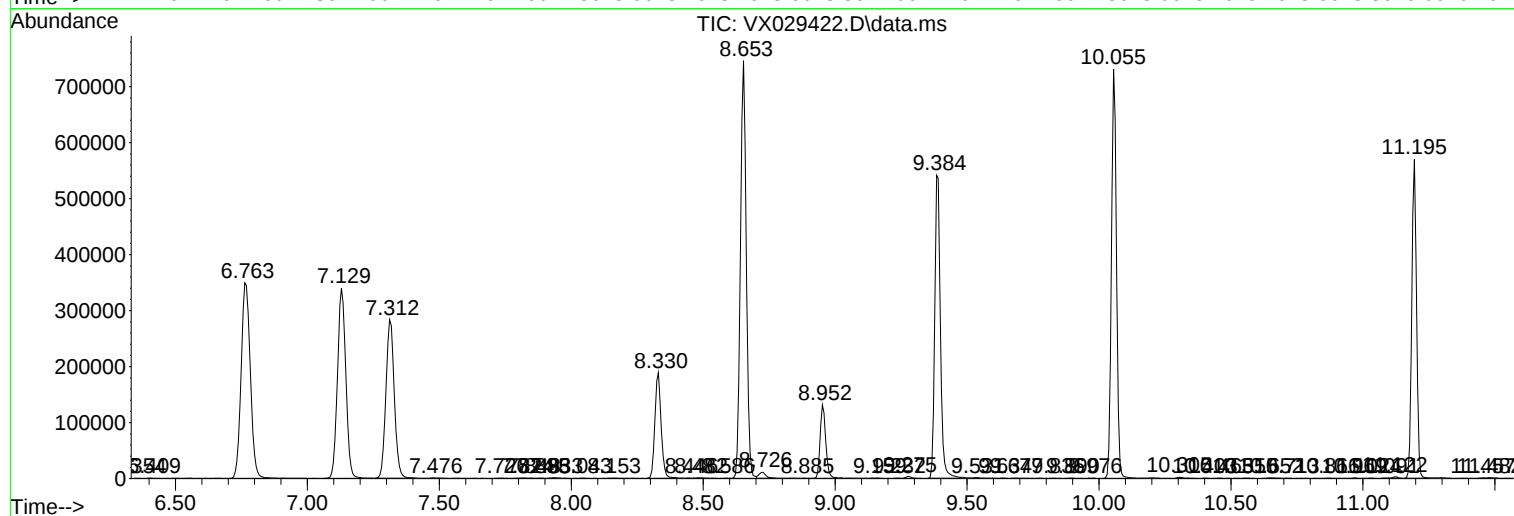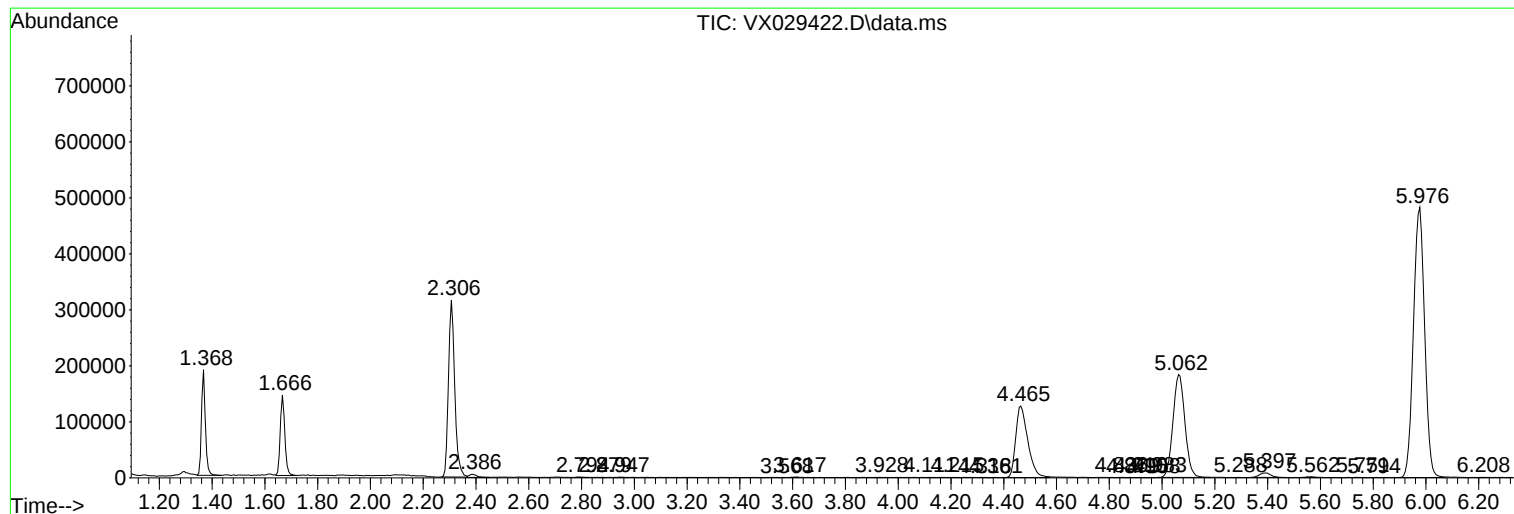

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029422.D
Acq On : 13 Jun 2022 18:56
Operator : JC/MD
Sample : N3291-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029422.D
Acq On : 13 Jun 2022 18:56
Operator : JC/MD
Sample : N3291-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------