

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029423.D
 Acq On : 13 Jun 2022 19:19
 Operator : JC/MD
 Sample : N3291-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CODY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029423.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	190837	193365	13.84%	1.797%
2	1.666	91	95	105	rVB	144631	169704	12.14%	1.577%
3	2.306	194	200	210	rBV	297809	472947	33.84%	4.396%
4	2.709	263	266	270	rVB4	598	874	0.06%	0.008%
5	2.898	295	297	300	rVB	365	277	0.02%	0.003%
6	3.062	322	324	326	rBV2	591	480	0.03%	0.004%
7	3.136	334	336	338	rBV	483	288	0.02%	0.003%
8	3.209	346	348	351	rBV3	262	362	0.03%	0.003%
9	3.355	370	372	374	rBV2	255	240	0.02%	0.002%
10	3.532	399	401	402	rBV	434	293	0.02%	0.003%
11	3.575	406	408	411	rBV2	328	339	0.02%	0.003%
12	3.648	419	420	421	rBV	483	240	0.02%	0.002%
13	3.745	435	436	440	rVB2	289	250	0.02%	0.002%
14	3.861	452	455	456	rBV	323	306	0.02%	0.003%
15	3.995	475	477	479	rBV3	319	366	0.03%	0.003%
16	4.148	501	502	507	rVB2	410	320	0.02%	0.003%
17	4.367	535	538	541	rBV2	265	375	0.03%	0.003%
18	4.465	544	554	573	rBV	120704	357281	25.56%	3.321%
19	4.867	619	620	637	rBV2	325	256	0.02%	0.002%
20	4.946	632	633	637	rVB2	346	350	0.03%	0.003%
21	4.983	637	639	640	rBV	375	318	0.02%	0.003%
22	5.062	640	652	668	rVV	185961	573944	41.07%	5.335%
23	5.239	680	681	683	rVB	474	241	0.02%	0.002%
24	5.257	683	684	687	rBV2	324	275	0.02%	0.003%
25	5.391	703	706	713	rVB4	716	1406	0.10%	0.013%
26	5.977	789	802	818	rBV2	474808	1397618	100.00%	12.991%
27	6.483	883	885	886	rBV2	314	244	0.02%	0.002%
28	6.611	904	906	908	rVB	382	345	0.02%	0.003%
29	6.629	908	909	911	rBV	272	280	0.02%	0.003%
30	6.763	922	931	946	rVV	344432	824433	58.99%	7.663%
31	7.031	974	975	978	rBV2	361	431	0.03%	0.004%
32	7.129	981	991	1001	rBV4	38079	88108	6.30%	0.819%
33	7.214	1003	1005	1006	rBV	467	283	0.02%	0.003%
34	7.312	1012	1021	1040	rBV	283755	619512	44.33%	5.758%
35	7.476	1046	1048	1049	rBV2	501	386	0.03%	0.004%
36	7.696	1082	1084	1087	rVB2	412	324	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029423.D
 Acq On : 13 Jun 2022 19:19
 Operator : JC/MD
 Sample : N3291-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CODY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.769	1093	1096	1097	rBV2	255	249	0.02%	0.002%
38	7.824	1102	1105	1107	rVV3	382	485	0.03%	0.005%
39	7.934	1121	1123	1128	rVV4	998	1690	0.12%	0.016%
40	8.007	1132	1135	1139	rBV3	438	671	0.05%	0.006%
41	8.171	1160	1162	1164	rBV	406	413	0.03%	0.004%
42	8.263	1175	1177	1179	rBV2	229	264	0.02%	0.002%
43	8.330	1181	1188	1201	rBV	184711	303594	21.72%	2.822%
44	8.653	1234	1241	1249	rBV	726779	1132633	81.04%	10.528%
45	8.720	1249	1252	1261	rVB	9848	17091	1.22%	0.159%
46	8.885	1276	1279	1280	rBV2	254	291	0.02%	0.003%
47	8.952	1285	1290	1303	rVV	127551	188584	13.49%	1.753%
48	9.281	1339	1344	1348	rBV5	2931	4228	0.30%	0.039%
49	9.391	1356	1362	1377	rBV	534480	792882	56.73%	7.370%
50	9.762	1422	1423	1427	rBV2	611	553	0.04%	0.005%
51	9.836	1432	1435	1436	rBV2	365	279	0.02%	0.003%
52	10.055	1465	1471	1481	rBV	733423	962522	68.87%	8.947%
53	10.311	1509	1513	1518	rBV3	1667	2774	0.20%	0.026%
54	10.439	1530	1534	1537	rBV	394	690	0.05%	0.006%
55	10.640	1565	1567	1571	rBV4	508	481	0.03%	0.004%
56	10.896	1605	1609	1610	rBV3	258	304	0.02%	0.003%
57	10.963	1617	1620	1625	rVB3	598	967	0.07%	0.009%
58	11.000	1625	1626	1628	rBV	481	310	0.02%	0.003%
59	11.085	1638	1640	1643	rBV3	797	915	0.07%	0.009%
60	11.122	1643	1646	1650	rVB	2828	3420	0.24%	0.032%
61	11.195	1652	1658	1669	rBV	556127	703328	50.32%	6.537%
62	11.378	1686	1688	1691	rBV2	380	475	0.03%	0.004%
63	11.457	1698	1701	1702	rBV	532	576	0.04%	0.005%
64	11.683	1736	1738	1742	rBV2	573	566	0.04%	0.005%
65	11.713	1742	1743	1745	rVV	449	341	0.02%	0.003%
66	11.750	1746	1749	1754	rVB3	3396	4315	0.31%	0.040%
67	11.805	1756	1758	1761	rVB	334	331	0.02%	0.003%
68	11.841	1761	1764	1768	rVB4	669	1021	0.07%	0.009%
69	11.872	1768	1769	1771	rBV	289	298	0.02%	0.003%
70	11.939	1776	1780	1782	rBV4	1415	1844	0.13%	0.017%
71	11.975	1784	1786	1788	rVB	634	350	0.03%	0.003%
72	12.024	1788	1794	1803	rBV	755577	940185	67.27%	8.739%
73	12.122	1808	1810	1813	rVV3	1683	2264	0.16%	0.021%
74	12.152	1813	1815	1819	rVB3	2199	2137	0.15%	0.020%
75	12.238	1826	1829	1830	rBV2	429	429	0.03%	0.004%
76	12.323	1837	1843	1852	rBV	764342	966811	69.18%	8.987%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029423.D
 Acq On : 13 Jun 2022 19:19
 Operator : JC/MD
 Sample : N3291-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.433	1857	1861	1864	rVB4	915	1008	0.07%	0.009%
78	12.463	1864	1866	1867	rBV	409	341	0.02%	0.003%
79	12.549	1876	1880	1881	rBV	377	396	0.03%	0.004%
80	12.756	1913	1914	1919	rVB3	345	236	0.02%	0.002%
81	12.798	1919	1921	1923	rBV	328	307	0.02%	0.003%
82	12.914	1938	1940	1941	rBV2	363	241	0.02%	0.002%
83	13.109	1970	1972	1976	rBV2	470	575	0.04%	0.005%
84	13.164	1979	1981	1985	rVB2	449	457	0.03%	0.004%
85	13.201	1985	1987	1988	rBV	243	252	0.02%	0.002%
86	13.359	2010	2013	2014	rBV2	279	240	0.02%	0.002%
87	13.542	2041	2043	2045	rVB	432	264	0.02%	0.002%
88	13.774	2078	2081	2083	rBV2	577	668	0.05%	0.006%
89	13.920	2102	2105	2106	rBV	351	413	0.03%	0.004%
90	13.969	2110	2113	2114	rBV2	252	274	0.02%	0.003%
91	14.018	2120	2121	2124	rVB2	375	281	0.02%	0.003%
92	14.469	2193	2195	2197	rVB	495	303	0.02%	0.003%
93	14.499	2197	2200	2201	rBV	474	418	0.03%	0.004%
94	14.865	2259	2260	2262	rBV	586	437	0.03%	0.004%
95	14.993	2279	2281	2282	rBV2	464	401	0.03%	0.004%
96	15.121	2300	2302	2303	rBV2	490	381	0.03%	0.004%
97	15.158	2307	2308	2309	rBV	485	280	0.02%	0.003%
98	15.237	2316	2321	2323	rBV4	788	1180	0.08%	0.011%
99	15.292	2328	2330	2332	rBV3	357	235	0.02%	0.002%
100	15.371	2342	2343	2345	rBV	468	272	0.02%	0.003%

Sum of corrected areas: 10758482




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029423.D
Acq On : 13 Jun 2022 19:19
Operator : JC/MD
Sample : N3291-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

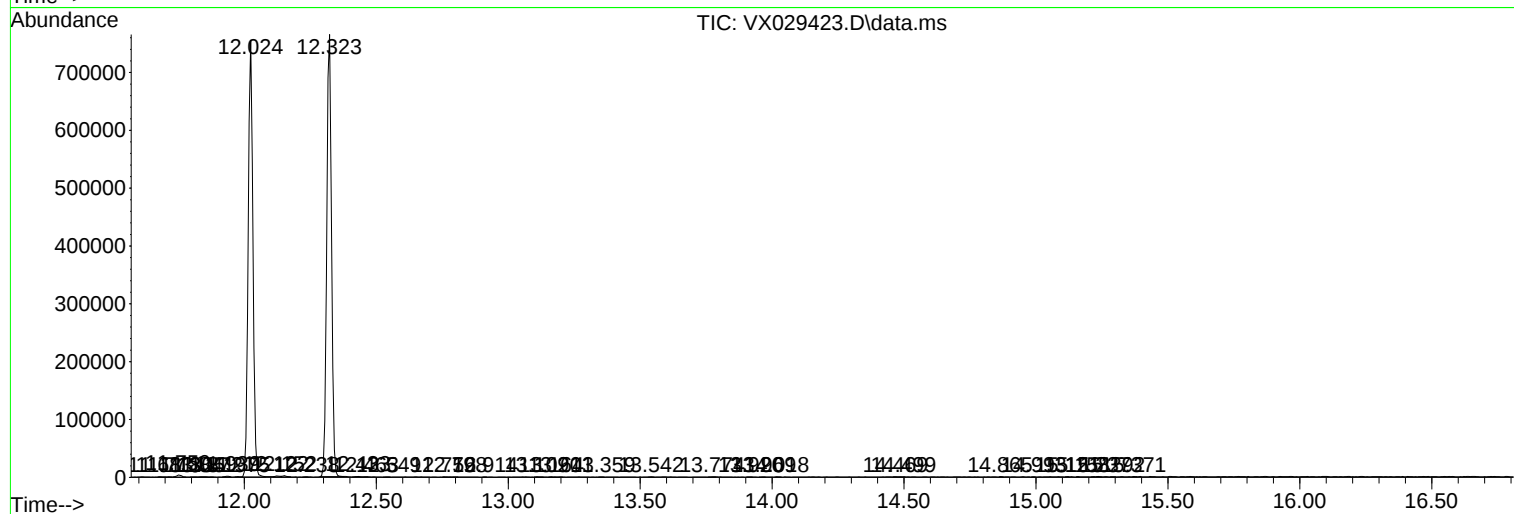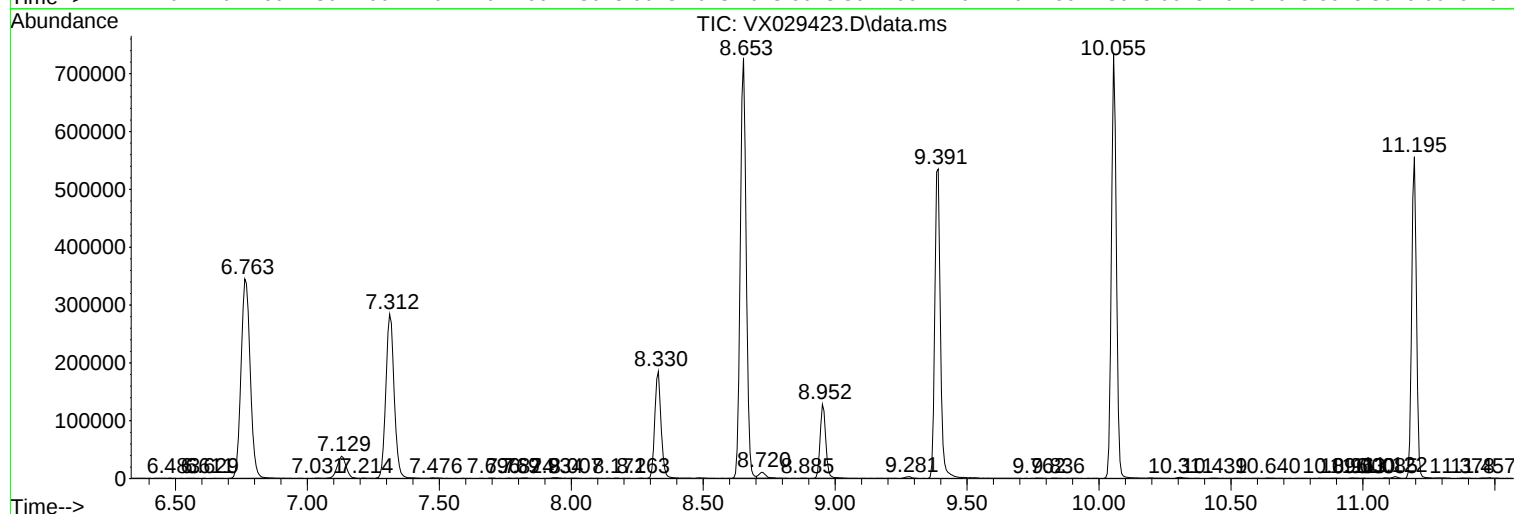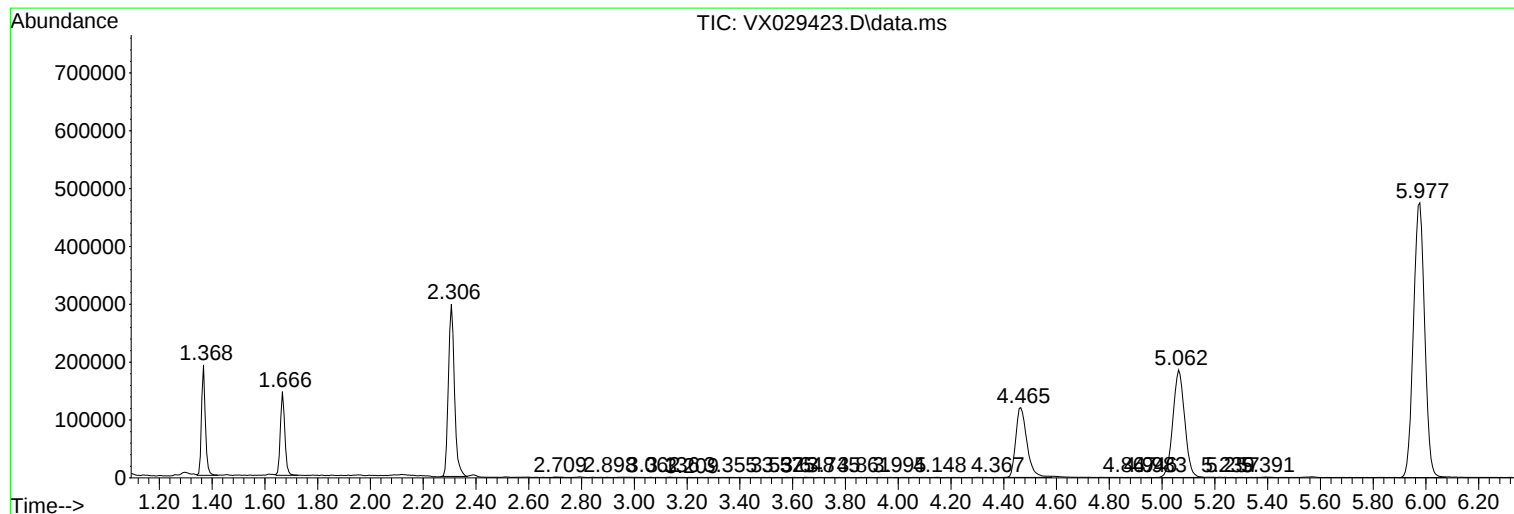

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029423.D
Acq On : 13 Jun 2022 19:19
Operator : JC/MD
Sample : N3291-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029423.D
Acq On : 13 Jun 2022 19:19
Operator : JC/MD
Sample : N3291-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------