

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029425.D
 Acq On : 13 Jun 2022 20:06
 Operator : JC/MD
 Sample : N3291-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CODY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M

Title : VOC Analysis

Signal : TIC: VX029425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	58	rVB	184357	188588	13.95%	1.793%
2	1.666	91	95	103	rVB	135103	161648	11.96%	1.537%
3	2.306	194	200	210	rBV	294410	462863	34.23%	4.400%
4	2.459	223	225	228	rVB3	465	363	0.03%	0.003%
5	2.562	240	242	243	rBV	503	299	0.02%	0.003%
6	2.636	252	254	257	rBV2	243	239	0.02%	0.002%
7	2.709	264	266	271	rVB4	654	785	0.06%	0.007%
8	2.782	275	278	279	rBV3	746	936	0.07%	0.009%
9	2.849	287	289	291	rBV2	400	286	0.02%	0.003%
10	2.892	294	296	299	rBV2	376	426	0.03%	0.004%
11	2.953	300	306	309	rBV3	940	1675	0.12%	0.016%
12	3.026	316	318	321	rBV	374	441	0.03%	0.004%
13	3.056	321	323	325	rVV2	380	374	0.03%	0.004%
14	3.251	353	355	359	rVB2	312	384	0.03%	0.004%
15	3.489	392	394	396	rVB2	407	339	0.03%	0.003%
16	3.507	396	397	400	rBV3	316	431	0.03%	0.004%
17	3.611	412	414	418	rBV3	489	724	0.05%	0.007%
18	4.160	502	504	507	rBV2	292	297	0.02%	0.003%
19	4.324	528	531	532	rVB2	369	363	0.03%	0.003%
20	4.465	544	554	570	rBV	119512	345378	25.54%	3.283%
21	4.867	619	620	625	rVB2	567	601	0.04%	0.006%
22	4.910	625	627	628	rBV2	326	299	0.02%	0.003%
23	5.062	639	652	669	rBV	178404	547919	40.52%	5.208%
24	5.275	684	687	689	rBV2	288	355	0.03%	0.003%
25	5.373	701	703	704	rBV	417	375	0.03%	0.004%
26	5.489	720	722	724	rVB2	397	302	0.02%	0.003%
27	5.538	724	730	731	rBV3	548	704	0.05%	0.007%
28	5.562	731	734	736	rBV4	633	856	0.06%	0.008%
29	5.727	759	761	764	rVB2	278	273	0.02%	0.003%
30	5.873	782	785	788	rBV3	304	411	0.03%	0.004%
31	5.976	788	802	817	rBV2	455395	1352114	100.00%	12.853%
32	6.153	829	831	836	rBV2	295	277	0.02%	0.003%
33	6.220	841	842	847	rVB2	471	455	0.03%	0.004%
34	6.361	863	865	868	rVV3	288	321	0.02%	0.003%
35	6.391	868	870	873	rVV3	386	320	0.02%	0.003%
36	6.476	882	884	888	rBV2	224	260	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029425.D
 Acq On : 13 Jun 2022 20:06
 Operator : JC/MD
 Sample : N3291-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CODY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	6.641	908	911	912	rBV	410	405	0.03%	0.004%
38	6.763	922	931	947	rBV	350568	836505	61.87%	7.952%
39	7.001	968	970	972	rVB2	457	347	0.03%	0.003%
40	7.031	972	975	977	rBV3	446	422	0.03%	0.004%
41	7.129	983	991	1002	rBV3	33844	81880	6.06%	0.778%
42	7.312	1012	1021	1039	rBV	274265	595002	44.01%	5.656%
43	7.482	1044	1049	1051	rBV2	783	930	0.07%	0.009%
44	7.738	1088	1091	1092	rBV2	356	371	0.03%	0.004%
45	7.824	1100	1105	1106	rBV3	756	1164	0.09%	0.011%
46	7.842	1106	1108	1111	rVB2	541	515	0.04%	0.005%
47	7.940	1120	1124	1129	rVB4	959	1743	0.13%	0.017%
48	8.043	1138	1141	1143	rBV	397	499	0.04%	0.005%
49	8.092	1148	1149	1152	rVB2	281	262	0.02%	0.002%
50	8.177	1160	1163	1164	rBV	237	254	0.02%	0.002%
51	8.330	1181	1188	1198	rBV	176645	291948	21.59%	2.775%
52	8.476	1208	1212	1213	rBV2	549	680	0.05%	0.006%
53	8.653	1234	1241	1249	rBV	706135	1101407	81.46%	10.470%
54	8.726	1249	1253	1258	rVB	8819	14751	1.09%	0.140%
55	8.952	1285	1290	1302	rBV	125931	181594	13.43%	1.726%
56	9.134	1318	1320	1321	rBV	360	261	0.02%	0.002%
57	9.220	1332	1334	1337	rVB2	365	302	0.02%	0.003%
58	9.275	1337	1343	1349	rBV2	2970	4401	0.33%	0.042%
59	9.384	1356	1361	1378	rBV	520211	770352	56.97%	7.323%
60	9.787	1425	1427	1430	rBV3	273	315	0.02%	0.003%
61	9.848	1435	1437	1441	rVB2	554	653	0.05%	0.006%
62	9.897	1441	1445	1448	rBV2	262	381	0.03%	0.004%
63	9.933	1450	1451	1453	rBV2	451	317	0.02%	0.003%
64	10.055	1465	1471	1480	rBV	716421	971767	71.87%	9.237%
65	10.244	1499	1502	1504	rVB4	405	467	0.03%	0.004%
66	10.311	1506	1513	1516	rBV3	1547	2636	0.19%	0.025%
67	10.646	1564	1568	1569	rBV	875	752	0.06%	0.007%
68	10.963	1617	1620	1623	rBV2	610	555	0.04%	0.005%
69	11.024	1627	1630	1631	rBV2	335	246	0.02%	0.002%
70	11.085	1637	1640	1641	rBV2	898	902	0.07%	0.009%
71	11.128	1643	1647	1652	rVV2	2544	3334	0.25%	0.032%
72	11.195	1652	1658	1672	rVV	542897	692607	51.22%	6.584%
73	11.384	1685	1689	1692	rBV3	480	694	0.05%	0.007%
74	11.457	1698	1701	1702	rBV2	590	616	0.05%	0.006%
75	11.482	1702	1705	1707	rBV3	894	1081	0.08%	0.010%
76	11.536	1713	1714	1716	rBV2	417	282	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029425.D
 Acq On : 13 Jun 2022 20:06
 Operator : JC/MD
 Sample : N3291-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CODY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.616	1726	1727	1729	rBV2	361	331	0.02%	0.003%
78	11.671	1734	1736	1738	rVV2	488	368	0.03%	0.003%
79	11.750	1744	1749	1754	rVB5	3447	4719	0.35%	0.045%
80	11.939	1776	1780	1783	rVB2	887	1100	0.08%	0.010%
81	12.024	1789	1794	1803	rBV	775676	938318	69.40%	8.919%
82	12.213	1822	1825	1828	rBV3	466	614	0.05%	0.006%
83	12.323	1836	1843	1855	rBV	741840	930657	68.83%	8.847%
84	12.945	1942	1945	1947	rBV2	402	431	0.03%	0.004%
85	13.042	1959	1961	1962	rBV2	323	313	0.02%	0.003%
86	13.122	1971	1974	1976	rBV2	489	515	0.04%	0.005%
87	13.250	1993	1995	1998	rBV2	422	414	0.03%	0.004%
88	13.469	2029	2031	2035	rBV2	334	337	0.02%	0.003%
89	13.518	2038	2039	2041	rBV	419	275	0.02%	0.003%
90	13.591	2049	2051	2054	rVB	524	452	0.03%	0.004%
91	13.634	2054	2058	2060	rBV	466	614	0.05%	0.006%
92	13.658	2060	2062	2063	rBV	393	278	0.02%	0.003%
93	13.780	2079	2082	2085	rVB3	345	509	0.04%	0.005%
94	13.810	2085	2087	2088	rBV	340	306	0.02%	0.003%
95	14.097	2133	2134	2138	rBV2	309	327	0.02%	0.003%
96	14.298	2164	2167	2168	rBV2	407	441	0.03%	0.004%
97	14.518	2202	2203	2207	rBV2	421	396	0.03%	0.004%
98	14.993	2279	2281	2284	rBV3	448	539	0.04%	0.005%
99	15.328	2334	2336	2339	rBV3	572	767	0.06%	0.007%
100	16.017	2447	2449	2450	rBV	813	610	0.05%	0.006%




Sum of corrected areas: 10519912

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029425.D
Acq On : 13 Jun 2022 20:06
Operator : JC/MD
Sample : N3291-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

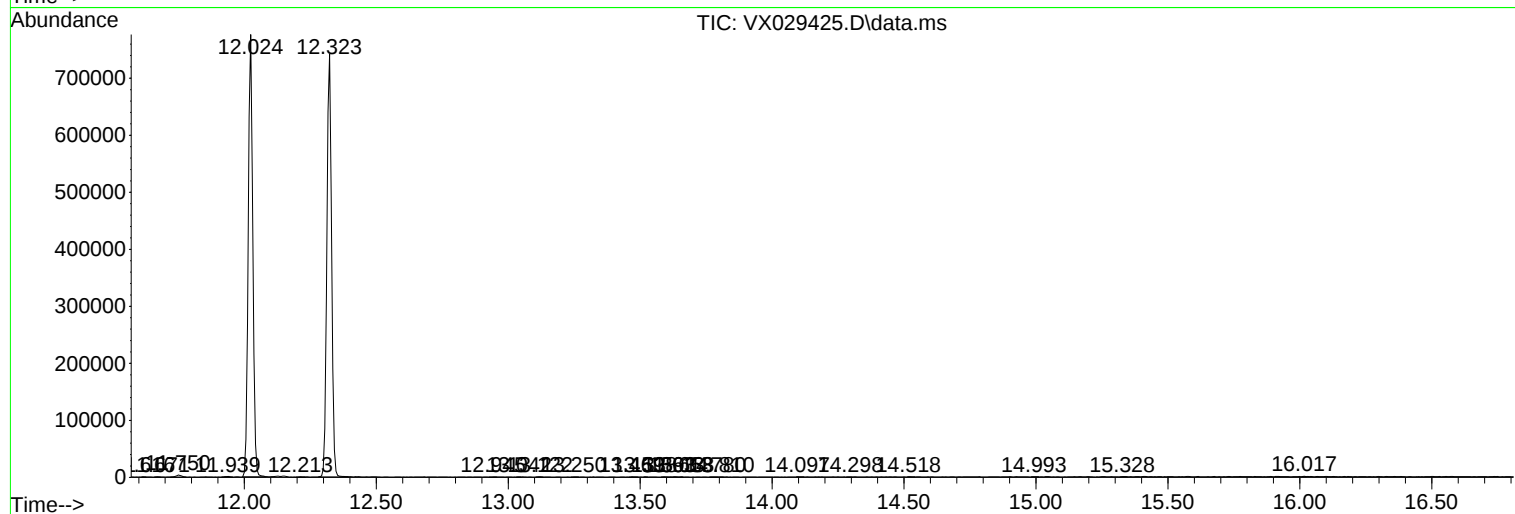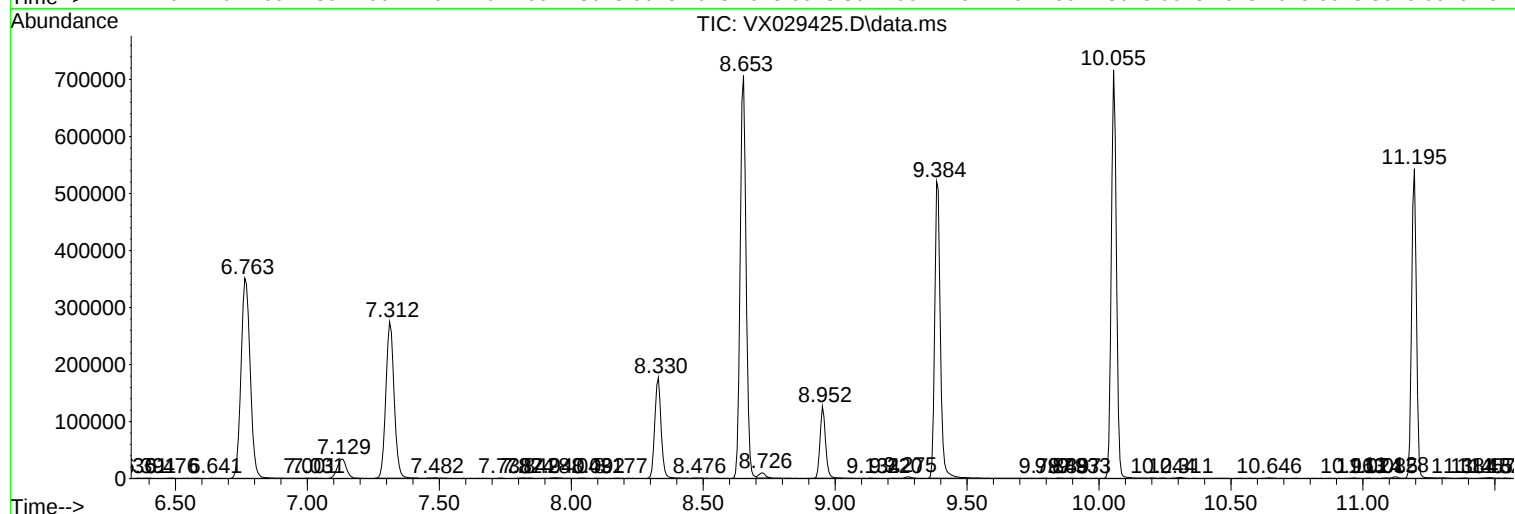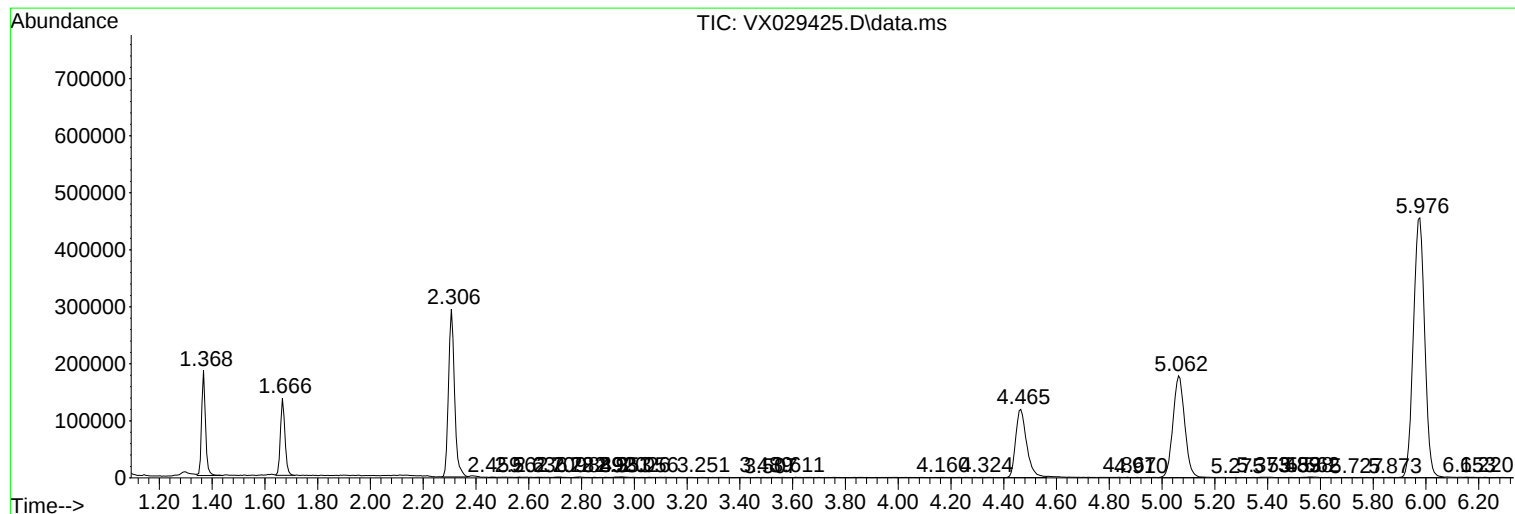

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029425.D
Acq On : 13 Jun 2022 20:06
Operator : JC/MD
Sample : N3291-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029425.D
Acq On : 13 Jun 2022 20:06
Operator : JC/MD
Sample : N3291-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc