

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029427.D
 Acq On : 13 Jun 2022 20:52
 Operator : JC/MD
 Sample : N3291-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	52	rVB	188821	184853	13.35%	1.725%
2	1.666	91	95	106	rVB	140893	167205	12.08%	1.560%
3	2.307	194	200	213	rBV	299296	471304	34.05%	4.397%
4	2.556	240	241	243	rBV2	422	396	0.03%	0.004%
5	2.788	276	279	284	rVB3	1559	2435	0.18%	0.023%
6	2.947	297	305	316	rVB	25512	57955	4.19%	0.541%
7	3.184	342	344	347	rVB	438	327	0.02%	0.003%
8	3.215	347	349	351	rBV2	406	372	0.03%	0.003%
9	3.258	354	356	358	rBV2	382	400	0.03%	0.004%
10	3.556	403	405	409	rVB2	380	421	0.03%	0.004%
11	3.654	419	421	424	rBV2	358	387	0.03%	0.004%
12	3.837	448	451	452	rBV2	348	399	0.03%	0.004%
13	3.922	463	465	467	rBV2	293	346	0.02%	0.003%
14	4.068	487	489	492	rBV2	251	376	0.03%	0.004%
15	4.465	545	554	567	rBV	123069	356644	25.76%	3.327%
16	4.715	593	595	597	rBV2	500	349	0.03%	0.003%
17	4.739	597	599	602	rVB	435	348	0.03%	0.003%
18	4.873	618	621	622	rBV3	315	259	0.02%	0.002%
19	4.891	622	624	626	rVB2	328	267	0.02%	0.002%
20	5.062	639	652	668	rVV	178735	558021	40.31%	5.206%
21	5.367	699	702	703	rBV3	246	272	0.02%	0.003%
22	5.550	729	732	735	rBV4	633	1070	0.08%	0.010%
23	5.971	789	801	817	rBV2	462687	1384289	100.00%	12.915%
24	6.141	827	829	830	rBV	338	281	0.02%	0.003%
25	6.361	863	865	867	rVB2	448	402	0.03%	0.004%
26	6.385	867	869	872	rVB3	307	269	0.02%	0.003%
27	6.409	872	873	876	rVB2	381	278	0.02%	0.003%
28	6.495	885	887	892	rVV2	265	361	0.03%	0.003%
29	6.598	901	904	907	rVB2	359	437	0.03%	0.004%
30	6.623	907	908	911	rBV2	331	372	0.03%	0.003%
31	6.763	922	931	949	rVV	344449	826580	59.71%	7.712%
32	6.928	956	958	961	rVB2	355	273	0.02%	0.003%
33	6.958	961	963	969	rVB4	334	524	0.04%	0.005%
34	7.062	978	980	983	rBV4	254	337	0.02%	0.003%
35	7.129	983	991	1002	rVV5	33011	76207	5.51%	0.711%
36	7.312	1012	1021	1037	rVV	279895	611459	44.17%	5.705%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029427.D
 Acq On : 13 Jun 2022 20:52
 Operator : JC/MD
 Sample : N3291-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.556	1059	1061	1063	rBV2	354	358	0.03%	0.003%
38	7.629	1070	1073	1075	rVV	312	303	0.02%	0.003%
39	7.659	1075	1078	1081	rVV2	256	256	0.02%	0.002%
40	7.732	1088	1090	1093	rVB	303	297	0.02%	0.003%
41	7.818	1099	1104	1105	rBV2	448	467	0.03%	0.004%
42	7.940	1118	1124	1126	rBV4	1238	2084	0.15%	0.019%
43	8.068	1143	1145	1148	rBV3	312	332	0.02%	0.003%
44	8.330	1181	1188	1200	rBV	179092	298215	21.54%	2.782%
45	8.653	1233	1241	1249	rBV	725112	1125496	81.30%	10.500%
46	8.854	1272	1274	1278	rVB3	322	393	0.03%	0.004%
47	8.952	1284	1290	1301	rBV	127899	185351	13.39%	1.729%
48	9.159	1321	1324	1327	rBV2	399	624	0.05%	0.006%
49	9.275	1339	1343	1348	rVB5	2846	4303	0.31%	0.040%
50	9.324	1348	1351	1353	rBV	397	581	0.04%	0.005%
51	9.385	1356	1361	1379	rBV	534134	787746	56.91%	7.349%
52	9.702	1410	1413	1418	rVB3	3064	4110	0.30%	0.038%
53	9.787	1425	1427	1429	rBV2	344	286	0.02%	0.003%
54	9.830	1432	1434	1436	rBV2	378	405	0.03%	0.004%
55	10.055	1465	1471	1481	rBV	729739	959840	69.34%	8.955%
56	10.201	1492	1495	1496	rBV2	637	549	0.04%	0.005%
57	10.305	1509	1512	1516	rVV3	1756	2297	0.17%	0.021%
58	10.647	1566	1568	1573	rVB	912	926	0.07%	0.009%
59	10.762	1585	1587	1590	rBV2	340	385	0.03%	0.004%
60	10.970	1619	1621	1624	rVB2	430	500	0.04%	0.005%
61	11.098	1639	1642	1643	rBV2	408	500	0.04%	0.005%
62	11.122	1643	1646	1650	rVB2	2656	3094	0.22%	0.029%
63	11.195	1652	1658	1667	rBV	551733	701702	50.69%	6.547%
64	11.323	1678	1679	1684	rVB3	732	552	0.04%	0.005%
65	11.384	1687	1689	1694	rBV2	411	611	0.04%	0.006%
66	11.555	1714	1717	1718	rVB2	539	456	0.03%	0.004%
67	11.616	1725	1727	1729	rBV2	304	363	0.03%	0.003%
68	11.689	1736	1739	1741	rBV2	518	590	0.04%	0.006%
69	11.750	1745	1749	1753	rVB2	3076	3691	0.27%	0.034%
70	11.841	1762	1764	1768	rVB3	663	756	0.05%	0.007%
71	11.939	1776	1780	1783	rVB3	1297	1681	0.12%	0.016%
72	11.976	1783	1786	1788	rBV3	756	821	0.06%	0.008%
73	12.024	1788	1794	1803	rBV	788645	943697	68.17%	8.804%
74	12.323	1837	1843	1850	rBV	774260	965582	69.75%	9.008%
75	12.518	1874	1875	1879	rVB2	300	280	0.02%	0.003%
76	12.579	1883	1885	1887	rVB2	623	454	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029427.D
 Acq On : 13 Jun 2022 20:52
 Operator : JC/MD
 Sample : N3291-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.610	1887	1890	1891	rBV2	362	331	0.02%	0.003%
78	12.677	1898	1901	1904	rVB2	525	480	0.03%	0.004%
79	12.701	1904	1905	1908	rBV2	289	338	0.02%	0.003%
80	12.768	1914	1916	1919	rVB2	585	601	0.04%	0.006%
81	12.805	1919	1922	1925	rBV2	255	414	0.03%	0.004%
82	12.866	1929	1932	1933	rBV2	299	282	0.02%	0.003%
83	12.920	1938	1941	1942	rBV	329	293	0.02%	0.003%
84	13.055	1959	1963	1968	rVB3	486	835	0.06%	0.008%
85	13.103	1968	1971	1973	rBV2	348	375	0.03%	0.003%
86	13.183	1982	1984	1987	rVB2	387	413	0.03%	0.004%
87	13.262	1995	1997	2000	rVB2	393	374	0.03%	0.003%
88	13.347	2010	2011	2014	rBV	329	341	0.02%	0.003%
89	13.652	2059	2061	2064	rBV3	317	346	0.02%	0.003%
90	13.780	2079	2082	2084	rBV2	405	511	0.04%	0.005%
91	13.908	2102	2103	2105	rBV	403	318	0.02%	0.003%
92	14.128	2137	2139	2143	rBV2	578	855	0.06%	0.008%
93	14.420	2186	2187	2194	rBV3	304	598	0.04%	0.006%
94	14.664	2226	2227	2230	rBV3	382	312	0.02%	0.003%
95	14.695	2230	2232	2233	rBV	548	372	0.03%	0.003%
96	14.865	2256	2260	2262	rBV2	503	762	0.06%	0.007%
97	15.036	2286	2288	2289	rBV	414	301	0.02%	0.003%
98	15.201	2311	2315	2317	rBV3	448	575	0.04%	0.005%
99	16.200	2477	2479	2482	rBV3	577	750	0.05%	0.007%
100	16.389	2508	2510	2512	rBV	682	400	0.03%	0.004%




Sum of corrected areas: 10718586

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029427.D
Acq On : 13 Jun 2022 20:52
Operator : JC/MD
Sample : N3291-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

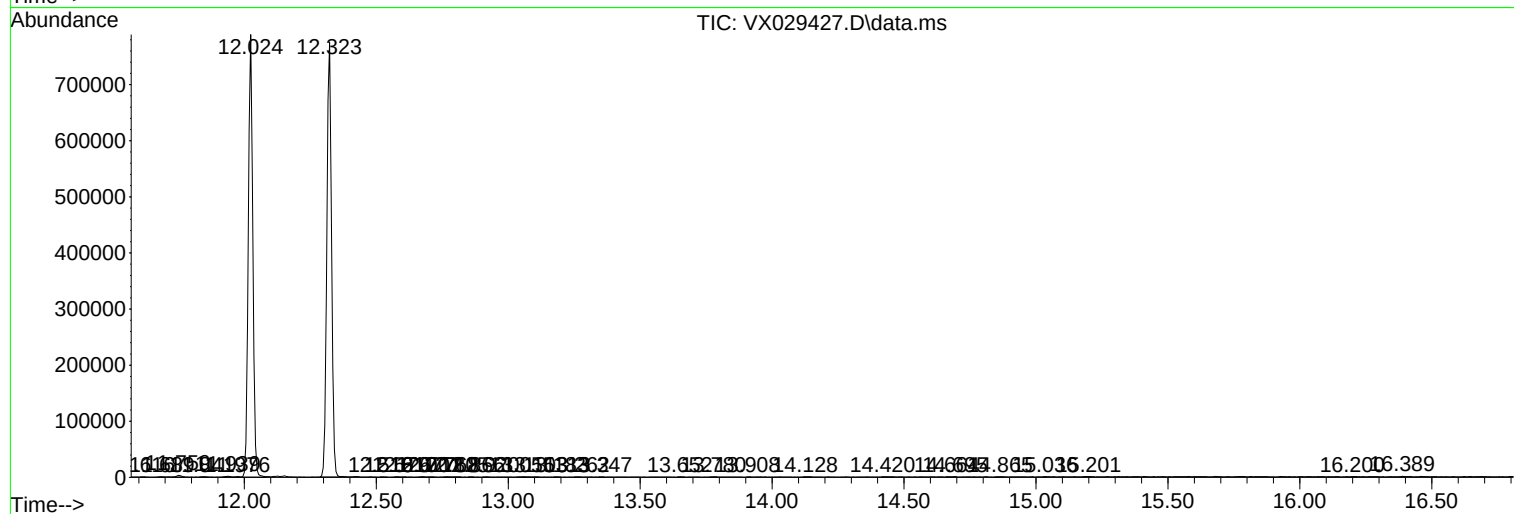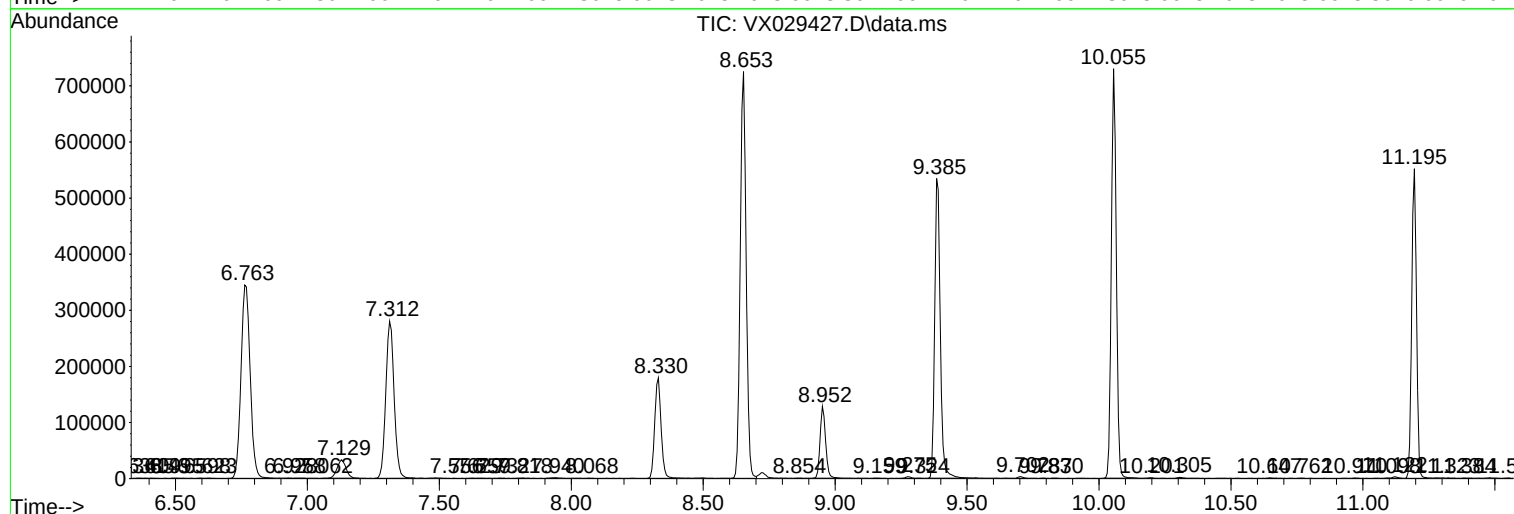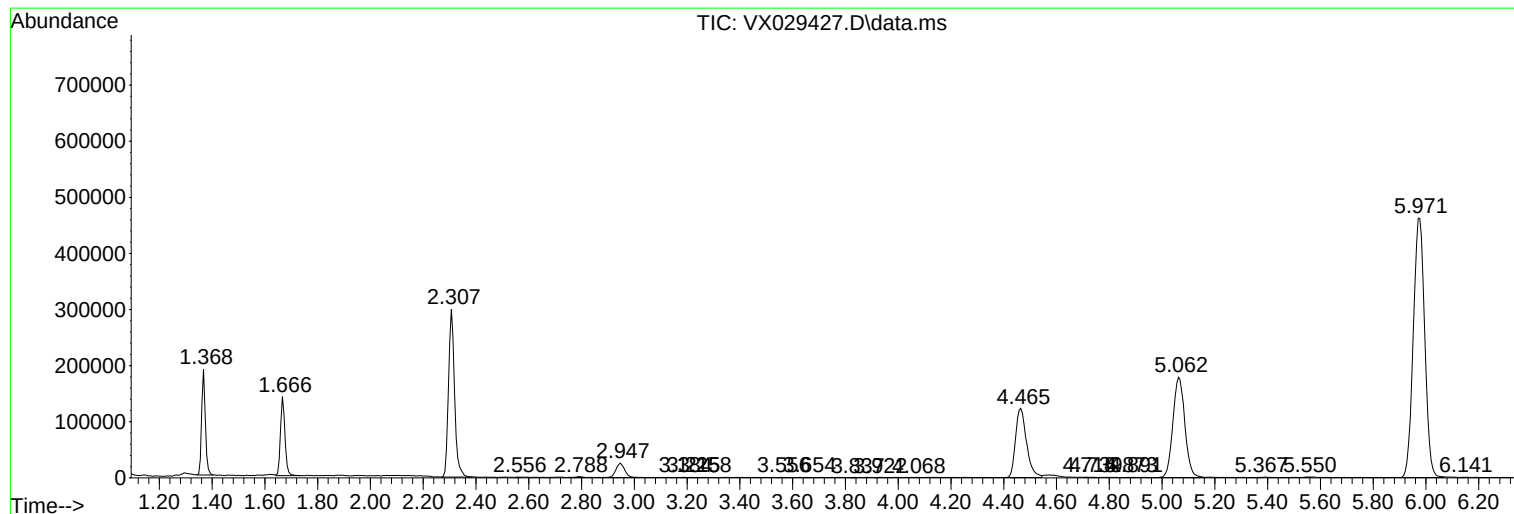

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029427.D
Acq On : 13 Jun 2022 20:52
Operator : JC/MD
Sample : N3291-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029427.D
Acq On : 13 Jun 2022 20:52
Operator : JC/MD
Sample : N3291-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------