

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029434.D
 Acq On : 13 Jun 2022 23:58
 Operator : JC/MD
 Sample : VX0613WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK659

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029434.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	56	rVB	222678	222186	14.18%	1.859%
2	1.666	91	95	103	rVB	150162	176465	11.26%	1.476%
3	2.306	194	200	218	rVB	343857	552874	35.28%	4.625%
4	2.568	241	243	246	rBV3	452	585	0.04%	0.005%
5	2.794	276	280	284	rVB2	1437	2278	0.15%	0.019%
6	2.861	290	291	294	rVB2	292	250	0.02%	0.002%
7	2.946	294	305	317	rBV2	40675	93156	5.94%	0.779%
8	3.367	373	374	376	rBV2	261	252	0.02%	0.002%
9	3.428	381	384	385	rBV2	389	425	0.03%	0.004%
10	3.580	407	409	411	rVB2	264	210	0.01%	0.002%
11	3.617	413	415	416	rBV2	382	227	0.01%	0.002%
12	3.641	416	419	422	rBV3	284	320	0.02%	0.003%
13	3.714	430	431	433	rBV2	422	265	0.02%	0.002%
14	3.745	435	436	440	rVV3	234	287	0.02%	0.002%
15	3.812	444	447	451	rBV3	328	380	0.02%	0.003%
16	3.928	464	466	468	rVB2	256	208	0.01%	0.002%
17	3.946	468	469	471	rBV2	348	308	0.02%	0.003%
18	3.995	475	477	478	rVB	320	193	0.01%	0.002%
19	4.013	478	480	483	rVB3	252	226	0.01%	0.002%
20	4.056	483	487	488	rBV2	386	413	0.03%	0.003%
21	4.123	495	498	500	rBV2	283	434	0.03%	0.004%
22	4.275	521	523	526	rBV2	269	367	0.02%	0.003%
23	4.464	545	554	567	rBV	133663	383108	24.45%	3.205%
24	4.787	605	607	611	rVB4	516	627	0.04%	0.005%
25	4.952	633	634	635	rBV	415	189	0.01%	0.002%
26	5.062	638	652	669	rBV	204635	627160	40.02%	5.246%
27	5.232	679	680	683	rBV2	315	292	0.02%	0.002%
28	5.299	689	691	694	rBV2	194	252	0.02%	0.002%
29	5.385	702	705	707	rBV4	495	713	0.05%	0.006%
30	5.562	728	734	738	rBV4	938	2029	0.13%	0.017%
31	5.726	757	761	762	rBV2	244	217	0.01%	0.002%
32	5.976	789	802	818	rBV2	522823	1567163	100.00%	13.110%
33	6.476	882	884	886	rVB	489	324	0.02%	0.003%
34	6.494	886	887	890	rBV3	304	318	0.02%	0.003%
35	6.616	903	907	908	rVV2	296	361	0.02%	0.003%
36	6.763	917	931	948	rBV	365944	886651	56.58%	7.417%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029434.D
 Acq On : 13 Jun 2022 23:58
 Operator : JC/MD
 Sample : VX0613WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK659

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	6.952	960	962	965	rBV3	342	361	0.02%	0.003%
38	7.128	981	991	1002	rBV5	27919	69617	4.44%	0.582%
39	7.311	1011	1021	1038	rBV	317041	688635	43.94%	5.761%
40	7.482	1043	1049	1051	rBV3	867	1469	0.09%	0.012%
41	7.647	1074	1076	1080	rVB2	305	290	0.02%	0.002%
42	7.738	1088	1091	1092	rBV3	195	192	0.01%	0.002%
43	7.817	1100	1104	1106	rBV2	743	927	0.06%	0.008%
44	7.872	1111	1113	1114	rBV2	328	187	0.01%	0.002%
45	8.043	1138	1141	1145	rBV2	247	486	0.03%	0.004%
46	8.122	1152	1154	1156	rVB2	333	332	0.02%	0.003%
47	8.146	1156	1158	1161	rBV2	311	307	0.02%	0.003%
48	8.171	1161	1162	1164	rVV2	231	214	0.01%	0.002%
49	8.244	1172	1174	1175	rVB	270	187	0.01%	0.002%
50	8.329	1181	1188	1201	rBV	191826	317716	20.27%	2.658%
51	8.543	1220	1223	1226	rBV	319	428	0.03%	0.004%
52	8.652	1233	1241	1249	rVV	830575	1286017	82.06%	10.758%
53	8.720	1249	1252	1259	rVB	12471	18868	1.20%	0.158%
54	8.951	1285	1290	1301	rBV	135386	198397	12.66%	1.660%
55	9.171	1324	1326	1328	rBV2	277	198	0.01%	0.002%
56	9.274	1339	1343	1348	rVB2	2628	3644	0.23%	0.030%
57	9.390	1356	1362	1379	rBV	575612	865154	55.21%	7.237%
58	9.701	1408	1413	1418	rBV	4039	5662	0.36%	0.047%
59	9.793	1427	1428	1432	rBV3	431	675	0.04%	0.006%
60	10.055	1465	1471	1485	rBV	772273	1028870	65.65%	8.607%
61	10.201	1492	1495	1501	rVB3	1190	1787	0.11%	0.015%
62	10.268	1505	1506	1509	rVV2	315	249	0.02%	0.002%
63	10.305	1509	1512	1519	rVB2	2349	3451	0.22%	0.029%
64	10.372	1521	1523	1525	rBV2	278	262	0.02%	0.002%
65	10.439	1532	1534	1536	rBV	311	234	0.01%	0.002%
66	10.597	1556	1560	1563	rBV2	270	350	0.02%	0.003%
67	10.652	1563	1569	1574	rBV5	1363	2614	0.17%	0.022%
68	10.884	1606	1607	1612	rVB2	271	236	0.02%	0.002%
69	10.963	1616	1620	1624	rVB3	469	856	0.05%	0.007%
70	11.122	1642	1646	1650	rVB2	4120	5428	0.35%	0.045%
71	11.195	1652	1658	1667	rBV	617992	776814	49.57%	6.498%
72	11.390	1687	1690	1692	rBV2	348	456	0.03%	0.004%
73	11.457	1697	1701	1703	rBV3	1381	1984	0.13%	0.017%
74	11.591	1721	1723	1724	rBV	312	272	0.02%	0.002%
75	11.676	1735	1737	1742	rVB4	387	439	0.03%	0.004%
76	11.750	1746	1749	1753	rVB2	4811	6128	0.39%	0.051%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029434.D
 Acq On : 13 Jun 2022 23:58
 Operator : JC/MD
 Sample : VX0613WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK659

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.841	1762	1764	1767	rVB2	693	668	0.04%	0.006%
78	11.926	1776	1778	1782	rBV3	1602	2168	0.14%	0.018%
79	11.975	1783	1786	1789	rVV	1230	1537	0.10%	0.013%
80	12.024	1789	1794	1806	rVV	836132	1017744	64.94%	8.514%
81	12.127	1808	1811	1812	rVV3	1850	2182	0.14%	0.018%
82	12.152	1812	1815	1819	rVB4	2645	3312	0.21%	0.028%
83	12.323	1835	1843	1851	rBV	880360	1101292	70.27%	9.213%
84	12.481	1867	1869	1870	rBV2	558	424	0.03%	0.004%
85	12.554	1879	1881	1884	rVB2	297	296	0.02%	0.002%
86	12.579	1884	1885	1887	rBV	313	231	0.01%	0.002%
87	13.115	1969	1973	1977	rBV5	1268	1838	0.12%	0.015%
88	13.469	2030	2031	2033	rBV2	394	333	0.02%	0.003%
89	13.597	2048	2052	2058	rBV3	1609	2240	0.14%	0.019%
90	13.688	2066	2067	2069	rBV	484	309	0.02%	0.003%
91	13.713	2069	2071	2074	rVB2	354	285	0.02%	0.002%
92	13.780	2080	2082	2086	rVB2	1720	1907	0.12%	0.016%
93	13.889	2098	2100	2101	rBV	434	207	0.01%	0.002%
94	13.963	2109	2112	2116	rVB4	1876	2345	0.15%	0.020%
95	13.999	2116	2118	2119	rBV	503	405	0.03%	0.003%
96	14.462	2192	2194	2195	rBV	329	219	0.01%	0.002%
97	14.603	2214	2217	2220	rVB	596	659	0.04%	0.006%
98	14.731	2237	2238	2240	rVB2	734	396	0.03%	0.003%
99	14.932	2269	2271	2273	rVB2	599	482	0.03%	0.004%
100	15.426	2350	2352	2354	rBV2	667	538	0.03%	0.005%

Sum of corrected areas: 11954123




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029434.D
Acq On : 13 Jun 2022 23:58
Operator : JC/MD
Sample : VX0613WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK659

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

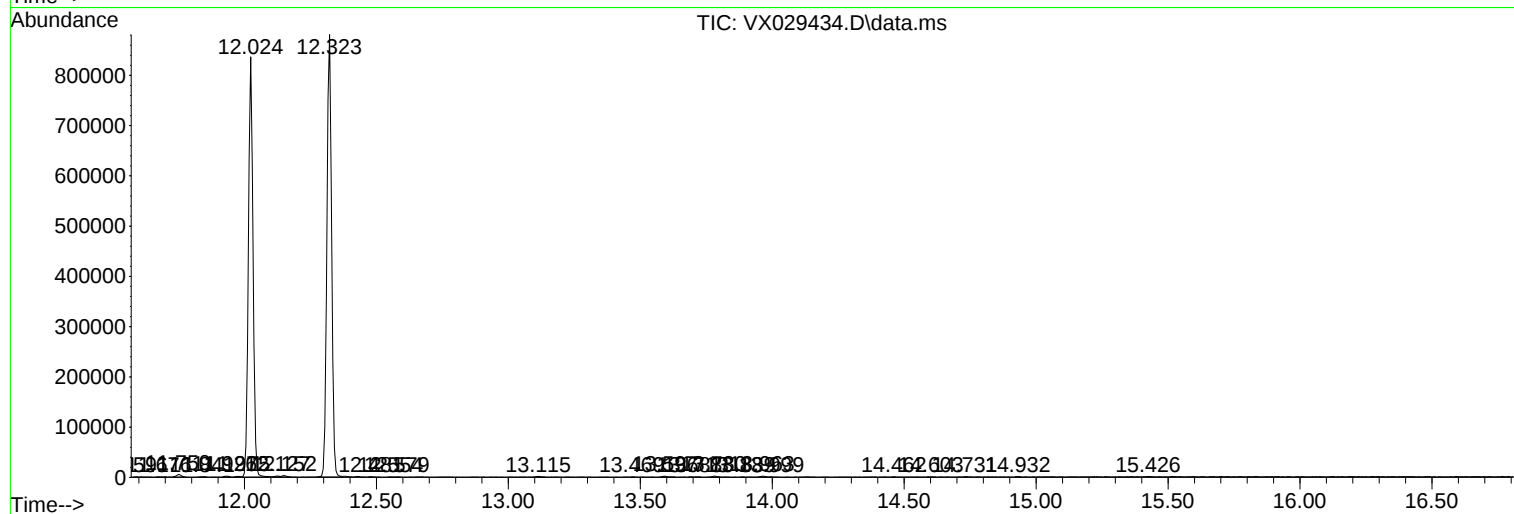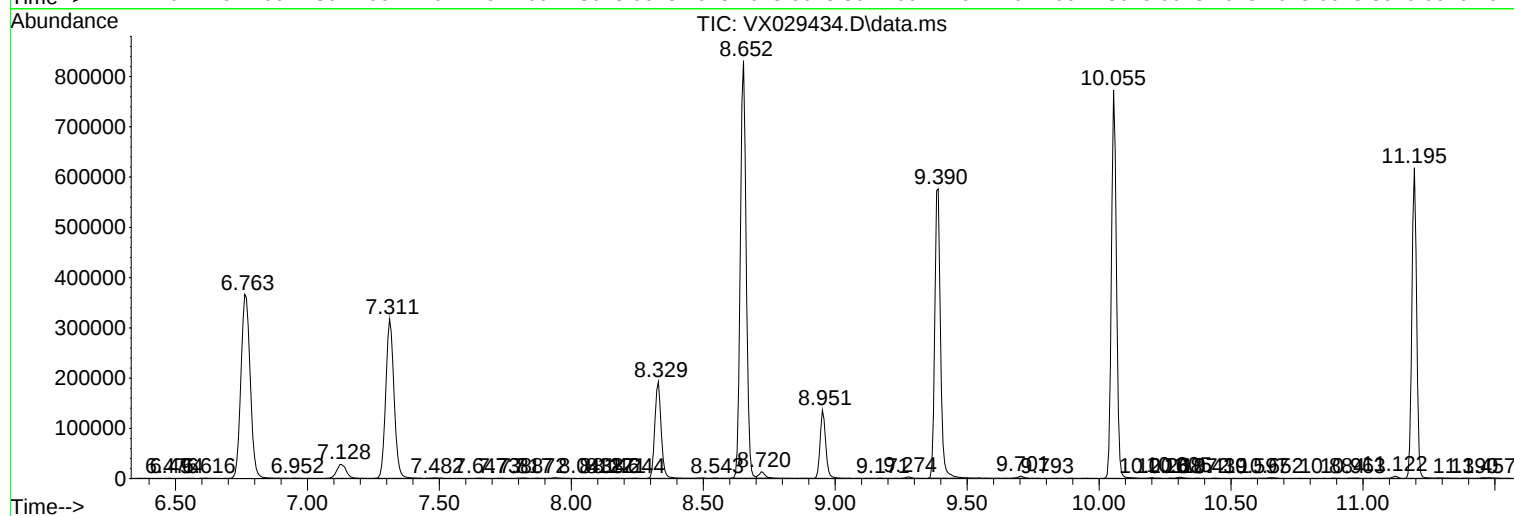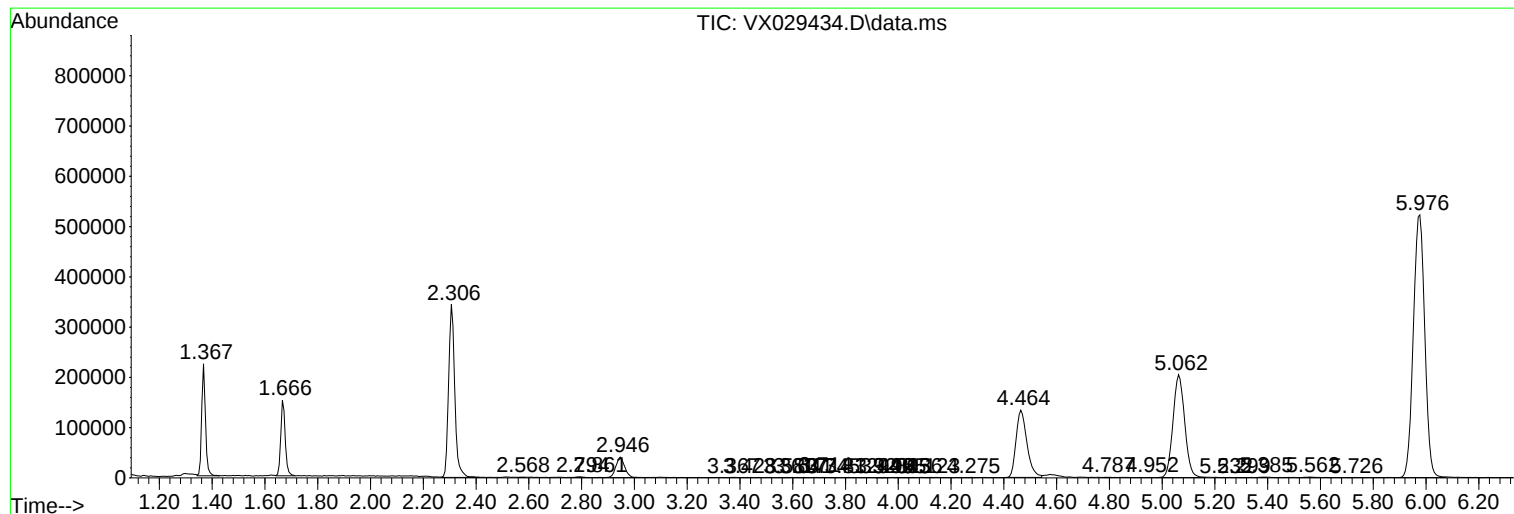

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029434.D
Acq On : 13 Jun 2022 23:58
Operator : JC/MD
Sample : VX0613WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK659

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029434.D
Acq On : 13 Jun 2022 23:58
Operator : JC/MD
Sample : VX0613WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK659

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------