

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029435.D
 Acq On : 14 Jun 2022 00:22
 Operator : JC/MD
 Sample : N3248-02DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYW7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M

Title : VOC Analysis

Signal : TIC: VX029435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	192110	191897	13.23%	1.536%
2	1.666	91	95	108	rVB	140316	166061	11.45%	1.329%
3	2.306	194	200	212	rBV2	336921	619899	42.75%	4.961%
4	2.514	230	234	239	rBV3	995	1725	0.12%	0.014%
5	2.794	275	280	283	rBV3	1354	2040	0.14%	0.016%
6	2.947	296	305	319	rVB	65052	149830	10.33%	1.199%
7	3.093	324	329	336	rVB2	4180	6974	0.48%	0.056%
8	3.373	374	375	378	rBV2	314	291	0.02%	0.002%
9	3.471	390	391	395	rBV2	358	328	0.02%	0.003%
10	3.544	401	403	406	rVB2	284	300	0.02%	0.002%
11	3.611	406	414	428	rBV	70796	167741	11.57%	1.342%
12	3.904	460	462	465	rBV	465	561	0.04%	0.004%
13	3.995	474	477	478	rBV	287	268	0.02%	0.002%
14	4.166	502	505	508	rBV3	252	333	0.02%	0.003%
15	4.306	527	528	530	rVB	511	260	0.02%	0.002%
16	4.465	545	554	567	rBV3	136765	469269	32.36%	3.755%
17	4.879	620	622	624	rBV3	314	240	0.02%	0.002%
18	5.062	639	652	670	rBV	189332	591196	40.77%	4.731%
19	5.233	679	680	683	rVB2	361	289	0.02%	0.002%
20	5.385	693	705	722	rBV2	188072	582779	40.19%	4.664%
21	5.556	727	733	735	rBV3	926	1579	0.11%	0.013%
22	5.739	760	763	765	rBV2	373	404	0.03%	0.003%
23	5.970	789	801	818	rBV2	490243	1450006	100.00%	11.604%
24	6.251	845	847	848	rVB2	563	343	0.02%	0.003%
25	6.263	848	849	852	rBV2	395	435	0.03%	0.003%
26	6.361	864	865	868	rVB3	533	381	0.03%	0.003%
27	6.678	913	917	919	rBV3	304	251	0.02%	0.002%
28	6.763	921	931	945	rBV	358852	859528	59.28%	6.878%
29	6.934	957	959	961	rBV2	406	294	0.02%	0.002%
30	6.995	966	969	971	rBV2	285	337	0.02%	0.003%
31	7.129	982	991	1002	rBV2	72068	164392	11.34%	1.316%
32	7.312	1010	1021	1036	rBV	298389	643256	44.36%	5.148%
33	7.476	1045	1048	1050	rBV2	850	1156	0.08%	0.009%
34	7.537	1056	1058	1060	rVB2	321	278	0.02%	0.002%
35	7.568	1060	1063	1067	rBV3	390	720	0.05%	0.006%
36	7.629	1071	1073	1075	rVV2	342	294	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029435.D
 Acq On : 14 Jun 2022 00:22
 Operator : JC/MD
 Sample : N3248-02DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYW7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.665	1077	1079	1081	rBV	304	279	0.02%	0.002%
38	7.702	1081	1085	1087	rBV2	343	497	0.03%	0.004%
39	7.818	1100	1104	1108	rBV3	469	1088	0.08%	0.009%
40	7.946	1119	1125	1130	rVV5	1049	2436	0.17%	0.019%
41	8.104	1149	1151	1154	rVB	479	402	0.03%	0.003%
42	8.220	1167	1170	1173	rVB2	277	314	0.02%	0.003%
43	8.250	1173	1175	1176	rBV	385	263	0.02%	0.002%
44	8.330	1181	1188	1201	rBV	179112	298477	20.58%	2.389%
45	8.482	1211	1213	1214	rBV	593	436	0.03%	0.003%
46	8.574	1225	1228	1233	rBV4	884	1439	0.10%	0.012%
47	8.653	1234	1241	1249	rVV	760283	1172113	80.84%	9.380%
48	8.726	1249	1253	1262	rVB2	10431	17869	1.23%	0.143%
49	8.952	1285	1290	1303	rBV	127065	188239	12.98%	1.506%
50	9.159	1320	1324	1328	rVB4	2451	3519	0.24%	0.028%
51	9.275	1337	1343	1352	rVB	101848	147093	10.14%	1.177%
52	9.384	1356	1361	1380	rVV	557991	821185	56.63%	6.572%
53	9.622	1399	1400	1403	rBV3	441	439	0.03%	0.004%
54	9.884	1442	1443	1445	rBV	475	240	0.02%	0.002%
55	9.933	1449	1451	1454	rBV2	280	245	0.02%	0.002%
56	9.976	1454	1458	1459	rVB2	429	433	0.03%	0.003%
57	10.055	1465	1471	1483	rBV	739332	1001286	69.05%	8.013%
58	10.195	1492	1494	1500	rVB3	900	1138	0.08%	0.009%
59	10.305	1506	1512	1517	rBV4	1792	3026	0.21%	0.024%
60	10.573	1553	1556	1560	rBV2	420	539	0.04%	0.004%
61	10.622	1560	1564	1565	rBV3	348	339	0.02%	0.003%
62	10.646	1565	1568	1572	rBV3	1246	1411	0.10%	0.011%
63	10.951	1616	1618	1619	rBV	362	352	0.02%	0.003%
64	10.969	1619	1621	1624	rVB3	637	646	0.04%	0.005%
65	11.122	1642	1646	1652	rVB	2534	2542	0.18%	0.020%
66	11.195	1652	1658	1665	rBV	583405	737203	50.84%	5.899%
67	11.451	1697	1700	1702	rBV3	811	905	0.06%	0.007%
68	11.475	1702	1704	1706	rVV2	704	614	0.04%	0.005%
69	11.543	1711	1715	1720	rVB2	327	593	0.04%	0.005%
70	11.677	1735	1737	1739	rBV3	348	286	0.02%	0.002%
71	11.725	1742	1745	1746	rVV	480	388	0.03%	0.003%
72	11.750	1746	1749	1755	rVB3	3602	4597	0.32%	0.037%
73	11.939	1776	1780	1783	rVB3	1145	1465	0.10%	0.012%
74	11.975	1783	1786	1788	rBV3	786	839	0.06%	0.007%
75	12.024	1789	1794	1805	rVV	817329	984250	67.88%	7.876%
76	12.225	1824	1827	1829	rBV2	370	351	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029435.D
 Acq On : 14 Jun 2022 00:22
 Operator : JC/MD
 Sample : N3248-02DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYW7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1852	rBV	793509	1008484	69.55%	8.070%
78	12.463	1864	1866	1868	rBV2	306	255	0.02%	0.002%
79	12.573	1881	1884	1886	rBV2	384	484	0.03%	0.004%
80	12.926	1936	1942	1943	rVB2	339	515	0.04%	0.004%
81	12.951	1943	1946	1950	rBV2	381	555	0.04%	0.004%
82	13.061	1961	1964	1965	rBV2	397	365	0.03%	0.003%
83	13.164	1978	1981	1984	rBV3	389	587	0.04%	0.005%
84	13.274	1997	1999	2002	rVV2	562	525	0.04%	0.004%
85	13.317	2004	2006	2008	rVV2	351	355	0.02%	0.003%
86	13.512	2036	2038	2039	rBV	404	237	0.02%	0.002%
87	13.597	2048	2052	2056	rBV3	1011	1367	0.09%	0.011%
88	13.725	2071	2073	2074	rBV2	310	302	0.02%	0.002%
89	13.786	2078	2083	2086	rBV4	1124	1722	0.12%	0.014%
90	13.963	2108	2112	2116	rBV4	569	775	0.05%	0.006%
91	14.195	2148	2150	2152	rBV2	248	318	0.02%	0.003%
92	14.298	2165	2167	2170	rBV2	376	493	0.03%	0.004%
93	14.548	2206	2208	2209	rBV	546	287	0.02%	0.002%
94	14.652	2223	2225	2227	rVB	513	302	0.02%	0.002%
95	14.847	2255	2257	2258	rVB	511	275	0.02%	0.002%
96	14.944	2271	2273	2275	rBV2	387	297	0.02%	0.002%
97	15.030	2285	2287	2288	rBV	549	461	0.03%	0.004%
98	15.091	2295	2297	2301	rBV2	460	729	0.05%	0.006%
99	15.146	2304	2306	2307	rVB	553	313	0.02%	0.003%
100	16.158	2470	2472	2473	rBV2	616	353	0.02%	0.003%




Sum of corrected areas: 12496067

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029435.D
Acq On : 14 Jun 2022 00:22
Operator : JC/MD
Sample : N3248-02DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYW7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

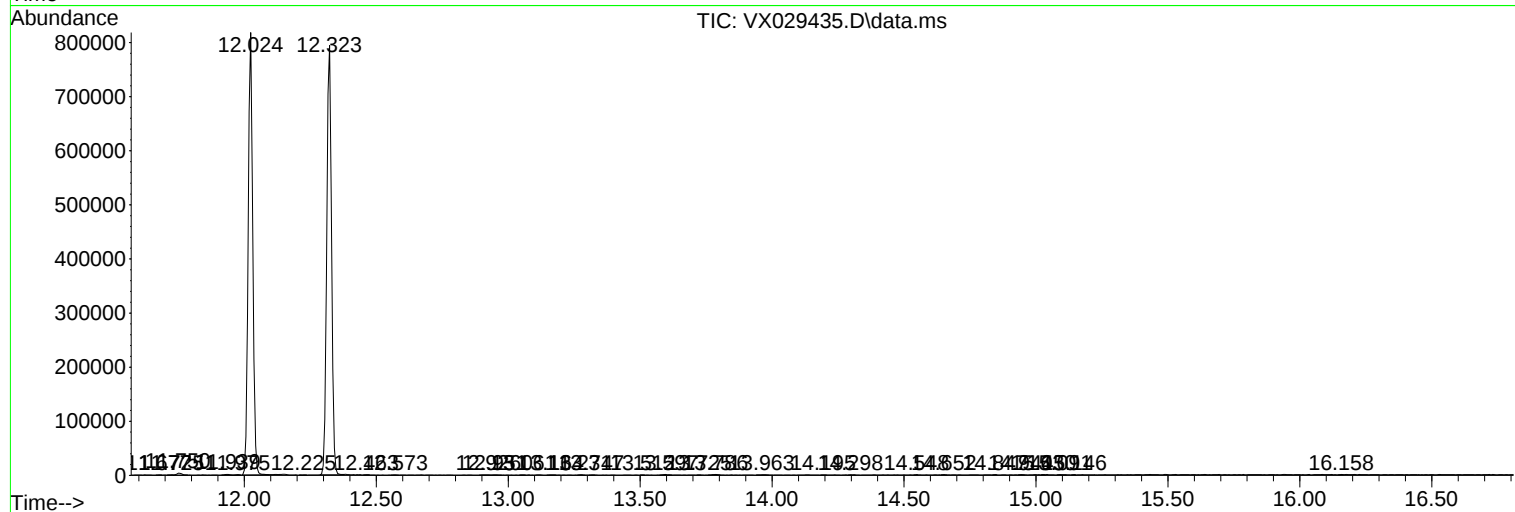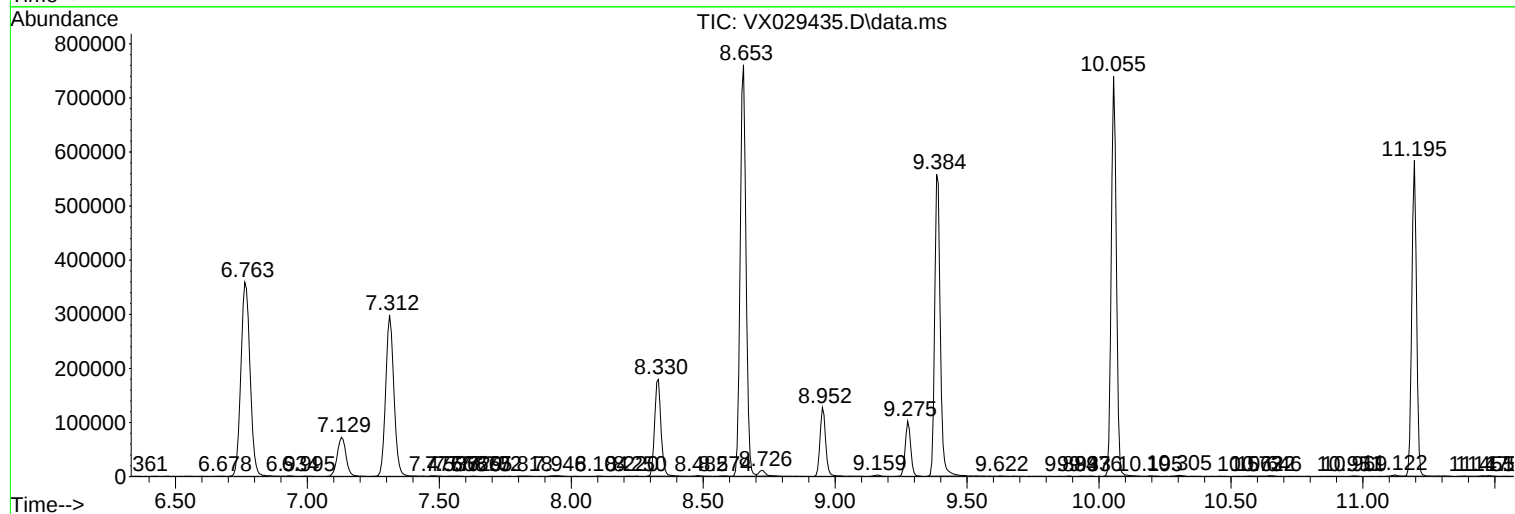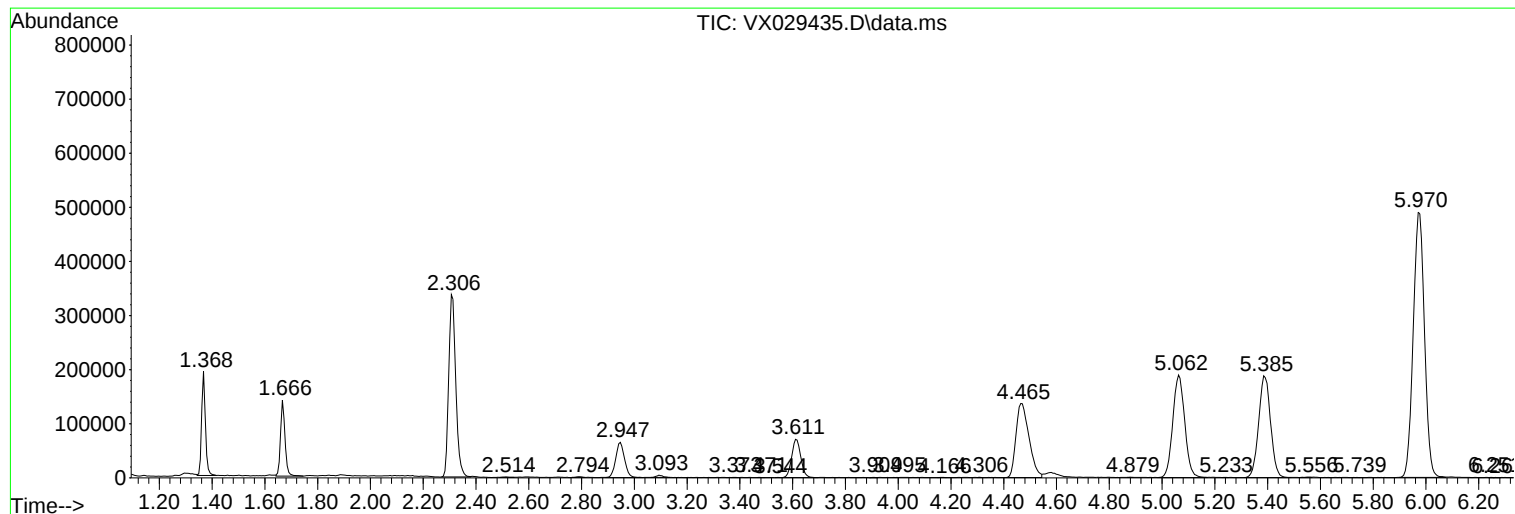

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029435.D
Acq On : 14 Jun 2022 00:22
Operator : JC/MD
Sample : N3248-02DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYW7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029435.D
Acq On : 14 Jun 2022 00:22
Operator : JC/MD
Sample : N3248-02DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYW7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc