

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029436.D
 Acq On : 14 Jun 2022 00:45
 Operator : JC/MD
 Sample : N3248-03DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYW8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	184026	184823	13.16%	1.540%
2	1.666	91	95	106	rVB	132912	154553	11.00%	1.288%
3	2.306	194	200	212	rBV2	326627	598707	42.63%	4.988%
4	2.788	275	279	284	rVB5	1455	2363	0.17%	0.020%
5	2.946	297	305	316	rVB	32877	76296	5.43%	0.636%
6	3.099	323	330	336	rBV5	3505	7577	0.54%	0.063%
7	3.276	357	359	361	rBV2	320	350	0.02%	0.003%
8	3.611	405	414	425	rVV	66926	156975	11.18%	1.308%
9	3.989	475	476	477	rBV	337	209	0.01%	0.002%
10	4.038	480	484	485	rBV2	402	464	0.03%	0.004%
11	4.306	525	528	529	rBV	313	367	0.03%	0.003%
12	4.397	541	543	544	rBV	365	220	0.02%	0.002%
13	4.465	544	554	567	rBV2	133498	455218	32.41%	3.792%
14	4.867	617	620	622	rBV2	186	253	0.02%	0.002%
15	5.062	640	652	669	rBV	181125	564974	40.23%	4.707%
16	5.281	686	688	689	rVB2	476	276	0.02%	0.002%
17	5.385	692	705	722	rVV2	175883	553151	39.39%	4.608%
18	5.531	726	729	730	rBV2	818	577	0.04%	0.005%
19	5.842	777	780	782	rBV2	282	376	0.03%	0.003%
20	5.976	788	802	817	rBV2	471867	1404460	100.00%	11.700%
21	6.281	850	852	853	rBV	182	182	0.01%	0.002%
22	6.318	857	858	861	rVV2	426	409	0.03%	0.003%
23	6.361	863	865	869	rVV2	309	299	0.02%	0.002%
24	6.623	906	908	910	rBV	261	194	0.01%	0.002%
25	6.763	920	931	950	rBV	349276	841271	59.90%	7.008%
26	6.915	955	956	957	rBV	454	188	0.01%	0.002%
27	7.049	976	978	980	rBV2	286	232	0.02%	0.002%
28	7.129	982	991	1004	rBV3	67499	156080	11.11%	1.300%
29	7.220	1004	1006	1009	rBV2	304	292	0.02%	0.002%
30	7.312	1011	1021	1036	rBV	286058	622005	44.29%	5.182%
31	7.488	1047	1050	1053	rBV3	767	867	0.06%	0.007%
32	7.586	1065	1066	1069	rBV2	324	413	0.03%	0.003%
33	7.647	1071	1076	1077	rVV2	368	459	0.03%	0.004%
34	7.738	1089	1091	1093	rBV2	221	222	0.02%	0.002%
35	7.763	1093	1095	1096	rVB2	353	217	0.02%	0.002%
36	7.781	1096	1098	1099	rBV	297	266	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029436.D
 Acq On : 14 Jun 2022 00:45
 Operator : JC/MD
 Sample : N3248-03DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYW8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.909	1116	1119	1120	rBV	424	407	0.03%	0.003%
38	8.061	1143	1144	1145	rBV	328	175	0.01%	0.001%
39	8.116	1150	1153	1154	rVV	223	208	0.01%	0.002%
40	8.202	1166	1167	1169	rBV	436	276	0.02%	0.002%
41	8.238	1171	1173	1175	rVV	339	202	0.01%	0.002%
42	8.330	1181	1188	1199	rBV	177222	289180	20.59%	2.409%
43	8.537	1220	1222	1225	rVB2	362	279	0.02%	0.002%
44	8.580	1225	1229	1231	rBV2	530	594	0.04%	0.005%
45	8.653	1234	1241	1248	rBV	715934	1130002	80.46%	9.414%
46	8.726	1249	1253	1258	rVB	9663	15364	1.09%	0.128%
47	8.872	1276	1277	1281	rVB3	521	517	0.04%	0.004%
48	8.952	1285	1290	1299	rBV	122427	177577	12.64%	1.479%
49	9.067	1307	1309	1311	rVB	435	304	0.02%	0.003%
50	9.159	1320	1324	1328	rVB4	2167	3473	0.25%	0.029%
51	9.275	1337	1343	1352	rBV	91602	133211	9.48%	1.110%
52	9.384	1356	1361	1377	rBV	566366	799113	56.90%	6.657%
53	9.646	1403	1404	1408	rBV	362	319	0.02%	0.003%
54	9.817	1429	1432	1433	rBV3	318	349	0.02%	0.003%
55	9.903	1443	1446	1447	rVB2	432	324	0.02%	0.003%
56	9.933	1449	1451	1455	rVB	339	307	0.02%	0.003%
57	9.970	1455	1457	1458	rBV	277	189	0.01%	0.002%
58	10.055	1465	1471	1485	rBV	744209	978864	69.70%	8.155%
59	10.195	1492	1494	1497	rVB3	829	820	0.06%	0.007%
60	10.256	1500	1504	1506	rBV2	401	541	0.04%	0.005%
61	10.311	1509	1513	1517	rVB3	1719	2441	0.17%	0.020%
62	10.354	1519	1520	1522	rVB2	345	200	0.01%	0.002%
63	10.390	1524	1526	1529	rBV	248	284	0.02%	0.002%
64	10.640	1565	1567	1570	rBV2	586	685	0.05%	0.006%
65	10.768	1585	1588	1591	rBV2	497	783	0.06%	0.007%
66	10.933	1613	1615	1617	rBV2	266	203	0.01%	0.002%
67	10.963	1617	1620	1622	rVV2	501	582	0.04%	0.005%
68	11.000	1625	1626	1628	rBV	319	217	0.02%	0.002%
69	11.091	1638	1641	1643	rBV4	507	584	0.04%	0.005%
70	11.122	1643	1646	1652	rVB3	2279	2709	0.19%	0.023%
71	11.195	1652	1658	1667	rBV	570336	711969	50.69%	5.931%
72	11.457	1698	1701	1703	rBV3	742	1072	0.08%	0.009%
73	11.555	1715	1717	1719	rBV	243	174	0.01%	0.001%
74	11.622	1724	1728	1729	rBV2	354	374	0.03%	0.003%
75	11.701	1739	1741	1743	rBV3	329	292	0.02%	0.002%
76	11.750	1746	1749	1754	rBV2	3408	4104	0.29%	0.034%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029436.D
 Acq On : 14 Jun 2022 00:45
 Operator : JC/MD
 Sample : N3248-03DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYW8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.841	1762	1764	1768	rVV	595	549	0.04%	0.005%
78	11.872	1768	1769	1770	rVB	489	179	0.01%	0.001%
79	11.933	1776	1779	1782	rBV3	1071	1231	0.09%	0.010%
80	12.024	1789	1794	1805	rBV	801370	963047	68.57%	8.023%
81	12.146	1812	1814	1818	rVB3	1551	1981	0.14%	0.017%
82	12.323	1837	1843	1852	rBV	791408	983041	69.99%	8.190%
83	12.390	1852	1854	1857	rVB3	849	788	0.06%	0.007%
84	12.548	1879	1880	1882	rBV	298	232	0.02%	0.002%
85	12.573	1882	1884	1888	rVV2	367	437	0.03%	0.004%
86	12.731	1909	1910	1911	rBV	375	185	0.01%	0.002%
87	12.786	1918	1919	1922	rBV2	259	290	0.02%	0.002%
88	13.054	1961	1963	1966	rVB2	424	361	0.03%	0.003%
89	13.121	1970	1974	1979	rVB3	589	803	0.06%	0.007%
90	13.158	1979	1980	1982	rBV	287	240	0.02%	0.002%
91	13.304	2000	2004	2008	rBV2	413	623	0.04%	0.005%
92	13.463	2028	2030	2031	rBV2	385	228	0.02%	0.002%
93	13.518	2038	2039	2041	rBV2	344	191	0.01%	0.002%
94	13.591	2048	2051	2055	rBV4	567	707	0.05%	0.006%
95	13.682	2064	2066	2068	rBV	307	241	0.02%	0.002%
96	13.780	2080	2082	2086	rVB3	776	920	0.07%	0.008%
97	13.999	2116	2118	2119	rBV2	418	276	0.02%	0.002%
98	15.176	2308	2311	2313	rBV2	670	840	0.06%	0.007%
99	15.901	2428	2430	2433	rBV3	696	696	0.05%	0.006%
100	15.981	2442	2443	2445	rBV2	581	504	0.04%	0.004%




Sum of corrected areas: 12003643

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029436.D
Acq On : 14 Jun 2022 00:45
Operator : JC/MD
Sample : N3248-03DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYW8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

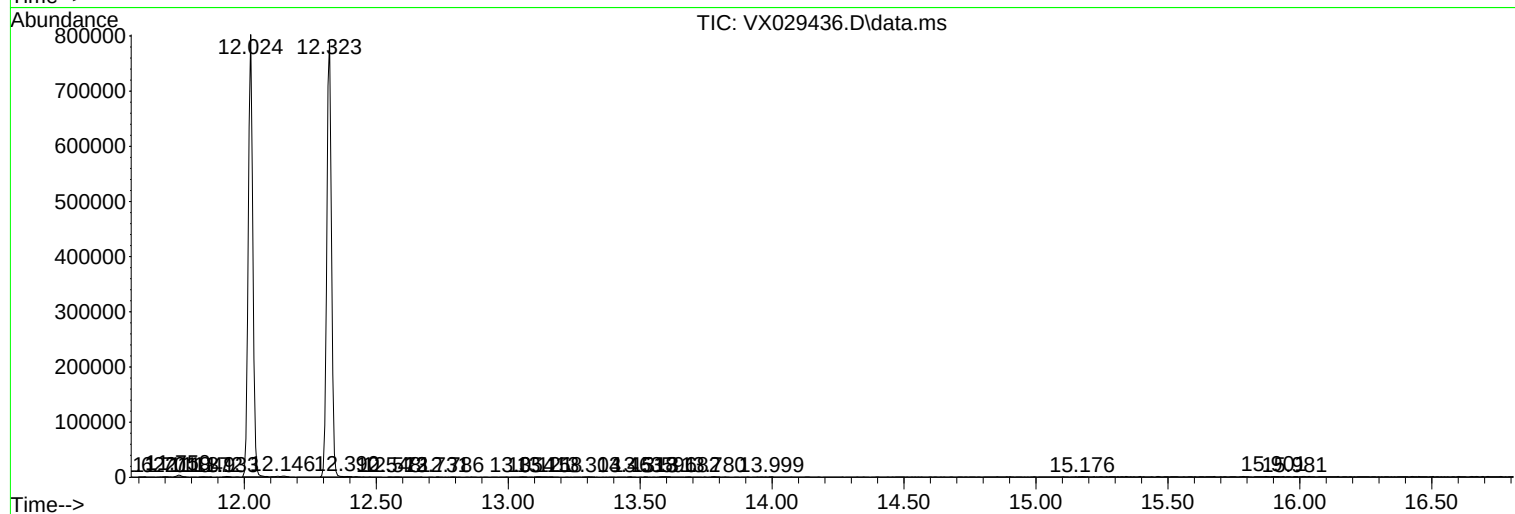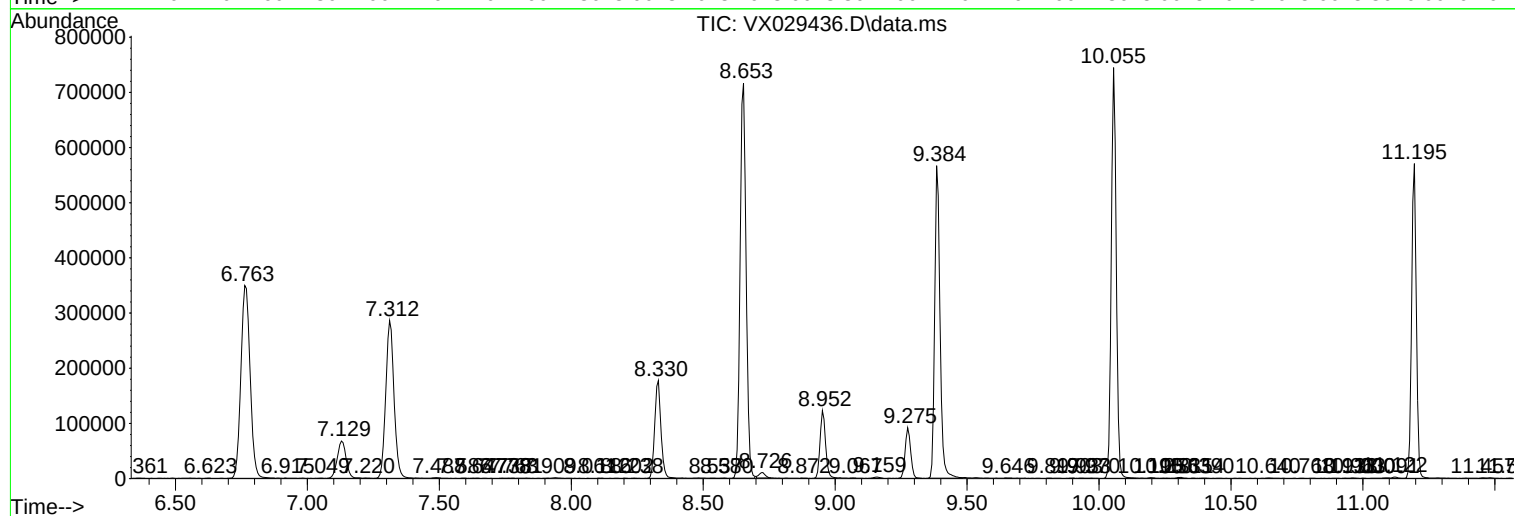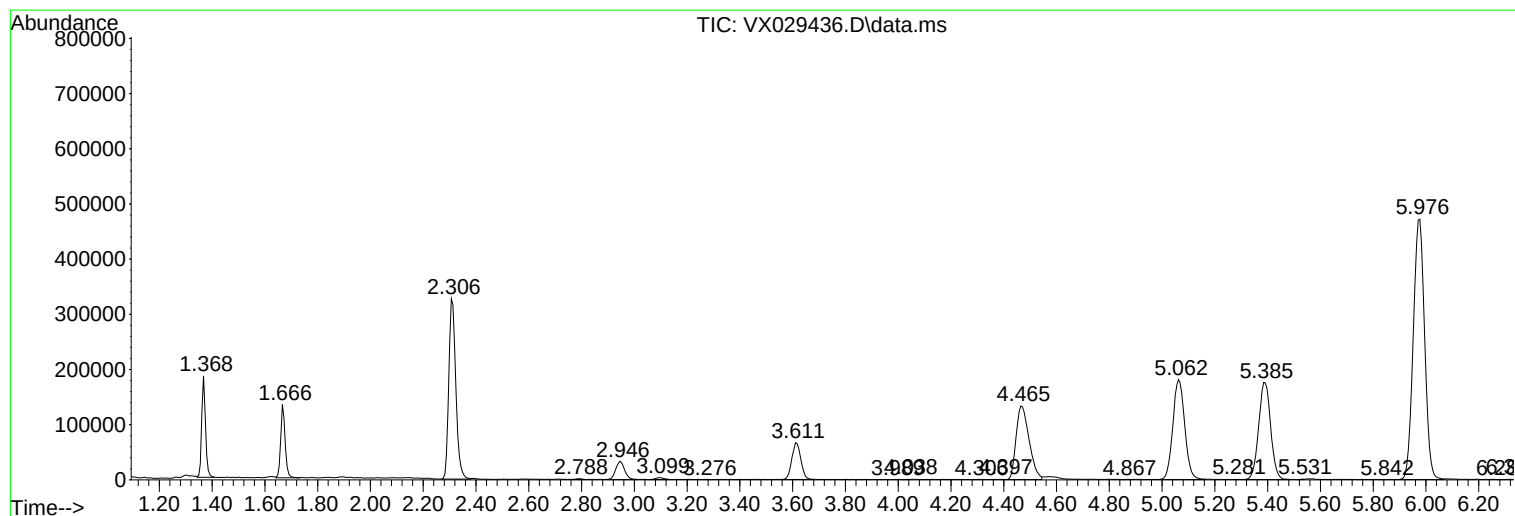

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029436.D
Acq On : 14 Jun 2022 00:45
Operator : JC/MD
Sample : N3248-03DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYW8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029436.D
Acq On : 14 Jun 2022 00:45
Operator : JC/MD
Sample : N3248-03DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYW8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------