

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029437.D
 Acq On : 14 Jun 2022 01:08
 Operator : JC/MD
 Sample : N3248-04DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYW9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029437.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB	187879	188688	13.43%	1.555%
2	1.666	91	95	104	rVB	132195	156122	11.12%	1.287%
3	2.306	194	200	211	rBV2	326249	600500	42.75%	4.950%
4	2.788	275	279	285	rVB4	1585	2997	0.21%	0.025%
5	2.892	292	296	297	rBV	465	628	0.04%	0.005%
6	2.947	297	305	318	rVV	63043	146178	10.41%	1.205%
7	3.099	325	330	336	rVB4	2506	4779	0.34%	0.039%
8	3.300	362	363	365	rBV	333	235	0.02%	0.002%
9	3.459	387	389	390	rBV2	248	194	0.01%	0.002%
10	3.556	402	405	406	rBV2	391	388	0.03%	0.003%
11	3.617	406	415	427	rVB	47492	114829	8.18%	0.947%
12	3.824	447	449	453	rBV3	257	329	0.02%	0.003%
13	3.971	470	473	477	rBV3	262	434	0.03%	0.004%
14	4.172	503	506	508	rBV3	271	308	0.02%	0.003%
15	4.355	534	536	538	rVB	407	273	0.02%	0.002%
16	4.404	542	544	545	rBV	352	299	0.02%	0.002%
17	4.471	545	555	568	rBV3	141326	511929	36.45%	4.220%
18	4.836	614	615	617	rBV	427	342	0.02%	0.003%
19	5.062	640	652	671	rBV	185404	569912	40.58%	4.698%
20	5.391	693	706	719	rVB	144761	449308	31.99%	3.704%
21	5.970	790	801	817	rBV2	471008	1404534	100.00%	11.578%
22	6.196	836	838	840	rVB	291	220	0.02%	0.002%
23	6.263	847	849	852	rBV2	259	276	0.02%	0.002%
24	6.336	859	861	863	rBV2	401	514	0.04%	0.004%
25	6.550	894	896	900	rBV2	264	357	0.03%	0.003%
26	6.763	920	931	948	rBV	357364	858702	61.14%	7.078%
27	6.879	948	950	953	rVB3	418	328	0.02%	0.003%
28	6.958	961	963	966	rBV3	399	461	0.03%	0.004%
29	7.129	983	991	1002	rBV	106968	239666	17.06%	1.976%
30	7.312	1012	1021	1034	rBV	289283	623481	44.39%	5.139%
31	7.427	1039	1040	1041	rBV	425	236	0.02%	0.002%
32	7.476	1045	1048	1049	rBV2	526	546	0.04%	0.005%
33	7.543	1057	1059	1060	rVB2	400	252	0.02%	0.002%
34	7.610	1069	1070	1072	rBV2	414	340	0.02%	0.003%
35	7.885	1113	1115	1117	rVB2	389	254	0.02%	0.002%
36	7.940	1117	1124	1131	rBV6	1268	3241	0.23%	0.027%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029437.D
 Acq On : 14 Jun 2022 01:08
 Operator : JC/MD
 Sample : N3248-04DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYW9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	8.074	1144	1146	1148	rBV2	209	210	0.01%	0.002%
38	8.190	1164	1165	1168	rBV2	244	191	0.01%	0.002%
39	8.257	1174	1176	1179	rBV2	181	204	0.01%	0.002%
40	8.330	1181	1188	1199	rVV	177356	288558	20.54%	2.379%
41	8.409	1199	1201	1204	rVB2	707	571	0.04%	0.005%
42	8.580	1227	1229	1234	rBV4	518	822	0.06%	0.007%
43	8.653	1234	1241	1249	rVV	726929	1137065	80.96%	9.373%
44	8.726	1249	1253	1261	rVB	9333	16283	1.16%	0.134%
45	8.854	1272	1274	1278	rVB3	443	458	0.03%	0.004%
46	8.952	1284	1290	1303	rBV	126002	182011	12.96%	1.500%
47	9.067	1308	1309	1312	rBV2	284	291	0.02%	0.002%
48	9.159	1320	1324	1329	rBV4	2706	3801	0.27%	0.031%
49	9.275	1337	1343	1352	rVB2	87830	128787	9.17%	1.062%
50	9.384	1356	1361	1374	rBV	548414	800825	57.02%	6.601%
51	9.665	1405	1407	1411	rVB2	344	364	0.03%	0.003%
52	9.927	1448	1450	1451	rVB	346	192	0.01%	0.002%
53	9.945	1451	1453	1456	rBV2	182	236	0.02%	0.002%
54	10.055	1465	1471	1485	rBV	745525	993617	70.74%	8.190%
55	10.305	1509	1512	1515	rBV2	1612	1821	0.13%	0.015%
56	10.366	1520	1522	1525	rVB3	353	266	0.02%	0.002%
57	10.451	1535	1536	1541	rBV3	237	368	0.03%	0.003%
58	10.592	1555	1559	1562	rBV2	270	398	0.03%	0.003%
59	10.701	1574	1577	1580	rVB2	455	580	0.04%	0.005%
60	10.732	1580	1582	1583	rBV	594	493	0.04%	0.004%
61	10.787	1588	1591	1592	rVB2	274	213	0.02%	0.002%
62	10.799	1592	1593	1596	rBV2	386	379	0.03%	0.003%
63	11.043	1631	1633	1636	rVB3	262	274	0.02%	0.002%
64	11.122	1642	1646	1649	rVB3	2294	2828	0.20%	0.023%
65	11.195	1652	1658	1668	rVV	567488	716479	51.01%	5.906%
66	11.378	1686	1688	1691	rVB	459	260	0.02%	0.002%
67	11.463	1698	1702	1703	rBV2	653	946	0.07%	0.008%
68	11.549	1713	1716	1718	rBV2	397	310	0.02%	0.003%
69	11.616	1725	1727	1729	rBV2	479	324	0.02%	0.003%
70	11.634	1729	1730	1733	rVB	652	501	0.04%	0.004%
71	11.658	1733	1734	1735	rBV	409	298	0.02%	0.002%
72	11.707	1740	1742	1745	rBV	396	481	0.03%	0.004%
73	11.756	1745	1750	1754	rBV3	2412	3803	0.27%	0.031%
74	11.829	1760	1762	1763	rBV	259	208	0.01%	0.002%
75	11.847	1763	1765	1767	rVB2	563	432	0.03%	0.004%
76	11.939	1776	1780	1782	rBV3	997	1033	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029437.D
 Acq On : 14 Jun 2022 01:08
 Operator : JC/MD
 Sample : N3248-04DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYW9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1805	rVB	799491	977142	69.57%	8.055%
78	12.238	1827	1829	1832	rBV2	304	358	0.03%	0.003%
79	12.323	1837	1843	1850	rBV	766198	976293	69.51%	8.048%
80	12.548	1878	1880	1881	rVB	492	261	0.02%	0.002%
81	12.567	1881	1883	1885	rBV2	342	380	0.03%	0.003%
82	12.622	1890	1892	1893	rBV	333	199	0.01%	0.002%
83	12.670	1896	1900	1903	rVB4	447	645	0.05%	0.005%
84	12.798	1920	1921	1923	rBV2	324	256	0.02%	0.002%
85	12.847	1927	1929	1930	rBV2	354	230	0.02%	0.002%
86	13.115	1971	1973	1975	rBV2	593	564	0.04%	0.005%
87	13.250	1994	1995	1996	rBV	400	287	0.02%	0.002%
88	13.487	2032	2034	2037	rBV	314	336	0.02%	0.003%
89	13.591	2048	2051	2056	rBV2	622	894	0.06%	0.007%
90	13.658	2060	2062	2064	rBV2	384	362	0.03%	0.003%
91	13.774	2079	2081	2082	rBV	519	310	0.02%	0.003%
92	13.792	2082	2084	2085	rVV	699	421	0.03%	0.003%
93	13.835	2089	2091	2094	rBV2	533	526	0.04%	0.004%
94	14.633	2220	2222	2226	rBV3	461	503	0.04%	0.004%
95	14.755	2240	2242	2243	rBV2	398	240	0.02%	0.002%
96	14.786	2246	2247	2250	rVV2	562	428	0.03%	0.004%
97	14.816	2250	2252	2254	rVV2	408	285	0.02%	0.002%
98	14.877	2261	2262	2263	rBV	601	308	0.02%	0.003%
99	15.603	2379	2381	2382	rBV	720	567	0.04%	0.005%
100	16.219	2480	2482	2484	rBV	478	387	0.03%	0.003%




Sum of corrected areas: 12131443

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029437.D
Acq On : 14 Jun 2022 01:08
Operator : JC/MD
Sample : N3248-04DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYW9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

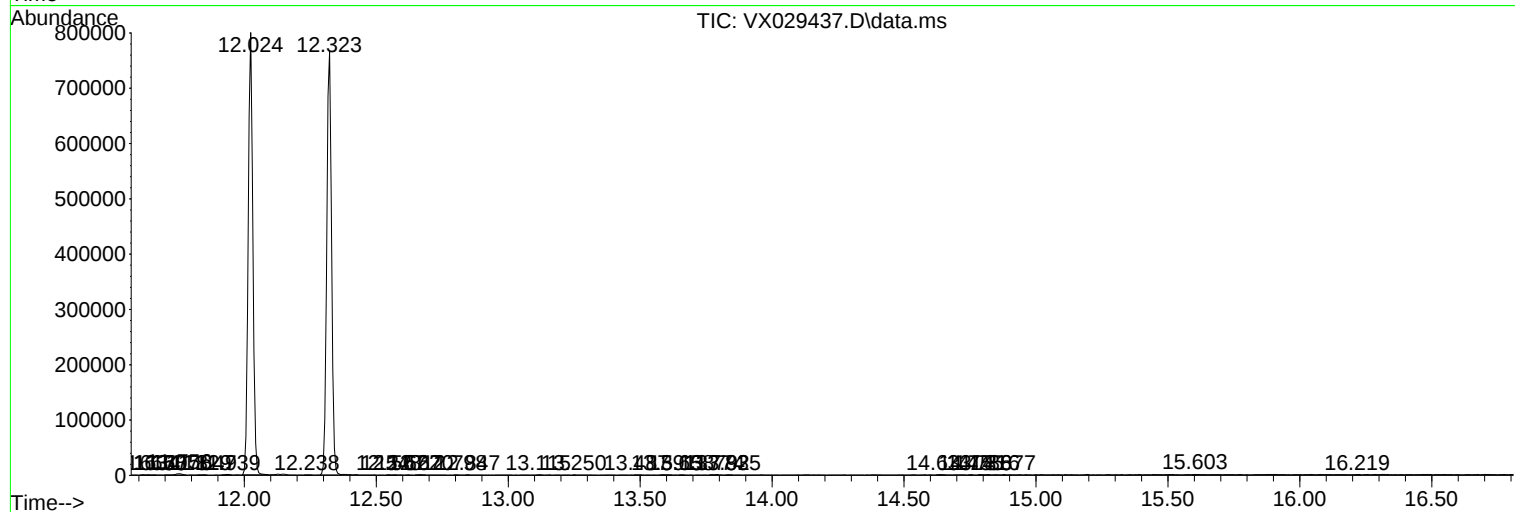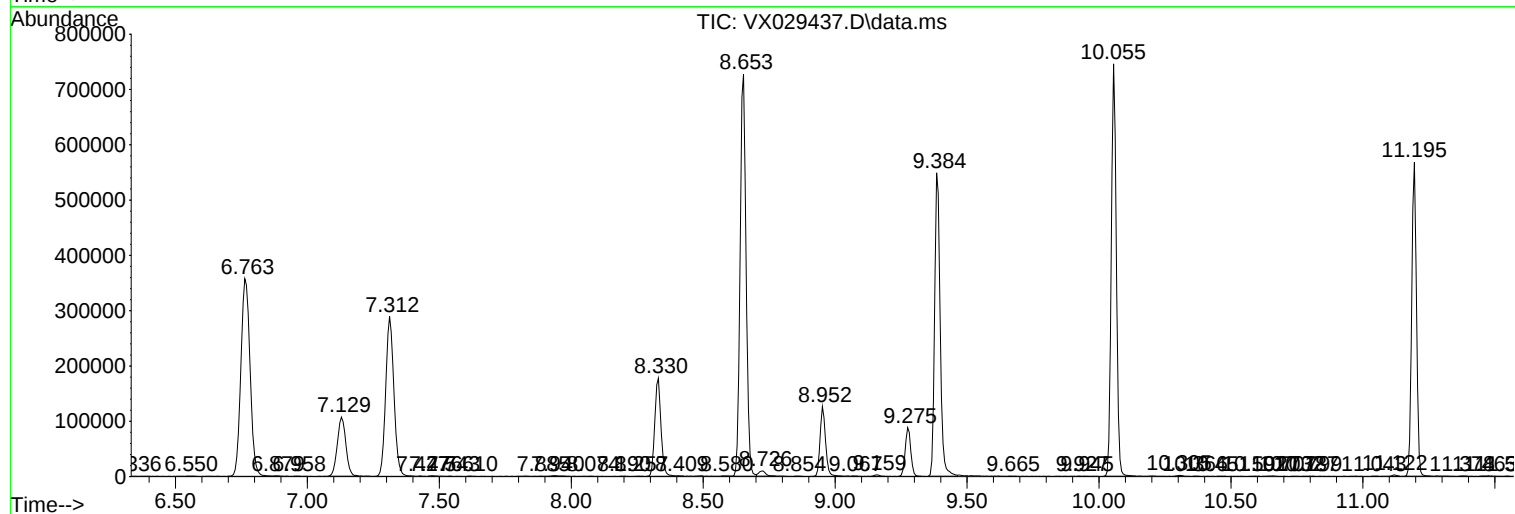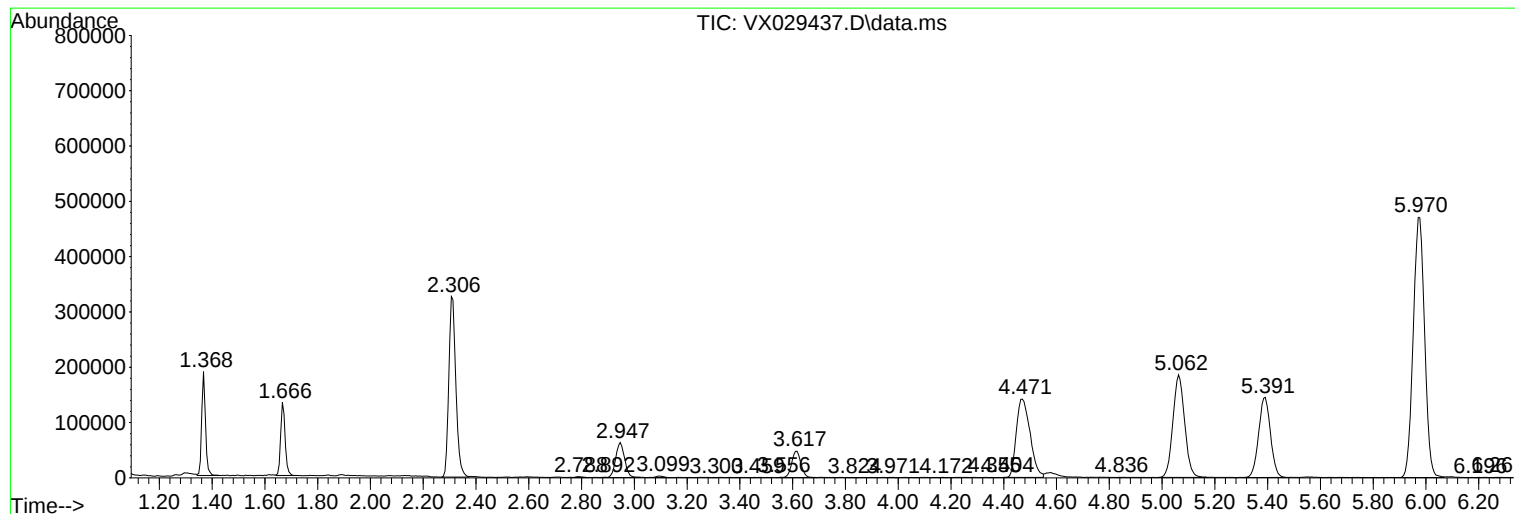

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029437.D
Acq On : 14 Jun 2022 01:08
Operator : JC/MD
Sample : N3248-04DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYW9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029437.D
Acq On : 14 Jun 2022 01:08
Operator : JC/MD
Sample : N3248-04DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYW9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------