

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029438.D
 Acq On : 14 Jun 2022 01:31
 Operator : JC/MD
 Sample : N3248-06DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYX6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB2	207619	224391	15.56%	1.886%
2	1.666	91	95	107	rVB2	99789	158650	11.00%	1.333%
3	2.306	193	200	210	rBV	297855	489703	33.96%	4.116%
4	2.709	264	266	273	rVB6	1040	1548	0.11%	0.013%
5	2.788	274	279	284	rVV3	1775	2767	0.19%	0.023%
6	2.946	296	305	323	rBV	73956	185141	12.84%	1.556%
7	3.093	324	329	338	rVB2	5223	11091	0.77%	0.093%
8	3.184	341	344	345	rBV2	314	278	0.02%	0.002%
9	3.306	363	364	367	rVB2	311	285	0.02%	0.002%
10	3.501	393	396	397	rBV2	239	283	0.02%	0.002%
11	3.611	401	414	426	rBV	113377	270193	18.74%	2.271%
12	3.824	446	449	453	rBV2	497	469	0.03%	0.004%
13	4.038	482	484	487	rVV2	306	315	0.02%	0.003%
14	4.105	493	495	497	rBV2	368	276	0.02%	0.002%
15	4.227	513	515	518	rBV	280	314	0.02%	0.003%
16	4.483	545	557	571	rBV2	185146	672747	46.65%	5.654%
17	4.885	622	623	626	rVB	292	236	0.02%	0.002%
18	5.062	638	652	667	rBV	187541	582382	40.38%	4.895%
19	5.385	694	705	720	rVV2	38798	121257	8.41%	1.019%
20	5.537	725	730	731	rBV3	472	513	0.04%	0.004%
21	5.623	743	744	750	rBV3	244	308	0.02%	0.003%
22	5.970	789	801	818	rBV2	489933	1442119	100.00%	12.120%
23	6.354	858	864	866	rBV3	1088	1851	0.13%	0.016%
24	6.531	891	893	894	rBV2	278	264	0.02%	0.002%
25	6.763	922	931	946	rBV	357298	864651	59.96%	7.267%
26	6.995	967	969	970	rBV2	397	318	0.02%	0.003%
27	7.074	980	982	983	rBV	411	314	0.02%	0.003%
28	7.129	983	991	1001	rVV4	31457	74146	5.14%	0.623%
29	7.312	1012	1021	1036	rBV	292100	638636	44.28%	5.367%
30	7.415	1036	1038	1044	rVB4	621	907	0.06%	0.008%
31	7.488	1044	1050	1053	rBV3	651	1350	0.09%	0.011%
32	7.592	1066	1067	1070	rBV2	296	240	0.02%	0.002%
33	7.696	1080	1084	1085	rBV	822	838	0.06%	0.007%
34	7.866	1110	1112	1114	rVB	354	237	0.02%	0.002%
35	7.897	1114	1117	1119	rBV	377	369	0.03%	0.003%
36	7.946	1120	1125	1130	rVV6	1173	2778	0.19%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029438.D
 Acq On : 14 Jun 2022 01:31
 Operator : JC/MD
 Sample : N3248-06DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYX6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	8.128	1152	1155	1156	rBV3	247	272	0.02%	0.002%
38	8.208	1166	1168	1170	rVB2	242	247	0.02%	0.002%
39	8.250	1173	1175	1176	rBV	356	240	0.02%	0.002%
40	8.330	1181	1188	1201	rBV	174824	293053	20.32%	2.463%
41	8.580	1224	1229	1233	rBV4	772	1208	0.08%	0.010%
42	8.653	1234	1241	1248	rVV	750327	1161046	80.51%	9.758%
43	8.720	1249	1252	1267	rVB	11751	21453	1.49%	0.180%
44	8.952	1284	1290	1305	rBV	124037	181452	12.58%	1.525%
45	9.110	1314	1316	1318	rBV2	238	273	0.02%	0.002%
46	9.165	1322	1325	1328	rVB	296	356	0.02%	0.003%
47	9.275	1336	1343	1349	rBV3	7924	11803	0.82%	0.099%
48	9.390	1356	1362	1379	rBV	526001	776223	53.83%	6.524%
49	9.750	1419	1421	1422	rVV	365	254	0.02%	0.002%
50	9.878	1440	1442	1443	rBV	354	252	0.02%	0.002%
51	9.921	1447	1449	1450	rVB2	529	274	0.02%	0.002%
52	10.055	1465	1471	1483	rBV	772659	1010195	70.05%	8.490%
53	10.195	1492	1494	1498	rVB2	1378	1668	0.12%	0.014%
54	10.305	1507	1512	1520	rBV4	1787	2754	0.19%	0.023%
55	10.390	1522	1526	1528	rBV2	312	455	0.03%	0.004%
56	10.421	1528	1531	1537	rVB3	172	315	0.02%	0.003%
57	10.543	1550	1551	1553	rBV2	352	238	0.02%	0.002%
58	10.652	1563	1569	1572	rBV3	1073	1716	0.12%	0.014%
59	10.963	1617	1620	1622	rBV3	651	669	0.05%	0.006%
60	11.061	1632	1636	1637	rBV2	287	349	0.02%	0.003%
61	11.116	1642	1645	1649	rBV2	2347	3155	0.22%	0.027%
62	11.195	1652	1658	1665	rBV	566524	698827	48.46%	5.873%
63	11.268	1668	1670	1671	rBV	451	324	0.02%	0.003%
64	11.384	1686	1689	1693	rVV4	334	566	0.04%	0.005%
65	11.457	1698	1701	1703	rBV2	684	1024	0.07%	0.009%
66	11.573	1718	1720	1722	rBV2	274	322	0.02%	0.003%
67	11.622	1724	1728	1731	rVV3	1443	2211	0.15%	0.019%
68	11.677	1734	1737	1738	rBV	359	454	0.03%	0.004%
69	11.707	1741	1742	1746	rVV	622	664	0.05%	0.006%
70	11.756	1746	1750	1756	rVB2	4650	6151	0.43%	0.052%
71	11.847	1763	1765	1768	rBV3	265	294	0.02%	0.002%
72	11.939	1775	1780	1782	rBV2	1641	1717	0.12%	0.014%
73	12.024	1789	1794	1803	rBV	798982	973680	67.52%	8.183%
74	12.244	1827	1830	1835	rVB3	935	1317	0.09%	0.011%
75	12.323	1837	1843	1856	rVB	769580	966286	67.00%	8.121%
76	12.481	1865	1869	1871	rBV2	440	489	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029438.D
 Acq On : 14 Jun 2022 01:31
 Operator : JC/MD
 Sample : N3248-06DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYX6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.548	1876	1880	1889	rVV2	7749	12643	0.88%	0.106%
78	12.786	1918	1919	1923	rVV2	441	330	0.02%	0.003%
79	12.859	1929	1931	1933	rVV2	347	351	0.02%	0.003%
80	12.884	1933	1935	1937	rVV2	295	261	0.02%	0.002%
81	12.957	1946	1947	1950	rVV	415	320	0.02%	0.003%
82	12.981	1950	1951	1954	rVV	478	279	0.02%	0.002%
83	13.048	1960	1962	1965	rBV2	372	387	0.03%	0.003%
84	13.189	1980	1985	1986	rBV2	288	399	0.03%	0.003%
85	13.408	2019	2021	2026	rBV2	383	649	0.05%	0.005%
86	13.597	2048	2052	2055	rBV2	543	724	0.05%	0.006%
87	13.731	2072	2074	2077	rBV3	306	412	0.03%	0.003%
88	13.945	2107	2109	2110	rVB	434	251	0.02%	0.002%
89	13.963	2110	2112	2117	rBV3	578	893	0.06%	0.008%
90	14.036	2122	2124	2125	rBV2	307	327	0.02%	0.003%
91	14.091	2131	2133	2135	rBV2	340	384	0.03%	0.003%
92	14.213	2151	2153	2155	rVB	447	289	0.02%	0.002%
93	14.231	2155	2156	2158	rBV2	492	410	0.03%	0.003%
94	14.371	2178	2179	2182	rBV	308	263	0.02%	0.002%
95	14.463	2192	2194	2195	rBV2	304	264	0.02%	0.002%
96	14.499	2198	2200	2202	rBV	614	581	0.04%	0.005%
97	14.658	2224	2226	2228	rBV	383	339	0.02%	0.003%
98	15.786	2409	2411	2413	rBV2	635	475	0.03%	0.004%
99	16.639	2549	2551	2553	rVV2	659	483	0.03%	0.004%
100	16.664	2553	2555	2557	rVB3	729	431	0.03%	0.004%


Sum of corrected areas: 11898556

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029438.D
Acq On : 14 Jun 2022 01:31
Operator : JC/MD
Sample : N3248-06DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYX6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

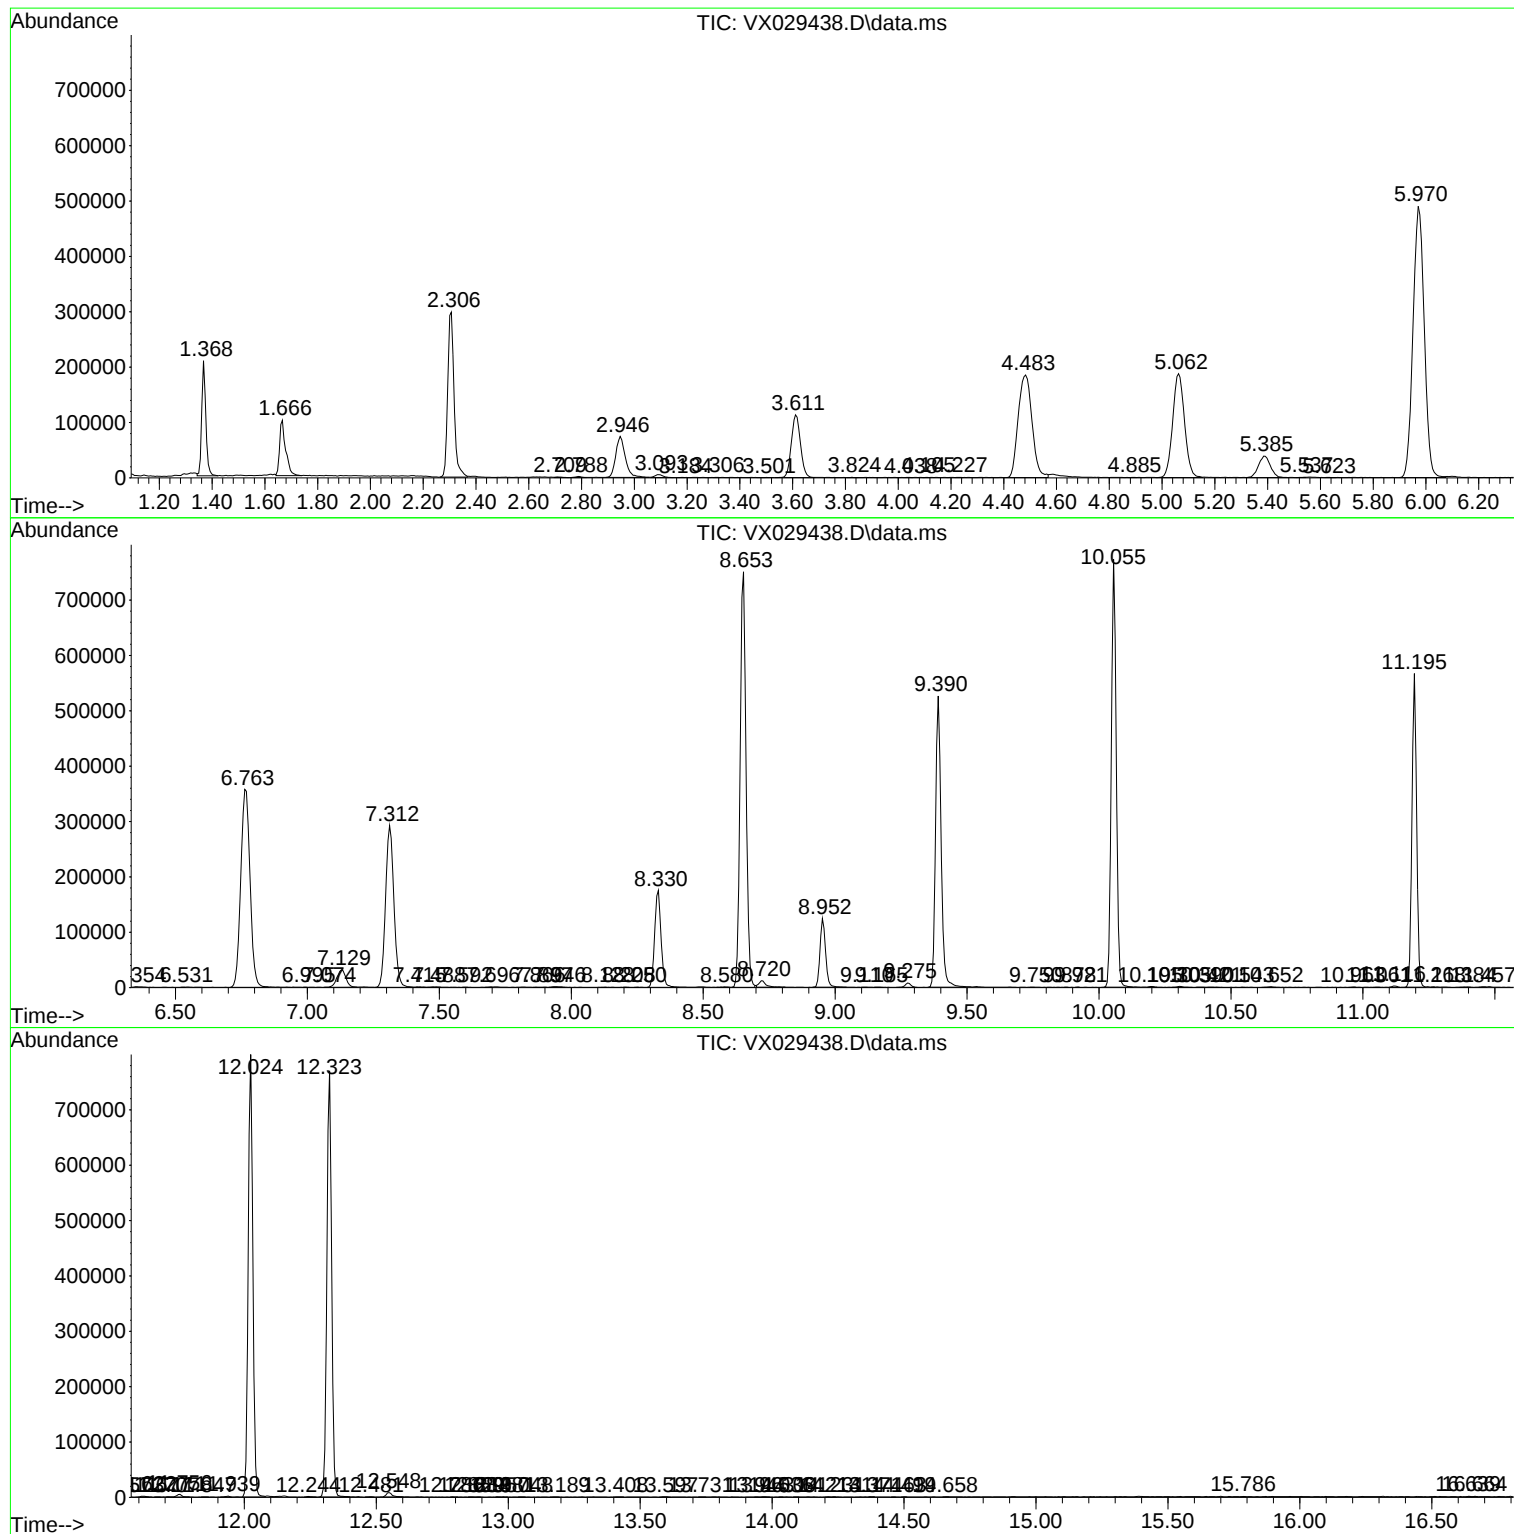

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029438.D
Acq On : 14 Jun 2022 01:31
Operator : JC/MD
Sample : N3248-06DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYX6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029438.D
Acq On : 14 Jun 2022 01:31
Operator : JC/MD
Sample : N3248-06DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYX6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc