

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029440.D
 Acq On : 14 Jun 2022 02:18
 Operator : JC/MD
 Sample : N3248-08DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYX9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029440.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	56	rVB	193395	196122	14.05%	1.692%
2	1.666	91	95	97	rBV	134902	169324	12.13%	1.461%
3	2.306	194	200	211	rBV	287746	463061	33.17%	3.996%
4	2.666	258	259	262	rBV2	377	370	0.03%	0.003%
5	2.703	262	265	266	rBV2	609	557	0.04%	0.005%
6	2.794	274	280	284	rVB5	1444	2639	0.19%	0.023%
7	2.946	296	305	322	rVB	57596	134056	9.60%	1.157%
8	3.099	325	330	334	rVV3	1564	2337	0.17%	0.020%
9	3.446	384	387	390	rBV2	308	486	0.03%	0.004%
10	3.611	405	414	427	rVV	62554	152051	10.89%	1.312%
11	3.715	430	431	434	rBV2	411	337	0.02%	0.003%
12	3.745	434	436	439	rBV2	318	396	0.03%	0.003%
13	3.904	458	462	463	rBV2	277	316	0.02%	0.003%
14	3.946	466	469	471	rBV	305	457	0.03%	0.004%
15	4.147	499	502	504	rBV2	398	428	0.03%	0.004%
16	4.184	506	508	510	rBV2	271	267	0.02%	0.002%
17	4.464	542	554	567	rBV2	138619	515257	36.91%	4.447%
18	5.062	639	652	666	rBV	184698	564493	40.44%	4.871%
19	5.391	693	706	718	rBV	78357	247962	17.76%	2.140%
20	5.556	727	733	735	rBV3	733	1332	0.10%	0.011%
21	5.623	741	744	746	rBV2	259	264	0.02%	0.002%
22	5.739	759	763	764	rBV	309	322	0.02%	0.003%
23	5.970	788	801	818	rBV3	470107	1395903	100.00%	12.046%
24	6.360	863	865	866	rBV	298	307	0.02%	0.003%
25	6.458	879	881	884	rVB2	338	277	0.02%	0.002%
26	6.763	921	931	946	rBV	361765	854316	61.20%	7.373%
27	6.982	965	967	971	rVB2	491	360	0.03%	0.003%
28	7.031	972	975	976	rBV2	287	250	0.02%	0.002%
29	7.129	983	991	1001	rVB4	27386	63672	4.56%	0.549%
30	7.311	1012	1021	1036	rBV	282317	623122	44.64%	5.377%
31	7.488	1044	1050	1053	rVB3	1015	1521	0.11%	0.013%
32	7.817	1101	1104	1108	rVB4	475	788	0.06%	0.007%
33	7.939	1116	1124	1127	rBV5	1024	2283	0.16%	0.020%
34	8.025	1136	1138	1140	rBV2	299	262	0.02%	0.002%
35	8.128	1153	1155	1157	rBV2	371	300	0.02%	0.003%
36	8.330	1181	1188	1199	rBV	169509	282585	20.24%	2.439%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029440.D
 Acq On : 14 Jun 2022 02:18
 Operator : JC/MD
 Sample : N3248-08DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYX9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	8.488	1210	1214	1218	rBV2	784	1417	0.10%	0.012%
38	8.580	1224	1229	1233	rBV3	1150	1762	0.13%	0.015%
39	8.653	1234	1241	1248	rVV	703563	1106396	79.26%	9.548%
40	8.720	1248	1252	1260	rVB	27192	45404	3.25%	0.392%
41	8.848	1270	1273	1274	rBV	389	404	0.03%	0.003%
42	8.951	1284	1290	1302	rBV	119596	180193	12.91%	1.555%
43	9.067	1308	1309	1312	rBV2	350	322	0.02%	0.003%
44	9.274	1339	1343	1349	rVB2	10414	15725	1.13%	0.136%
45	9.384	1356	1361	1379	rVV	536869	797124	57.10%	6.879%
46	9.689	1409	1411	1413	rBV	369	315	0.02%	0.003%
47	9.726	1416	1417	1420	rBV2	318	249	0.02%	0.002%
48	9.933	1450	1451	1454	rVB3	331	258	0.02%	0.002%
49	10.055	1465	1471	1484	rBV	748947	983381	70.45%	8.486%
50	10.201	1489	1495	1500	rBV	7294	10027	0.72%	0.087%
51	10.305	1507	1512	1517	rVB	14314	18576	1.33%	0.160%
52	10.506	1542	1545	1546	rBV	371	336	0.02%	0.003%
53	10.646	1564	1568	1574	rBV2	8342	11622	0.83%	0.100%
54	10.695	1574	1576	1581	rBV2	180	266	0.02%	0.002%
55	10.939	1614	1616	1618	rBV2	239	282	0.02%	0.002%
56	10.963	1618	1620	1625	rVV2	1491	1934	0.14%	0.017%
57	11.024	1628	1630	1633	rVB3	333	309	0.02%	0.003%
58	11.122	1643	1646	1650	rVB2	1965	2543	0.18%	0.022%
59	11.195	1652	1658	1667	rBV	558170	711621	50.98%	6.141%
60	11.305	1673	1676	1682	rVB	2787	3755	0.27%	0.032%
61	11.384	1684	1689	1696	rBV2	7377	11962	0.86%	0.103%
62	11.457	1697	1701	1704	rBV	3597	4664	0.33%	0.040%
63	11.616	1722	1727	1733	rVB	7428	8613	0.62%	0.074%
64	11.719	1740	1744	1745	rBV4	779	786	0.06%	0.007%
65	11.756	1745	1750	1757	rVB	20927	27343	1.96%	0.236%
66	11.890	1769	1772	1775	rVB2	915	868	0.06%	0.007%
67	11.933	1776	1779	1783	rBV3	1056	1293	0.09%	0.011%
68	11.969	1783	1785	1788	rVB3	1321	1282	0.09%	0.011%
69	12.024	1789	1794	1801	rVV	790054	962539	68.95%	8.307%
70	12.091	1801	1805	1808	rVV2	9175	12221	0.88%	0.105%
71	12.146	1812	1814	1820	rVB4	1812	2694	0.19%	0.023%
72	12.243	1825	1830	1833	rBV2	3691	5136	0.37%	0.044%
73	12.323	1837	1843	1852	rBV	747395	954379	68.37%	8.236%
74	12.469	1863	1867	1870	rVB3	1024	1461	0.10%	0.013%
75	12.500	1870	1872	1874	rBV	241	246	0.02%	0.002%
76	12.615	1888	1891	1894	rVB2	1387	1583	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029440.D
 Acq On : 14 Jun 2022 02:18
 Operator : JC/MD
 Sample : N3248-08DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYX9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.701	1902	1905	1907	rBV2	916	791	0.06%	0.007%
78	12.841	1926	1928	1932	rVV4	396	573	0.04%	0.005%
79	12.920	1939	1941	1945	rVV2	741	852	0.06%	0.007%
80	12.963	1945	1948	1953	rVB2	1298	1386	0.10%	0.012%
81	13.030	1955	1959	1960	rBV2	250	319	0.02%	0.003%
82	13.146	1974	1978	1979	rBV2	485	472	0.03%	0.004%
83	13.249	1993	1995	1997	rVB	464	294	0.02%	0.003%
84	13.292	1997	2002	2005	rBV4	1598	2379	0.17%	0.021%
85	13.451	2026	2028	2032	rVB	582	532	0.04%	0.005%
86	13.536	2038	2042	2043	rBV2	428	434	0.03%	0.004%
87	13.585	2048	2050	2054	rBV3	568	848	0.06%	0.007%
88	13.780	2077	2082	2087	rBV2	2110	3138	0.22%	0.027%
89	14.085	2130	2132	2135	rVB2	469	380	0.03%	0.003%
90	14.127	2135	2139	2141	rBV3	715	1031	0.07%	0.009%
91	14.170	2144	2146	2147	rBV2	406	297	0.02%	0.003%
92	14.420	2186	2187	2190	rBV2	341	300	0.02%	0.003%
93	14.487	2197	2198	2200	rBV2	375	276	0.02%	0.002%
94	14.676	2227	2229	2230	rBV	478	343	0.02%	0.003%
95	14.792	2246	2248	2251	rVB	583	411	0.03%	0.004%
96	14.926	2269	2270	2271	rBV	548	277	0.02%	0.002%
97	15.139	2301	2305	2306	rBV3	378	450	0.03%	0.004%
98	15.316	2332	2334	2336	rBV2	636	433	0.03%	0.004%
99	15.773	2406	2409	2412	rBV4	663	1078	0.08%	0.009%
100	16.450	2518	2520	2522	rBV3	461	351	0.03%	0.003%




Sum of corrected areas: 11587716

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029440.D
Acq On : 14 Jun 2022 02:18
Operator : JC/MD
Sample : N3248-08DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYX9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

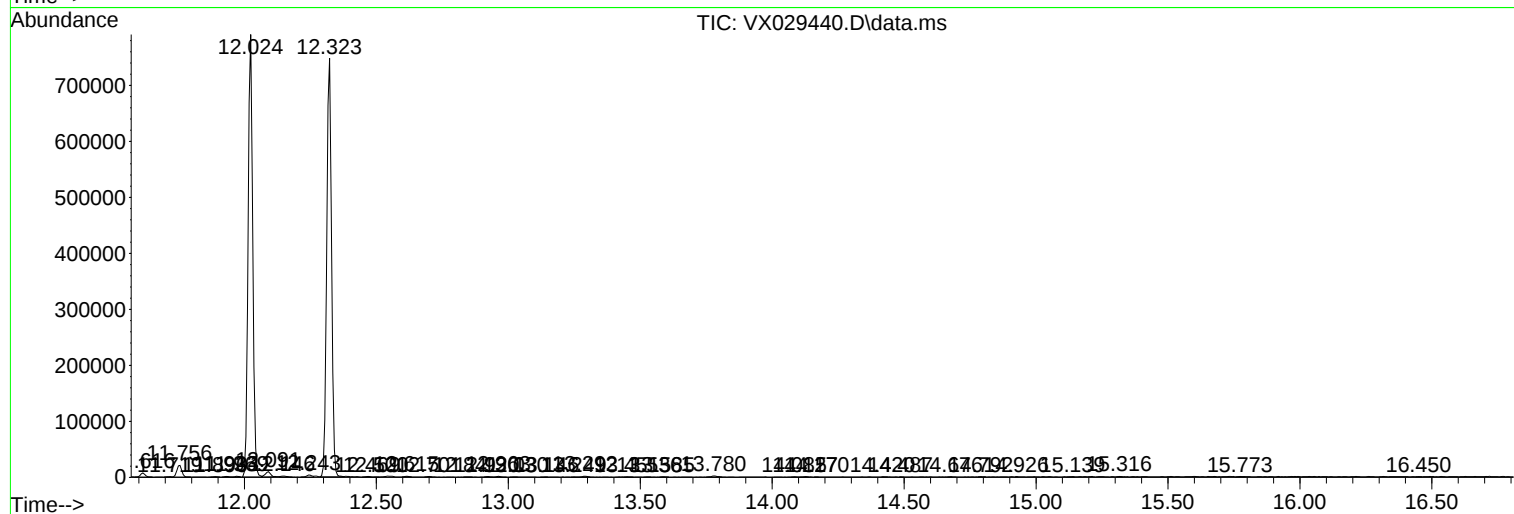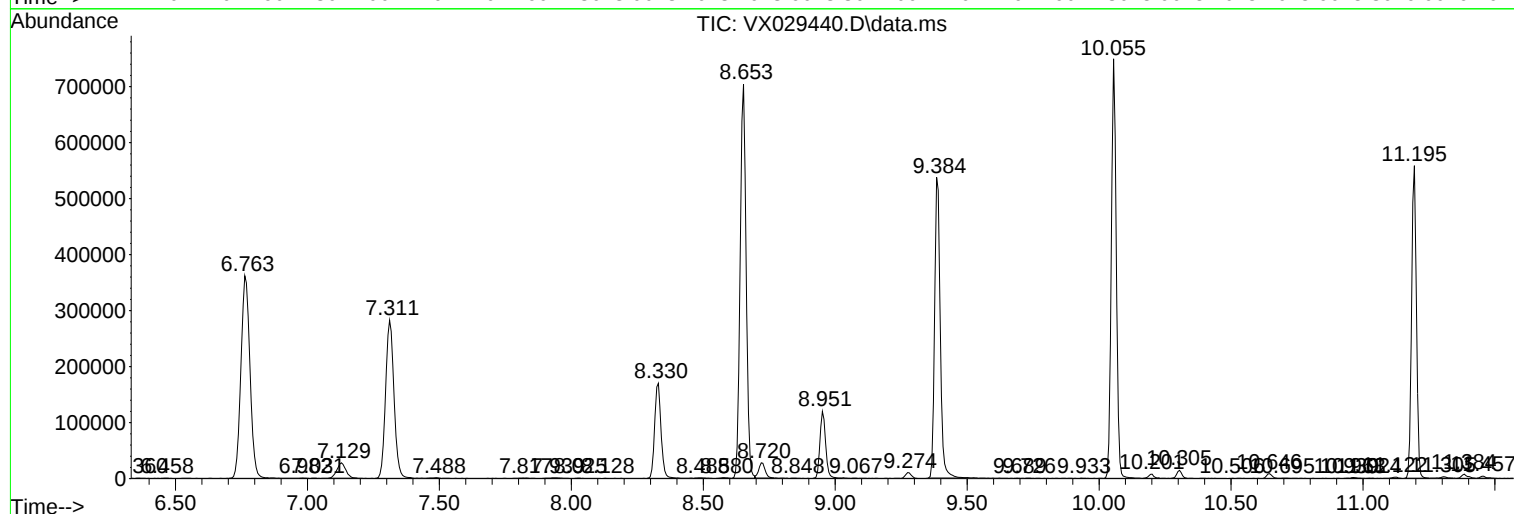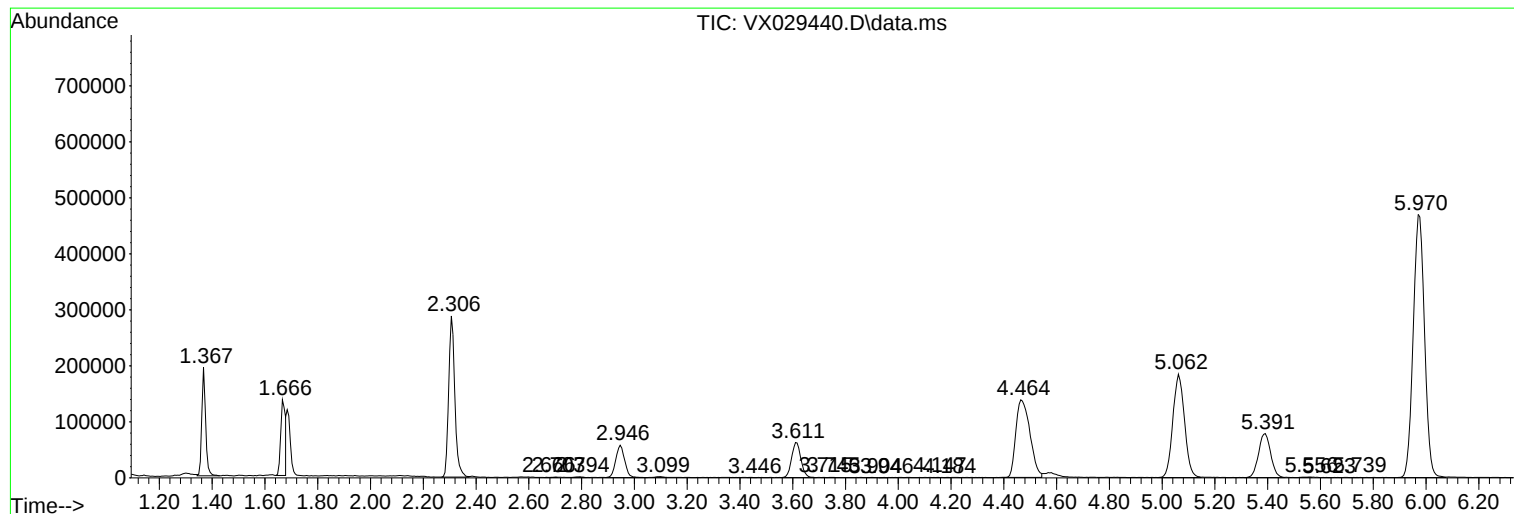

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029440.D
Acq On : 14 Jun 2022 02:18
Operator : JC/MD
Sample : N3248-08DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYX9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029440.D
Acq On : 14 Jun 2022 02:18
Operator : JC/MD
Sample : N3248-08DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYX9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc