

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029443.D
 Acq On : 14 Jun 2022 03:27
 Operator : JC/MD
 Sample : N3248-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M

Title : VOC Analysis

Signal : TIC: VX029443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	183600	183380	13.18%	1.513%
2	1.666	91	95	103	rVB	133416	154249	11.09%	1.272%
3	2.306	194	200	212	rBV2	298967	504402	36.26%	4.160%
4	2.703	262	265	266	rBV2	474	593	0.04%	0.005%
5	2.782	275	278	281	rBV3	480	691	0.05%	0.006%
6	2.934	300	303	304	rBV3	448	508	0.04%	0.004%
7	3.093	324	329	339	rVB6	3085	8176	0.59%	0.067%
8	3.166	339	341	343	rVB3	303	267	0.02%	0.002%
9	3.611	405	414	426	rBV	72393	173698	12.49%	1.433%
10	3.776	440	441	444	rVV2	366	342	0.02%	0.003%
11	3.837	450	451	454	rBV2	230	277	0.02%	0.002%
12	3.934	465	467	469	rBV2	370	295	0.02%	0.002%
13	4.056	484	487	490	rVB2	209	313	0.02%	0.003%
14	4.135	497	500	502	rBV2	300	300	0.02%	0.002%
15	4.178	504	507	511	rBV2	360	631	0.05%	0.005%
16	4.343	532	534	537	rVB2	294	288	0.02%	0.002%
17	4.373	537	539	541	rBV2	194	261	0.02%	0.002%
18	4.465	544	554	574	rBV	125091	404307	29.06%	3.335%
19	4.660	585	586	592	rVB2	442	526	0.04%	0.004%
20	5.062	639	652	670	rVV	181474	566008	40.68%	4.668%
21	5.391	690	706	723	rBV	326311	1023076	73.54%	8.438%
22	5.544	727	731	734	rBV4	426	640	0.05%	0.005%
23	5.976	787	802	817	rBV2	468765	1391247	100.00%	11.475%
24	6.129	825	827	828	rBV	495	382	0.03%	0.003%
25	6.172	833	834	837	rVV3	521	380	0.03%	0.003%
26	6.367	863	866	867	rBV2	315	371	0.03%	0.003%
27	6.501	886	888	890	rBV2	320	274	0.02%	0.002%
28	6.617	904	907	911	rBV3	240	420	0.03%	0.003%
29	6.763	922	931	947	rBV	353725	844202	60.68%	6.963%
30	7.129	982	991	1003	rBV3	40612	94525	6.79%	0.780%
31	7.238	1008	1009	1012	rVB2	364	301	0.02%	0.002%
32	7.312	1012	1021	1037	rBV	285281	618732	44.47%	5.103%
33	7.494	1045	1051	1059	rVB3	946	2752	0.20%	0.023%
34	7.610	1067	1070	1071	rBV3	304	278	0.02%	0.002%
35	7.635	1071	1074	1076	rBV3	204	272	0.02%	0.002%
36	7.744	1091	1092	1095	rBV2	344	344	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029443.D
 Acq On : 14 Jun 2022 03:27
 Operator : JC/MD
 Sample : N3248-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.933	1119	1123	1131	rBV3	1121	2291	0.16%	0.019%
38	8.061	1143	1144	1147	rBV2	270	292	0.02%	0.002%
39	8.232	1169	1172	1177	rBV2	361	597	0.04%	0.005%
40	8.330	1181	1188	1199	rBV	166736	282214	20.28%	2.328%
41	8.494	1211	1215	1218	rVB4	720	1274	0.09%	0.011%
42	8.653	1234	1241	1249	rBV	711459	1126956	81.00%	9.295%
43	8.726	1249	1253	1262	rVB	10193	17546	1.26%	0.145%
44	8.884	1277	1279	1281	rVB2	409	334	0.02%	0.003%
45	8.952	1284	1290	1301	rBV	119251	178566	12.83%	1.473%
46	9.067	1307	1309	1312	rVB2	653	593	0.04%	0.005%
47	9.092	1312	1313	1317	rBV2	391	278	0.02%	0.002%
48	9.165	1318	1325	1328	rVB5	995	1810	0.13%	0.015%
49	9.275	1337	1343	1349	rBV	56369	82462	5.93%	0.680%
50	9.384	1356	1361	1377	rBV	545148	795390	57.17%	6.560%
51	9.561	1389	1390	1393	rBV2	459	466	0.03%	0.004%
52	9.866	1436	1440	1441	rBV	443	346	0.02%	0.003%
53	9.884	1441	1443	1447	rVB2	416	408	0.03%	0.003%
54	9.939	1447	1452	1453	rBV2	325	619	0.04%	0.005%
55	10.055	1465	1471	1479	rBV	733010	983433	70.69%	8.111%
56	10.305	1509	1512	1517	rVB	1328	1758	0.13%	0.015%
57	10.445	1532	1535	1536	rBV2	397	268	0.02%	0.002%
58	10.482	1540	1541	1544	rVB2	470	408	0.03%	0.003%
59	10.512	1544	1546	1548	rBV2	439	473	0.03%	0.004%
60	10.567	1554	1555	1560	rVB2	293	368	0.03%	0.003%
61	10.652	1564	1569	1570	rBV4	495	673	0.05%	0.006%
62	10.701	1576	1577	1582	rBV2	329	541	0.04%	0.004%
63	10.939	1613	1616	1617	rBV2	224	275	0.02%	0.002%
64	11.085	1637	1640	1642	rBV2	362	420	0.03%	0.003%
65	11.122	1642	1646	1650	rVB3	2203	2936	0.21%	0.024%
66	11.195	1652	1658	1667	rVV	565445	714067	51.33%	5.890%
67	11.280	1670	1672	1674	rVV2	495	415	0.03%	0.003%
68	11.305	1674	1676	1679	rVB2	477	412	0.03%	0.003%
69	11.329	1679	1680	1683	rVB2	574	448	0.03%	0.004%
70	11.384	1686	1689	1691	rBV3	394	476	0.03%	0.004%
71	11.457	1696	1701	1702	rBV3	572	677	0.05%	0.006%
72	11.482	1702	1705	1708	rVV3	961	1153	0.08%	0.010%
73	11.750	1745	1749	1752	rBV2	2187	2992	0.22%	0.025%
74	11.884	1769	1771	1774	rBV2	272	266	0.02%	0.002%
75	11.933	1776	1779	1782	rVB3	976	1199	0.09%	0.010%
76	12.024	1788	1794	1804	rBV	789920	966110	69.44%	7.969%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029443.D
 Acq On : 14 Jun 2022 03:27
 Operator : JC/MD
 Sample : N3248-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1852	rBV	756635	964802	69.35%	7.958%
78	12.518	1873	1875	1878	rBV3	287	308	0.02%	0.003%
79	12.597	1887	1888	1890	rBV	368	295	0.02%	0.002%
80	12.798	1917	1921	1925	rBV3	319	528	0.04%	0.004%
81	12.859	1929	1931	1934	rVV2	462	418	0.03%	0.003%
82	12.890	1934	1936	1940	rVB2	304	272	0.02%	0.002%
83	12.951	1945	1946	1948	rBV2	357	263	0.02%	0.002%
84	13.006	1952	1955	1956	rBV2	271	287	0.02%	0.002%
85	13.182	1982	1984	1987	rVB2	389	391	0.03%	0.003%
86	13.256	1994	1996	1998	rBV	258	276	0.02%	0.002%
87	13.359	2011	2013	2017	rBV2	276	366	0.03%	0.003%
88	13.390	2017	2018	2023	rVB2	395	380	0.03%	0.003%
89	13.707	2069	2070	2073	rBV2	420	395	0.03%	0.003%
90	13.762	2075	2079	2080	rBV2	471	463	0.03%	0.004%
91	13.786	2080	2083	2084	rBV2	530	503	0.04%	0.004%
92	14.005	2118	2119	2123	rVB	429	374	0.03%	0.003%
93	14.048	2123	2126	2127	rBV	254	269	0.02%	0.002%
94	14.194	2146	2150	2153	rBV3	364	594	0.04%	0.005%
95	14.225	2153	2155	2157	rBV	323	339	0.02%	0.003%
96	14.335	2171	2173	2176	rBV2	378	450	0.03%	0.004%
97	14.640	2221	2223	2224	rVB	523	324	0.02%	0.003%
98	15.213	2315	2317	2319	rBV2	684	518	0.04%	0.004%
99	16.273	2489	2491	2492	rBV2	772	588	0.04%	0.005%
100	16.383	2507	2509	2511	rBV2	598	726	0.05%	0.006%


Sum of corrected areas: 12124047

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029443.D
Acq On : 14 Jun 2022 03:27
Operator : JC/MD
Sample : N3248-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

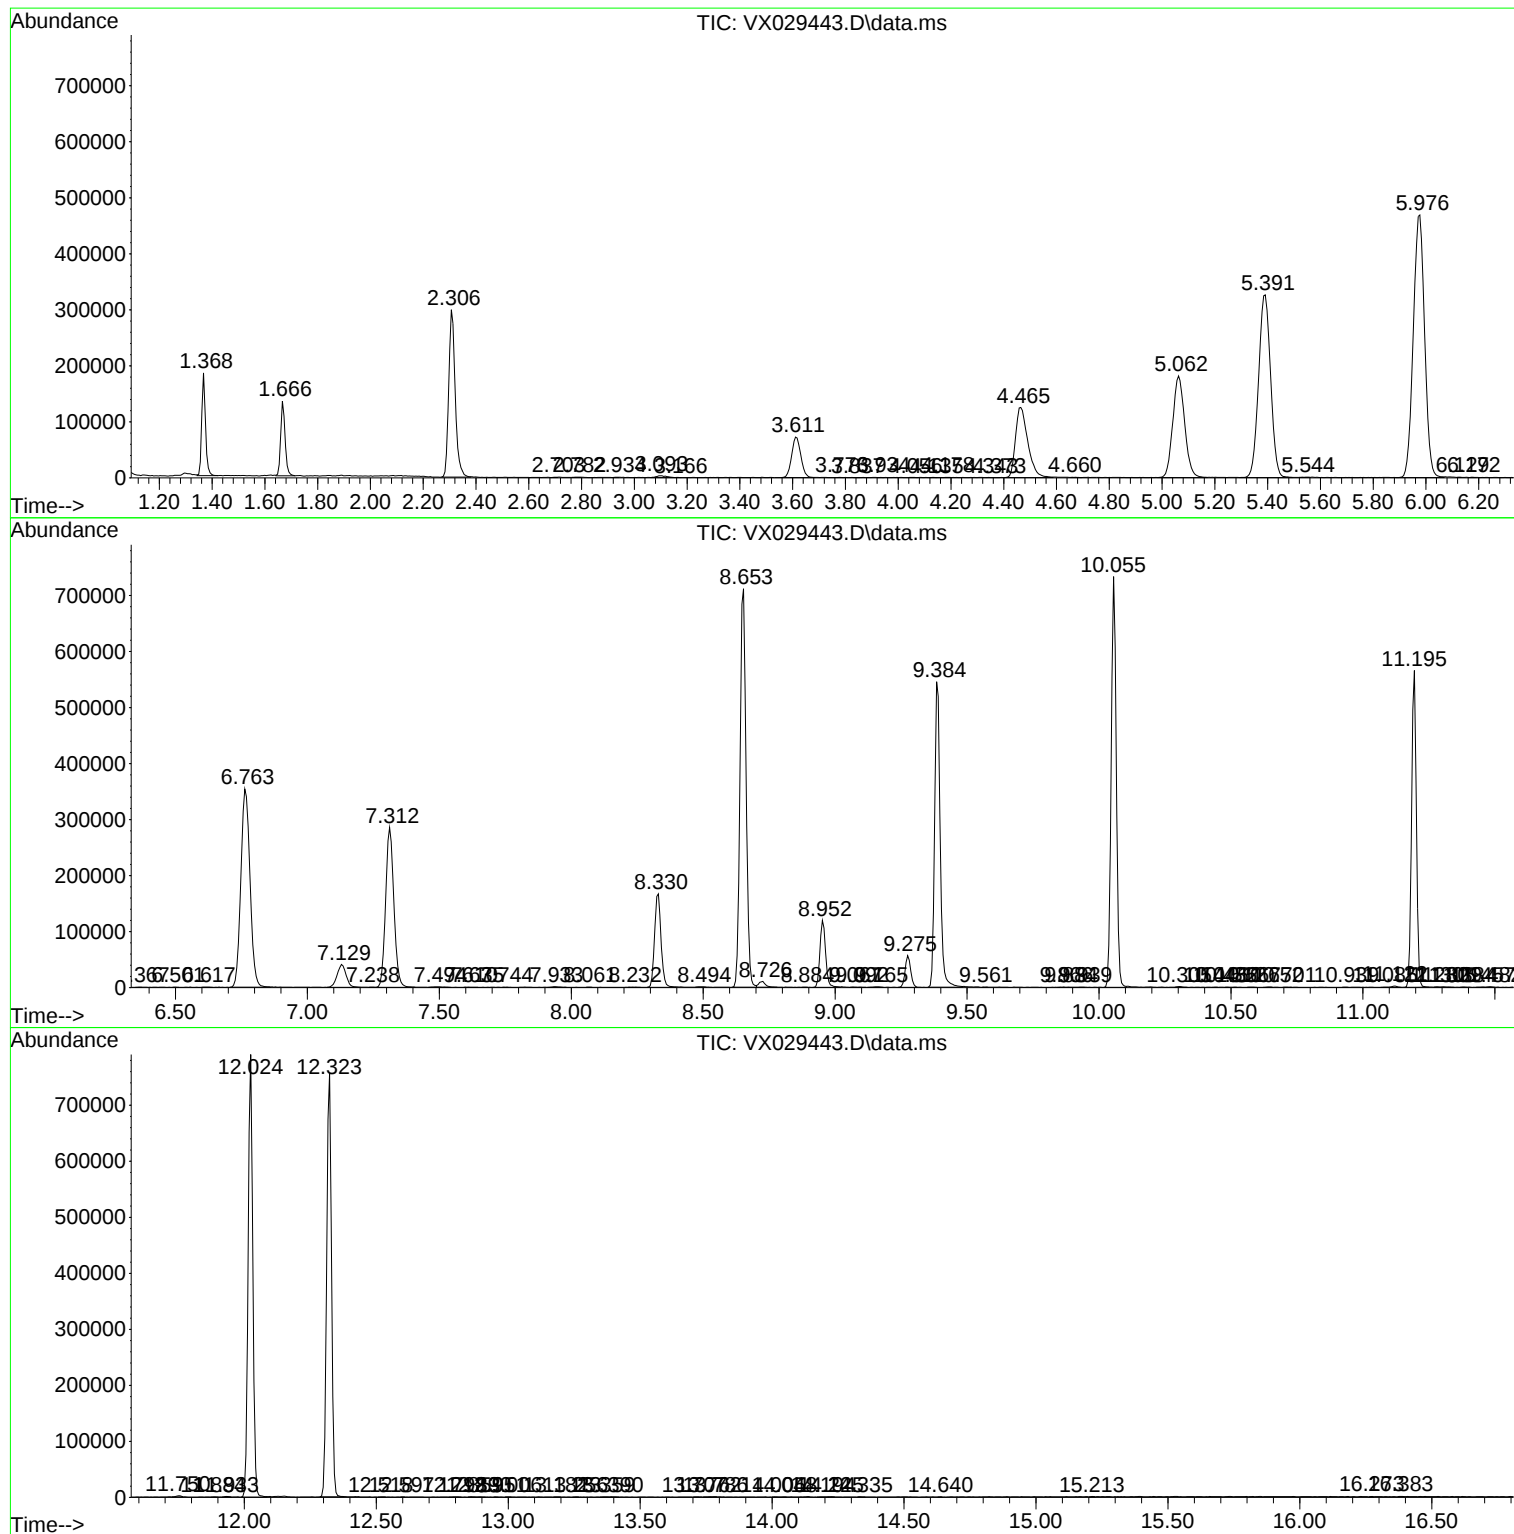

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029443.D
Acq On : 14 Jun 2022 03:27
Operator : JC/MD
Sample : N3248-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029443.D
Acq On : 14 Jun 2022 03:27
Operator : JC/MD
Sample : N3248-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc