

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029444.D
 Acq On : 14 Jun 2022 03:50
 Operator : JC/MD
 Sample : N3248-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029444.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	175632	175391	12.85%	1.502%
2	1.666	91	95	105	rVB	133804	162275	11.89%	1.390%
3	2.307	194	200	210	rBV2	295669	488924	35.83%	4.188%
4	2.508	229	233	237	rVB2	675	800	0.06%	0.007%
5	2.544	237	239	240	rBV	510	336	0.02%	0.003%
6	2.563	240	242	245	rVV	688	510	0.04%	0.004%
7	2.672	258	260	262	rBV	335	261	0.02%	0.002%
8	2.709	264	266	269	rVB2	510	555	0.04%	0.005%
9	2.788	276	279	284	rVB3	880	1166	0.09%	0.010%
10	2.947	300	305	310	rBV4	995	2114	0.15%	0.018%
11	3.038	319	320	323	rVB2	485	361	0.03%	0.003%
12	3.105	325	331	339	rVB7	2702	7273	0.53%	0.062%
13	3.245	351	354	355	rBV	347	375	0.03%	0.003%
14	3.611	404	414	427	rBV2	65770	154434	11.32%	1.323%
15	3.837	449	451	453	rVV2	309	272	0.02%	0.002%
16	3.953	468	470	473	rBV2	218	244	0.02%	0.002%
17	4.050	484	486	488	rBV2	458	454	0.03%	0.004%
18	4.257	519	520	523	rVB2	309	279	0.02%	0.002%
19	4.312	523	529	530	rBV3	301	524	0.04%	0.004%
20	4.465	544	554	572	rBV	114636	369900	27.10%	3.168%
21	4.709	590	594	595	rBV2	360	439	0.03%	0.004%
22	4.952	633	634	638	rVB2	426	374	0.03%	0.003%
23	5.062	638	652	669	rBV	179817	560103	41.04%	4.797%
24	5.391	693	706	722	rBV	282325	889347	65.17%	7.617%
25	5.977	790	802	822	rVV2	458948	1364716	100.00%	11.689%
26	6.227	839	843	845	rBV2	394	529	0.04%	0.005%
27	6.275	849	851	854	rVB3	425	355	0.03%	0.003%
28	6.342	859	862	863	rBV	260	336	0.02%	0.003%
29	6.562	897	898	900	rVB2	611	365	0.03%	0.003%
30	6.580	900	901	904	rBV2	411	346	0.03%	0.003%
31	6.763	921	931	944	rBV	348045	825804	60.51%	7.073%
32	7.001	968	970	971	rBV	423	370	0.03%	0.003%
33	7.062	977	980	982	rBV	204	275	0.02%	0.002%
34	7.129	982	991	1004	rVB3	41369	96628	7.08%	0.828%
35	7.312	1012	1021	1036	rBV	280739	607925	44.55%	5.207%
36	7.495	1043	1051	1054	rBV4	1079	2294	0.17%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029444.D
 Acq On : 14 Jun 2022 03:50
 Operator : JC/MD
 Sample : N3248-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.574	1061	1064	1066	rBV2	211	259	0.02%	0.002%
38	7.708	1084	1086	1088	rVV2	387	279	0.02%	0.002%
39	7.824	1101	1105	1108	rBV2	489	788	0.06%	0.007%
40	7.934	1120	1123	1124	rBV	836	800	0.06%	0.007%
41	8.031	1136	1139	1141	rBV2	325	363	0.03%	0.003%
42	8.092	1147	1149	1151	rVB	331	255	0.02%	0.002%
43	8.135	1153	1156	1158	rBV3	258	284	0.02%	0.002%
44	8.220	1167	1170	1173	rBV2	264	488	0.04%	0.004%
45	8.269	1176	1178	1181	rVV3	275	251	0.02%	0.002%
46	8.330	1181	1188	1203	rVV	164768	280494	20.55%	2.402%
47	8.555	1223	1225	1227	rBV2	298	291	0.02%	0.002%
48	8.653	1234	1241	1248	rVV	696945	1099831	80.59%	9.420%
49	8.720	1249	1252	1262	rVB2	9420	16502	1.21%	0.141%
50	8.866	1273	1276	1277	rBV2	343	378	0.03%	0.003%
51	8.952	1284	1290	1302	rBV	121680	175914	12.89%	1.507%
52	9.153	1321	1323	1329	rBV4	1062	1774	0.13%	0.015%
53	9.275	1338	1343	1351	rVB	50836	74100	5.43%	0.635%
54	9.385	1356	1361	1380	rBV	491404	738868	54.14%	6.328%
55	9.830	1433	1434	1436	rVB	462	251	0.02%	0.002%
56	9.860	1436	1439	1444	rBV3	497	619	0.05%	0.005%
57	9.903	1444	1446	1448	rBV2	352	312	0.02%	0.003%
58	10.000	1459	1462	1465	rBV2	378	506	0.04%	0.004%
59	10.055	1465	1471	1486	rBV	704762	954117	69.91%	8.172%
60	10.305	1508	1512	1516	rBV3	1335	1955	0.14%	0.017%
61	10.409	1526	1529	1530	rBV2	327	291	0.02%	0.002%
62	10.439	1530	1534	1536	rBV2	239	359	0.03%	0.003%
63	10.647	1565	1568	1570	rBV2	579	570	0.04%	0.005%
64	10.927	1612	1614	1617	rBV2	271	364	0.03%	0.003%
65	10.964	1617	1620	1623	rVB3	450	521	0.04%	0.004%
66	11.092	1637	1641	1642	rBV	633	578	0.04%	0.005%
67	11.122	1642	1646	1649	rVB2	1967	2747	0.20%	0.024%
68	11.195	1652	1658	1669	rBV	525874	696472	51.03%	5.965%
69	11.311	1675	1677	1682	rVB	2024	2414	0.18%	0.021%
70	11.402	1689	1692	1695	rVB3	372	489	0.04%	0.004%
71	11.457	1698	1701	1702	rBV	754	726	0.05%	0.006%
72	11.531	1711	1713	1715	rBV	369	413	0.03%	0.004%
73	11.591	1720	1723	1724	rVB2	372	346	0.03%	0.003%
74	11.628	1724	1729	1730	rBV3	551	770	0.06%	0.007%
75	11.671	1735	1736	1738	rBV2	268	248	0.02%	0.002%
76	11.756	1746	1750	1756	rVB4	2749	3827	0.28%	0.033%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029444.D
 Acq On : 14 Jun 2022 03:50
 Operator : JC/MD
 Sample : N3248-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.799	1756	1757	1760	rBV	242	281	0.02%	0.002%
78	11.841	1762	1764	1769	rVB3	470	691	0.05%	0.006%
79	11.933	1776	1779	1783	rBV4	728	1070	0.08%	0.009%
80	12.024	1788	1794	1806	rBV	772475	941521	68.99%	8.064%
81	12.323	1837	1843	1850	rBV	744202	946315	69.34%	8.105%
82	12.475	1866	1868	1871	rVB	668	624	0.05%	0.005%
83	12.506	1871	1873	1876	rBV	296	277	0.02%	0.002%
84	12.768	1909	1916	1919	rVB3	701	1239	0.09%	0.011%
85	12.841	1926	1928	1931	rVB2	313	271	0.02%	0.002%
86	12.872	1931	1933	1935	rBV2	436	382	0.03%	0.003%
87	13.049	1960	1962	1965	rVB2	507	599	0.04%	0.005%
88	13.201	1985	1987	1989	rBV2	307	295	0.02%	0.003%
89	13.225	1989	1991	1993	rVB2	310	255	0.02%	0.002%
90	13.323	2005	2007	2009	rVB	319	274	0.02%	0.002%
91	13.750	2074	2077	2078	rBV2	254	275	0.02%	0.002%
92	13.774	2080	2081	2084	rVB3	311	306	0.02%	0.003%
93	13.835	2089	2091	2093	rVB2	370	255	0.02%	0.002%
94	14.018	2120	2121	2125	rVB2	364	243	0.02%	0.002%
95	14.335	2171	2173	2175	rBV2	417	420	0.03%	0.004%
96	14.713	2233	2235	2236	rBV2	467	303	0.02%	0.003%
97	15.060	2290	2292	2294	rBV2	410	338	0.02%	0.003%
98	15.359	2339	2341	2342	rBV	595	525	0.04%	0.004%
99	16.237	2483	2485	2486	rBV2	422	288	0.02%	0.002%
100	16.438	2514	2518	2520	rBV4	600	852	0.06%	0.007%




Sum of corrected areas: 11675367

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029444.D
Acq On : 14 Jun 2022 03:50
Operator : JC/MD
Sample : N3248-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

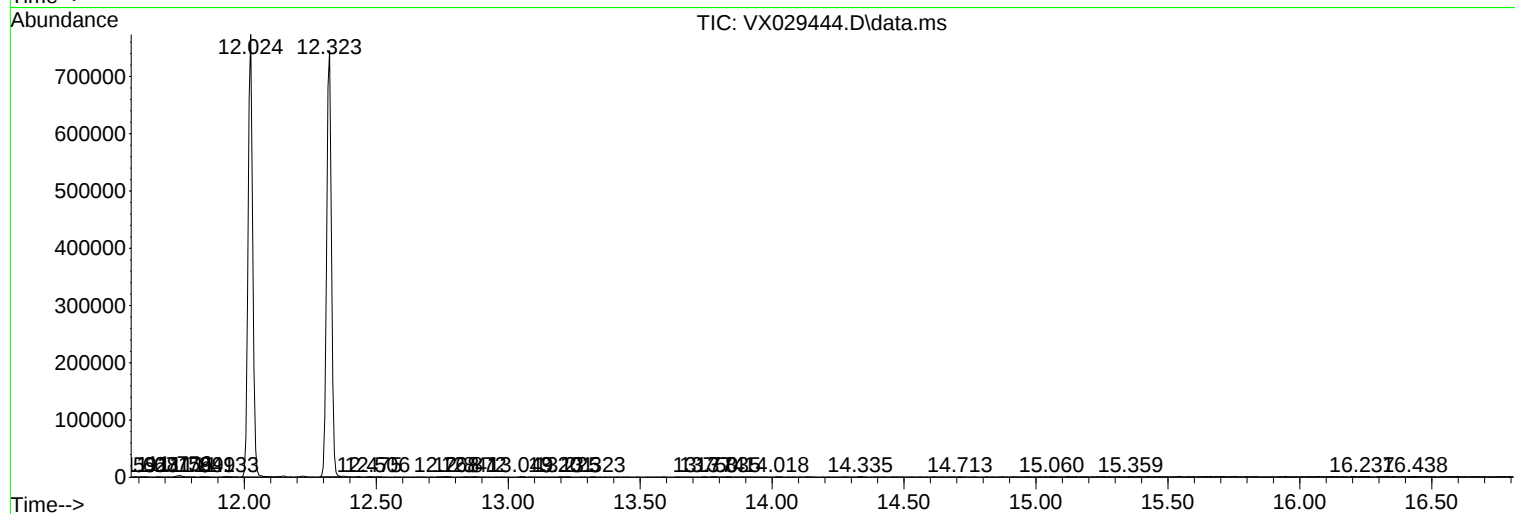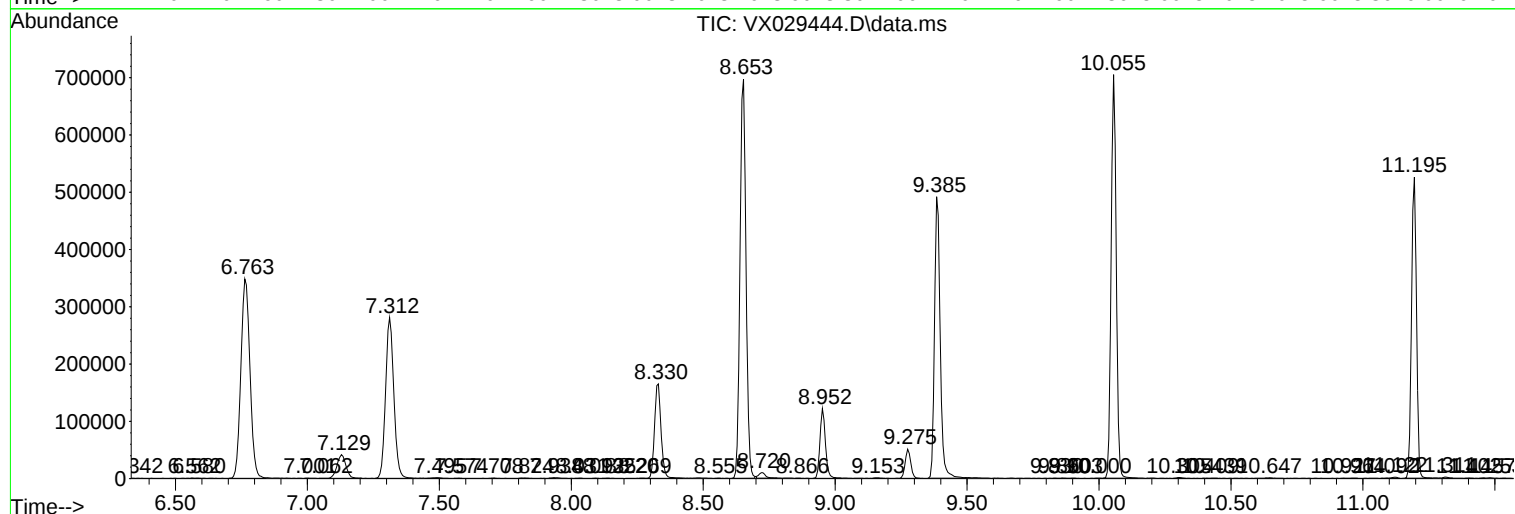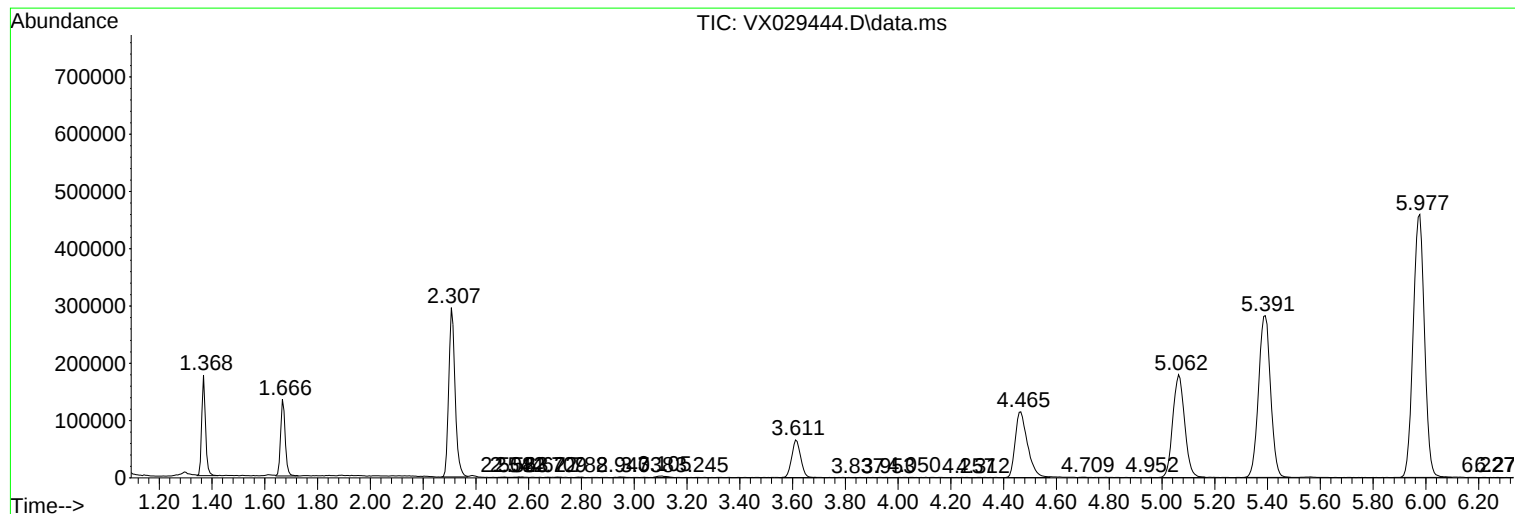

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029444.D
Acq On : 14 Jun 2022 03:50
Operator : JC/MD
Sample : N3248-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029444.D
Acq On : 14 Jun 2022 03:50
Operator : JC/MD
Sample : N3248-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------