

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029445.D
 Acq On : 14 Jun 2022 04:13
 Operator : JC/MD
 Sample : N3249-01DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYZ2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029445.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	183752	186824	13.73%	1.579%
2	1.666	91	95	104	rVB	128717	176836	12.99%	1.495%
3	2.307	194	200	211	rBV	284956	459119	33.73%	3.881%
4	2.782	274	278	285	rVB5	1501	2755	0.20%	0.023%
5	2.874	292	293	295	rBV2	414	336	0.02%	0.003%
6	2.947	296	305	317	rVV	58265	136239	10.01%	1.152%
7	3.099	325	330	338	rVB5	3523	7187	0.53%	0.061%
8	3.337	367	369	370	rVV	484	291	0.02%	0.002%
9	3.355	370	372	375	rVB	575	433	0.03%	0.004%
10	3.532	400	401	406	rBV2	320	362	0.03%	0.003%
11	3.611	406	414	426	rVV	67866	158115	11.62%	1.337%
12	3.739	433	435	438	rVB3	415	401	0.03%	0.003%
13	3.837	449	451	453	rBV	377	244	0.02%	0.002%
14	3.953	469	470	474	rBV	371	360	0.03%	0.003%
15	4.282	520	524	527	rVB2	227	401	0.03%	0.003%
16	4.489	544	558	569	rBV2	253152	923279	67.83%	7.805%
17	5.062	640	652	670	rVB	181454	547034	40.19%	4.624%
18	5.294	688	690	693	rBV2	344	318	0.02%	0.003%
19	5.391	693	706	723	rVV2	89702	284524	20.90%	2.405%
20	5.538	729	730	731	rBV	573	335	0.02%	0.003%
21	5.971	787	801	817	rBV2	456117	1361150	100.00%	11.506%
22	6.477	882	884	890	rVB2	290	462	0.03%	0.004%
23	6.544	890	895	896	rBV	407	679	0.05%	0.006%
24	6.617	904	907	909	rBV2	349	363	0.03%	0.003%
25	6.678	916	917	920	rBV	324	251	0.02%	0.002%
26	6.763	922	931	949	rVB	345269	827182	60.77%	6.992%
27	6.940	959	960	965	rVB2	593	614	0.05%	0.005%
28	7.056	977	979	981	rVV	315	249	0.02%	0.002%
29	7.129	981	991	1003	rVV3	25336	61981	4.55%	0.524%
30	7.312	1011	1021	1038	rBV	277500	608373	44.70%	5.143%
31	7.476	1045	1048	1055	rBV4	709	1328	0.10%	0.011%
32	7.629	1071	1073	1079	rVB2	230	388	0.03%	0.003%
33	7.787	1098	1099	1101	rBV2	232	242	0.02%	0.002%
34	7.940	1119	1124	1129	rBV5	1210	3145	0.23%	0.027%
35	8.001	1132	1134	1136	rVV2	370	321	0.02%	0.003%
36	8.049	1139	1142	1144	rBV	335	341	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029445.D
 Acq On : 14 Jun 2022 04:13
 Operator : JC/MD
 Sample : N3249-01DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYZ2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	8.116	1150	1153	1154	rVV	272	241	0.02%	0.002%
38	8.184	1161	1164	1165	rBV	314	291	0.02%	0.002%
39	8.257	1174	1176	1178	rBV	322	319	0.02%	0.003%
40	8.324	1181	1187	1202	rBV	163225	275727	20.26%	2.331%
41	8.494	1209	1215	1218	rBV6	598	1282	0.09%	0.011%
42	8.574	1226	1228	1234	rBV3	1314	2205	0.16%	0.019%
43	8.653	1234	1241	1248	rVV	711209	1095862	80.51%	9.264%
44	8.720	1249	1252	1265	rVB	15006	24563	1.80%	0.208%
45	8.952	1283	1290	1302	rBV	117839	172898	12.70%	1.462%
46	9.153	1321	1323	1324	rBV2	353	242	0.02%	0.002%
47	9.196	1328	1330	1335	rVB2	343	436	0.03%	0.004%
48	9.281	1338	1344	1348	rBV	11050	16892	1.24%	0.143%
49	9.385	1356	1361	1377	rBV	538827	782227	57.47%	6.612%
50	9.848	1433	1437	1439	rVB3	300	312	0.02%	0.003%
51	10.055	1465	1471	1481	rBV	737518	967433	71.07%	8.178%
52	10.201	1491	1495	1500	rVB	3068	3837	0.28%	0.032%
53	10.305	1508	1512	1518	rVB2	5742	8096	0.59%	0.068%
54	10.647	1564	1568	1572	rBV	10815	14850	1.09%	0.126%
55	10.775	1585	1589	1590	rBV2	238	261	0.02%	0.002%
56	10.964	1618	1620	1625	rVB	601	691	0.05%	0.006%
57	11.079	1638	1639	1642	rBV2	259	289	0.02%	0.002%
58	11.122	1642	1646	1652	rVV3	1603	2168	0.16%	0.018%
59	11.195	1652	1658	1668	rVV	546376	697378	51.23%	5.895%
60	11.305	1673	1676	1681	rVV3	1659	2278	0.17%	0.019%
61	11.396	1685	1691	1696	rVV3	4054	8836	0.65%	0.075%
62	11.451	1696	1700	1708	rVB	9683	13770	1.01%	0.116%
63	11.555	1715	1717	1718	rVB	558	281	0.02%	0.002%
64	11.573	1718	1720	1722	rBV	344	341	0.03%	0.003%
65	11.616	1722	1727	1736	rVB	12131	15939	1.17%	0.135%
66	11.677	1736	1737	1739	rBV	411	300	0.02%	0.003%
67	11.720	1740	1744	1745	rBV2	591	594	0.04%	0.005%
68	11.756	1745	1750	1753	rBV2	9815	12282	0.90%	0.104%
69	11.890	1771	1772	1775	rVB3	458	434	0.03%	0.004%
70	11.933	1777	1779	1782	rVV2	899	778	0.06%	0.007%
71	11.976	1782	1786	1789	rVV3	1324	1473	0.11%	0.012%
72	12.024	1789	1794	1801	rVV	769974	944780	69.41%	7.987%
73	12.091	1801	1805	1810	rVB	15443	20523	1.51%	0.173%
74	12.244	1826	1830	1837	rBV3	4837	6859	0.50%	0.058%
75	12.323	1837	1843	1851	rBV	757534	951319	69.89%	8.042%
76	12.469	1863	1867	1873	rVB2	1184	1869	0.14%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029445.D
 Acq On : 14 Jun 2022 04:13
 Operator : JC/MD
 Sample : N3249-01DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYZ2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.549	1875	1880	1887	rVV3	5230	8036	0.59%	0.068%
78	12.616	1887	1891	1893	rVB3	1620	1760	0.13%	0.015%
79	12.707	1902	1906	1909	rBV5	953	1582	0.12%	0.013%
80	12.853	1926	1930	1933	rBV3	1183	1406	0.10%	0.012%
81	12.963	1945	1948	1951	rBV2	1456	1669	0.12%	0.014%
82	13.042	1959	1961	1962	rBV	362	322	0.02%	0.003%
83	13.091	1967	1969	1971	rVV	361	306	0.02%	0.003%
84	13.140	1975	1977	1980	rBV3	233	240	0.02%	0.002%
85	13.286	1999	2001	2006	rVB3	1686	2176	0.16%	0.018%
86	13.420	2021	2023	2027	rVB3	685	729	0.05%	0.006%
87	13.487	2033	2034	2036	rBV	376	277	0.02%	0.002%
88	13.609	2053	2054	2056	rBV	307	252	0.02%	0.002%
89	13.780	2079	2082	2087	rVB2	1694	2074	0.15%	0.018%
90	13.987	2114	2116	2119	rVB2	318	269	0.02%	0.002%
91	14.085	2128	2132	2134	rBV2	347	407	0.03%	0.003%
92	14.231	2153	2156	2158	rBV3	449	572	0.04%	0.005%
93	14.378	2178	2180	2183	rBV2	705	540	0.04%	0.005%
94	14.542	2205	2207	2212	rBV2	387	406	0.03%	0.003%
95	14.609	2216	2218	2219	rBV	587	419	0.03%	0.004%
96	14.737	2238	2239	2241	rBV2	422	293	0.02%	0.002%
97	14.859	2257	2259	2262	rVB2	629	518	0.04%	0.004%
98	15.042	2286	2289	2290	rBV3	469	608	0.04%	0.005%
99	15.499	2362	2364	2367	rBV3	708	679	0.05%	0.006%
100	16.761	2569	2571	2573	rVB	707	432	0.03%	0.004%




Sum of corrected areas: 11829590

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029445.D
Acq On : 14 Jun 2022 04:13
Operator : JC/MD
Sample : N3249-01DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYZ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

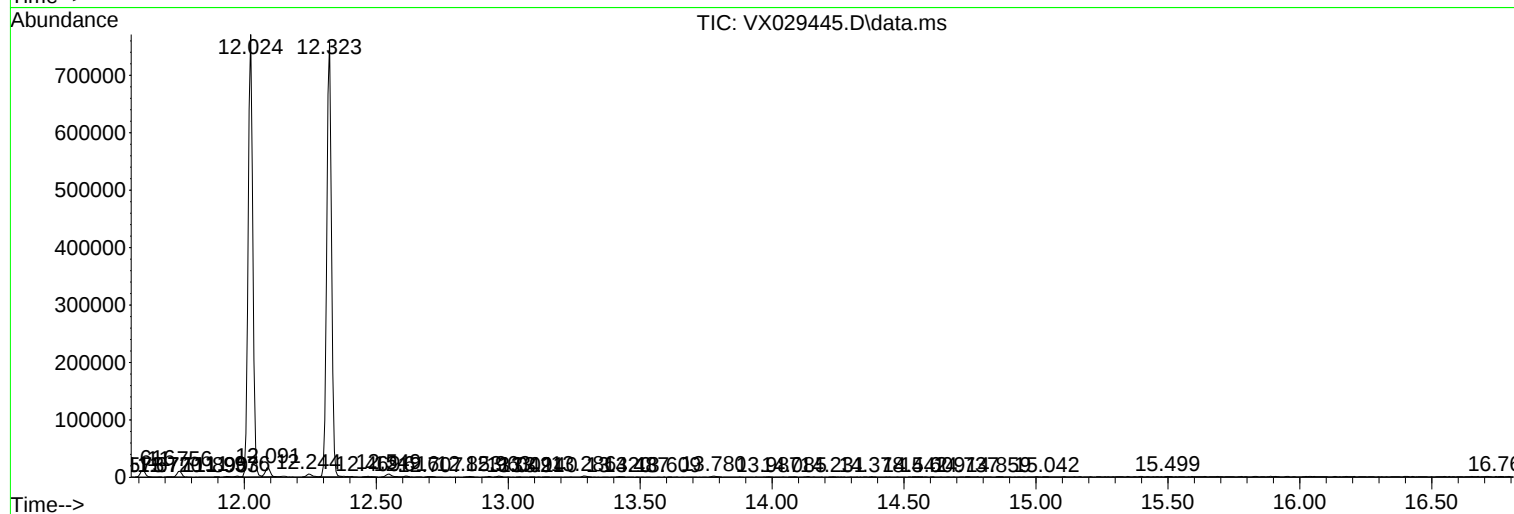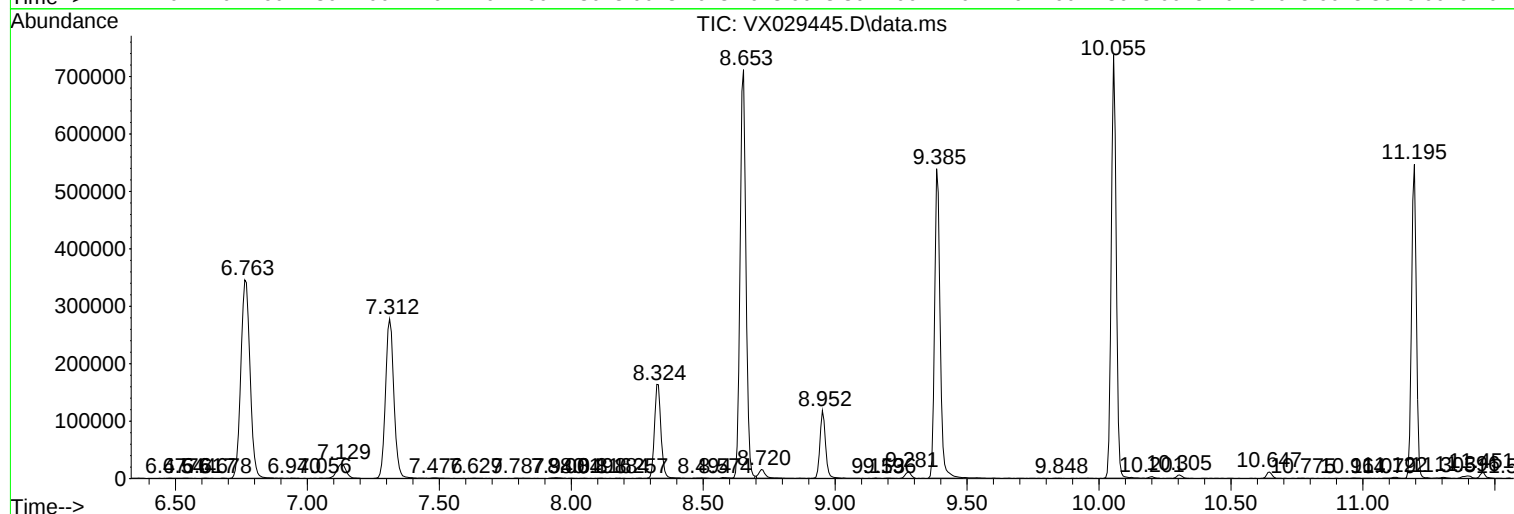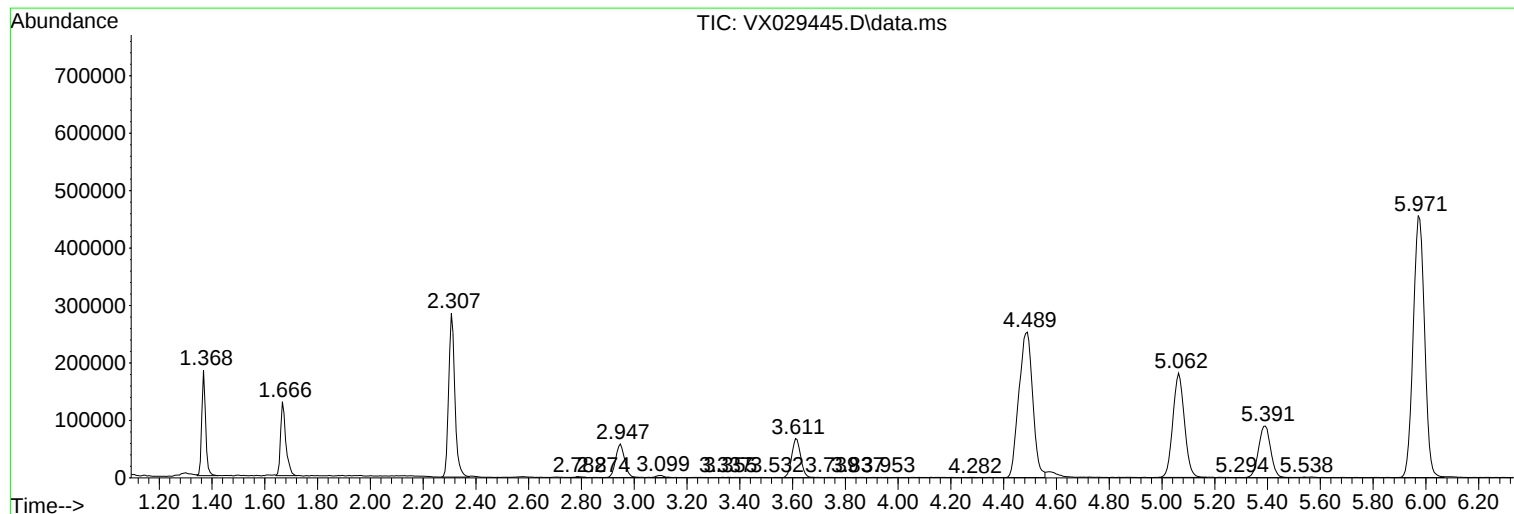

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029445.D
Acq On : 14 Jun 2022 04:13
Operator : JC/MD
Sample : N3249-01DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYZ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029445.D
Acq On : 14 Jun 2022 04:13
Operator : JC/MD
Sample : N3249-01DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYZ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------