

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029446.D
 Acq On : 14 Jun 2022 04:36
 Operator : JC/MD
 Sample : N3249-08DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYT2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029446.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB2	195590	206143	15.30%	1.803%
2	1.666	91	95	104	rVB	128160	155253	11.52%	1.358%
3	2.306	194	200	212	rBV	265663	430182	31.92%	3.762%
4	2.550	238	240	242	rBV3	447	346	0.03%	0.003%
5	2.575	242	244	248	rBV4	558	960	0.07%	0.008%
6	2.648	254	256	258	rVV	472	336	0.02%	0.003%
7	2.794	275	280	284	rVB5	1459	1989	0.15%	0.017%
8	2.947	297	305	316	rVB	39007	90991	6.75%	0.796%
9	3.099	323	330	338	rVB	8894	17127	1.27%	0.150%
10	3.294	360	362	366	rVB3	286	296	0.02%	0.003%
11	3.611	404	414	429	rVB	129781	304983	22.63%	2.667%
12	3.715	429	431	433	rBV2	354	316	0.02%	0.003%
13	3.837	450	451	454	rVB	423	241	0.02%	0.002%
14	3.861	454	455	458	rBV2	350	283	0.02%	0.002%
15	4.099	492	494	498	rVB2	255	303	0.02%	0.003%
16	4.166	503	505	507	rBV2	260	337	0.03%	0.003%
17	4.489	545	558	570	rBV2	254877	923349	68.52%	8.075%
18	4.849	615	617	622	rVB3	335	462	0.03%	0.004%
19	4.916	626	628	630	rVB	317	260	0.02%	0.002%
20	5.062	639	652	668	rBV	179114	549663	40.79%	4.807%
21	5.385	694	705	721	rVB2	46147	143283	10.63%	1.253%
22	5.495	721	723	727	rVB	402	472	0.04%	0.004%
23	5.538	727	730	731	rBV2	587	610	0.05%	0.005%
24	5.641	745	747	749	rBV2	310	291	0.02%	0.003%
25	5.818	773	776	780	rVB2	360	446	0.03%	0.004%
26	5.855	780	782	787	rBV2	330	556	0.04%	0.005%
27	5.970	787	801	816	rBV2	453587	1347512	100.00%	11.785%
28	6.300	852	855	856	rBV	286	240	0.02%	0.002%
29	6.361	864	865	869	rVB2	395	459	0.03%	0.004%
30	6.452	874	880	881	rBV2	265	450	0.03%	0.004%
31	6.513	888	890	893	rBV	378	519	0.04%	0.005%
32	6.763	921	931	944	rBV	337219	810961	60.18%	7.092%
33	6.976	964	966	968	rVB2	286	242	0.02%	0.002%
34	7.129	982	991	1003	rVV4	37701	90613	6.72%	0.792%
35	7.312	1012	1021	1036	rBV	276232	602498	44.71%	5.269%
36	7.470	1045	1047	1048	rBV	391	393	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029446.D
 Acq On : 14 Jun 2022 04:36
 Operator : JC/MD
 Sample : N3249-08DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYT2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.610	1066	1070	1072	rVB3	252	393	0.03%	0.003%
38	7.659	1076	1078	1082	rBV2	207	297	0.02%	0.003%
39	7.702	1083	1085	1086	rVV2	475	258	0.02%	0.002%
40	7.793	1098	1100	1103	rBV2	241	268	0.02%	0.002%
41	7.818	1103	1104	1108	rBV2	322	419	0.03%	0.004%
42	7.933	1118	1123	1128	rBV2	1206	2411	0.18%	0.021%
43	8.330	1181	1188	1198	rBV	162050	272867	20.25%	2.386%
44	8.482	1210	1213	1214	rBV3	800	712	0.05%	0.006%
45	8.580	1227	1229	1231	rVV2	812	597	0.04%	0.005%
46	8.653	1234	1241	1249	rBV	663856	1035331	76.83%	9.055%
47	8.720	1249	1252	1263	rVV	9487	15987	1.19%	0.140%
48	8.799	1263	1265	1267	rVB	385	266	0.02%	0.002%
49	8.830	1267	1270	1272	rBV4	363	523	0.04%	0.005%
50	8.903	1280	1282	1285	rBV2	378	340	0.03%	0.003%
51	8.952	1285	1290	1300	rBV	117180	173857	12.90%	1.521%
52	9.153	1321	1323	1327	rBV3	1162	1450	0.11%	0.013%
53	9.275	1336	1343	1350	rBV	14229	21087	1.56%	0.184%
54	9.384	1356	1361	1380	rBV	526951	790135	58.64%	6.910%
55	9.738	1416	1419	1420	rBV2	275	356	0.03%	0.003%
56	9.854	1436	1438	1439	rBV	337	270	0.02%	0.002%
57	9.945	1450	1453	1454	rBV	430	247	0.02%	0.002%
58	10.055	1465	1471	1489	rBV	692900	925768	68.70%	8.097%
59	10.195	1491	1494	1498	rVV4	631	1029	0.08%	0.009%
60	10.244	1501	1502	1504	rBV	411	272	0.02%	0.002%
61	10.305	1508	1512	1517	rBV2	1447	2142	0.16%	0.019%
62	10.378	1522	1524	1527	rBV2	344	311	0.02%	0.003%
63	10.506	1544	1545	1547	rBV	444	320	0.02%	0.003%
64	10.640	1565	1567	1570	rBV2	612	581	0.04%	0.005%
65	10.774	1587	1589	1592	rBV2	306	358	0.03%	0.003%
66	10.805	1592	1594	1596	rBV3	232	275	0.02%	0.002%
67	11.049	1630	1634	1635	rBV3	289	268	0.02%	0.002%
68	11.079	1637	1639	1642	rBV2	400	349	0.03%	0.003%
69	11.122	1642	1646	1650	rVB3	2062	2314	0.17%	0.020%
70	11.195	1652	1658	1667	rBV	561565	704032	52.25%	6.157%
71	11.384	1686	1689	1690	rBV2	284	396	0.03%	0.003%
72	11.433	1695	1697	1698	rBV	543	392	0.03%	0.003%
73	11.713	1741	1743	1745	rBV	540	546	0.04%	0.005%
74	11.750	1745	1749	1758	rVB3	2333	3331	0.25%	0.029%
75	11.841	1761	1764	1765	rBV2	408	436	0.03%	0.004%
76	11.933	1776	1779	1785	rBV3	1155	1482	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029446.D
 Acq On : 14 Jun 2022 04:36
 Operator : JC/MD
 Sample : N3249-08DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYT2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.975	1785	1786	1788	rVB	453	240	0.02%	0.002%
78	12.024	1788	1794	1804	rBV	730847	886173	65.76%	7.750%
79	12.323	1837	1843	1850	rBV	700975	893379	66.30%	7.813%
80	12.798	1919	1921	1923	rVB	384	294	0.02%	0.003%
81	12.829	1923	1926	1928	rVB	416	333	0.02%	0.003%
82	12.859	1928	1931	1933	rBV	405	470	0.03%	0.004%
83	12.969	1946	1949	1952	rVB3	375	540	0.04%	0.005%
84	13.000	1952	1954	1955	rBV	329	238	0.02%	0.002%
85	13.061	1961	1964	1968	rVB2	348	451	0.03%	0.004%
86	13.280	1998	2000	2002	rBV	373	379	0.03%	0.003%
87	13.426	2020	2024	2026	rBV2	278	319	0.02%	0.003%
88	13.524	2039	2040	2042	rBV	308	246	0.02%	0.002%
89	13.695	2067	2068	2069	rBV	474	244	0.02%	0.002%
90	13.731	2073	2074	2079	rBV2	400	442	0.03%	0.004%
91	13.780	2079	2082	2085	rBV3	513	810	0.06%	0.007%
92	13.963	2111	2112	2115	rBV2	250	271	0.02%	0.002%
93	14.432	2187	2189	2192	rVB2	362	329	0.02%	0.003%
94	14.548	2206	2208	2210	rBV	360	314	0.02%	0.003%
95	14.664	2224	2227	2228	rBV2	403	265	0.02%	0.002%
96	14.743	2238	2240	2244	rBV2	508	544	0.04%	0.005%
97	15.615	2381	2383	2385	rBV2	520	421	0.03%	0.004%
98	16.097	2460	2462	2463	rBV	770	396	0.03%	0.003%
99	16.597	2543	2544	2547	rBV3	572	421	0.03%	0.004%
100	16.712	2560	2563	2564	rBV3	549	616	0.05%	0.005%


Sum of corrected areas: 11434173

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029446.D
Acq On : 14 Jun 2022 04:36
Operator : JC/MD
Sample : N3249-08DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYT2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

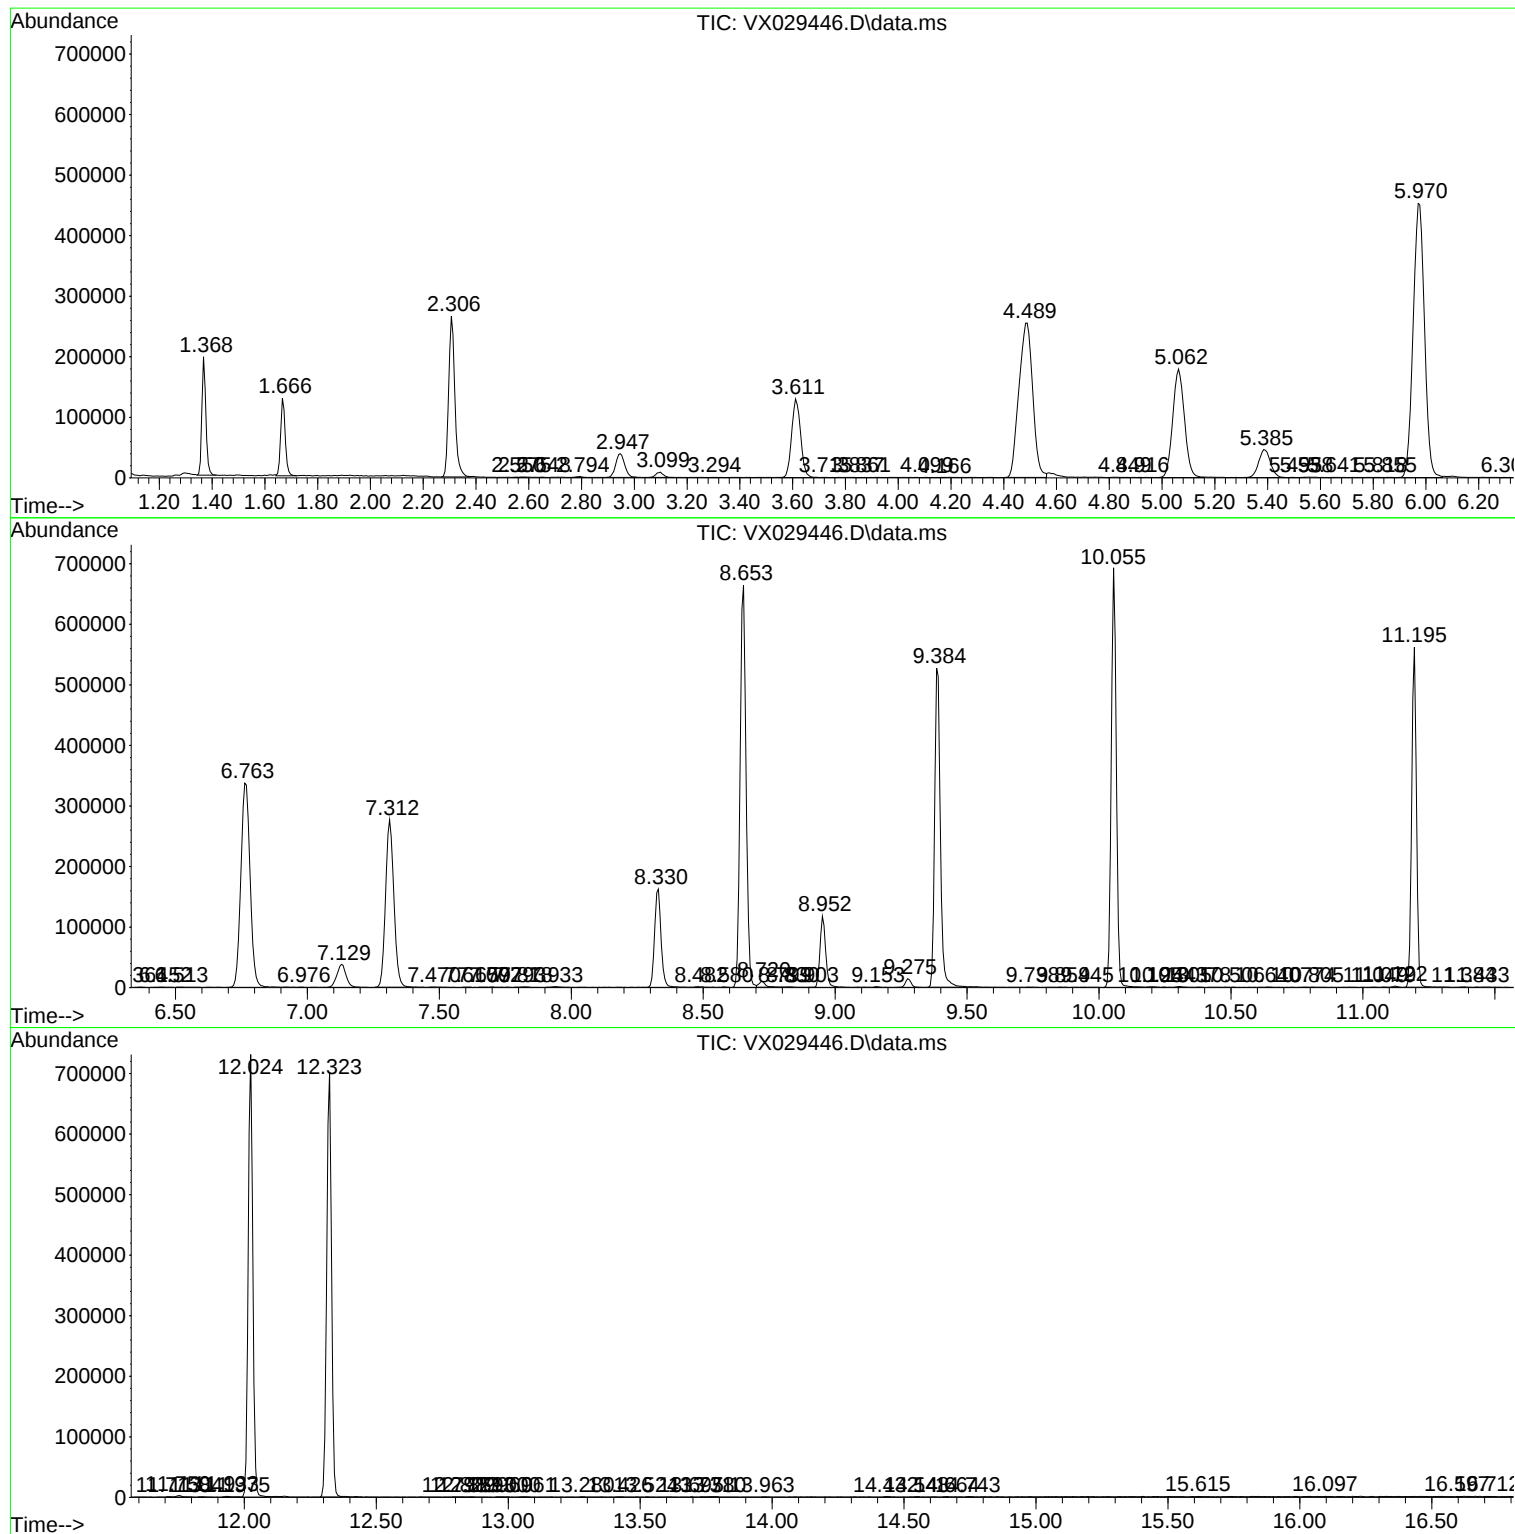

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029446.D
Acq On : 14 Jun 2022 04:36
Operator : JC/MD
Sample : N3249-08DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYT2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029446.D
Acq On : 14 Jun 2022 04:36
Operator : JC/MD
Sample : N3249-08DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYT2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------