

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029448.D
 Acq On : 14 Jun 2022 05:23
 Operator : JC/MD
 Sample : N3249-17DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYX5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	26	28	30	rBV2	2374	2575	0.20%	0.023%
2	1.368	42	46	54	rVB2	195130	209456	15.90%	1.906%
3	1.666	91	95	106	rVB	128637	153167	11.62%	1.394%
4	2.306	194	200	213	rBV	257145	416746	31.63%	3.793%
5	2.502	231	232	234	rBV2	360	317	0.02%	0.003%
6	2.703	263	265	267	rBV2	379	325	0.02%	0.003%
7	2.788	275	279	286	rVB3	1742	3318	0.25%	0.030%
8	2.886	292	295	297	rVB2	363	343	0.03%	0.003%
9	2.947	297	305	318	rBV	43682	102217	7.76%	0.930%
10	3.099	323	330	337	rBV4	4465	9606	0.73%	0.087%
11	3.611	404	414	428	rVV	94285	221065	16.78%	2.012%
12	3.709	428	430	434	rVV3	411	516	0.04%	0.005%
13	3.800	443	445	450	rVB2	389	427	0.03%	0.004%
14	4.245	516	518	521	rBV3	253	304	0.02%	0.003%
15	4.483	545	557	569	rBV2	220271	825400	62.64%	7.512%
16	4.885	621	623	626	rBV2	417	458	0.03%	0.004%
17	5.062	640	652	666	rVV2	174560	532108	40.38%	4.843%
18	5.312	691	693	695	rBV2	311	290	0.02%	0.003%
19	5.397	695	707	715	rVB4	3984	12421	0.94%	0.113%
20	5.550	728	732	735	rBV4	855	1386	0.11%	0.013%
21	5.708	754	758	760	rBV	395	413	0.03%	0.004%
22	5.745	762	764	765	rVB2	490	296	0.02%	0.003%
23	5.842	778	780	783	rBV	230	305	0.02%	0.003%
24	5.897	786	789	790	rBV	333	318	0.02%	0.003%
25	5.970	790	801	817	rBV3	446202	1317687	100.00%	11.993%
26	6.178	832	835	837	rBV4	262	323	0.02%	0.003%
27	6.294	853	854	857	rVV2	312	315	0.02%	0.003%
28	6.361	860	865	867	rBV3	333	514	0.04%	0.005%
29	6.464	878	882	884	rBV2	281	494	0.04%	0.004%
30	6.763	921	931	946	rBV	328575	786856	59.71%	7.162%
31	7.129	982	991	1004	rVB3	31926	77883	5.91%	0.709%
32	7.312	1011	1021	1032	rBV	275778	590113	44.78%	5.371%
33	7.482	1045	1049	1053	rBV4	683	1241	0.09%	0.011%
34	7.635	1073	1074	1078	rVB2	358	350	0.03%	0.003%
35	7.818	1100	1104	1108	rVB3	825	1003	0.08%	0.009%
36	7.940	1121	1124	1133	rBV4	1067	2098	0.16%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029448.D
 Acq On : 14 Jun 2022 05:23
 Operator : JC/MD
 Sample : N3249-17DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYX5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	8.141	1154	1157	1160	rBV	267	387	0.03%	0.004%
38	8.208	1166	1168	1170	rBV2	332	316	0.02%	0.003%
39	8.269	1176	1178	1180	rBV2	319	326	0.02%	0.003%
40	8.330	1181	1188	1201	rVV	158117	266542	20.23%	2.426%
41	8.494	1211	1215	1217	rBV2	705	1090	0.08%	0.010%
42	8.574	1224	1228	1233	rVB4	1054	1646	0.12%	0.015%
43	8.653	1233	1241	1248	rBV	640319	1010856	76.71%	9.200%
44	8.720	1248	1252	1259	rVB	10575	18212	1.38%	0.166%
45	8.897	1276	1281	1282	rBV2	304	410	0.03%	0.004%
46	8.952	1284	1290	1299	rBV	115174	166404	12.63%	1.515%
47	9.159	1321	1324	1327	rVB4	847	1091	0.08%	0.010%
48	9.275	1339	1343	1348	rVB4	2654	3664	0.28%	0.033%
49	9.384	1356	1361	1381	rBV	533971	777683	59.02%	7.078%
50	9.695	1408	1412	1414	rBV4	424	572	0.04%	0.005%
51	9.878	1440	1442	1445	rBV2	250	347	0.03%	0.003%
52	10.012	1462	1464	1465	rBV	318	328	0.02%	0.003%
53	10.055	1465	1471	1480	rVV	671863	894644	67.90%	8.143%
54	10.195	1491	1494	1500	rVB	3944	5227	0.40%	0.048%
55	10.244	1500	1502	1505	rVB2	375	388	0.03%	0.004%
56	10.305	1507	1512	1520	rVV	7120	10367	0.79%	0.094%
57	10.390	1524	1526	1528	rBV2	349	302	0.02%	0.003%
58	10.646	1564	1568	1574	rVB2	10668	15549	1.18%	0.142%
59	10.695	1574	1576	1579	rBV	292	286	0.02%	0.003%
60	10.744	1583	1584	1587	rBV	326	362	0.03%	0.003%
61	10.799	1592	1593	1596	rVV2	364	342	0.03%	0.003%
62	10.866	1600	1604	1605	rBV2	306	336	0.03%	0.003%
63	10.915	1610	1612	1615	rVB2	294	347	0.03%	0.003%
64	10.970	1618	1621	1626	rBV5	1694	2474	0.19%	0.023%
65	11.055	1633	1635	1638	rVB2	452	462	0.04%	0.004%
66	11.085	1638	1640	1642	rBV3	547	595	0.05%	0.005%
67	11.122	1642	1646	1650	rVB3	1666	2149	0.16%	0.020%
68	11.195	1652	1658	1666	rBV	552376	693493	52.63%	6.312%
69	11.305	1672	1676	1684	rVB4	2338	3892	0.30%	0.035%
70	11.384	1684	1689	1697	rBV	10226	15503	1.18%	0.141%
71	11.451	1697	1700	1711	rVV3	5775	8483	0.64%	0.077%
72	11.616	1722	1727	1731	rBV	7953	9760	0.74%	0.089%
73	11.719	1739	1744	1745	rBV4	455	492	0.04%	0.004%
74	11.756	1745	1750	1757	rVB	28417	34774	2.64%	0.316%
75	11.835	1761	1763	1767	rBV2	308	313	0.02%	0.003%
76	11.890	1770	1772	1775	rBV2	274	333	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029448.D
 Acq On : 14 Jun 2022 05:23
 Operator : JC/MD
 Sample : N3249-17DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYX5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.933	1777	1779	1783	rVB3	1088	1130	0.09%	0.010%
78	11.975	1783	1786	1788	rBV4	607	625	0.05%	0.006%
79	12.024	1788	1794	1801	rBV	693265	857463	65.07%	7.804%
80	12.091	1801	1805	1809	rVB	13701	16491	1.25%	0.150%
81	12.244	1826	1830	1833	rBV4	3871	5234	0.40%	0.048%
82	12.323	1837	1843	1852	rVV	672330	868506	65.91%	7.905%
83	12.469	1866	1867	1873	rVB2	639	833	0.06%	0.008%
84	12.542	1875	1879	1885	rVV3	2919	4551	0.35%	0.041%
85	12.616	1889	1891	1895	rBV	816	832	0.06%	0.008%
86	12.756	1912	1914	1915	rBV2	539	403	0.03%	0.004%
87	13.103	1968	1971	1976	rVB2	315	426	0.03%	0.004%
88	13.390	2016	2018	2021	rVV2	335	352	0.03%	0.003%
89	13.439	2024	2026	2028	rVV	391	366	0.03%	0.003%
90	13.591	2049	2051	2054	rBV3	427	414	0.03%	0.004%
91	13.634	2055	2058	2060	rBV	368	371	0.03%	0.003%
92	13.780	2078	2082	2086	rVV2	1302	1964	0.15%	0.018%
93	13.853	2091	2094	2095	rBV2	247	300	0.02%	0.003%
94	14.134	2138	2140	2143	rVB2	1098	979	0.07%	0.009%
95	14.188	2146	2149	2153	rBV2	446	577	0.04%	0.005%
96	14.231	2155	2156	2159	rBV2	398	394	0.03%	0.004%
97	14.262	2159	2161	2164	rBV2	269	309	0.02%	0.003%
98	14.597	2214	2216	2219	rBV3	389	550	0.04%	0.005%
99	14.816	2250	2252	2254	rVB2	570	388	0.03%	0.004%
100	15.457	2355	2357	2358	rBV	470	354	0.03%	0.003%


Sum of corrected areas: 10987213

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029448.D
Acq On : 14 Jun 2022 05:23
Operator : JC/MD
Sample : N3249-17DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYX5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

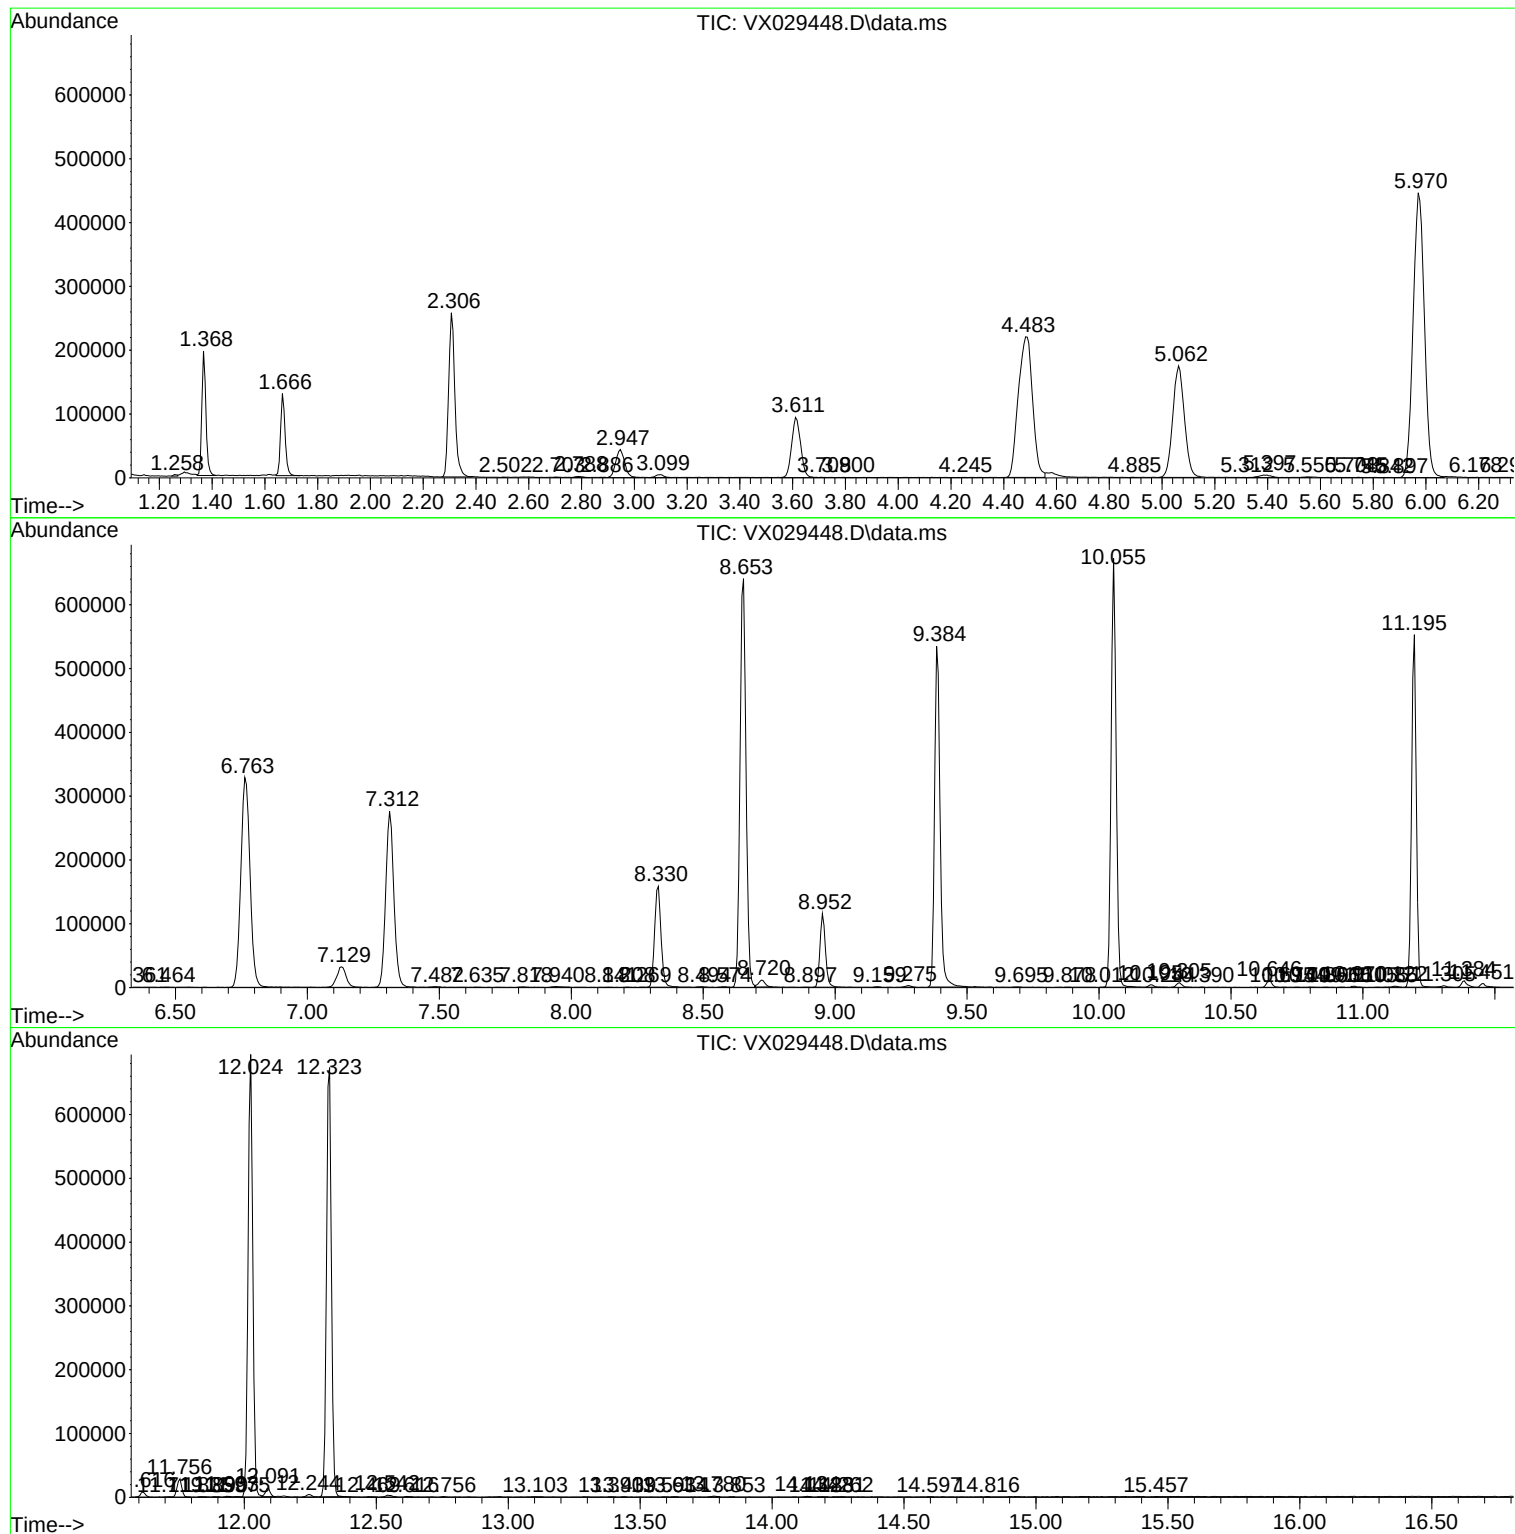

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029448.D
Acq On : 14 Jun 2022 05:23
Operator : JC/MD
Sample : N3249-17DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYX5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029448.D
Acq On : 14 Jun 2022 05:23
Operator : JC/MD
Sample : N3249-17DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYX5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc