

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029449.D
 Acq On : 14 Jun 2022 05:46
 Operator : JC/MD
 Sample : N3311-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DZ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	171883	173307	12.76%	1.647%
2	1.666	91	95	104	rVB	120069	145228	10.69%	1.380%
3	2.307	194	200	211	rBV	282059	447852	32.97%	4.257%
4	2.788	275	279	284	rVB3	671	1393	0.10%	0.013%
5	2.953	299	306	311	rBV5	770	2073	0.15%	0.020%
6	3.081	326	327	329	rBV2	320	246	0.02%	0.002%
7	3.178	342	343	347	rBV3	419	529	0.04%	0.005%
8	3.526	398	400	402	rVB2	382	270	0.02%	0.003%
9	3.599	408	412	413	rVB3	329	372	0.03%	0.004%
10	3.739	432	435	437	rBV2	365	457	0.03%	0.004%
11	3.904	461	462	465	rVB2	325	252	0.02%	0.002%
12	3.946	465	469	471	rBV2	244	309	0.02%	0.003%
13	4.038	482	484	485	rBV	359	350	0.03%	0.003%
14	4.361	535	537	539	rVB2	408	251	0.02%	0.002%
15	4.465	545	554	571	rBV	120742	351026	25.85%	3.336%
16	4.776	604	605	608	rBV3	368	279	0.02%	0.003%
17	4.879	621	622	625	rVB2	611	422	0.03%	0.004%
18	4.940	631	632	636	rBV2	239	279	0.02%	0.003%
19	5.062	639	652	670	rBV2	179410	551188	40.58%	5.239%
20	5.300	688	691	692	rBV	265	237	0.02%	0.002%
21	5.367	700	702	703	rBV2	401	271	0.02%	0.003%
22	5.391	703	706	709	rVV4	710	943	0.07%	0.009%
23	5.416	709	710	714	rVB2	744	535	0.04%	0.005%
24	5.562	727	734	743	rVB3	1255	2920	0.21%	0.028%
25	5.696	753	756	758	rBV2	260	275	0.02%	0.003%
26	5.769	766	768	771	rBV2	347	419	0.03%	0.004%
27	5.971	786	801	818	rVV2	455352	1358176	100.00%	12.909%
28	6.214	839	841	844	rVB2	337	262	0.02%	0.002%
29	6.556	895	897	902	rVB3	558	597	0.04%	0.006%
30	6.598	902	904	907	rVB	372	255	0.02%	0.002%
31	6.641	907	911	912	rBV2	363	368	0.03%	0.003%
32	6.678	916	917	921	rVB	360	324	0.02%	0.003%
33	6.763	921	931	951	rBV	351766	842759	62.05%	8.010%
34	7.001	969	970	971	rBV	404	234	0.02%	0.002%
35	7.129	982	991	1004	rVB3	20973	55217	4.07%	0.525%
36	7.312	1012	1021	1033	rBV	280940	602480	44.36%	5.726%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029449.D
 Acq On : 14 Jun 2022 05:46
 Operator : JC/MD
 Sample : N3311-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DZ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.482	1044	1049	1050	rBV3	902	1126	0.08%	0.011%
38	7.586	1060	1066	1075	rBV3	8164	18220	1.34%	0.173%
39	7.726	1087	1089	1091	rVB2	345	242	0.02%	0.002%
40	7.940	1120	1124	1125	rBV2	1158	1213	0.09%	0.012%
41	8.092	1147	1149	1152	rVB2	338	270	0.02%	0.003%
42	8.123	1152	1154	1155	rBV	564	375	0.03%	0.004%
43	8.330	1181	1188	1200	rVV	162003	272568	20.07%	2.591%
44	8.452	1204	1208	1210	rVV3	390	451	0.03%	0.004%
45	8.482	1210	1213	1219	rVV5	667	1258	0.09%	0.012%
46	8.598	1231	1232	1234	rVV2	340	275	0.02%	0.003%
47	8.653	1234	1241	1248	rVV	701958	1090321	80.28%	10.363%
48	8.720	1248	1252	1266	rVB	15631	28515	2.10%	0.271%
49	8.952	1285	1290	1300	rBV	117528	170513	12.55%	1.621%
50	9.226	1333	1335	1340	rVV2	273	394	0.03%	0.004%
51	9.275	1340	1343	1348	rVV5	2031	2813	0.21%	0.027%
52	9.317	1348	1350	1351	rVB	477	294	0.02%	0.003%
53	9.385	1356	1361	1379	rBV	529956	776084	57.14%	7.376%
54	9.525	1380	1384	1390	rVB4	6350	10235	0.75%	0.097%
55	9.695	1410	1412	1415	rBV2	357	321	0.02%	0.003%
56	9.982	1455	1459	1460	rBV2	328	334	0.02%	0.003%
57	10.055	1465	1471	1485	rBV	727661	972479	71.60%	9.243%
58	10.189	1492	1493	1497	rVB4	632	821	0.06%	0.008%
59	10.275	1505	1507	1508	rBV2	261	228	0.02%	0.002%
60	10.305	1508	1512	1515	rVV2	2681	3691	0.27%	0.035%
61	10.360	1519	1521	1524	rVB3	219	250	0.02%	0.002%
62	10.665	1565	1571	1577	rVB6	5188	8456	0.62%	0.080%
63	10.866	1599	1604	1607	rVB3	1987	2521	0.19%	0.024%
64	10.921	1611	1613	1614	rBV	262	236	0.02%	0.002%
65	10.957	1618	1619	1622	rBV3	317	308	0.02%	0.003%
66	11.092	1637	1641	1642	rVB2	627	593	0.04%	0.006%
67	11.122	1642	1646	1649	rVB3	1716	2302	0.17%	0.022%
68	11.153	1649	1651	1652	rBV	282	232	0.02%	0.002%
69	11.195	1652	1658	1668	rBV	557379	695454	51.20%	6.610%
70	11.390	1683	1690	1695	rVB3	528	1142	0.08%	0.011%
71	11.451	1698	1700	1703	rBV3	591	901	0.07%	0.009%
72	11.616	1724	1727	1729	rBV	499	636	0.05%	0.006%
73	11.713	1740	1743	1745	rVB2	553	554	0.04%	0.005%
74	11.756	1745	1750	1756	rVB5	3149	4719	0.35%	0.045%
75	11.805	1756	1758	1760	rBV2	326	393	0.03%	0.004%
76	11.841	1762	1764	1767	rBV3	575	611	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029449.D
 Acq On : 14 Jun 2022 05:46
 Operator : JC/MD
 Sample : N3311-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DZ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.872	1767	1769	1770	rBV	407	249	0.02%	0.002%
78	11.933	1776	1779	1782	rVB2	1627	1784	0.13%	0.017%
79	12.024	1788	1794	1806	rBV	791890	956686	70.44%	9.093%
80	12.116	1808	1809	1810	rBV	723	393	0.03%	0.004%
81	12.323	1837	1843	1851	rBV	737926	937124	69.00%	8.907%
82	12.421	1857	1859	1861	rVB	505	358	0.03%	0.003%
83	12.543	1877	1879	1882	rBV2	382	452	0.03%	0.004%
84	12.573	1882	1884	1887	rVB2	329	259	0.02%	0.002%
85	12.634	1892	1894	1895	rBV	410	298	0.02%	0.003%
86	12.853	1928	1930	1936	rBV3	1009	1628	0.12%	0.015%
87	12.969	1947	1949	1952	rBV2	264	233	0.02%	0.002%
88	13.055	1960	1963	1965	rVB2	374	409	0.03%	0.004%
89	13.451	2026	2028	2029	rBV2	305	257	0.02%	0.002%
90	13.981	2113	2115	2118	rBV3	313	385	0.03%	0.004%
91	14.024	2120	2122	2125	rVV3	360	308	0.02%	0.003%
92	14.109	2133	2136	2140	rBV2	352	427	0.03%	0.004%
93	14.359	2176	2177	2179	rBV2	377	235	0.02%	0.002%
94	14.439	2188	2190	2192	rBV2	393	344	0.03%	0.003%
95	14.603	2212	2217	2219	rBV3	713	1112	0.08%	0.011%
96	15.103	2297	2299	2301	rBV2	488	500	0.04%	0.005%
97	15.152	2305	2307	2309	rVV	505	292	0.02%	0.003%
98	15.743	2402	2404	2408	rBV3	606	623	0.05%	0.006%
99	16.213	2479	2481	2485	rBV3	669	1120	0.08%	0.011%
100	16.505	2527	2529	2532	rBV2	712	876	0.06%	0.008%

Sum of corrected areas: 10521056




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029449.D
Acq On : 14 Jun 2022 05:46
Operator : JC/MD
Sample : N3311-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

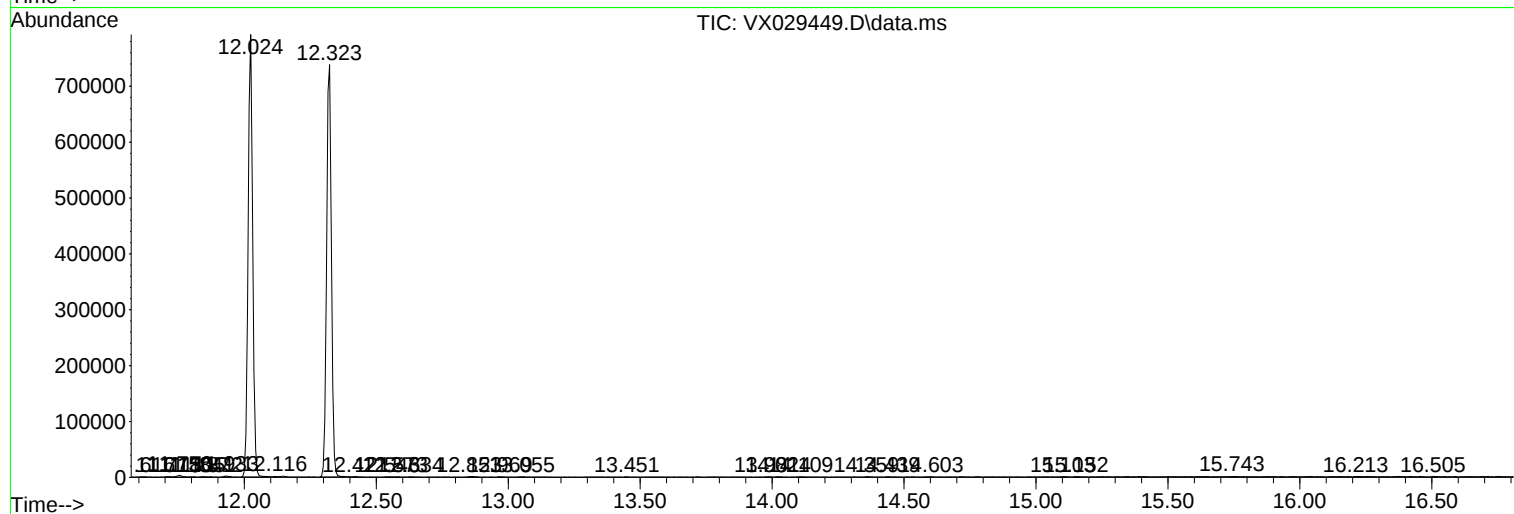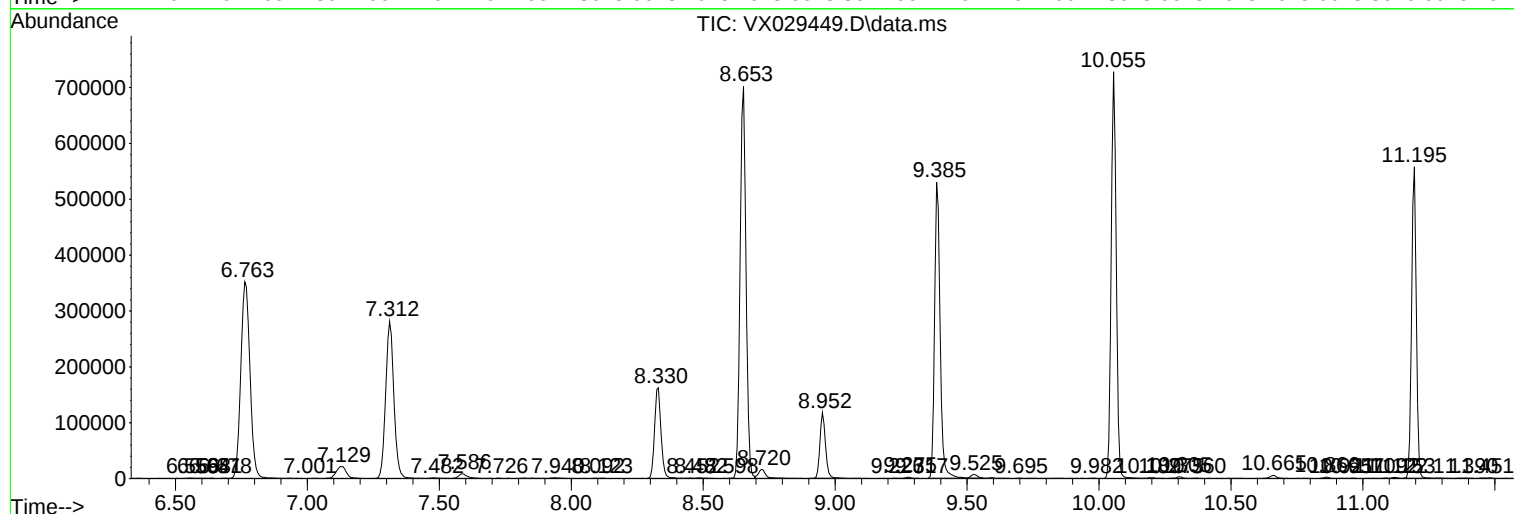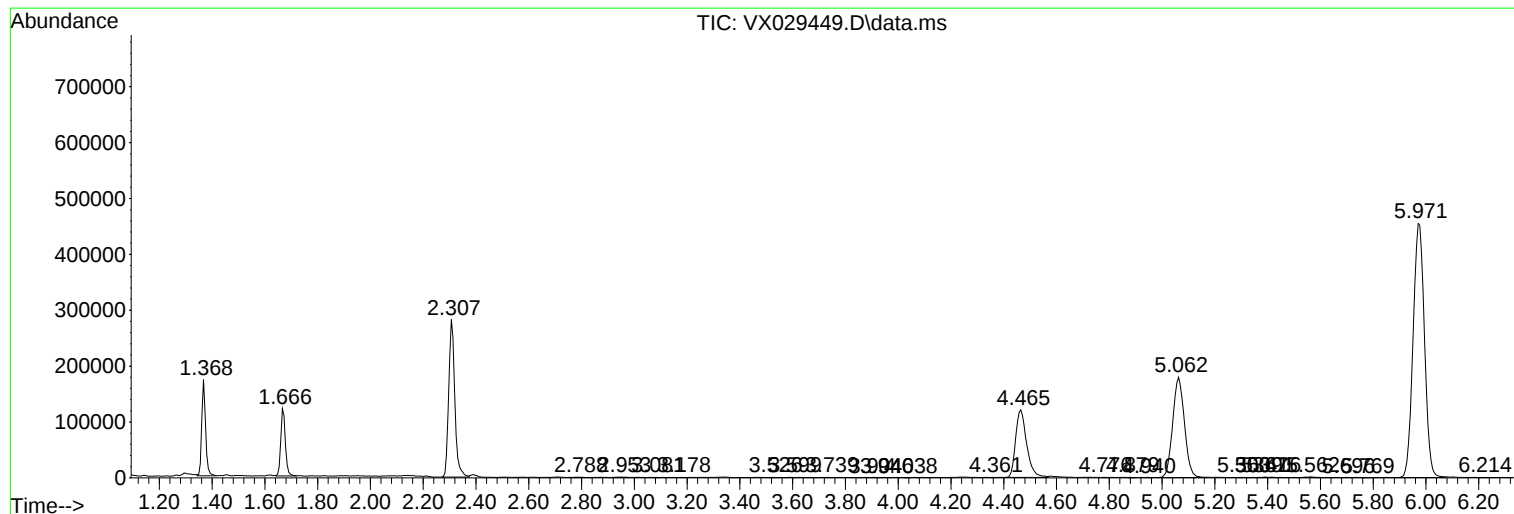

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029449.D
Acq On : 14 Jun 2022 05:46
Operator : JC/MD
Sample : N3311-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029449.D
Acq On : 14 Jun 2022 05:46
Operator : JC/MD
Sample : N3311-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
