

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029450.D
 Acq On : 14 Jun 2022 06:09
 Operator : JC/MD
 Sample : N3311-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	172569	173148	12.77%	1.497%
2	1.666	91	95	104	rVB	125699	152209	11.22%	1.316%
3	2.306	194	200	212	rBV2	287307	498255	36.74%	4.307%
4	2.514	233	234	237	rVB	544	305	0.02%	0.003%
5	2.709	263	266	271	rVB4	645	1163	0.09%	0.010%
6	2.794	275	280	284	rVB5	648	1318	0.10%	0.011%
7	3.136	332	336	338	rBV2	216	271	0.02%	0.002%
8	3.282	359	360	364	rBV2	405	450	0.03%	0.004%
9	3.459	387	389	391	rBV2	349	332	0.02%	0.003%
10	3.532	399	401	403	rBV	410	311	0.02%	0.003%
11	3.568	405	407	409	rBV2	393	350	0.03%	0.003%
12	3.593	409	411	412	rVV	420	353	0.03%	0.003%
13	3.605	412	413	420	rVB4	819	1325	0.10%	0.011%
14	4.294	524	526	531	rVB3	232	356	0.03%	0.003%
15	4.337	531	533	536	rBV	341	334	0.02%	0.003%
16	4.465	545	554	570	rBV	124214	397648	29.32%	3.437%
17	5.062	638	652	669	rBV	179056	550024	40.56%	4.754%
18	5.385	697	705	711	rBV5	5800	15885	1.17%	0.137%
19	5.544	727	731	732	rBV2	806	1062	0.08%	0.009%
20	5.629	744	745	747	rVB2	353	238	0.02%	0.002%
21	5.842	777	780	781	rBV	258	243	0.02%	0.002%
22	5.976	789	802	817	rBV2	457962	1356220	100.00%	11.722%
23	6.147	828	830	833	rVB2	419	324	0.02%	0.003%
24	6.300	850	855	856	rBV3	277	353	0.03%	0.003%
25	6.336	859	861	862	rBV2	344	266	0.02%	0.002%
26	6.543	894	895	898	rBV2	409	392	0.03%	0.003%
27	6.647	909	912	914	rBV2	528	549	0.04%	0.005%
28	6.763	920	931	952	rBV	352159	840170	61.95%	7.262%
29	6.958	959	963	965	rVB3	439	523	0.04%	0.005%
30	7.043	976	977	981	rVB2	290	236	0.02%	0.002%
31	7.129	981	991	1006	rBV	475227	1021546	75.32%	8.830%
32	7.312	1012	1021	1036	rVB	281772	604181	44.55%	5.222%
33	7.476	1045	1048	1049	rBV2	702	708	0.05%	0.006%
34	7.598	1065	1068	1069	rBV2	310	274	0.02%	0.002%
35	7.696	1082	1084	1086	rBV2	294	283	0.02%	0.002%
36	7.738	1089	1091	1094	rVB3	244	277	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029450.D
 Acq On : 14 Jun 2022 06:09
 Operator : JC/MD
 Sample : N3311-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.811	1100	1103	1104	rBV	537	431	0.03%	0.004%
38	7.940	1119	1124	1128	rBV3	1012	1934	0.14%	0.017%
39	8.086	1144	1148	1150	rBV2	209	359	0.03%	0.003%
40	8.171	1159	1162	1163	rBV2	334	359	0.03%	0.003%
41	8.232	1170	1172	1175	rVB	302	272	0.02%	0.002%
42	8.330	1181	1188	1198	rBV	162962	272723	20.11%	2.357%
43	8.482	1209	1213	1215	rBV3	820	1121	0.08%	0.010%
44	8.653	1234	1241	1249	rBV	698371	1096090	80.82%	9.474%
45	8.720	1249	1252	1258	rVB	9846	16241	1.20%	0.140%
46	8.952	1284	1290	1301	rBV	117865	170879	12.60%	1.477%
47	9.165	1321	1325	1328	rVB2	630	789	0.06%	0.007%
48	9.275	1339	1343	1350	rVB3	1958	3351	0.25%	0.029%
49	9.384	1355	1361	1378	rBV	533821	774929	57.14%	6.698%
50	9.665	1404	1407	1410	rBV4	406	387	0.03%	0.003%
51	9.823	1430	1433	1435	rBV3	377	463	0.03%	0.004%
52	10.055	1465	1471	1483	rBV	759016	979049	72.19%	8.462%
53	10.201	1493	1495	1499	rVB2	883	920	0.07%	0.008%
54	10.250	1501	1503	1505	rBV	376	301	0.02%	0.003%
55	10.299	1509	1511	1519	rBV3	1303	2515	0.19%	0.022%
56	10.585	1556	1558	1560	rVB	397	297	0.02%	0.003%
57	10.646	1564	1568	1570	rBV3	638	744	0.05%	0.006%
58	10.707	1577	1578	1581	rBV	332	341	0.03%	0.003%
59	11.012	1625	1628	1629	rVB2	383	261	0.02%	0.002%
60	11.030	1629	1631	1633	rBV2	284	341	0.03%	0.003%
61	11.122	1642	1646	1650	rVB3	1586	2244	0.17%	0.019%
62	11.195	1652	1658	1666	rBV	562570	699037	51.54%	6.042%
63	11.305	1673	1676	1683	rVB3	912	1619	0.12%	0.014%
64	11.457	1698	1701	1702	rBV3	451	477	0.04%	0.004%
65	11.652	1729	1733	1738	rBV2	366	610	0.04%	0.005%
66	11.707	1740	1742	1746	rVV2	407	566	0.04%	0.005%
67	11.756	1746	1750	1755	rVB3	2864	3369	0.25%	0.029%
68	11.841	1762	1764	1767	rVB2	603	493	0.04%	0.004%
69	11.872	1767	1769	1772	rBV2	272	386	0.03%	0.003%
70	11.933	1776	1779	1783	rVB3	1063	1209	0.09%	0.010%
71	11.963	1783	1784	1785	rBV	418	264	0.02%	0.002%
72	12.024	1788	1794	1803	rBV	790691	956170	70.50%	8.265%
73	12.323	1836	1843	1854	rVV	753523	946244	69.77%	8.179%
74	12.427	1858	1860	1864	rVV3	922	1007	0.07%	0.009%
75	12.475	1866	1868	1871	rVB2	640	587	0.04%	0.005%
76	12.524	1875	1876	1880	rVB3	342	277	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029450.D
 Acq On : 14 Jun 2022 06:09
 Operator : JC/MD
 Sample : N3311-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.616	1889	1891	1893	rVB	525	282	0.02%	0.002%
78	12.725	1907	1909	1910	rVB	393	237	0.02%	0.002%
79	12.780	1914	1918	1920	rBV3	239	313	0.02%	0.003%
80	12.926	1940	1942	1945	rVB2	314	244	0.02%	0.002%
81	13.109	1970	1972	1975	rVB	399	351	0.03%	0.003%
82	13.134	1975	1976	1978	rBV	475	353	0.03%	0.003%
83	13.304	2002	2004	2006	rVB2	272	255	0.02%	0.002%
84	13.329	2006	2008	2010	rBV2	246	288	0.02%	0.002%
85	13.579	2048	2049	2051	rBV2	361	275	0.02%	0.002%
86	13.603	2051	2053	2054	rVV	509	278	0.02%	0.002%
87	13.756	2076	2078	2080	rBV	374	372	0.03%	0.003%
88	13.920	2103	2105	2106	rBV	606	318	0.02%	0.003%
89	13.999	2116	2118	2120	rBV3	302	246	0.02%	0.002%
90	14.219	2151	2154	2158	rBV3	390	569	0.04%	0.005%
91	14.329	2169	2172	2173	rBV2	337	313	0.02%	0.003%
92	14.566	2209	2211	2213	rBV2	366	266	0.02%	0.002%
93	14.615	2217	2219	2220	rBV	362	277	0.02%	0.002%
94	14.829	2253	2254	2257	rBV2	449	423	0.03%	0.004%
95	15.085	2293	2296	2298	rBV2	445	473	0.03%	0.004%
96	15.213	2315	2317	2318	rBV2	482	302	0.02%	0.003%
97	15.335	2335	2337	2338	rBV	604	376	0.03%	0.003%
98	15.706	2397	2398	2399	rBV	514	317	0.02%	0.003%
99	16.158	2470	2472	2474	rBV	707	314	0.02%	0.003%
100	16.267	2488	2490	2492	rBV	582	500	0.04%	0.004%




Sum of corrected areas: 11569480

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029450.D
Acq On : 14 Jun 2022 06:09
Operator : JC/MD
Sample : N3311-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

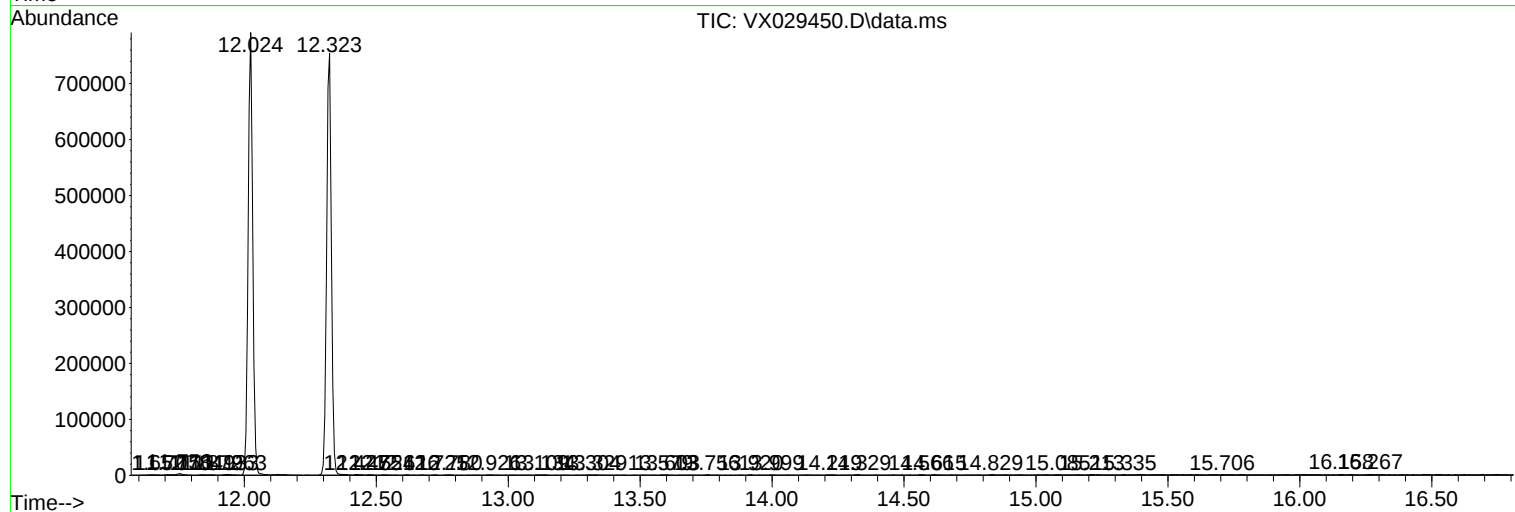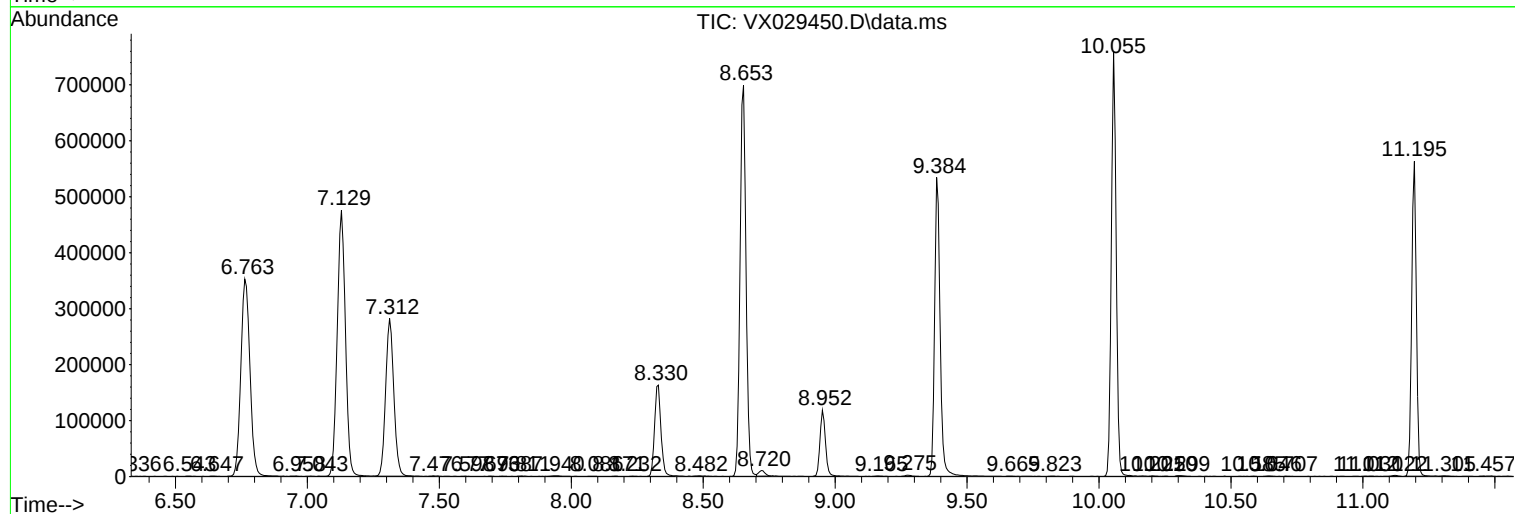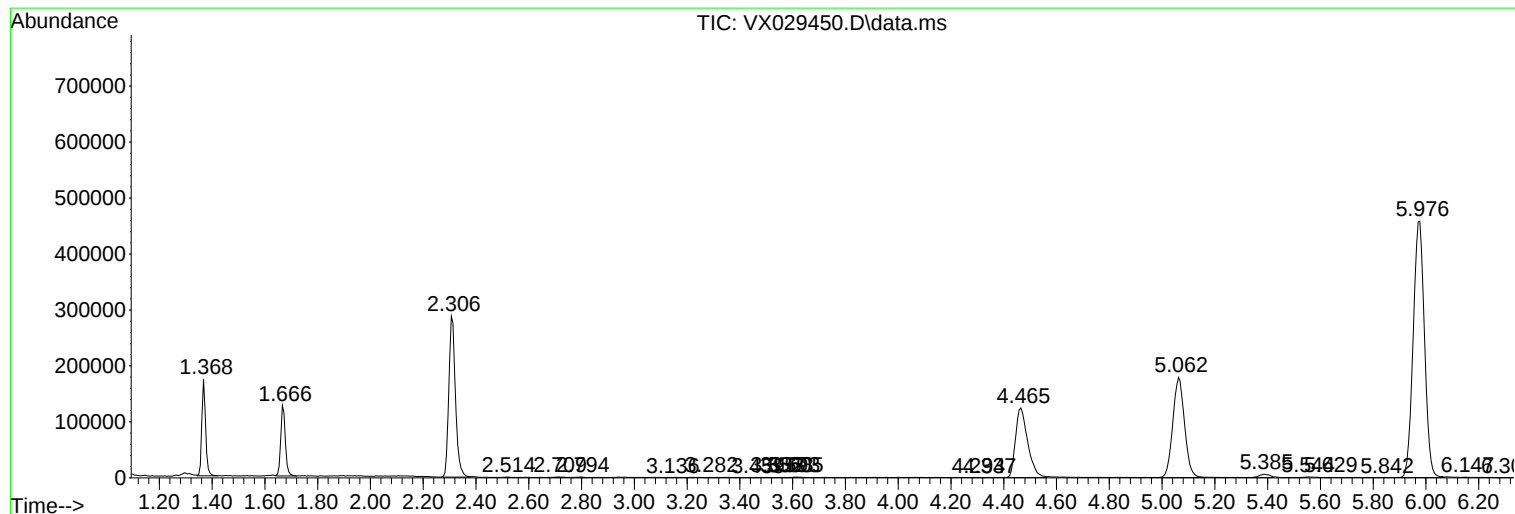

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029450.D
Acq On : 14 Jun 2022 06:09
Operator : JC/MD
Sample : N3311-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029450.D
Acq On : 14 Jun 2022 06:09
Operator : JC/MD
Sample : N3311-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------