

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029451.D
 Acq On : 14 Jun 2022 06:32
 Operator : JC/MD
 Sample : N3311-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0E00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	173940	171310	12.51%	1.624%
2	1.666	91	95	103	rVB	130872	156135	11.40%	1.480%
3	2.306	194	200	210	rBV	277630	445986	32.57%	4.228%
4	2.556	239	241	243	rBV2	374	367	0.03%	0.003%
5	2.660	257	258	260	rBV2	262	227	0.02%	0.002%
6	2.782	276	278	279	rBV2	710	495	0.04%	0.005%
7	2.843	286	288	290	rVB	408	283	0.02%	0.003%
8	2.892	292	296	298	rBV2	305	479	0.03%	0.005%
9	3.075	323	326	327	rBV2	187	218	0.02%	0.002%
10	3.172	341	342	345	rBV3	471	475	0.03%	0.005%
11	3.331	366	368	370	rBV2	355	224	0.02%	0.002%
12	3.428	381	384	386	rBV3	300	355	0.03%	0.003%
13	3.532	400	401	404	rVB2	331	236	0.02%	0.002%
14	3.581	406	409	410	rBV2	316	234	0.02%	0.002%
15	3.599	410	412	414	rBV2	405	342	0.02%	0.003%
16	3.666	422	423	426	rVB2	525	333	0.02%	0.003%
17	3.690	426	427	430	rBV	267	234	0.02%	0.002%
18	4.050	483	486	488	rVB3	244	247	0.02%	0.002%
19	4.154	502	503	507	rBV2	233	258	0.02%	0.002%
20	4.465	545	554	571	rBV	119550	350953	25.63%	3.327%
21	4.806	608	610	611	rVB2	365	262	0.02%	0.002%
22	4.824	611	613	620	rBV3	491	930	0.07%	0.009%
23	5.062	639	652	670	rBV	180830	559290	40.84%	5.302%
24	5.251	681	683	685	rBV2	359	386	0.03%	0.004%
25	5.336	693	697	698	rVB2	292	308	0.02%	0.003%
26	5.525	725	728	729	rVV2	309	287	0.02%	0.003%
27	5.550	729	732	736	rVV3	895	1250	0.09%	0.012%
28	5.720	757	760	764	rBV3	397	554	0.04%	0.005%
29	5.970	789	801	821	rVV2	456373	1369373	100.00%	12.981%
30	6.153	829	831	839	rVB4	507	864	0.06%	0.008%
31	6.354	863	864	866	rVB	579	275	0.02%	0.003%
32	6.409	872	873	876	rVB	449	221	0.02%	0.002%
33	6.446	876	879	880	rBV2	224	299	0.02%	0.003%
34	6.507	887	889	891	rVB	244	214	0.02%	0.002%
35	6.550	891	896	897	rBV3	384	553	0.04%	0.005%
36	6.763	922	931	943	rBV	355175	852168	62.23%	8.078%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029451.D
 Acq On : 14 Jun 2022 06:32
 Operator : JC/MD
 Sample : N3311-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0E00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.019	972	973	976	rVB2	351	219	0.02%	0.002%
38	7.129	982	991	1002	rBV4	22049	54195	3.96%	0.514%
39	7.312	1012	1021	1036	rBV	274378	605780	44.24%	5.743%
40	7.488	1047	1050	1053	rBV4	606	789	0.06%	0.007%
41	7.629	1072	1073	1077	rVB2	243	243	0.02%	0.002%
42	7.665	1077	1079	1084	rBV2	176	312	0.02%	0.003%
43	7.811	1101	1103	1104	rBV	479	370	0.03%	0.004%
44	7.933	1120	1123	1124	rBV	849	902	0.07%	0.009%
45	8.049	1136	1142	1144	rBV2	387	579	0.04%	0.005%
46	8.196	1165	1166	1170	rBV2	208	217	0.02%	0.002%
47	8.275	1177	1179	1181	rBV2	339	251	0.02%	0.002%
48	8.330	1181	1188	1199	rBV	164742	271125	19.80%	2.570%
49	8.653	1234	1241	1249	rBV	703811	1092693	79.80%	10.358%
50	8.720	1249	1252	1259	rVB	9896	16385	1.20%	0.155%
51	8.952	1281	1290	1299	rBV	115050	172595	12.60%	1.636%
52	9.281	1339	1344	1346	rBV2	1767	2370	0.17%	0.022%
53	9.348	1353	1355	1356	rBV	259	215	0.02%	0.002%
54	9.384	1356	1361	1375	rBV	539215	780857	57.02%	7.402%
55	9.829	1432	1434	1437	rVB3	385	492	0.04%	0.005%
56	9.915	1446	1448	1451	rBV	256	225	0.02%	0.002%
57	10.055	1465	1471	1482	rBV	752660	991709	72.42%	9.401%
58	10.256	1502	1504	1507	rBV3	299	372	0.03%	0.004%
59	10.305	1507	1512	1518	rVV5	1410	2302	0.17%	0.022%
60	10.476	1536	1540	1541	rVB2	280	335	0.02%	0.003%
61	10.604	1560	1561	1564	rVB2	406	402	0.03%	0.004%
62	10.646	1564	1568	1570	rBV3	651	948	0.07%	0.009%
63	10.762	1585	1587	1589	rBV	323	349	0.03%	0.003%
64	10.854	1601	1602	1606	rVB	294	248	0.02%	0.002%
65	11.122	1639	1646	1649	rVB3	1542	2463	0.18%	0.023%
66	11.195	1652	1658	1670	rBV	560495	705139	51.49%	6.685%
67	11.347	1681	1683	1684	rBV	297	259	0.02%	0.002%
68	11.451	1698	1700	1702	rBV2	641	661	0.05%	0.006%
69	11.616	1725	1727	1728	rBV2	278	238	0.02%	0.002%
70	11.634	1728	1730	1733	rVB	350	253	0.02%	0.002%
71	11.719	1740	1744	1745	rBV2	423	526	0.04%	0.005%
72	11.756	1746	1750	1754	rVB3	1895	2415	0.18%	0.023%
73	11.835	1762	1763	1765	rVB2	487	295	0.02%	0.003%
74	11.872	1765	1769	1771	rVB2	211	300	0.02%	0.003%
75	11.902	1771	1774	1775	rBV	373	324	0.02%	0.003%
76	12.024	1789	1794	1804	rVV	800408	966285	70.56%	9.160%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029451.D
 Acq On : 14 Jun 2022 06:32
 Operator : JC/MD
 Sample : N3311-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0E00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.189	1819	1821	1824	rVB	304	276	0.02%	0.003%
78	12.323	1837	1843	1850	rVV	763070	946553	69.12%	8.973%
79	12.420	1857	1859	1864	rVB2	674	559	0.04%	0.005%
80	12.701	1904	1905	1907	rVB	297	213	0.02%	0.002%
81	12.762	1909	1915	1917	rBV2	361	520	0.04%	0.005%
82	12.835	1924	1927	1929	rBV2	256	268	0.02%	0.003%
83	12.859	1929	1931	1933	rVV2	360	263	0.02%	0.002%
84	12.896	1935	1937	1941	rVB	202	264	0.02%	0.003%
85	13.128	1972	1975	1978	rVV2	357	407	0.03%	0.004%
86	13.170	1981	1982	1986	rVB2	366	378	0.03%	0.004%
87	13.268	1996	1998	2001	rBV2	262	313	0.02%	0.003%
88	13.432	2023	2025	2028	rVV	343	395	0.03%	0.004%
89	13.780	2080	2082	2086	rBV2	382	646	0.05%	0.006%
90	13.932	2104	2107	2110	rVV3	284	386	0.03%	0.004%
91	13.969	2111	2113	2115	rVB2	505	357	0.03%	0.003%
92	13.993	2115	2117	2119	rBV	460	387	0.03%	0.004%
93	14.243	2156	2158	2160	rBV3	224	308	0.02%	0.003%
94	14.426	2186	2188	2189	rBV2	243	247	0.02%	0.002%
95	14.829	2253	2254	2256	rBV2	351	214	0.02%	0.002%
96	14.932	2269	2271	2272	rVB	557	310	0.02%	0.003%
97	14.950	2272	2274	2277	rBV3	405	527	0.04%	0.005%
98	15.316	2332	2334	2336	rBV2	584	568	0.04%	0.005%
99	15.420	2350	2351	2354	rVB3	867	632	0.05%	0.006%
100	16.645	2550	2552	2554	rBV	722	538	0.04%	0.005%

Sum of corrected areas: 10548791




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029451.D
Acq On : 14 Jun 2022 06:32
Operator : JC/MD
Sample : N3311-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0E00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

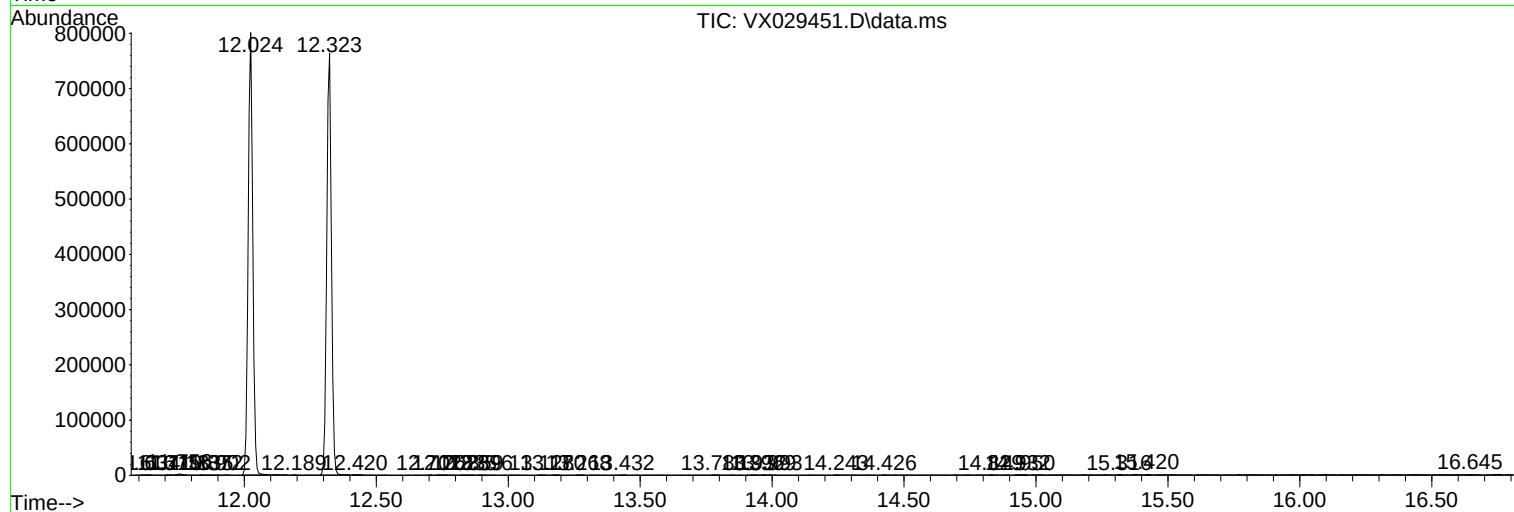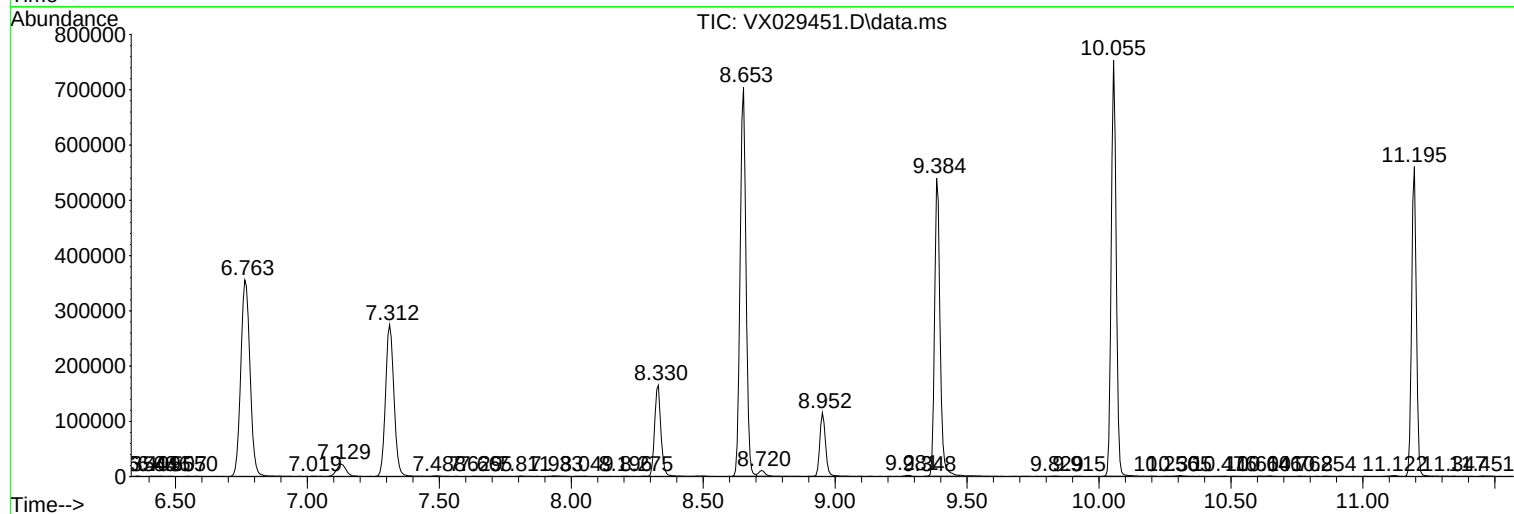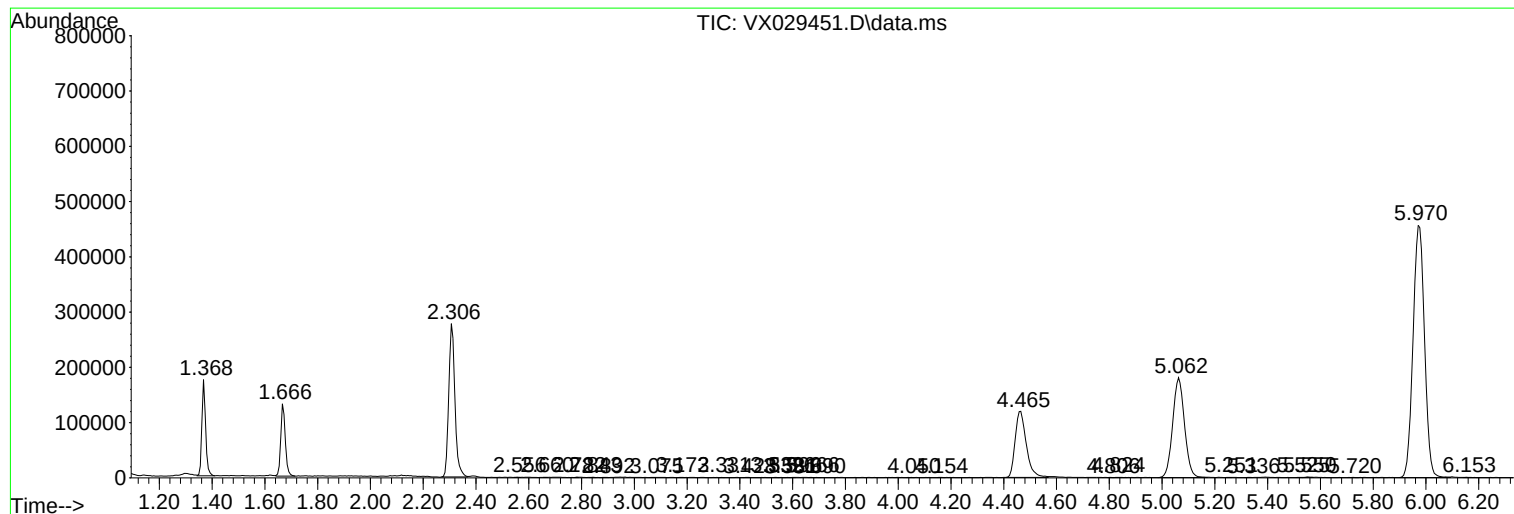

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029451.D
Acq On : 14 Jun 2022 06:32
Operator : JC/MD
Sample : N3311-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0E00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029451.D
Acq On : 14 Jun 2022 06:32
Operator : JC/MD
Sample : N3311-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0E00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc