

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029452.D
 Acq On : 14 Jun 2022 06:55
 Operator : JC/MD
 Sample : N3311-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0E03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029452.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	172659	170634	12.63%	1.624%
2	1.666	91	95	102	rVB	123923	146452	10.84%	1.394%
3	2.306	194	200	210	rBV	274940	439734	32.54%	4.186%
4	2.709	262	266	268	rBV2	606	877	0.06%	0.008%
5	2.879	292	294	297	rBV2	298	383	0.03%	0.004%
6	2.947	300	305	306	rBV2	965	1282	0.09%	0.012%
7	3.026	316	318	320	rVB	462	325	0.02%	0.003%
8	3.136	335	336	338	rBV2	392	279	0.02%	0.003%
9	3.190	342	345	347	rBV2	263	326	0.02%	0.003%
10	3.245	351	354	356	rBV2	186	253	0.02%	0.002%
11	3.264	356	357	361	rBV3	291	267	0.02%	0.003%
12	3.379	374	376	378	rVV2	225	314	0.02%	0.003%
13	3.587	408	410	413	rBV2	299	389	0.03%	0.004%
14	3.611	413	414	418	rVV3	291	355	0.03%	0.003%
15	3.715	429	431	433	rBV2	234	244	0.02%	0.002%
16	3.885	454	459	462	rBV2	301	484	0.04%	0.005%
17	4.050	484	486	488	rVV2	412	267	0.02%	0.003%
18	4.343	533	534	536	rBV2	333	243	0.02%	0.002%
19	4.458	543	553	569	rBV	119268	349846	25.89%	3.330%
20	4.715	593	595	597	rVB2	328	264	0.02%	0.003%
21	4.739	597	599	600	rBV	298	262	0.02%	0.002%
22	4.800	607	609	610	rVB2	428	265	0.02%	0.003%
23	5.062	637	652	670	rBV	177715	567943	42.02%	5.406%
24	5.294	688	690	693	rBV2	379	431	0.03%	0.004%
25	5.397	702	707	712	rBV4	629	1525	0.11%	0.015%
26	5.556	727	733	736	rBV3	724	1637	0.12%	0.016%
27	5.867	780	784	787	rVB2	282	315	0.02%	0.003%
28	5.970	787	801	820	rBV2	453198	1351524	100.00%	12.866%
29	6.293	851	854	857	rBV2	498	566	0.04%	0.005%
30	6.361	861	865	866	rBV2	282	304	0.02%	0.003%
31	6.763	922	931	949	rBV	353262	853841	63.18%	8.128%
32	7.056	977	979	981	rBV	486	332	0.02%	0.003%
33	7.129	981	991	1001	rVV5	21872	52853	3.91%	0.503%
34	7.312	1012	1021	1038	rVV	274703	601687	44.52%	5.728%
35	7.482	1044	1049	1050	rBV2	1003	1120	0.08%	0.011%
36	7.555	1058	1061	1063	rBV2	238	248	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029452.D
 Acq On : 14 Jun 2022 06:55
 Operator : JC/MD
 Sample : N3311-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0E03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.720	1086	1088	1090	rBV3	358	387	0.03%	0.004%
38	7.818	1099	1104	1107	rBV2	531	933	0.07%	0.009%
39	7.872	1110	1113	1116	rBV2	402	482	0.04%	0.005%
40	7.940	1118	1124	1125	rBV	831	1396	0.10%	0.013%
41	8.037	1137	1140	1143	rBV2	355	379	0.03%	0.004%
42	8.080	1145	1147	1150	rBV2	302	262	0.02%	0.002%
43	8.171	1159	1162	1167	rBV2	446	583	0.04%	0.006%
44	8.330	1181	1188	1200	rBV	158946	269231	19.92%	2.563%
45	8.488	1209	1214	1220	rBV4	1060	2117	0.16%	0.020%
46	8.580	1226	1229	1234	rVB3	615	933	0.07%	0.009%
47	8.653	1234	1241	1248	rBV	686071	1086201	80.37%	10.340%
48	8.720	1248	1252	1258	rVB	18605	30055	2.22%	0.286%
49	8.891	1277	1280	1284	rBV2	249	251	0.02%	0.002%
50	8.952	1284	1290	1298	rBV	114330	166908	12.35%	1.589%
51	9.281	1340	1344	1347	rVB3	1413	2193	0.16%	0.021%
52	9.384	1356	1361	1379	rBV	534973	774655	57.32%	7.374%
53	9.586	1392	1394	1396	rBV2	690	654	0.05%	0.006%
54	9.634	1400	1402	1405	rBV3	440	503	0.04%	0.005%
55	9.744	1418	1420	1424	rBV2	340	443	0.03%	0.004%
56	9.897	1442	1445	1448	rBV2	250	388	0.03%	0.004%
57	10.055	1465	1471	1482	rBV	739875	991059	73.33%	9.434%
58	10.195	1491	1494	1498	rVB3	1776	2589	0.19%	0.025%
59	10.232	1498	1500	1503	rBV	213	282	0.02%	0.003%
60	10.305	1507	1512	1517	rVV	5098	7516	0.56%	0.072%
61	10.518	1545	1547	1549	rVV2	236	252	0.02%	0.002%
62	10.646	1564	1568	1572	rVV2	2747	3689	0.27%	0.035%
63	10.762	1586	1587	1589	rBV	347	338	0.03%	0.003%
64	10.848	1600	1601	1605	rVB2	252	249	0.02%	0.002%
65	11.122	1642	1646	1652	rVB5	1751	2367	0.18%	0.023%
66	11.195	1652	1658	1668	rBV	536358	691310	51.15%	6.581%
67	11.384	1685	1689	1695	rBV2	1100	1671	0.12%	0.016%
68	11.457	1698	1701	1702	rBV2	653	634	0.05%	0.006%
69	11.549	1714	1716	1717	rBV	455	385	0.03%	0.004%
70	11.616	1721	1727	1730	rVV2	841	988	0.07%	0.009%
71	11.713	1741	1743	1745	rVB2	737	473	0.03%	0.005%
72	11.756	1745	1750	1755	rBV4	4149	5523	0.41%	0.053%
73	11.829	1760	1762	1763	rBV	365	260	0.02%	0.002%
74	11.933	1775	1779	1784	rBV3	760	952	0.07%	0.009%
75	12.024	1789	1794	1801	rVV	786347	966409	71.51%	9.200%
76	12.225	1825	1827	1828	rBV	371	351	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029452.D
 Acq On : 14 Jun 2022 06:55
 Operator : JC/MD
 Sample : N3311-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0E03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.244	1828	1830	1835	rVB	918	876	0.06%	0.008%
78	12.323	1837	1843	1851	rBV	714559	928100	68.67%	8.835%
79	12.567	1879	1883	1884	rVB3	340	391	0.03%	0.004%
80	12.774	1915	1917	1921	rVB	388	354	0.03%	0.003%
81	12.963	1944	1948	1952	rBV2	840	1069	0.08%	0.010%
82	13.048	1960	1962	1963	rVV	443	272	0.02%	0.003%
83	13.103	1968	1971	1972	rBV	464	364	0.03%	0.003%
84	13.292	2000	2002	2005	rVB3	414	237	0.02%	0.002%
85	13.365	2013	2014	2019	rBV2	398	503	0.04%	0.005%
86	13.542	2040	2043	2046	rBV3	493	732	0.05%	0.007%
87	13.603	2052	2053	2055	rBV	415	328	0.02%	0.003%
88	13.676	2063	2065	2066	rBV	421	269	0.02%	0.003%
89	13.774	2079	2081	2087	rVV2	829	1320	0.10%	0.013%
90	14.085	2130	2132	2134	rVB	424	389	0.03%	0.004%
91	14.127	2138	2139	2140	rBV	413	246	0.02%	0.002%
92	14.377	2178	2180	2186	rVB3	488	749	0.06%	0.007%
93	14.481	2195	2197	2200	rBV2	530	652	0.05%	0.006%
94	14.755	2240	2242	2243	rBV2	421	382	0.03%	0.004%
95	15.060	2291	2292	2293	rBV	603	297	0.02%	0.003%
96	15.176	2308	2311	2314	rBV3	680	840	0.06%	0.008%
97	16.456	2518	2521	2522	rBV3	592	542	0.04%	0.005%
98	16.572	2538	2540	2541	rBV2	446	248	0.02%	0.002%
99	16.676	2553	2557	2560	rBV4	535	840	0.06%	0.008%
100	16.743	2566	2568	2570	rBV2	790	546	0.04%	0.005%


Sum of corrected areas: 10504868

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029452.D
Acq On : 14 Jun 2022 06:55
Operator : JC/MD
Sample : N3311-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0E03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

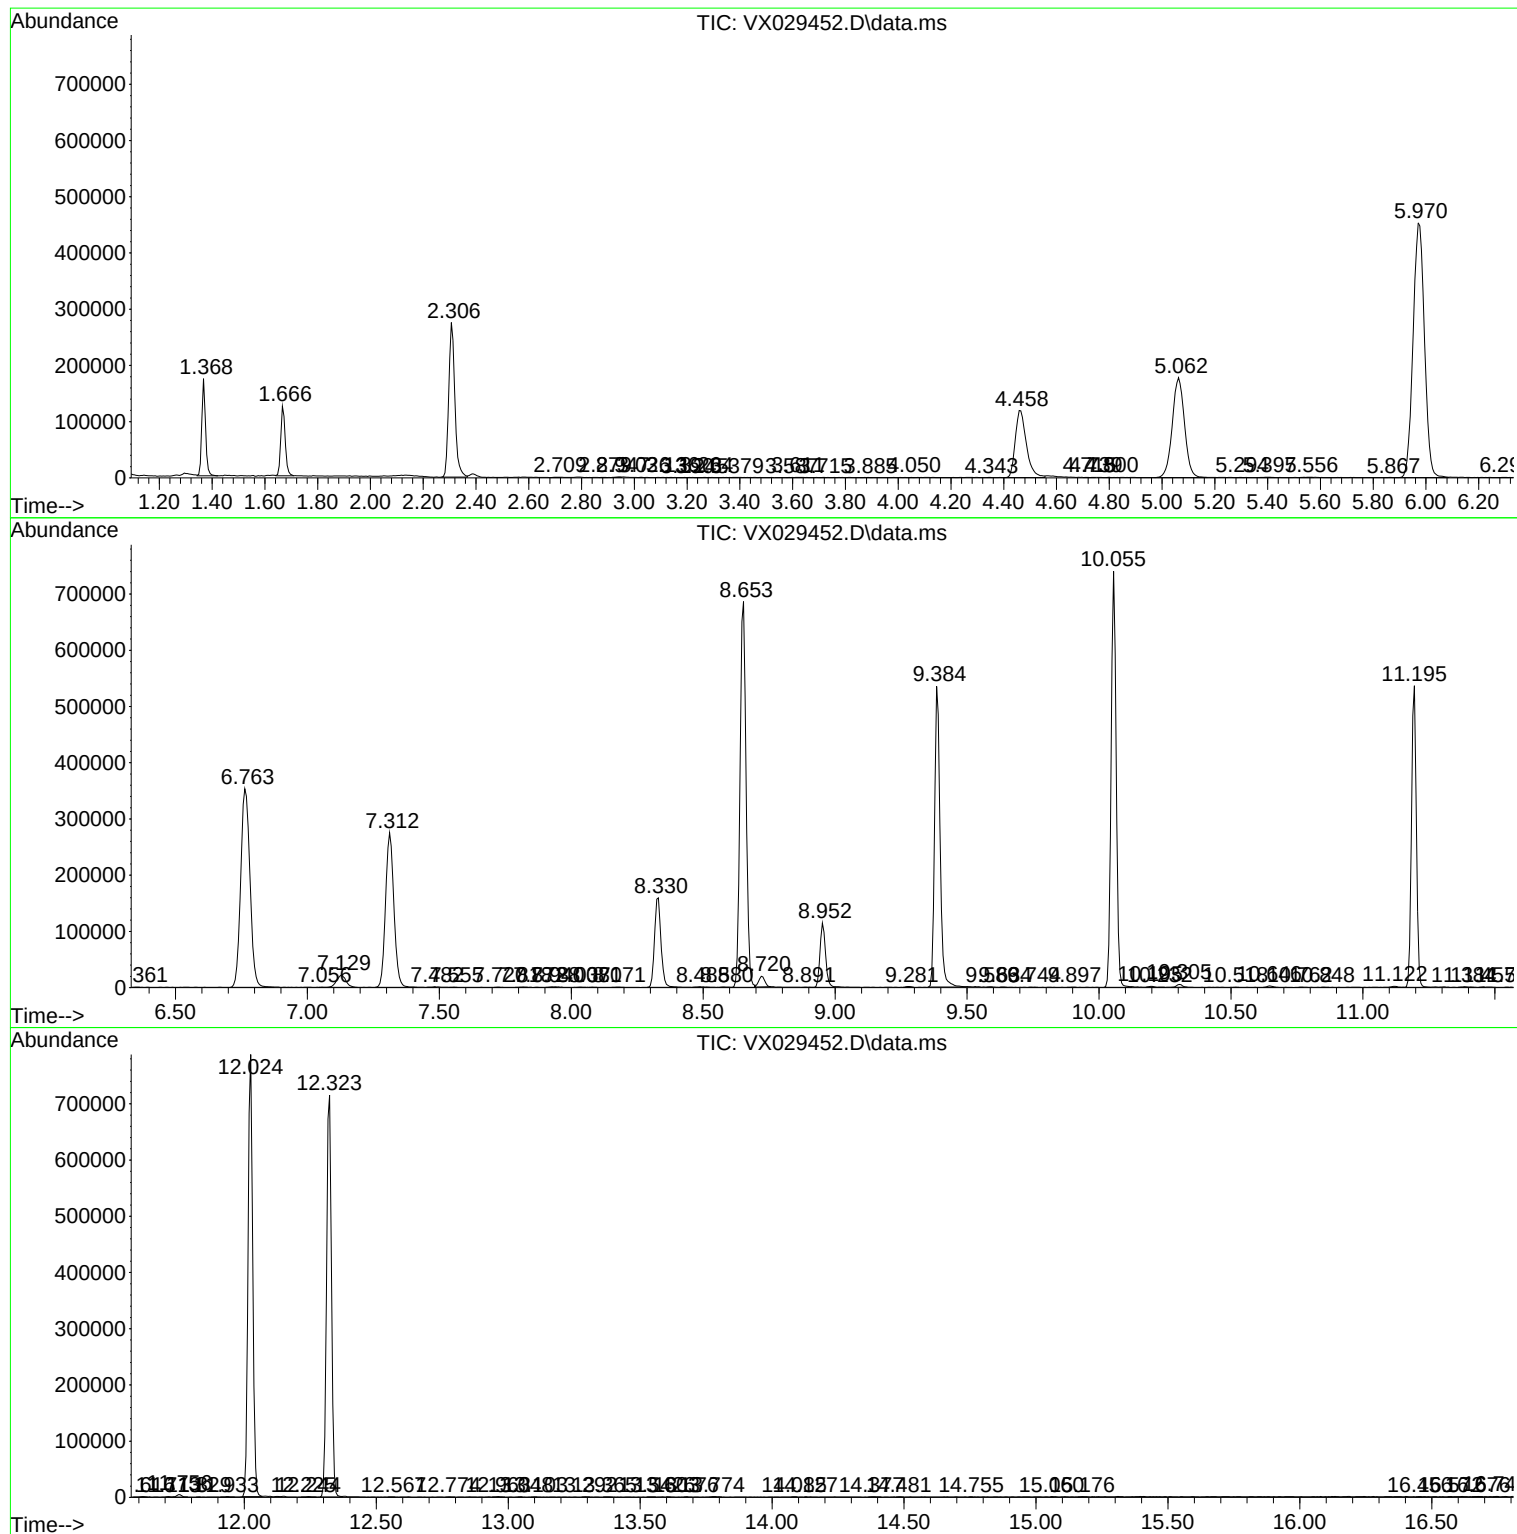

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029452.D
Acq On : 14 Jun 2022 06:55
Operator : JC/MD
Sample : N3311-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0E03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029452.D
Acq On : 14 Jun 2022 06:55
Operator : JC/MD
Sample : N3311-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0E03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc