

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029453.D
 Acq On : 14 Jun 2022 07:18
 Operator : JC/MD
 Sample : N3311-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0E04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	163311	164382	12.40%	1.523%
2	1.666	91	95	103	rVB	122226	148642	11.21%	1.377%
3	2.307	194	200	210	rBV2	276383	455414	34.35%	4.220%
4	2.788	273	279	285	rBV3	933	1520	0.11%	0.014%
5	2.861	289	291	294	rVB2	346	331	0.02%	0.003%
6	2.934	301	303	306	rBV4	607	937	0.07%	0.009%
7	3.105	329	331	333	rVB2	344	239	0.02%	0.002%
8	3.130	333	335	339	rVV2	277	401	0.03%	0.004%
9	3.349	369	371	373	rBV2	330	284	0.02%	0.003%
10	3.508	395	397	399	rVB	367	308	0.02%	0.003%
11	3.538	399	402	407	rBV3	321	621	0.05%	0.006%
12	3.593	409	411	413	rVV	293	325	0.02%	0.003%
13	3.623	413	416	420	rVB3	671	928	0.07%	0.009%
14	3.977	473	474	477	rBV2	313	383	0.03%	0.004%
15	4.105	493	495	496	rBV2	229	230	0.02%	0.002%
16	4.233	514	516	518	rBV	287	200	0.02%	0.002%
17	4.300	525	527	528	rBV	254	249	0.02%	0.002%
18	4.373	538	539	543	rBV	351	369	0.03%	0.003%
19	4.465	545	554	575	rVV	116803	360434	27.19%	3.340%
20	4.769	601	604	607	rVB2	384	549	0.04%	0.005%
21	4.855	615	618	619	rBV2	403	531	0.04%	0.005%
22	5.062	640	652	669	rBV	178630	542513	40.92%	5.027%
23	5.306	689	692	697	rBV2	297	396	0.03%	0.004%
24	5.349	697	699	700	rBV	499	332	0.03%	0.003%
25	5.385	700	705	707	rBV4	2342	3684	0.28%	0.034%
26	5.562	729	734	738	rBV3	727	1533	0.12%	0.014%
27	5.629	742	745	747	rBV2	231	258	0.02%	0.002%
28	5.775	767	769	771	rVB2	248	246	0.02%	0.002%
29	5.970	790	801	819	rBV2	447385	1325704	100.00%	12.285%
30	6.172	832	834	835	rVB2	402	236	0.02%	0.002%
31	6.251	846	847	848	rBV	382	272	0.02%	0.003%
32	6.281	851	852	855	rVV2	474	435	0.03%	0.004%
33	6.312	855	857	861	rVV3	173	203	0.02%	0.002%
34	6.537	891	894	895	rBV2	368	410	0.03%	0.004%
35	6.653	911	913	919	rVB2	378	476	0.04%	0.004%
36	6.763	922	931	946	rBV	340858	811584	61.22%	7.521%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029453.D
 Acq On : 14 Jun 2022 07:18
 Operator : JC/MD
 Sample : N3311-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0E04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.129	982	991	1004	rBV	268379	580409	43.78%	5.378%
38	7.312	1012	1021	1033	rBV	270207	587534	44.32%	5.444%
39	7.476	1046	1048	1053	rBV3	781	1102	0.08%	0.010%
40	7.714	1084	1087	1090	rBV2	468	630	0.05%	0.006%
41	7.769	1095	1096	1099	rBV2	265	276	0.02%	0.003%
42	7.806	1101	1102	1104	rBV	324	215	0.02%	0.002%
43	7.903	1116	1118	1120	rBV2	358	286	0.02%	0.003%
44	7.934	1120	1123	1127	rBV2	863	1466	0.11%	0.014%
45	8.129	1153	1155	1156	rBV	279	265	0.02%	0.002%
46	8.147	1156	1158	1159	rVB2	386	257	0.02%	0.002%
47	8.330	1181	1188	1198	rBV	155681	264610	19.96%	2.452%
48	8.482	1211	1213	1221	rVB3	782	1477	0.11%	0.014%
49	8.574	1226	1228	1229	rBV2	388	330	0.02%	0.003%
50	8.653	1234	1241	1248	rVV	675427	1065381	80.36%	9.873%
51	8.720	1248	1252	1260	rVB	13989	23445	1.77%	0.217%
52	8.872	1275	1277	1280	rVB2	257	298	0.02%	0.003%
53	8.909	1280	1283	1284	rVB2	276	264	0.02%	0.002%
54	8.952	1284	1290	1300	rBV	116567	167584	12.64%	1.553%
55	9.153	1321	1323	1326	rVB2	462	452	0.03%	0.004%
56	9.250	1337	1339	1340	rBV	299	219	0.02%	0.002%
57	9.275	1340	1343	1348	rVV4	1633	2299	0.17%	0.021%
58	9.385	1356	1361	1378	rBV	524764	760666	57.38%	7.049%
59	9.921	1447	1449	1453	rVB2	332	362	0.03%	0.003%
60	9.958	1453	1455	1459	rBV3	280	413	0.03%	0.004%
61	10.055	1465	1471	1487	rBV	707435	944490	71.24%	8.752%
62	10.305	1508	1512	1516	rVB2	3557	4641	0.35%	0.043%
63	10.372	1521	1523	1525	rBV	304	219	0.02%	0.002%
64	10.457	1534	1537	1541	rBV2	370	634	0.05%	0.006%
65	10.579	1555	1557	1559	rBV2	344	355	0.03%	0.003%
66	10.598	1559	1560	1561	rVV	418	206	0.02%	0.002%
67	10.653	1564	1569	1576	rVV6	1105	2358	0.18%	0.022%
68	10.817	1595	1596	1599	rBV2	330	293	0.02%	0.003%
69	11.006	1626	1627	1630	rBV2	322	346	0.03%	0.003%
70	11.122	1643	1646	1650	rVB3	1592	1834	0.14%	0.017%
71	11.195	1652	1658	1667	rBV	532103	688277	51.92%	6.378%
72	11.348	1681	1683	1685	rVB2	335	205	0.02%	0.002%
73	11.384	1685	1689	1690	rBV3	756	805	0.06%	0.007%
74	11.451	1699	1700	1702	rVB	440	232	0.02%	0.002%
75	11.476	1702	1704	1711	rVB3	976	1291	0.10%	0.012%
76	11.567	1716	1719	1720	rBV	459	495	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029453.D
 Acq On : 14 Jun 2022 07:18
 Operator : JC/MD
 Sample : N3311-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0E04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.713	1741	1743	1744	rVV	513	321	0.02%	0.003%
78	11.750	1746	1749	1754	rVB3	2774	3911	0.30%	0.036%
79	11.793	1754	1756	1759	rBV2	342	344	0.03%	0.003%
80	11.823	1759	1761	1763	rBV2	267	275	0.02%	0.003%
81	11.896	1771	1773	1777	rBV2	312	513	0.04%	0.005%
82	11.939	1777	1780	1785	rVB4	755	1033	0.08%	0.010%
83	12.024	1789	1794	1804	rVV	750334	921294	69.49%	8.537%
84	12.323	1837	1843	1851	rBV	747035	925146	69.79%	8.573%
85	12.689	1901	1903	1906	rVB	413	410	0.03%	0.004%
86	12.823	1921	1925	1928	rBV3	230	461	0.03%	0.004%
87	12.853	1928	1930	1934	rVV2	418	508	0.04%	0.005%
88	13.219	1989	1990	1994	rVB	351	264	0.02%	0.002%
89	13.420	2021	2023	2024	rBV	354	240	0.02%	0.002%
90	13.469	2030	2031	2034	rVB	373	266	0.02%	0.002%
91	13.780	2080	2082	2088	rVB3	914	1034	0.08%	0.010%
92	13.841	2090	2092	2093	rVB2	364	195	0.01%	0.002%
93	13.865	2093	2096	2097	rBV	248	278	0.02%	0.003%
94	13.914	2103	2104	2106	rVB	363	205	0.02%	0.002%
95	13.939	2106	2108	2110	rBV	365	267	0.02%	0.002%
96	13.963	2110	2112	2113	rBV2	359	309	0.02%	0.003%
97	14.810	2250	2251	2252	rBV	534	272	0.02%	0.003%
98	15.536	2368	2370	2373	rBV2	612	663	0.05%	0.006%
99	16.341	2500	2502	2503	rBV2	429	225	0.02%	0.002%
100	16.639	2550	2551	2553	rBV2	574	471	0.04%	0.004%




Sum of corrected areas: 10791385

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029453.D
Acq On : 14 Jun 2022 07:18
Operator : JC/MD
Sample : N3311-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0E04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

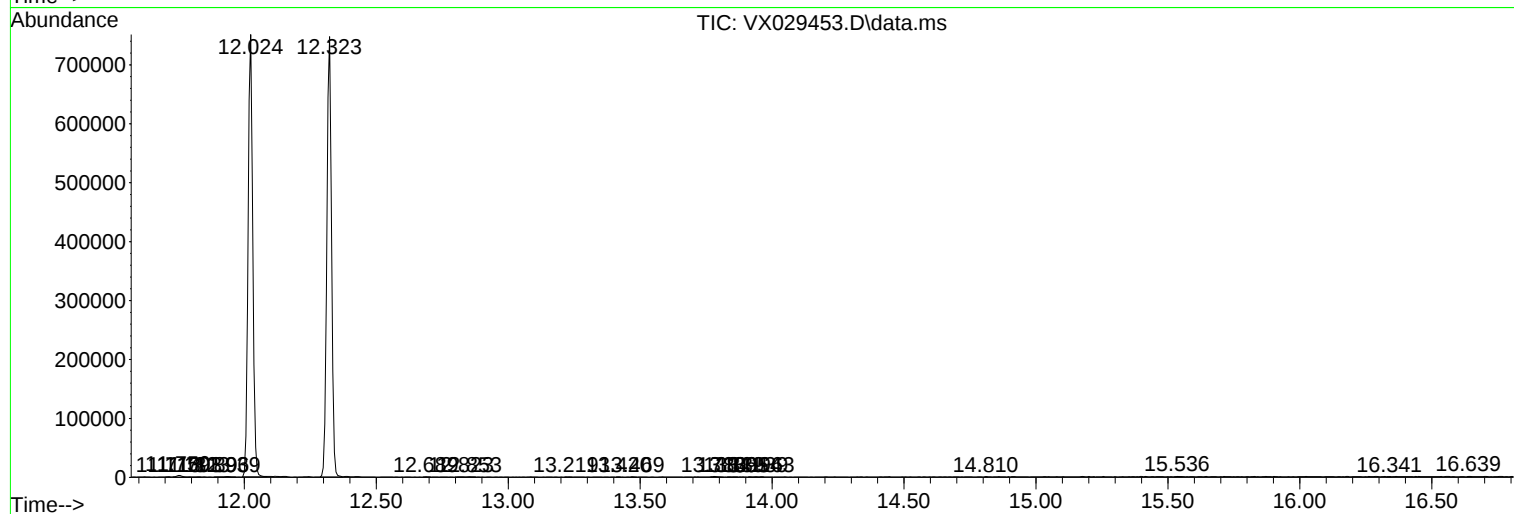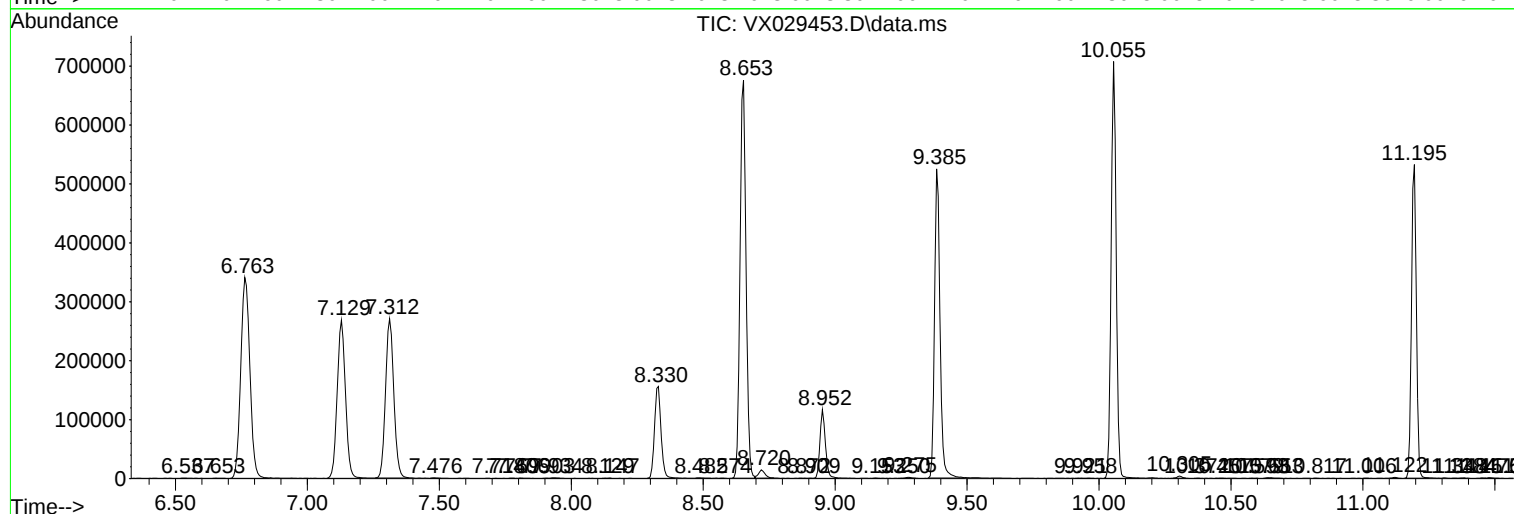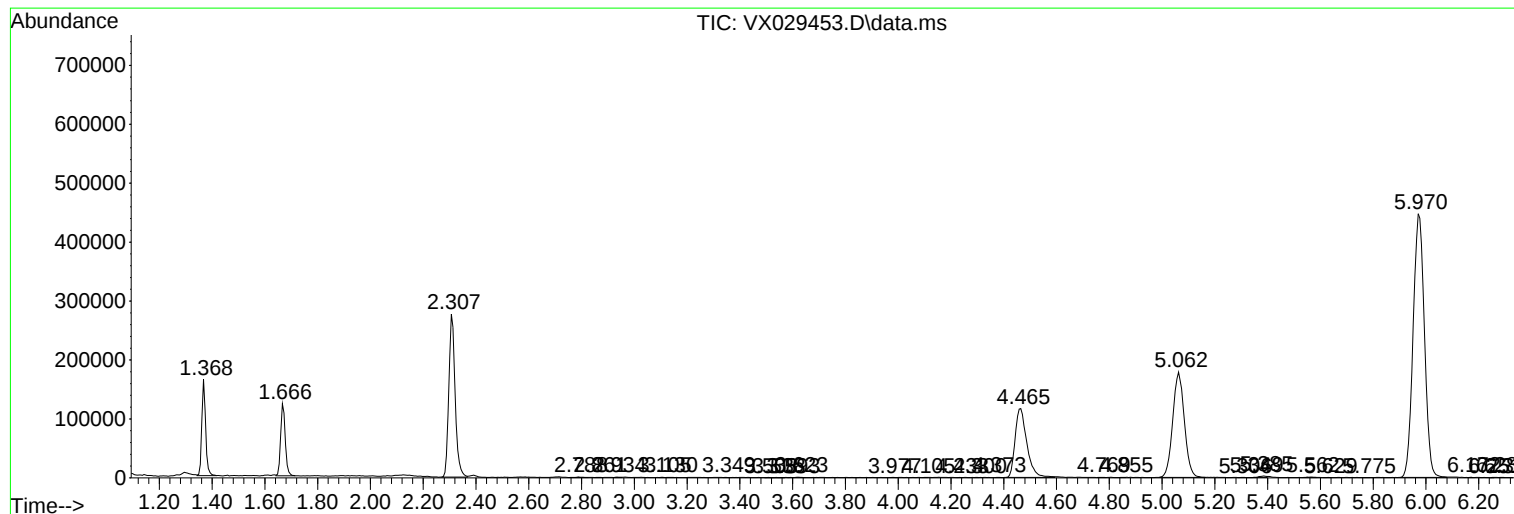

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029453.D
Acq On : 14 Jun 2022 07:18
Operator : JC/MD
Sample : N3311-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0E04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
Data File : VX029453.D
Acq On : 14 Jun 2022 07:18
Operator : JC/MD
Sample : N3311-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0E04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------