
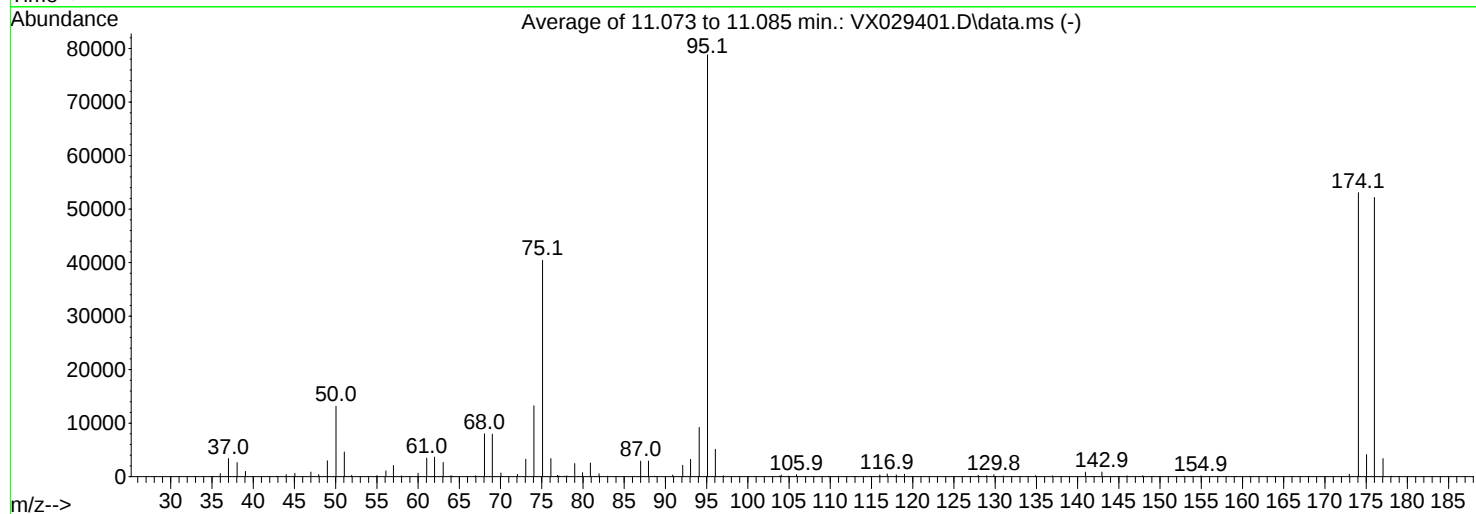


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061322\
 Data File : VX029401.D
 Acq On : 13 Jun 2022 09:46
 Operator : JC/MD
 Sample : BFB636
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB636

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM061322WMA.M
 Title : VOC Analysis
 Last Update : Wed Jun 15 07:14:08 2022

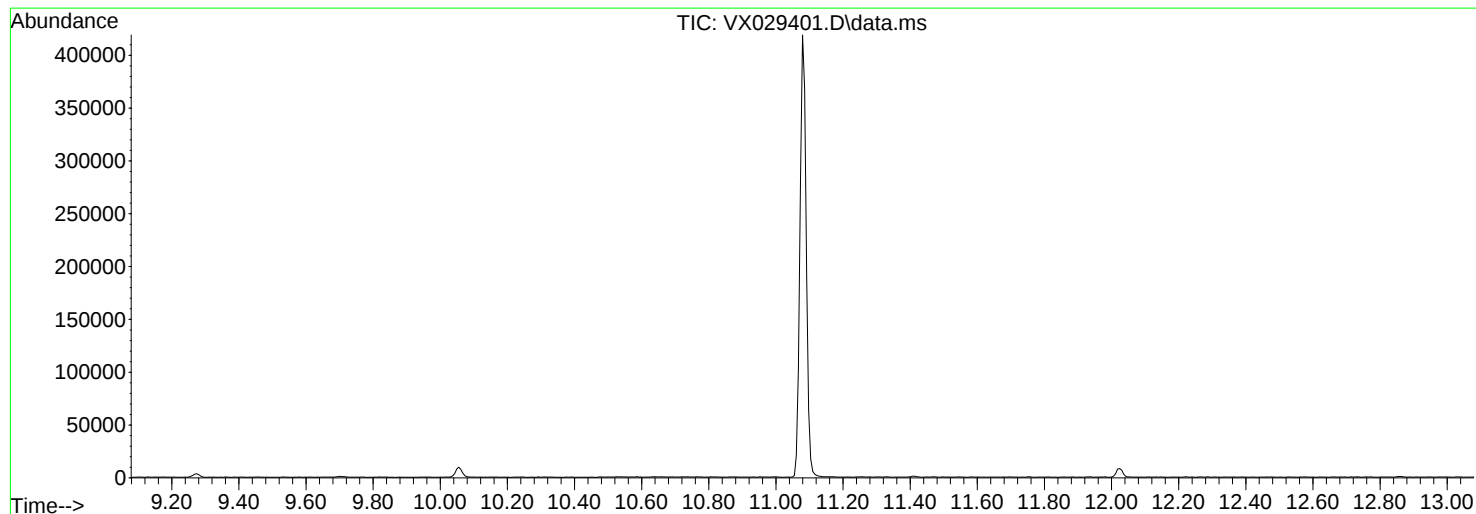

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	13151	PASS
75	95	30	80	51.3	40432	PASS
95	95	100	100	100.0	78821	PASS
96	95	5	9	6.5	5102	PASS
173	174	0.00	2	0.9	461	PASS
174	95	50	120	67.3	53061	PASS
175	174	5	9	7.8	4130	PASS
176	174	95	101	98.3	52176	PASS
177	176	5	9	6.5	3380	PASS

m/z	Abundance
36.00	143.0
38.10	62.0
40.00	404.0
43.90	207.0

Instrument :
MSVOA_X
ClientSampleId :
BFB636

m/z	Abundance
35.20	55.0
36.00	735.0
37.00	2982.0
38.10	2503.0
39.00	897.0
40.00	536.0
42.90	56.0
44.00	495.0
45.20	407.0
47.00	891.0
48.00	374.0
49.00	2641.0
50.10	11450.0
51.00	4266.0
52.00	258.0
54.90	166.0
56.10	976.0
57.00	1680.0
58.00	80.0
60.00	459.0
61.00	2886.0
62.00	2996.0
63.00	2158.0
64.00	265.0
67.00	162.0
68.00	6466.0
69.00	6740.0
70.10	625.0
72.10	302.0
73.00	2658.0
74.00	11209.0
75.10	34392.0
76.10	2851.0
76.90	315.0
78.10	184.0
79.00	2057.0
79.90	569.0
80.90	2147.0
81.90	542.0
87.10	2282.0
87.90	2587.0
88.70	236.0
90.90	296.0
92.10	1686.0
93.00	2690.0
94.10	7633.0
95.10	64224.0
96.00	4259.0
97.10	75.0
103.90	426.0
104.90	126.0
105.90	292.0
109.80	53.0
111.00	63.0
116.00	240.0
116.90	453.0
118.00	312.0
119.00	373.0
127.90	228.0
128.90	122.0
129.80	305.0
131.00	76.0
134.80	114.0
136.90	147.0
141.10	511.0
142.00	107.0
142.90	575.0
145.90	108.0
147.80	176.0
152.90	81.0
154.90	78.0
157.00	95.0
173.00	412.0
174.10	36480.0
175.10	3176.0
176.00	35336.0
177.10	2174.0
178.00	117.0

Instrument :
MSVOA_X
ClientSampleId :
BFB636

m/z	Abundance
36.00	834.0
37.00	4036.0
38.10	3225.0
39.10	1071.0
40.00	421.0
42.90	105.0
44.10	602.0
45.00	849.0
47.00	789.0
47.90	447.0
49.00	3489.0
50.00	15899.0
51.10	5378.0
52.00	236.0
55.00	316.0
56.10	1233.0
57.00	2593.0
58.00	140.0
60.00	992.0
61.10	4161.0
62.00	4515.0
63.10	3366.0
64.00	259.0
66.90	247.0
68.00	9683.0
69.00	9439.0
70.00	832.0
72.10	532.0
73.10	4120.0
74.10	16186.0
75.10	48304.0
76.10	4309.0
77.10	375.0
77.80	306.0
79.00	2905.0
80.00	917.0
80.90	2945.0
82.00	569.0
83.00	129.0
87.00	3636.0
88.00	3351.0
90.90	371.0
92.10	2548.0
93.10	3968.0
94.10	10678.0
95.10	91200.0
96.10	5956.0
97.10	255.0
104.10	479.0
104.90	128.0
105.80	443.0
109.70	90.0
110.90	89.0
114.90	184.0
116.00	322.0
116.90	517.0
118.10	294.0
118.90	458.0
127.90	314.0
129.00	248.0
129.90	507.0
131.10	147.0
134.90	173.0
137.00	107.0
140.90	1001.0
143.00	919.0
144.00	60.0
146.00	102.0
147.10	87.0
147.90	163.0
150.00	158.0
152.90	96.0
154.90	180.0
156.90	78.0
161.00	129.0
172.90	447.0
174.00	62080.0
175.00	5216.0
176.00	60920.0
177.00	4232.0
178.10	87.0

Instrument :
MSVOA_X
ClientSampleId :
BFB636

m/z	Abundance
36.00	560.0
37.00	3122.0
38.00	2398.0
39.10	1014.0
39.90	381.0
42.80	90.0
44.10	664.0
45.10	528.0
45.90	53.0
47.00	941.0
48.00	371.0
49.00	2715.0
50.10	12104.0
51.10	4204.0
51.90	220.0
55.10	191.0
56.10	1033.0
57.00	1986.0
57.90	201.0
60.00	562.0
61.00	3358.0
62.00	3466.0
63.10	2514.0
64.20	239.0
67.00	169.0
68.10	7923.0
69.00	7703.0
70.00	626.0
72.00	415.0
73.00	2992.0
74.00	12392.0
75.10	38600.0
76.10	2985.0
76.90	407.0
78.00	257.0
79.00	2419.0
79.90	743.0
80.90	2534.0
82.00	524.0
82.90	106.0
86.90	2840.0
88.00	2770.0
90.90	239.0
92.10	2170.0
93.00	3075.0
94.10	9363.0
95.10	81040.0
96.00	5090.0
97.00	116.0
104.00	393.0
105.00	150.0
106.00	393.0
107.00	61.0
110.90	117.0
111.80	61.0
112.80	81.0
115.00	78.0
116.00	456.0
116.90	542.0
117.90	363.0
119.10	484.0
128.00	268.0
129.00	189.0
129.80	335.0
130.90	149.0
135.00	225.0
137.00	155.0
141.00	997.0
141.70	102.0
143.00	1146.0
143.90	75.0
145.00	103.0
146.00	212.0
147.00	128.0
148.00	213.0
149.00	70.0
150.00	65.0
152.90	117.0
155.00	235.0
157.20	117.0
159.20	75.0
160.80	104.0
171.20	72.0
173.00	525.0
174.00	60624.0
175.00	3998.0
176.00	60272.0
177.10	3735.0
178.10	109.0

Instrument :
MSVOA_X
ClientSampleId :
BFB636