

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061323\
 Data File : VX036144.D
 Acq On : 13 Jun 2023 15:15
 Operator : JC/MD
 Sample : 03178-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-2A

Quant Time: Jun 14 00:55:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053123W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 31 12:50:30 2023
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/14/2023
 Supervised By : Mahesh Dadoda 06/14/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	201312	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	332732	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	298288	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	138945	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	158586	48.512	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	97.020%		
35) Dibromofluoromethane	5.385	113	105205	47.010	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	94.020%		
50) Toluene-d8	8.647	98	397826	49.531	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	99.060%		
62) 4-Bromofluorobenzene	11.079	95	155187	48.945	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	97.900%		
Target Compounds					Qvalue	
16) Acetone	2.404	43	2201	1.632	ug/l	98
31) Cyclohexane	5.471	56	1103m	0.322	ug/l	
85) sec-Butylbenzene	11.890	105	2759	0.286	ug/l	100
91) 1,2-Dichlorobenzene	12.335	146	1555	0.342	ug/l	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061323\
Data File : VX036144.D
Acq On : 13 Jun 2023 15:15
Operator : JC/MD
Sample : 03178-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
MW-2A

Quant Time: Jun 14 00:55:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053123W.M
Quant Title : SW846 8260
QLast Update : Wed May 31 12:50:30 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : John Carlone 06/14/2023
Supervised By : Mahesh Dadoda 06/14/2023

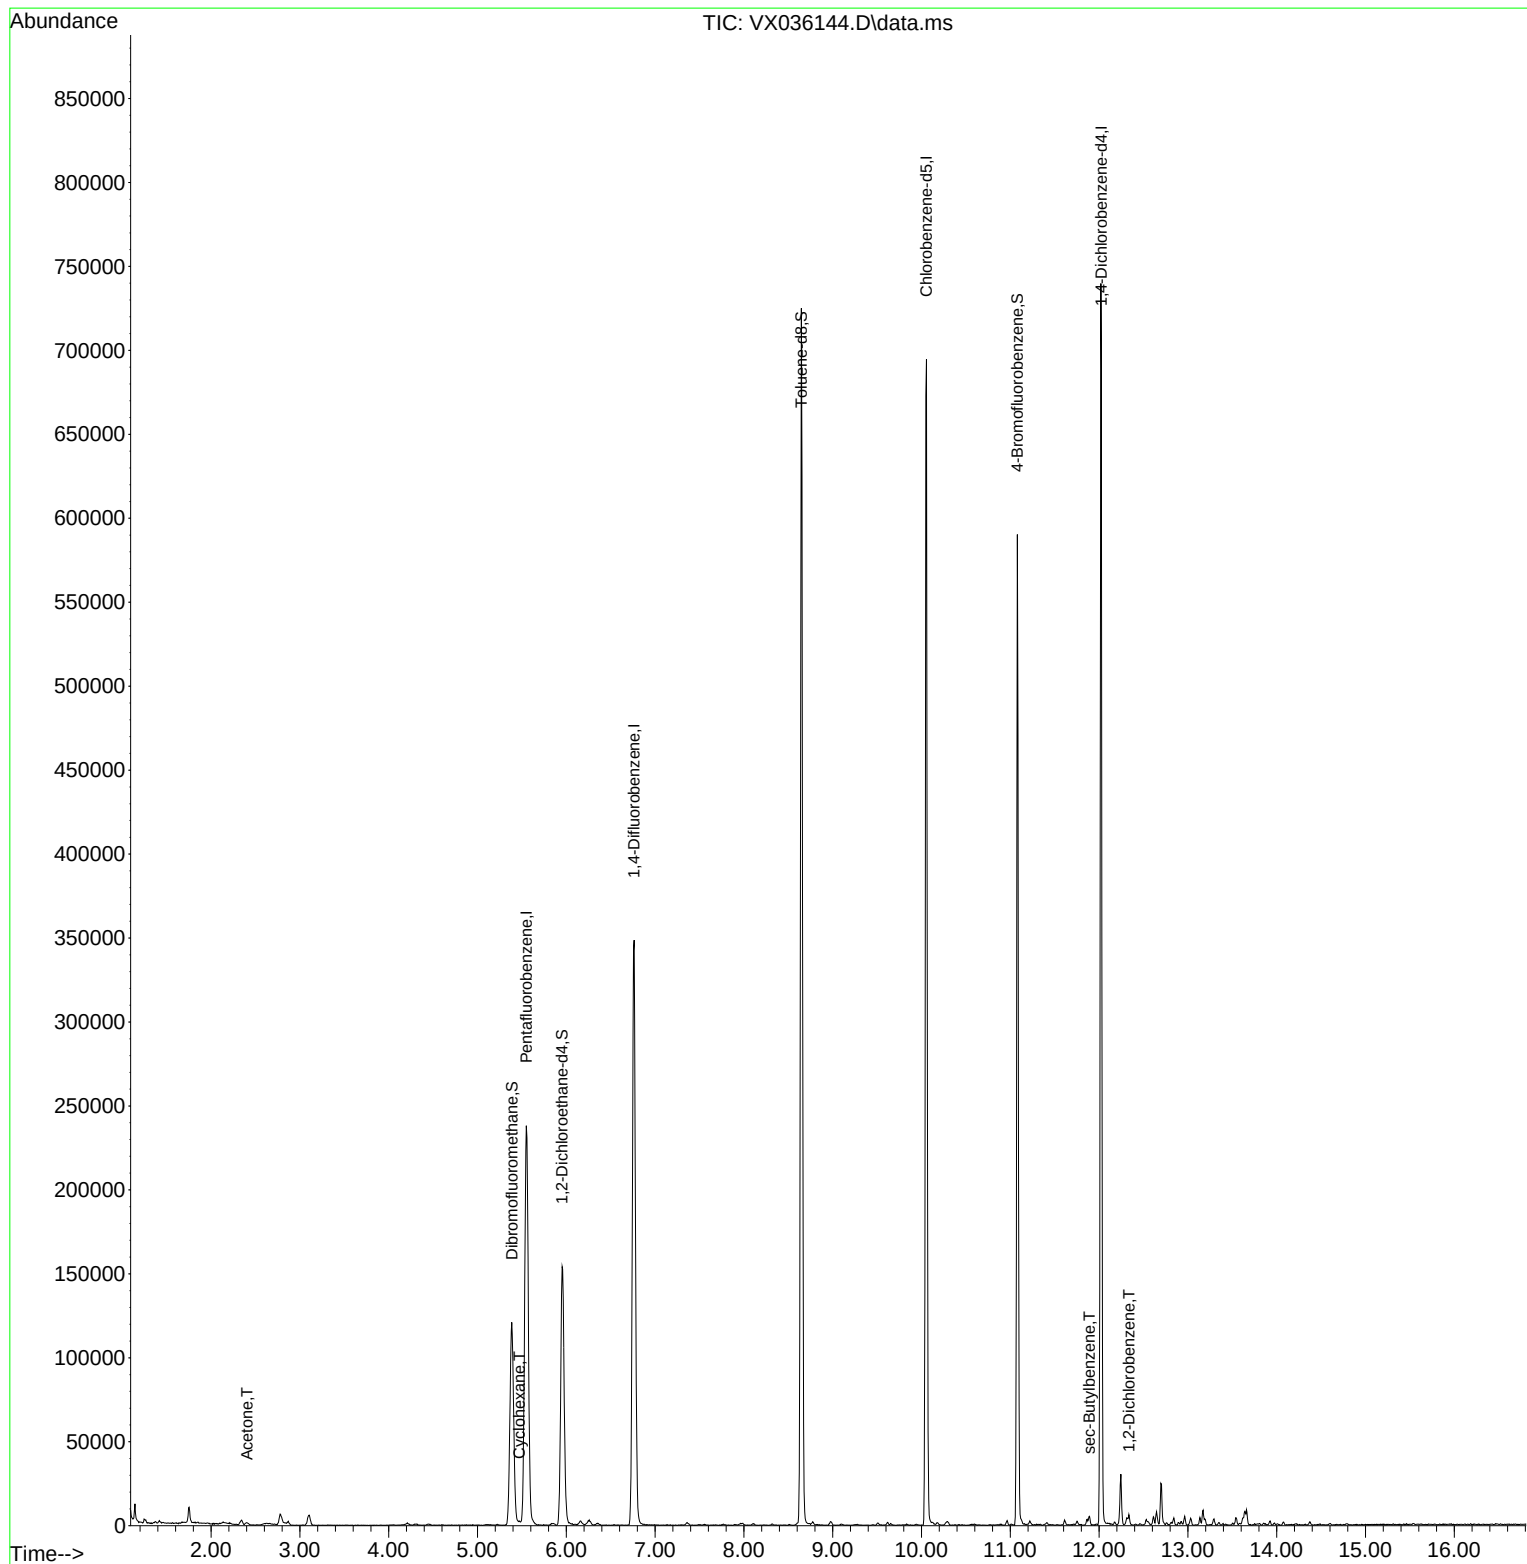

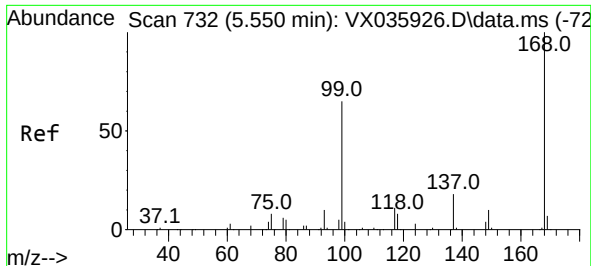

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 732
Delta R.T. 0.001 min
Lab File: VX036144.D
Acq: 13 Jun 2023 15:15




Instrument :
MSVOA_X
ClientSampleId :
MW-2A



Tgt Ion:168 Resp: 20131
Ion Ratio Lower Upper
168 100
99 73.0 57.0 85.6




Manual Integrations
APPROVED


Reviewed By :John Carlone 06/14/2023
Supervised By :Mahesh Dadoda 06/14/2023

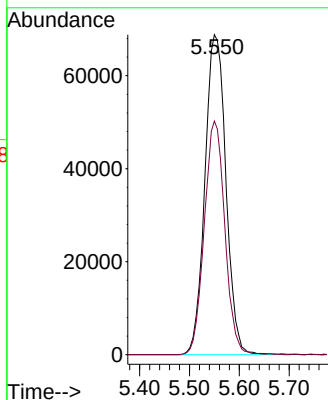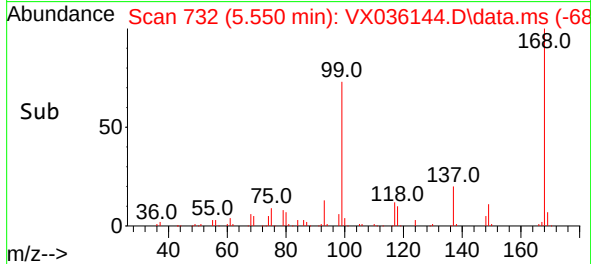

#16
Acetone
Concen: 1.632 ug/l
RT: 2.404 min Scan# 216
Delta R.T. 0.013 min
Lab File: VX036144.D
Acq: 13 Jun 2023 15:15


Tgt Ion: 43 Resp: 2201
Ion Ratio Lower Upper
43 100
58 26.5 22.2 33.2

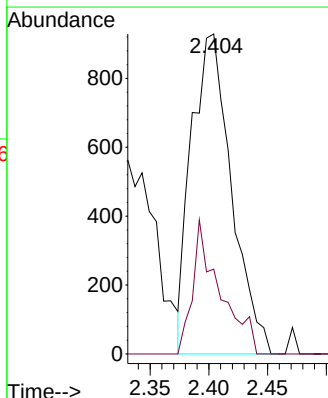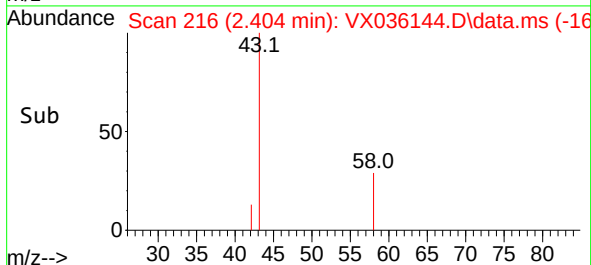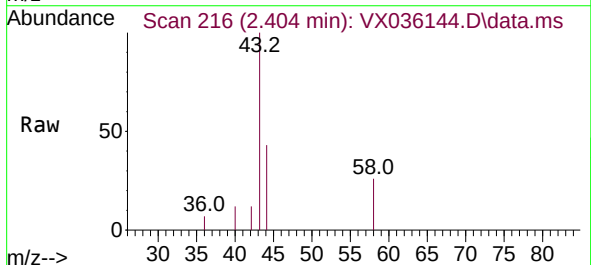



#31
Cyclohexane
Concen: 0.322 ug/l m
RT: 5.471 min Scan# 719
Delta R.T. 0.001 min
Lab File: VX036144.D
Acq: 13 Jun 2023 15:15




Instrument :
MSVOA_X
ClientSampleId :
MW-2A



Tgt Ion: 56 Resp: 110
Ion Ratio Lower Upper
56 100
69 19.4 25.9 38.9
84 83.2 67.6 101.4




Manual Integrations
APPROVED


Reviewed By :John Carlone 06/14/2023
Supervised By :Mahesh Dadoda 06/14/2023

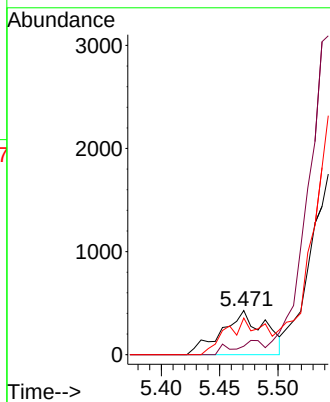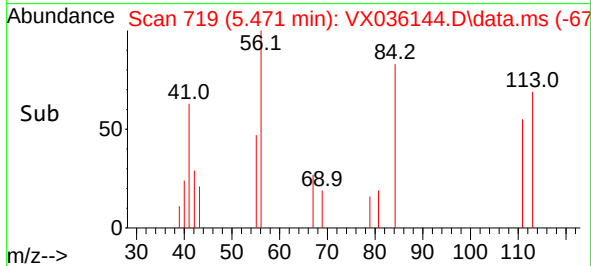

#33
1,2-Dichloroethane-d4
Concen: 48.512 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX036144.D
Acq: 13 Jun 2023 15:15

Tgt Ion: 65 Resp: 158586
Ion Ratio Lower Upper
65 100
67 49.7 0.0 99.6

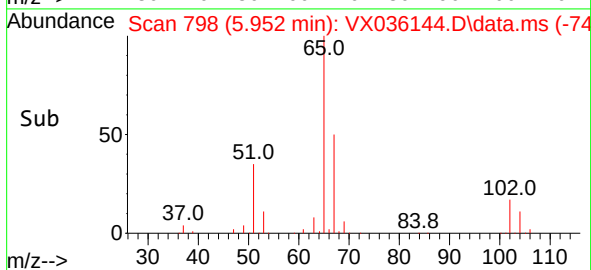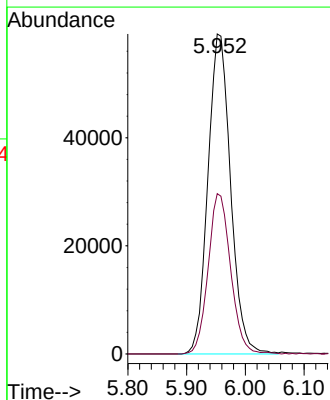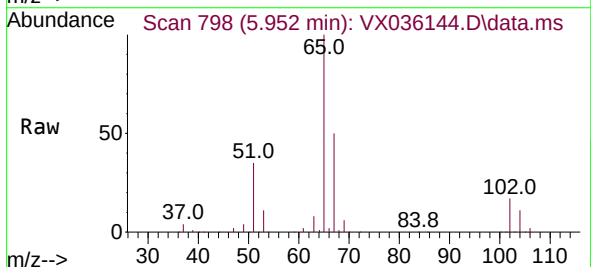

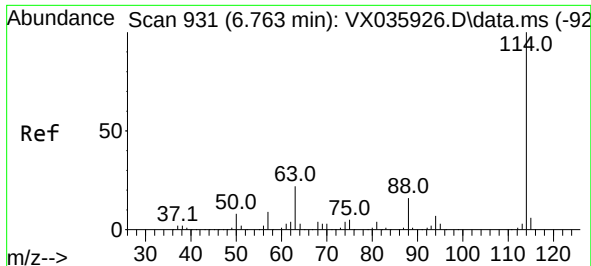





#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 914
Delta R.T. 0.000 min
Lab File: VX036144.D
Acq: 13 Jun 2023 15:15

Instrument :
MSVOA_X
ClientSampleId :
MW-2A

Tgt Ion:114 Resp: 332732
Ion Ratio Lower Upper
114 100
63 22.5 0.0 46.0
88 18.0 0.0 35.2




Manual Integrations
APPROVED


Reviewed By :John Carlone 06/14/2023
Supervised By :Mahesh Dadoda 06/14/2023

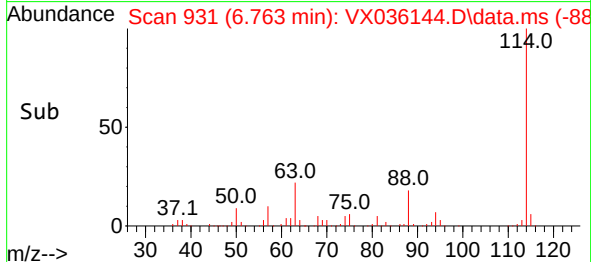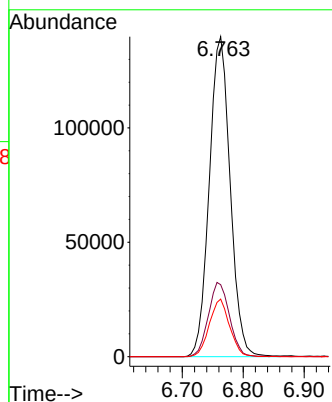

#35
Dibromofluoromethane
Concen: 47.010 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX036144.D
Acq: 13 Jun 2023 15:15


Tgt Ion:113 Resp: 105205
Ion Ratio Lower Upper
113 100
111 102.3 81.7 122.5
192 16.2 13.5 20.3

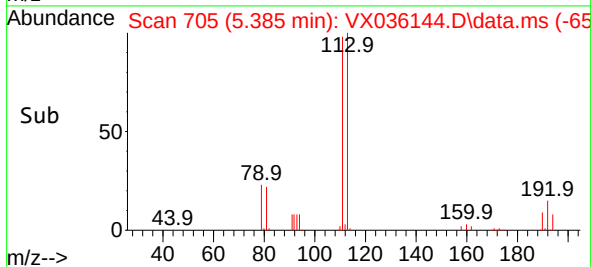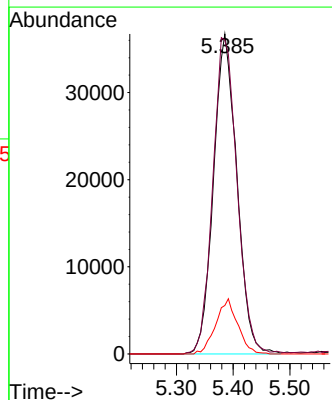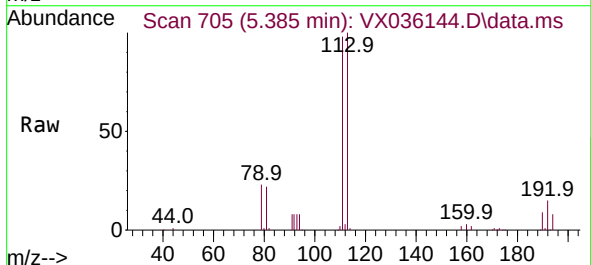

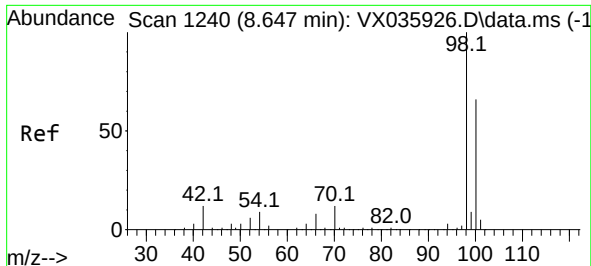

#50
Toluene-d8
Concen: 49.531 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.001 min
Lab File: VX036144.D
Acq: 13 Jun 2023 15:15




Instrument :
MSVOA_X
ClientSampleId :
MW-2A




Tgt Ion: 98 Resp: 397820
Ion Ratio Lower Upper
98 100
100 66.8 53.4 80.0

Manual Integrations
APPROVED



Reviewed By :John Carlone 06/14/2023
Supervised By :Mahesh Dadoda 06/14/2023

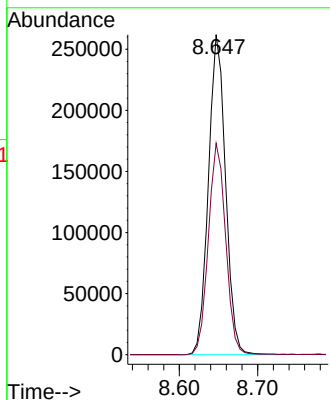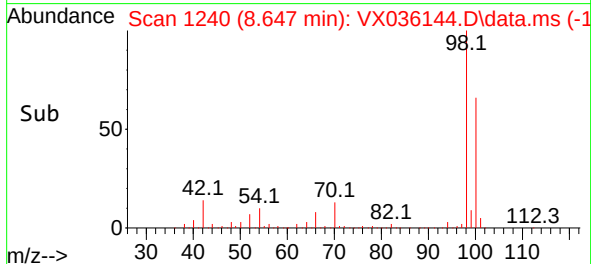


#62
4-Bromofluorobenzene
Concen: 48.945 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX036144.D
Acq: 13 Jun 2023 15:15

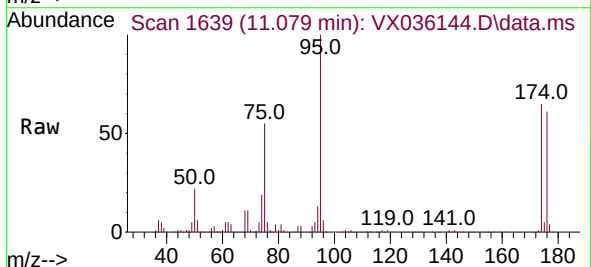


Tgt Ion: 95 Resp: 155187
Ion Ratio Lower Upper
95 100
174 66.8 0.0 132.6
176 63.8 0.0 128.0

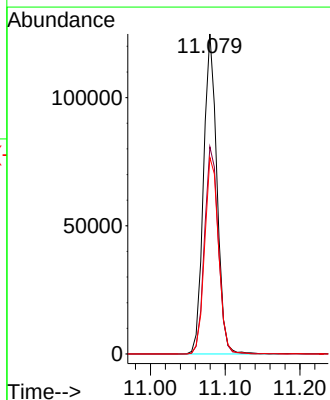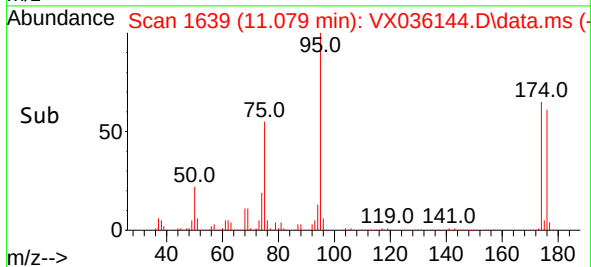



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX036144.D
Acq: 13 Jun 2023 15:15




Instrument :
MSVOA_X
ClientSampleId :
MW-2A




Tgt Ion:117 Resp: 298288
Ion Ratio Lower Upper
117 100
82 59.1 46.6 69.8
119 31.4 25.4 38.2

Manual Integrations
APPROVED



Reviewed By :John Carlone 06/14/2023
Supervised By :Mahesh Dadoda 06/14/2023

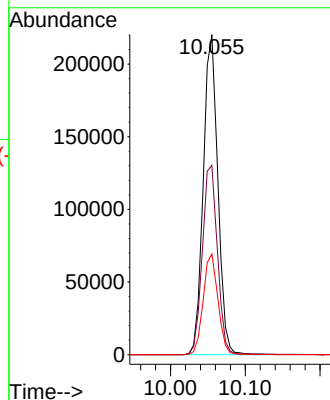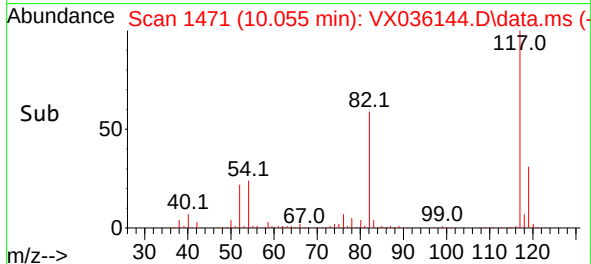


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX036144.D
Acq: 13 Jun 2023 15:15

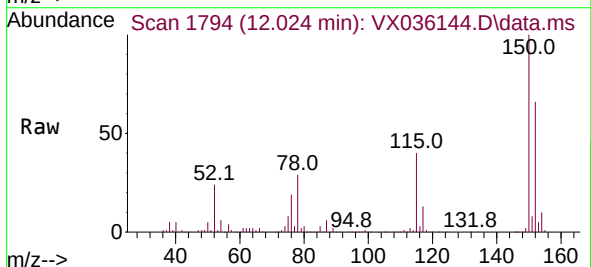


Tgt Ion:152 Resp: 138945
Ion Ratio Lower Upper
152 100
115 65.3 45.5 136.5
150 156.7 0.0 345.2

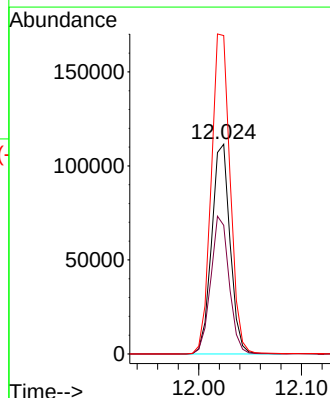



#85
 sec-Butylbenzene
 Concen: 0.286 ug/l
 RT: 11.890 min Scan# 1772
 Delta R.T. 0.000 min
 Lab File: VX036144.D
 Acq: 13 Jun 2023 15:15




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-2A




Tgt Ion:105 Resp: 2759
 Ion Ratio Lower Upper
 105 100
 134 19.4 9.7 28.9

Manual Integrations
 APPROVED

Reviewed By :John Carlone 06/14/2023
 Supervised By :Mahesh Dadoda 06/14/2023

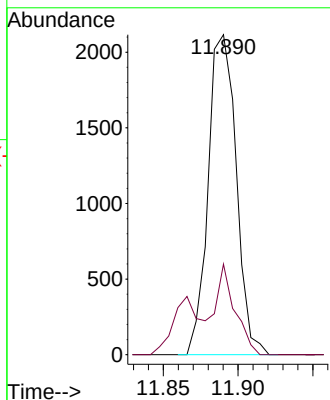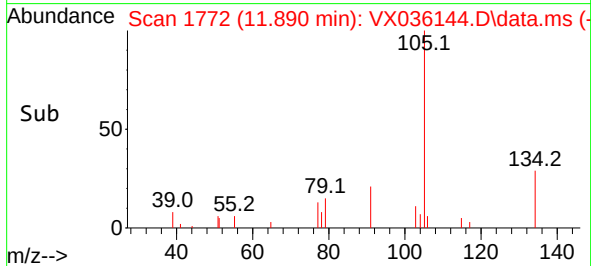

#91
 1,2-Dichlorobenzene
 Concen: 0.342 ug/l
 RT: 12.335 min Scan# 1845
 Delta R.T. 0.000 min
 Lab File: VX036144.D
 Acq: 13 Jun 2023 15:15

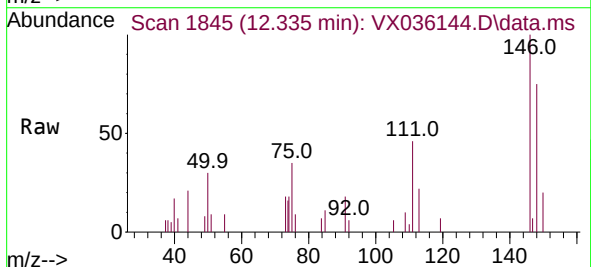

Tgt Ion:146 Resp: 1555
 Ion Ratio Lower Upper
 146 100
 111 49.8 23.3 69.9
 148 71.5 31.9 95.7

