

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061323\
 Data File : VX036149.D
 Acq On : 13 Jun 2023 17:13
 Operator : JC/MD
 Sample : 03170-01 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 AUD-1917

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053123W.M

Title : SW846 8260

Signal : TIC: VX036149.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.398	208	215	230	rBV	130857	312061	27.11%	4.763%
2	4.593	564	575	579	rBV3	5115	17185	1.49%	0.262%
3	5.385	694	705	719	rBV	123933	363035	31.53%	5.541%
4	5.550	721	732	748	rVB	252937	716345	62.22%	10.934%
5	5.952	788	798	815	rBV2	157266	423100	36.75%	6.458%
6	6.763	920	931	949	rBV	365739	874161	75.93%	13.343%
7	8.647	1233	1240	1248	rBV	755159	1151267	100.00%	17.573%
8	8.720	1248	1252	1262	rVB2	7481	13810	1.20%	0.211%
9	10.055	1465	1471	1482	rBV	732942	1001947	87.03%	15.294%
10	11.079	1634	1639	1649	rBV	570349	725124	62.98%	11.068%
11	12.018	1788	1793	1802	rBV	672988	866042	75.23%	13.219%
12	12.335	1838	1845	1850	rVB3	7681	12712	1.10%	0.194%
13	13.292	1993	2002	2006	rBV4	9712	18369	1.60%	0.280%
14	13.774	2077	2081	2087	rVB	14407	18742	1.63%	0.286%
15	14.231	2147	2156	2163	rVB3	11725	21312	1.85%	0.325%
16	14.481	2189	2197	2203	rBV4	9178	16071	1.40%	0.245%




Sum of corrected areas: 6551283

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061323\
Data File : VX036149.D
Acq On : 13 Jun 2023 17:13
Operator : JC/MD
Sample : 03170-01 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

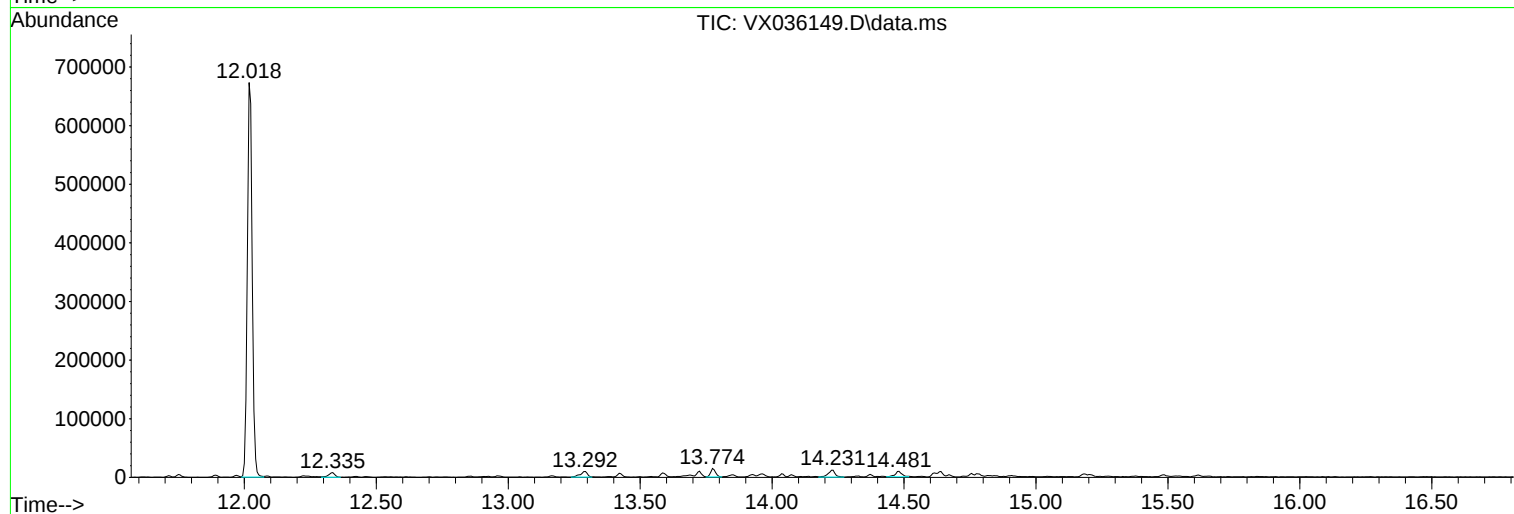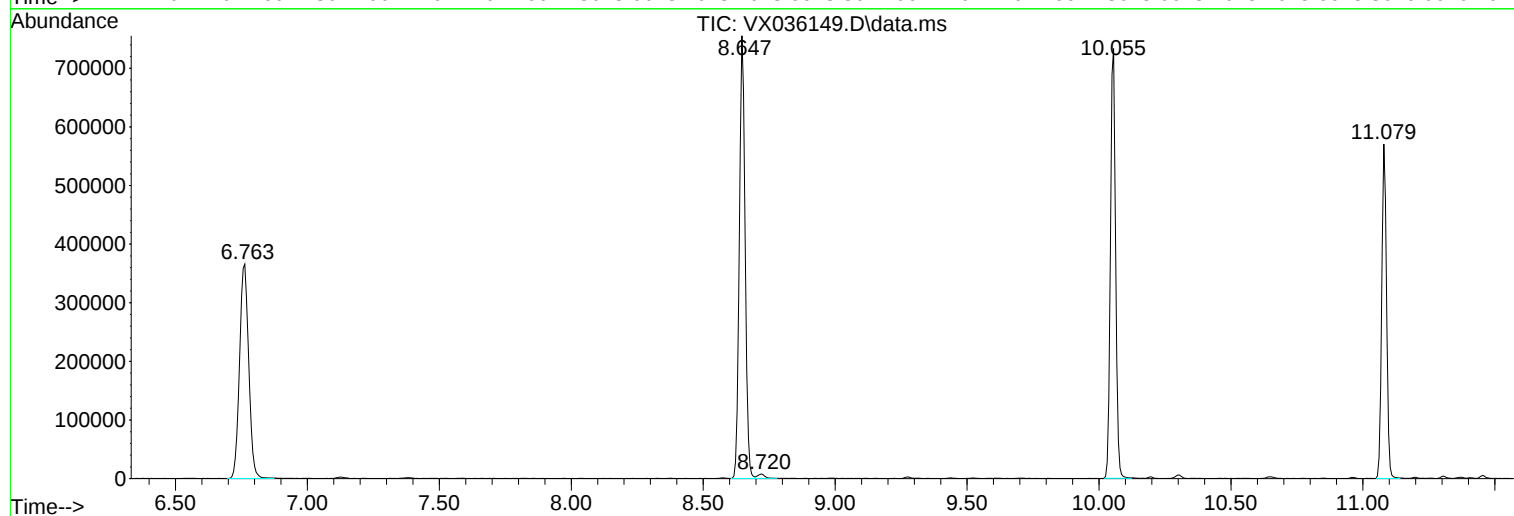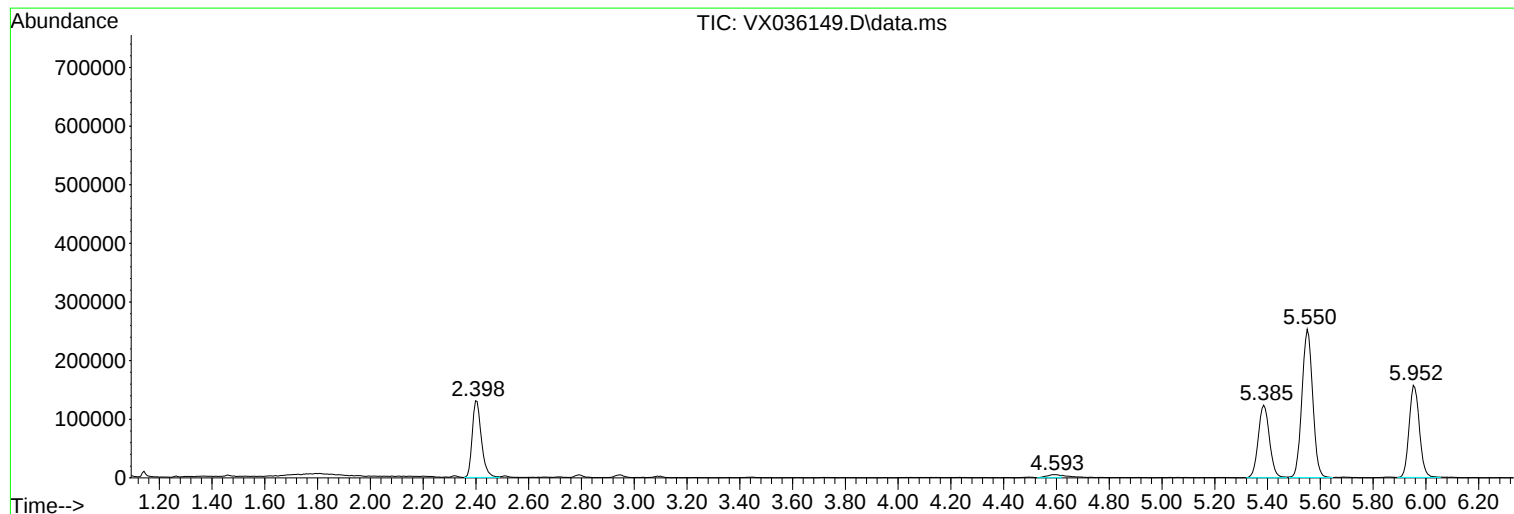

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061323\
Data File : VX036149.D
Acq On : 13 Jun 2023 17:13
Operator : JC/MD
Sample : 03170-01 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061323\
Data File : VX036149.D
Acq On : 13 Jun 2023 17:13
Operator : JC/MD
Sample : 03170-01 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------