


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061323\
Data File : VX036130.D
Acq On : 13 Jun 2023 08:28
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053123W.M
Title : SW846 8260
Last Update : Wed May 31 12:50:30 2023

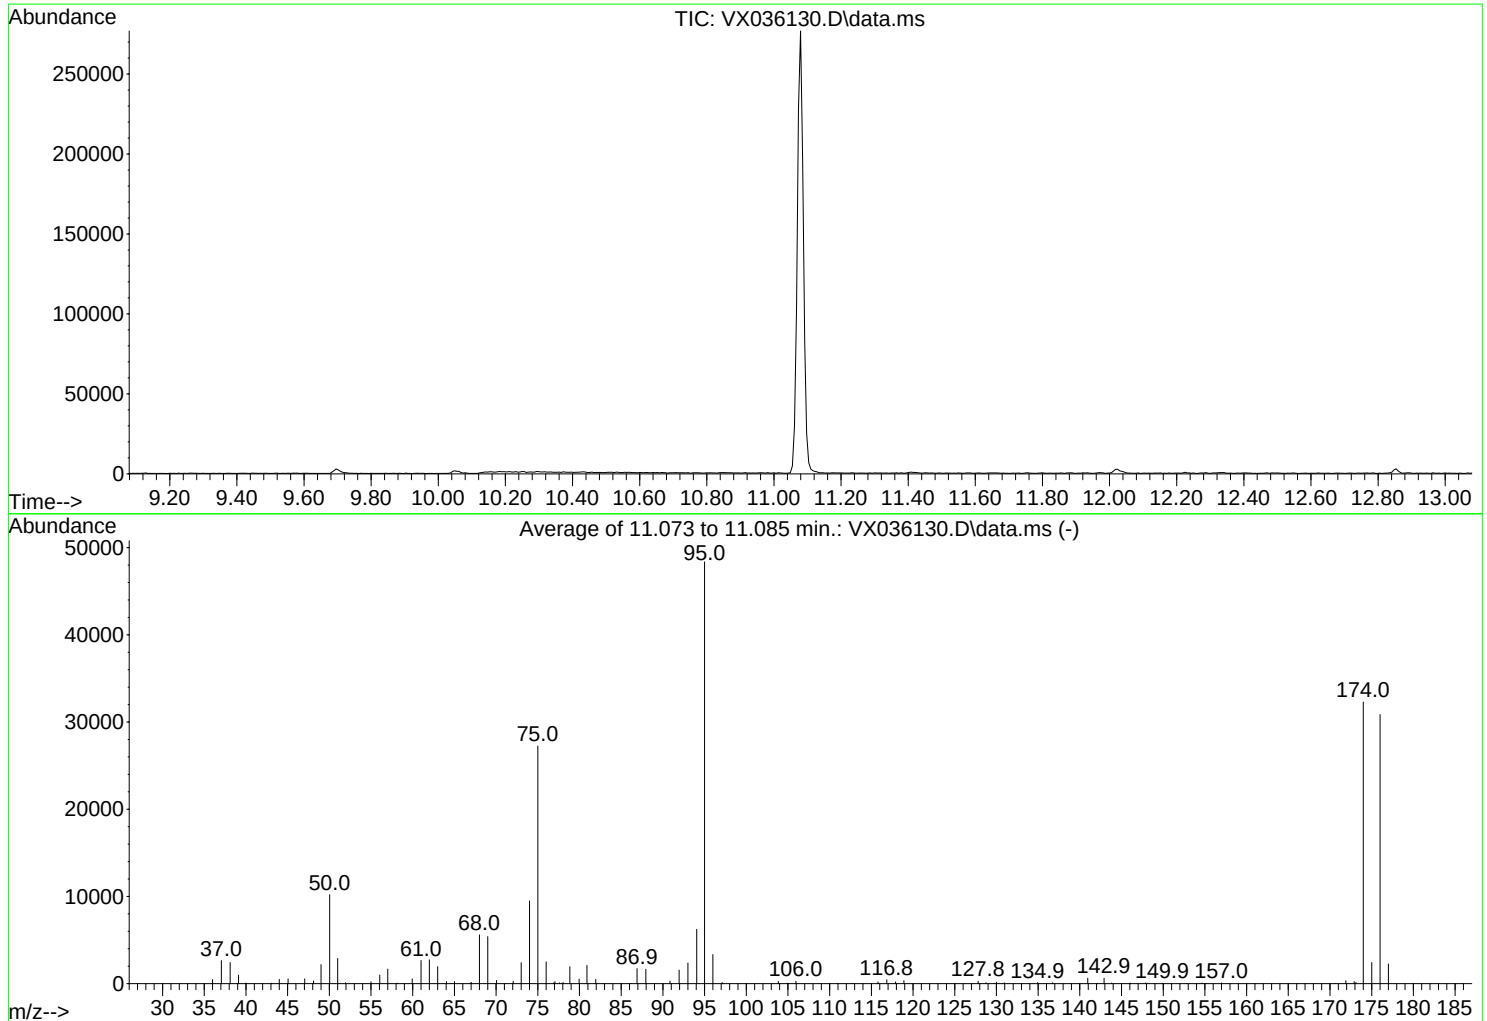

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.1	10213	PASS
75	95	30	60	56.3	27256	PASS
95	95	100	100	100.0	48376	PASS
96	95	5	9	6.9	3337	PASS
173	174	0.00	2	0.7	242	PASS
174	95	50	100	66.8	32299	PASS
175	174	5	9	7.5	2421	PASS
176	174	95	101	95.6	30869	PASS
177	176	5	9	7.3	2263	PASS