

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061324\
 Data File : VX041844.D
 Acq On : 13 Jun 2024 11:25
 Operator : JC/MD
 Sample : PB161467TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jun 14 00:54:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 30 07:36:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	166828	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.757	114	261909	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	258872	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	127111	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	87361	42.697	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	85.400%
35) Dibromofluoromethane	5.385	113	79676	44.000	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	88.000%
50) Toluene-d8	8.647	98	310542	49.080	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.160%
62) 4-Bromofluorobenzene	11.079	95	116499	49.887	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.780%
Target Compounds						
						Qvalue
3) Chloromethane	1.294	50	357	0.223	ug/l	# 43
5) Bromomethane	1.599	94	682	0.595	ug/l	94
11) Tert butyl alcohol	3.013	59	831	2.296	ug/l	# 78
13) Acrolein	2.233	56	151	0.448	ug/l	# 47
14) Allyl chloride	2.648	41	1580	0.646	ug/l	# 41
15) Acrylonitrile	3.080	53	203	0.229	ug/l	# 77
16) Acetone	2.392	43	86298	94.298	ug/l	90
18) Methyl Acetate	2.709	43	2603	1.332	ug/l	96
20) Methylene Chloride	2.788	84	9505	5.191	ug/l	88
25) 2-Butanone	4.574	43	21488	16.898	ug/l	98
29) Tetrahydrofuran	5.019	42	3471	4.328	ug/l	94
31) Cyclohexane	5.537	56	2470	1.022	ug/l	# 1
36) 1,1-Dichloropropene	5.543	75	9902	4.516	ug/l	# 51
37) Ethyl Acetate	4.726	43	677	0.245	ug/l	# 69
38) Carbon Tetrachloride	5.550	117	14209	5.704	ug/l	# 17
41) Methacrylonitrile	5.031	41	2016	1.490	ug/l	# 47
43) Isopropyl Acetate	6.342	43	121596	29.105	ug/l	95
48) Methyl methacrylate	7.616	41	4153	2.070	ug/l	# 16
49) 1,4-Dioxane	7.689	88	114	2.601	ug/l	# 1
51) 4-Methyl-2-Pentanone	8.549	43	99642	36.780	ug/l	# 47
53) t-1,3-Dichloropropene	8.957	75	991	0.435	ug/l	# 43
54) cis-1,3-Dichloropropene	8.549	75	46388	18.408	ug/l	# 52
57) 1,3-Dichloropropane	9.482	76	6580	2.261	ug/l	# 42
59) 2-Hexanone	9.482	43	82022	39.712	ug/l	# 55
74) N-amyl acetate	10.640	43	26422	7.565	ug/l	# 54
76) 1,2,3-Trichloropropane	11.079	75	53711	24.218	ug/l	# 39
81) trans-1,4-Dichloro-2-b...	11.079	75	53711	66.006	ug/l	# 5
93) 1,2,4-Trichlorobenzene	13.597	180	736	0.264	ug/l	92
95) Naphthalene	13.780	128	3038	0.369	ug/l	96
96) 1,2,3-Trichlorobenzene	13.963	180	794	0.276	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061324\
Data File : VX041844.D
Acq On : 13 Jun 2024 11:25
Operator : JC/MD
Sample : PB161467TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jun 14 00:54:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
Quant Title : SW846 8260
QLast Update : Thu May 30 07:36:24 2024
Response via : Initial Calibration

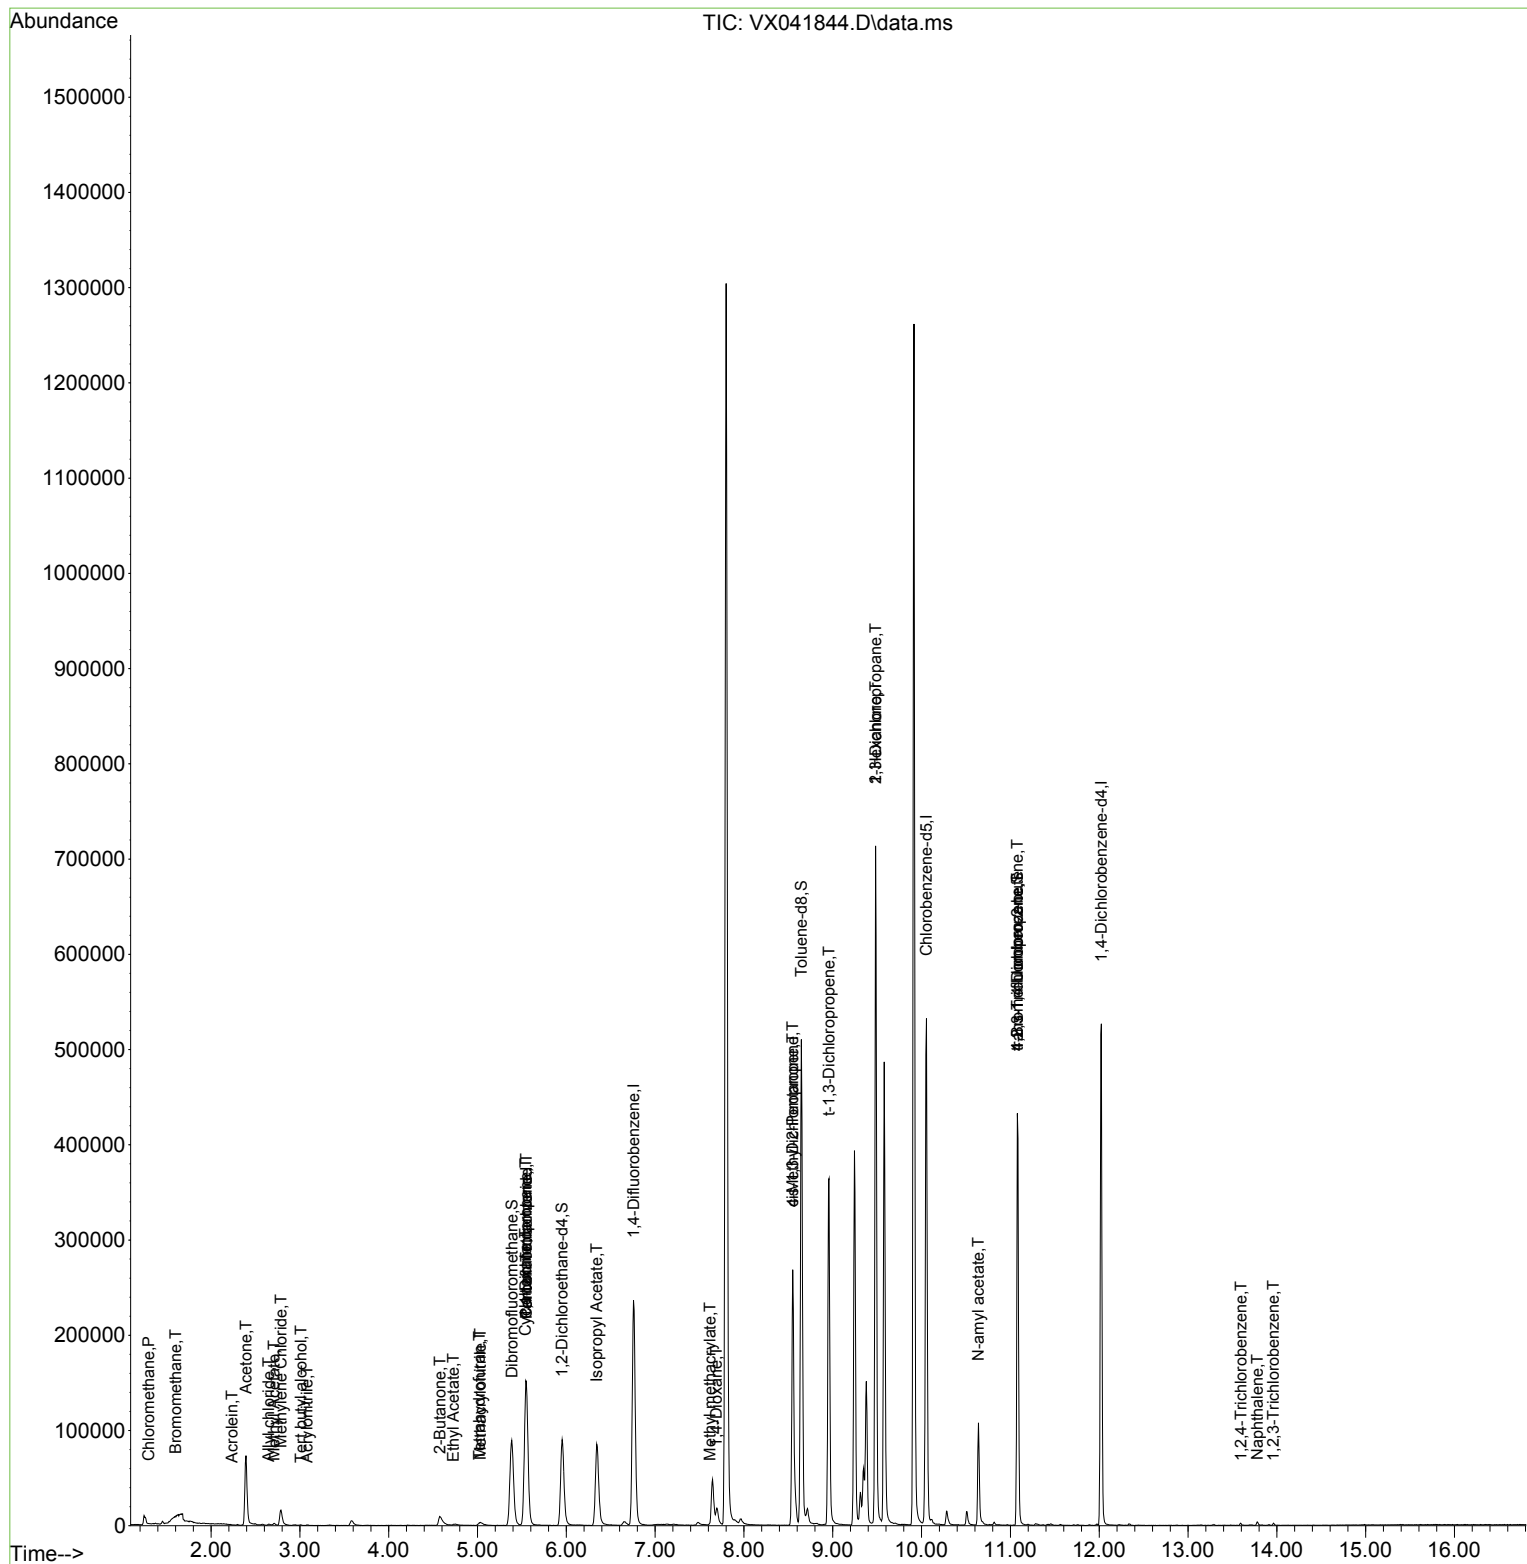



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.550 min Scan# 71

Delta R.T. -0.000 min

Lab File: VX041844.D

Acq: 13 Jun 2024 11:25

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:168 Resp: 166828

Ion Ratio Lower Upper

168 100

99 49.0 56.6 85.0#

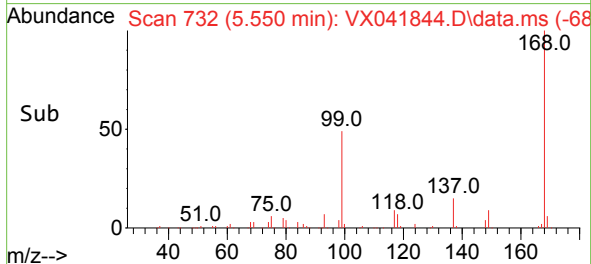

#3

Chloromethane

Concen: 0.223 ug/l

RT: 1.294 min Scan# 34

Delta R.T. -0.006 min

Lab File: VX041844.D




Acq: 13 Jun 2024 11:25


Tgt Ion: 50 Resp: 357

Ion Ratio Lower Upper

50 100


52 0.0 25.5 38.3#

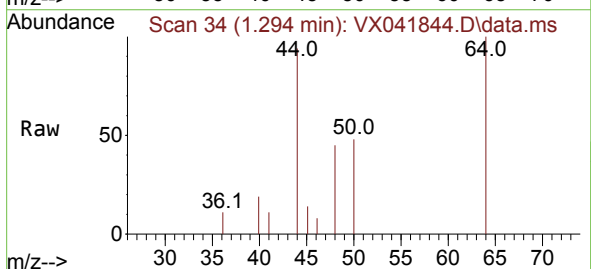



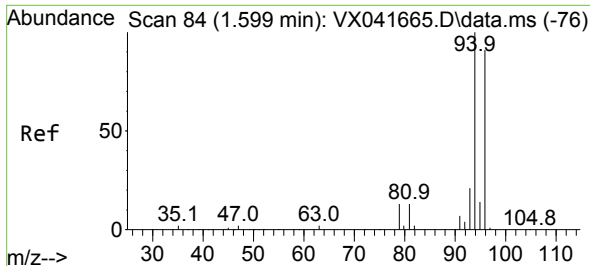


#5
Bromomethane
Concen: 0.595 ug/l
RT: 1.599 min Scan# 84
Delta R.T. -0.000 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25

Instrument :
MSVOA_X
ClientSampleId :



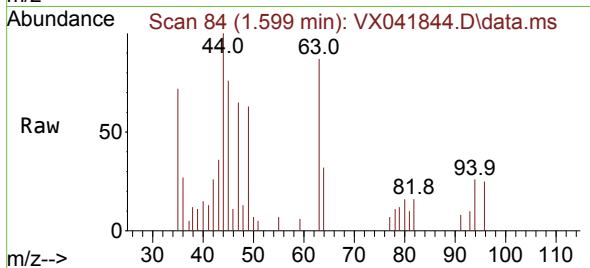



Tgt Ion: 94 Resp: 682
Ion Ratio Lower Upper
94 100
96 99.0 74.6 111.8

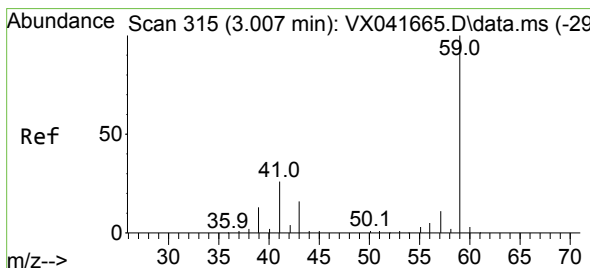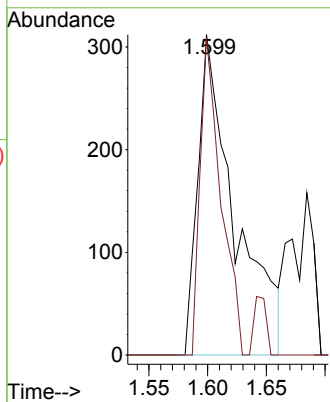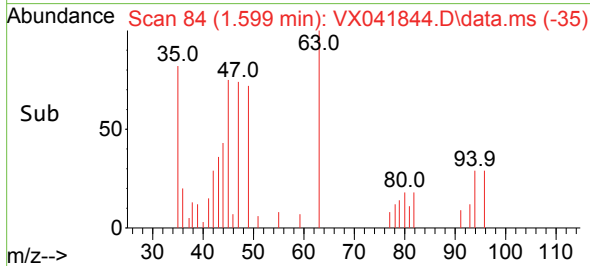

#11
Tert butyl alcohol
Concen: 2.296 ug/l
RT: 3.013 min Scan# 316
Delta R.T. 0.006 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25

Tgt Ion: 59 Resp: 831
Ion Ratio Lower Upper
59 100
57 0.0 6.0 9.0#

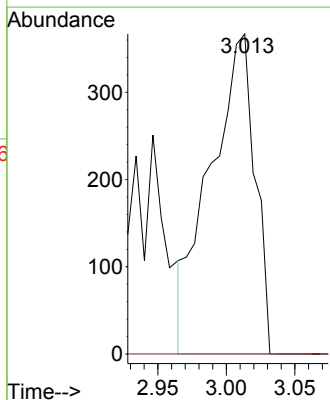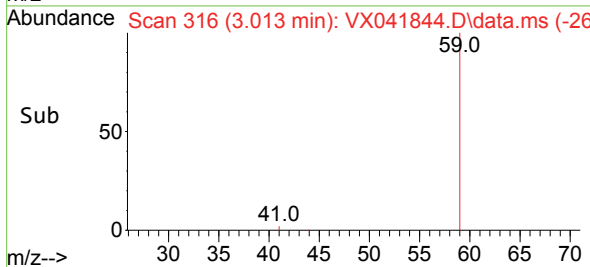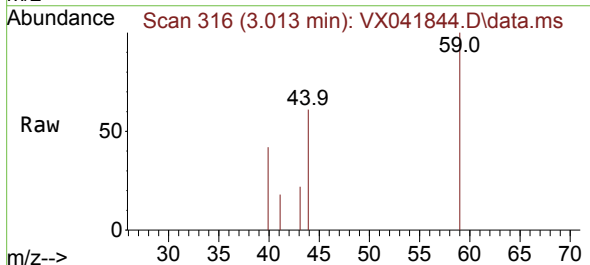



#13

Acrolein

Concen: 0.448 ug/l

RT: 2.233 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX041844.D

Acq: 13 Jun 2024 11:25

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 56 Resp: 151

Ion Ratio Lower Upper

56 100

55 27.8 57.1 85.7#

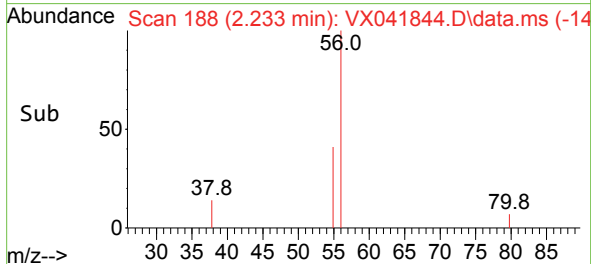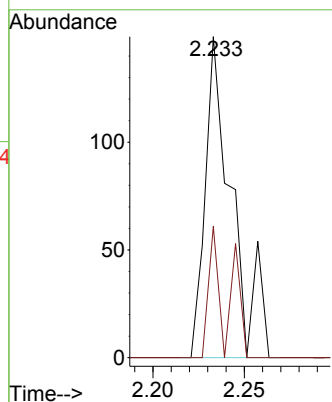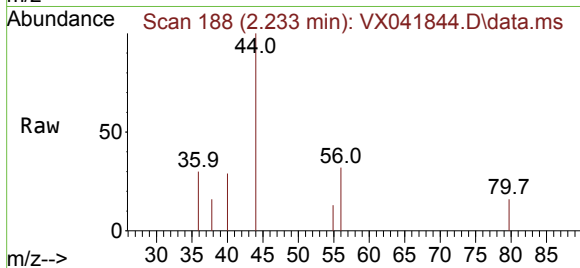

#14

Allyl chloride

Concen: 0.646 ug/l

RT: 2.648 min Scan# 256

Delta R.T. -0.012 min

Lab File: VX041844.D

Acq: 13 Jun 2024 11:25




Tgt Ion: 41 Resp: 1580


Ion Ratio Lower Upper

41 100

39 20.1 55.8 83.6#


76 0.0 24.3 36.5#

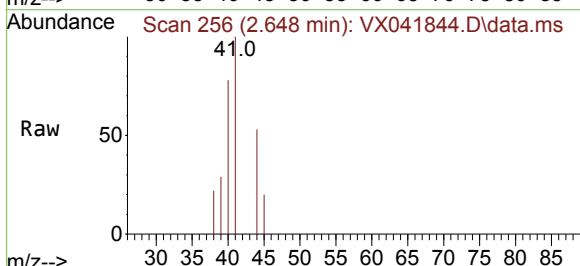






#15
Acrylonitrile
Concen: 0.229 ug/l
RT: 3.080 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 53 Resp: 203
Ion Ratio Lower Upper
53 100
52 86.7 66.0 99.0
51 0.0 29.8 44.6#

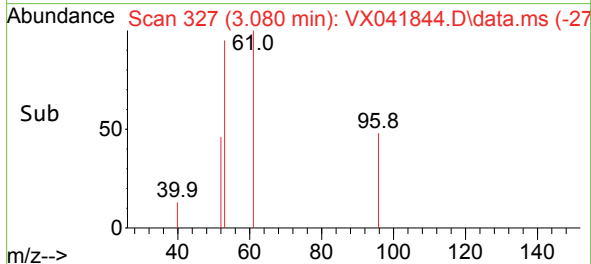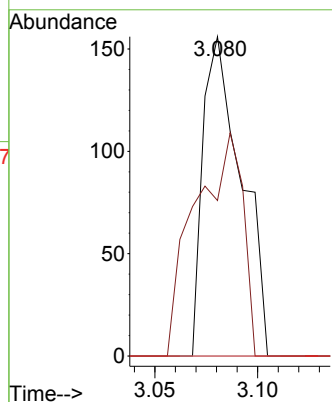

#16
Acetone
Concen: 94.298 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25

Tgt Ion: 43 Resp: 86298
Ion Ratio Lower Upper
43 100
58 32.4 21.9 32.9


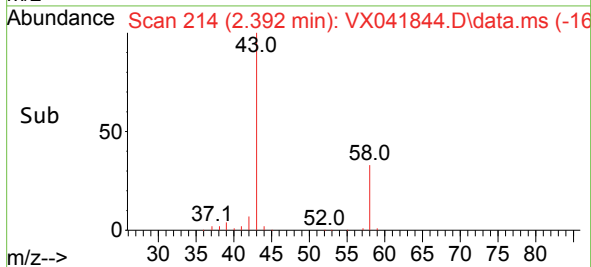
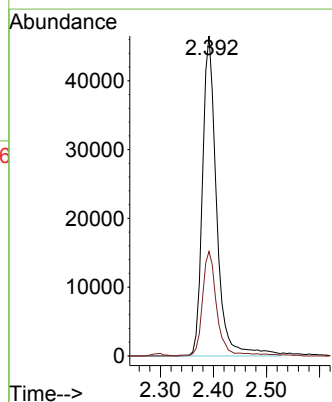
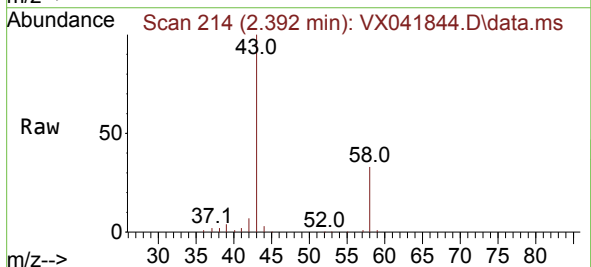




#18
Methyl Acetate
Concen: 1.332 ug/l
RT: 2.709 min Scan# 266
Delta R.T. -0.000 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 2603
Ion Ratio Lower Upper
43 100
74 20.5 17.8 26.8

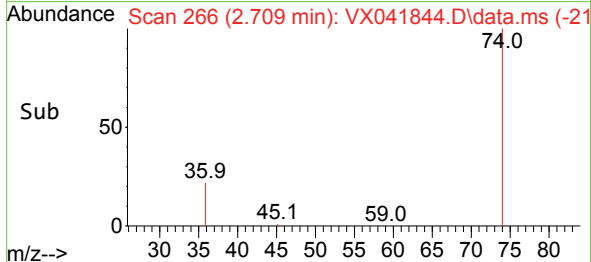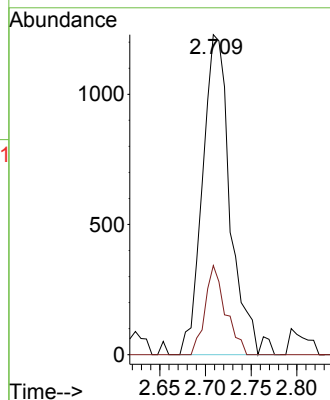

#20
Methylene Chloride
Concen: 5.191 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25

Tgt Ion: 84 Resp: 9505
Ion Ratio Lower Upper
84 100
49 113.5 103.6 155.4
51 33.8 33.8 50.6
86 67.2 49.4 74.0


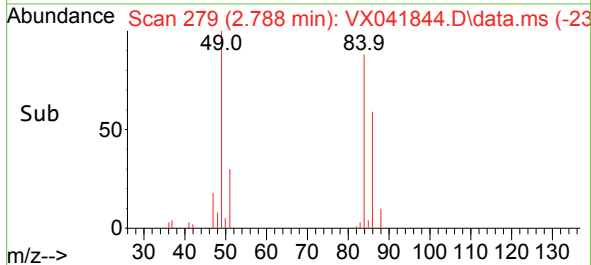
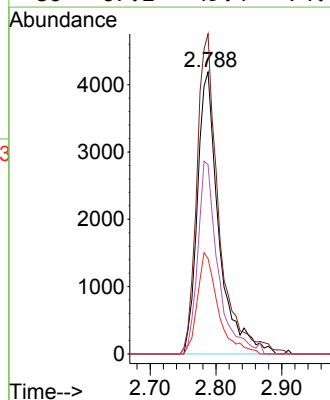
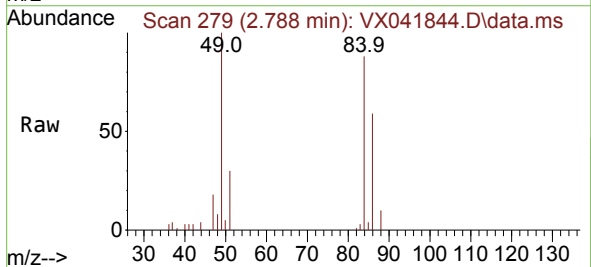


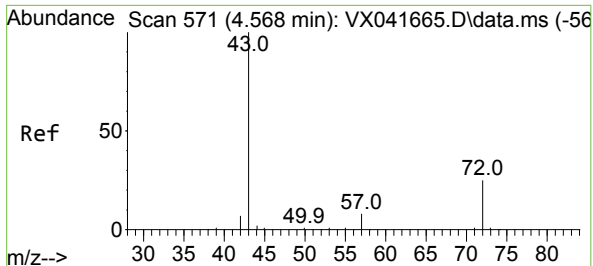

#25
2-Butanone
Concen: 16.898 ug/l
RT: 4.574 min Scan# 51
Delta R.T. 0.006 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 21488
Ion Ratio Lower Upper
43 100
72 25.1 19.4 29.2

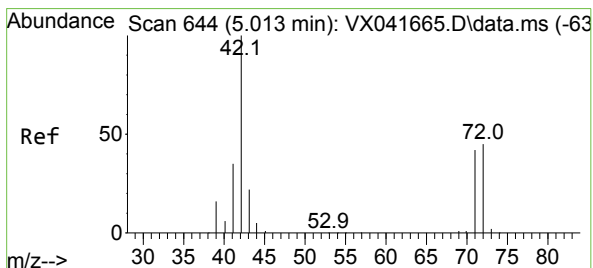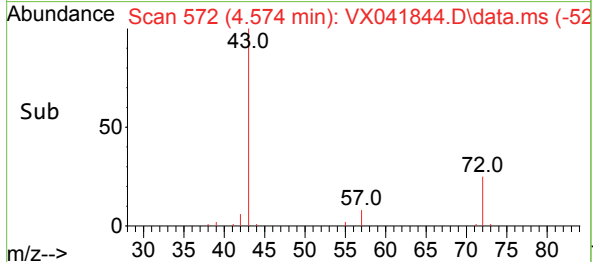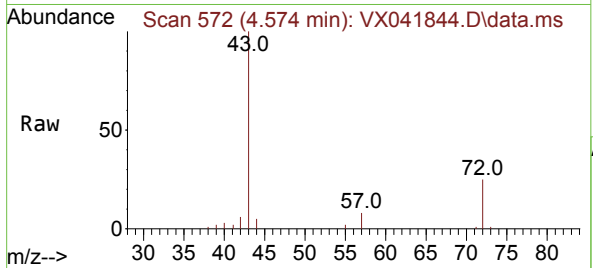

#29
Tetrahydrofuran
Concen: 4.328 ug/l
RT: 5.019 min Scan# 645
Delta R.T. 0.006 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25


Tgt Ion: 42 Resp: 3471
Ion Ratio Lower Upper
42 100
72 49.7 34.2 51.4
71 41.2 32.2 48.2

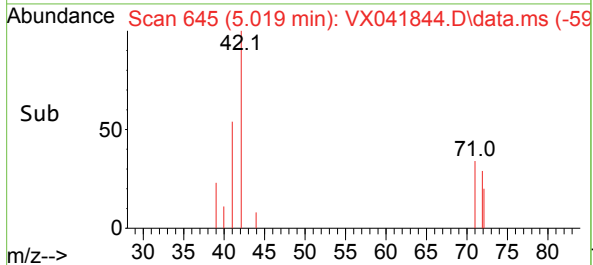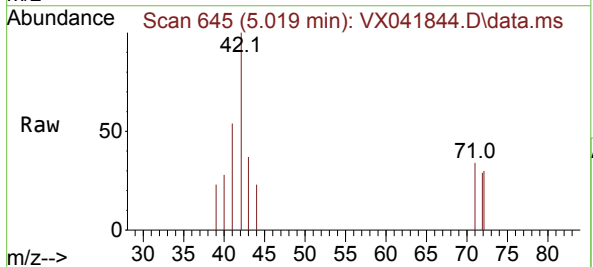



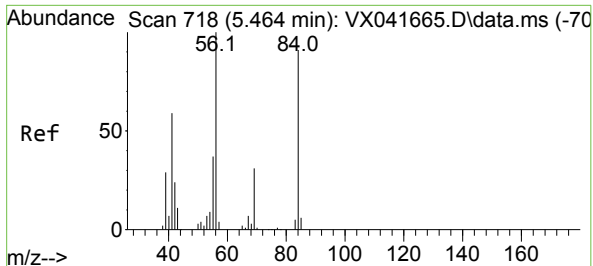


#31
Cyclohexane
Concen: 1.022 ug/l
RT: 5.537 min Scan# 718
Delta R.T. 0.073 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25

Instrument :
MSVOA_X
ClientSampleId :



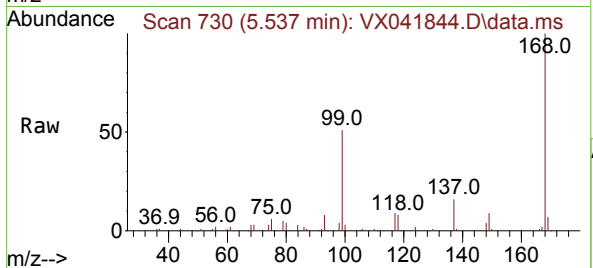



Tgt Ion: 56 Resp: 2470
Ion Ratio Lower Upper
56 100
69 172.2 23.4 35.2#
84 146.8 65.9 98.9#

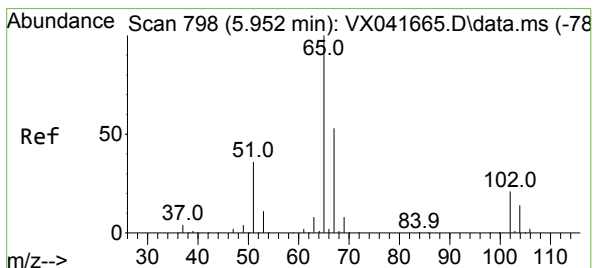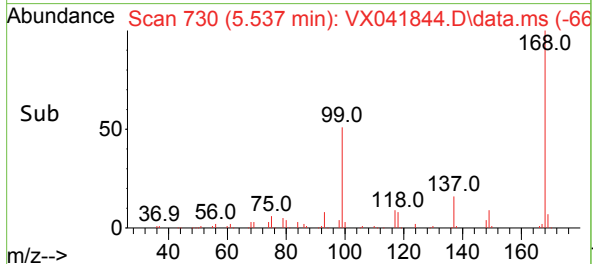

#33
1,2-Dichloroethane-d4
Concen: 42.697 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25

Tgt Ion: 65 Resp: 87361
Ion Ratio Lower Upper
65 100
67 53.5 0.0 100.2


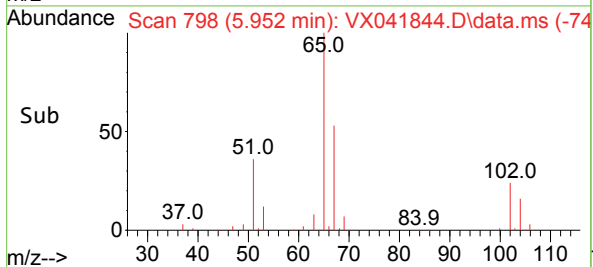

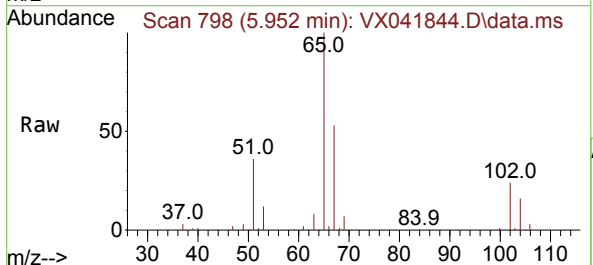




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 261909
Ion Ratio Lower Upper
114 100
63 18.9 0.0 45.0
88 15.0 0.0 36.6

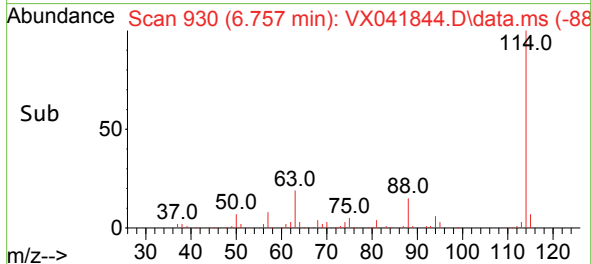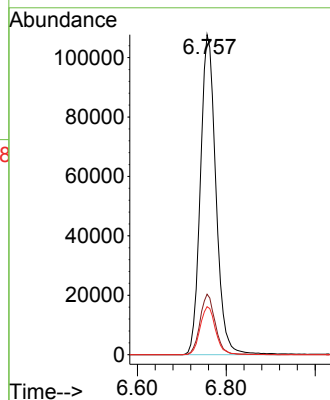

#35
Dibromofluoromethane
Concen: 44.000 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25

Tgt Ion:113 Resp: 79676
Ion Ratio Lower Upper
113 100
111 103.7 82.9 124.3
192 25.4 13.3 19.9#



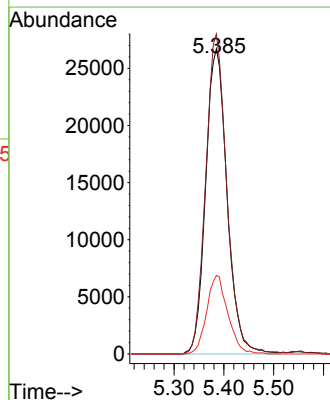
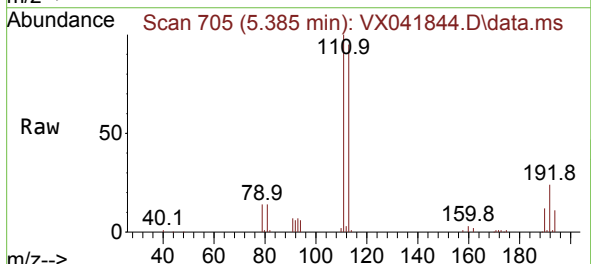




#36
1,1-Dichloropropene
Concen: 4.516 ug/l
RT: 5.543 min Scan# 71
Delta R.T. -0.146 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 9902
Ion Ratio Lower Upper
75 100
110 9.2 17.0 50.9#
77 0.0 24.7 37.1#

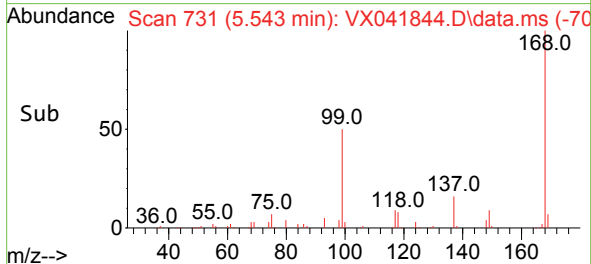

#37
Ethyl Acetate
Concen: 0.245 ug/l
RT: 4.726 min Scan# 597
Delta R.T. 0.006 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25


Tgt Ion: 43 Resp: 677
Ion Ratio Lower Upper
43 100
61 0.0 10.6 16.0#
70 0.0 8.3 12.5#

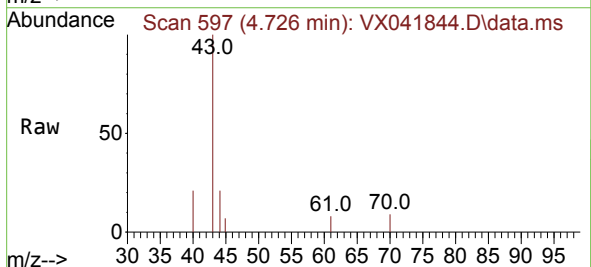






#38
Carbon Tetrachloride
Concen: 5.704 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 14209
Ion Ratio Lower Upper
117 100
119 7.4 78.2 117.2#
121 0.0 24.4 36.6#

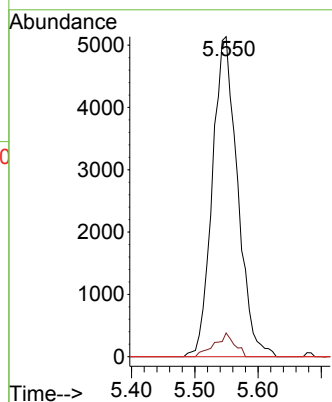

#41
Methacrylonitrile
Concen: 1.490 ug/l
RT: 5.031 min Scan# 647
Delta R.T. 0.110 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25

Tgt Ion: 41 Resp: 2016
Ion Ratio Lower Upper
41 100
39 44.2 45.2 67.8#
67 0.0 52.6 78.8#
52 0.0 22.7 34.1#


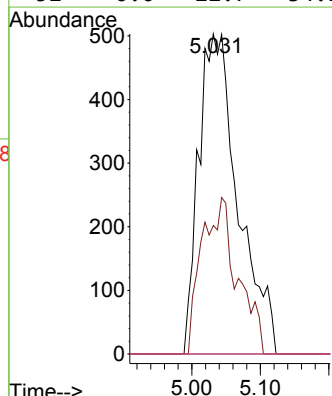






#43
Isopropyl Acetate
Concen: 29.105 ug/l
RT: 6.342 min Scan# 862
Delta R.T. -0.000 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 121596
Ion Ratio Lower Upper
43 100
61 21.0 15.2 22.8
87 14.4 9.8 14.6

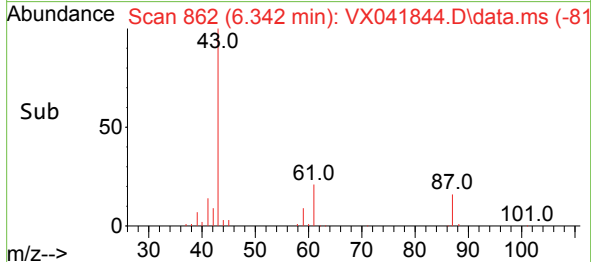

#48
Methyl methacrylate
Concen: 2.070 ug/l
RT: 7.616 min Scan# 1071
Delta R.T. -0.079 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25


Tgt Ion: 41 Resp: 4153
Ion Ratio Lower Upper
41 100
69 0.0 59.2 88.8#
39 0.0 47.7 71.5#

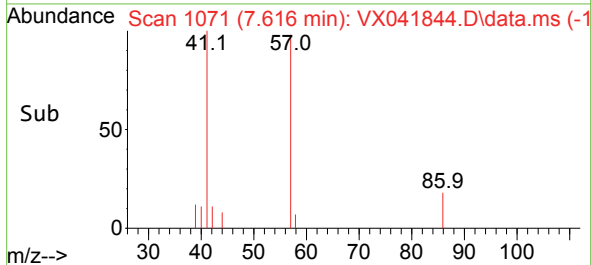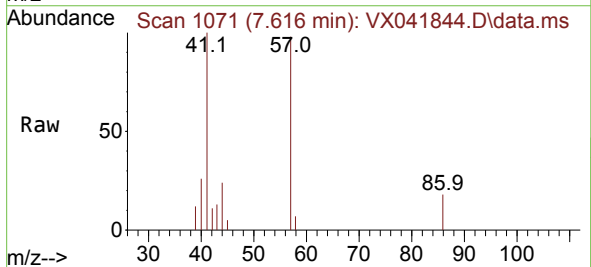






#49
1,4-Dioxane
Concen: 2.601 ug/l
RT: 7.689 min Scan# 1083
Delta R.T. 0.018 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 88 Resp: 114
Ion Ratio Lower Upper
88 100
43 0.0 0.0 0.0
58 631.6 60.1 90.1#



#50
Toluene-d8
Concen: 49.080 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25

Tgt Ion: 98 Resp: 310542
Ion Ratio Lower Upper
98 100
100 66.5 53.1 79.7


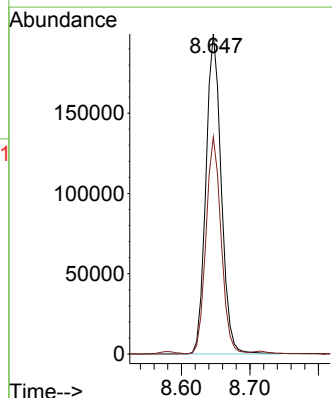

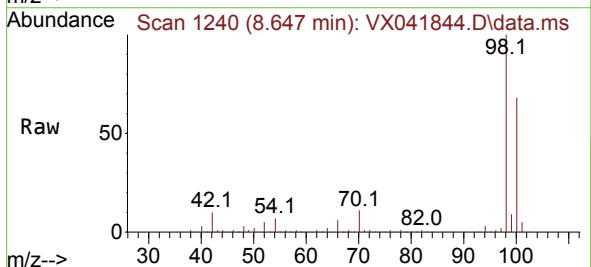




#51
4-Methyl-2-Pentanone
Concen: 36.780 ug/l
RT: 8.549 min Scan# 11
Delta R.T. -0.031 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 99642
Ion Ratio Lower Upper
43 100
58 5.8 30.4 45.6#

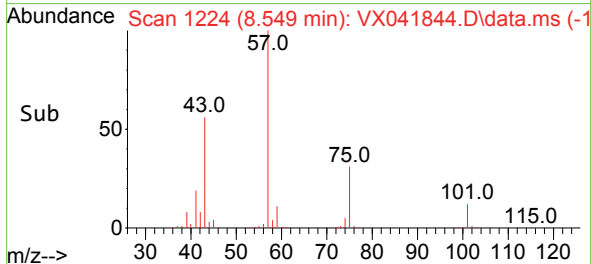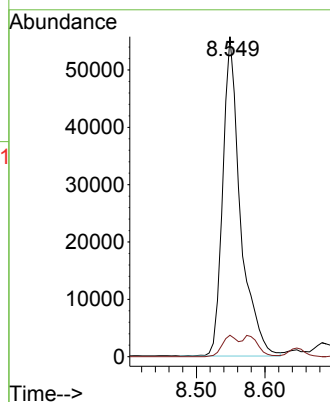

#53
t-1,3-Dichloropropene
Concen: 0.435 ug/l
RT: 8.957 min Scan# 1291
Delta R.T. -0.018 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25

Tgt Ion: 75 Resp: 991
Ion Ratio Lower Upper
75 100
77 0.0 25.7 38.5#



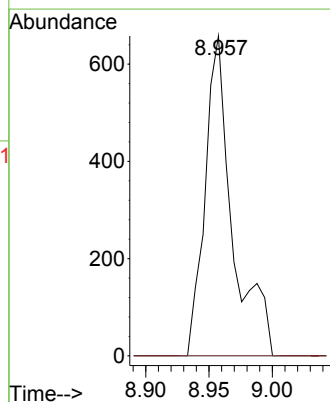
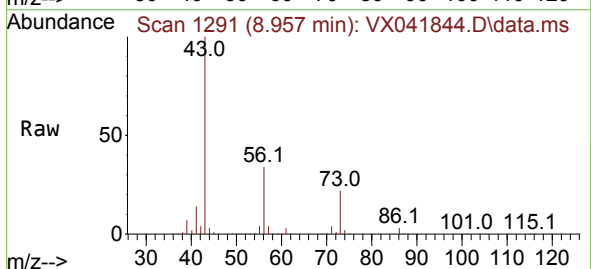




#54
 cis-1,3-Dichloropropene
 Concen: 18.408 ug/l
 RT: 8.549 min Scan# 1194
 Delta R.T. 0.183 min
 Lab File: VX041844.D
 Acq: 13 Jun 2024 11:25




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 75 Resp: 46388
 Ion Ratio Lower Upper
 75 100
 77 0.5 25.3 37.9#
 39 25.7 46.7 70.1#

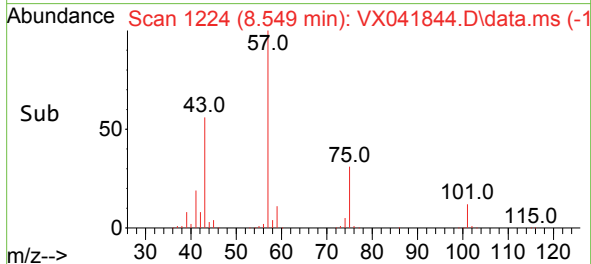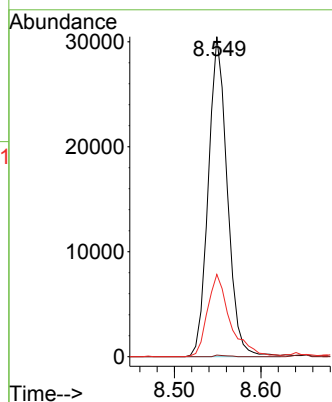

#57
 1,3-Dichloropropane
 Concen: 2.261 ug/l
 RT: 9.482 min Scan# 1377
 Delta R.T. 0.177 min
 Lab File: VX041844.D
 Acq: 13 Jun 2024 11:25

Tgt Ion: 76 Resp: 6580
 Ion Ratio Lower Upper
 76 100
 78 0.0 26.1 39.1#




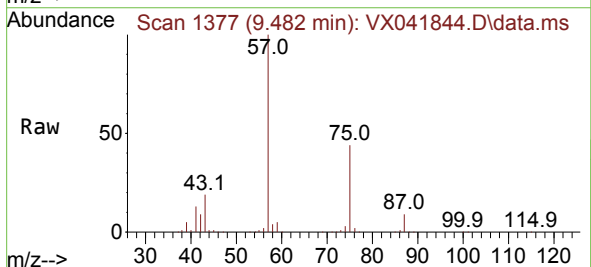




#59
2-Hexanone
Concen: 39.712 ug/l
RT: 9.482 min Scan# 11
Delta R.T. 0.049 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 82022
Ion Ratio Lower Upper
43 100
58 20.3 26.2 78.5#

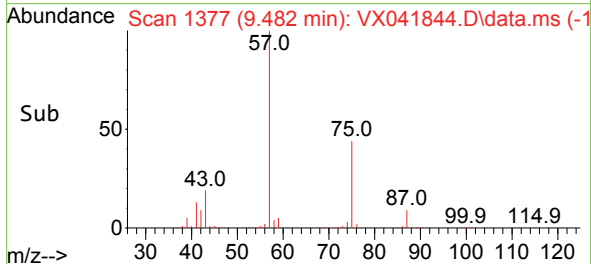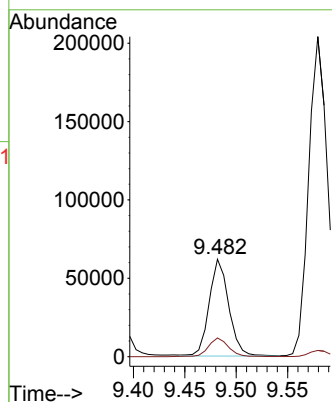

#62
4-Bromofluorobenzene
Concen: 49.887 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25

Tgt Ion: 95 Resp: 116499
Ion Ratio Lower Upper
95 100
174 97.0 0.0 135.6
176 94.8 0.0 131.0




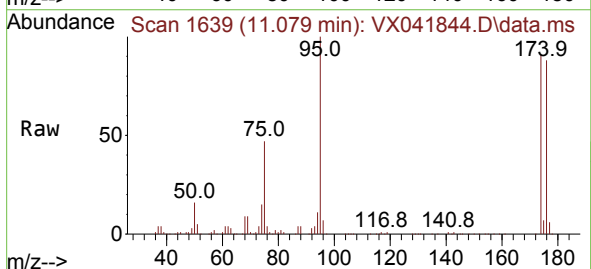




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 258872
Ion Ratio Lower Upper
117 100
82 50.5 46.2 69.4
119 32.2 25.5 38.3

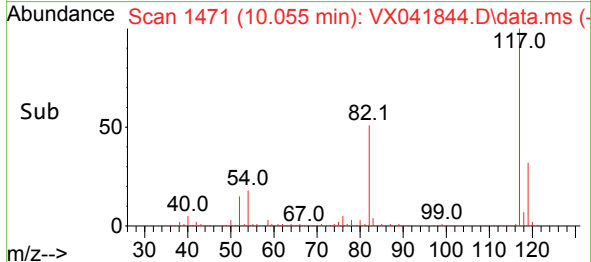

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25

Tgt Ion:152 Resp: 127111
Ion Ratio Lower Upper
152 100
115 53.9 43.3 129.9
150 156.8 0.0 345.0

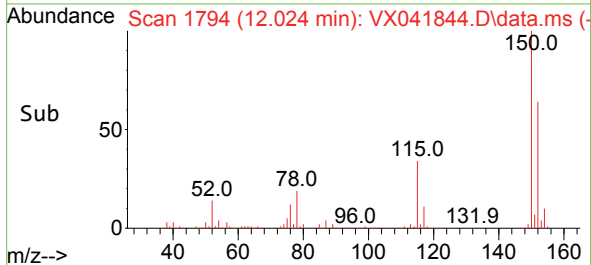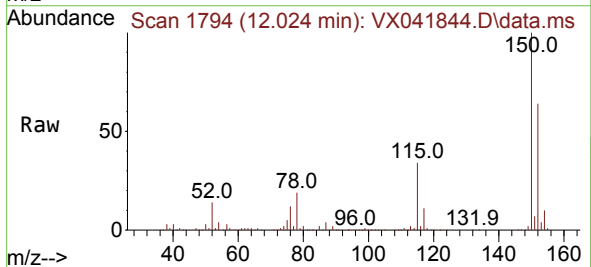



#74

N-amy1 acetate

Concen: 7.565 ug/l

RT: 10.640 min Scan# 1639

Delta R.T. -0.201 min


Lab File: VX041844.D

Acq: 13 Jun 2024 11:25

Instrument :

MSVOA_X

ClientSampleId :



Tgt Ion: 43 Resp: 26422




Ion Ratio Lower Upper

43 100

70 1.9 32.9 49.3#

55 4.7 19.3 28.9#

61 11.7 18.8 28.2#



#76

1,2,3-Trichloropropane

Concen: 24.218 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX041844.D




Acq: 13 Jun 2024 11:25


Tgt Ion: 75 Resp: 53711

Ion Ratio Lower Upper

75 100

77 1.4 19.1 57.5#









#81
trans-1,4-Dichloro-2-butene
Concen: 66.006 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 53711
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

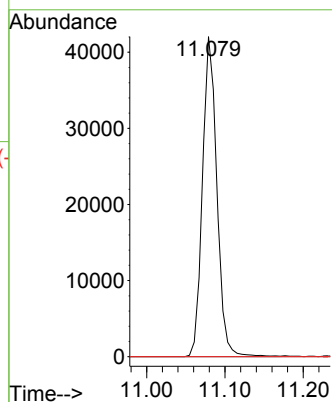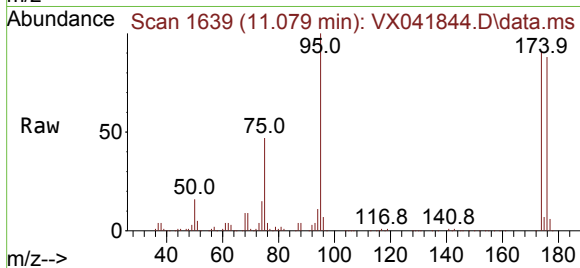

#93
1,2,4-Trichlorobenzene
Concen: 0.264 ug/l
RT: 13.597 min Scan# 2052
Delta R.T. 0.012 min
Lab File: VX041844.D
Acq: 13 Jun 2024 11:25

Tgt Ion:180 Resp: 736
Ion Ratio Lower Upper
180 100
182 99.7 48.3 144.8
145 24.6 18.0 54.0

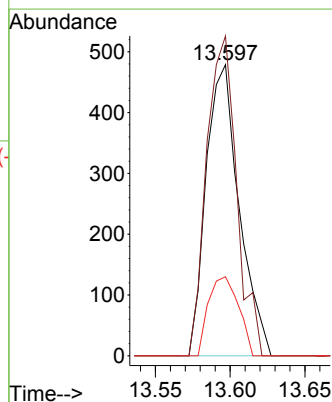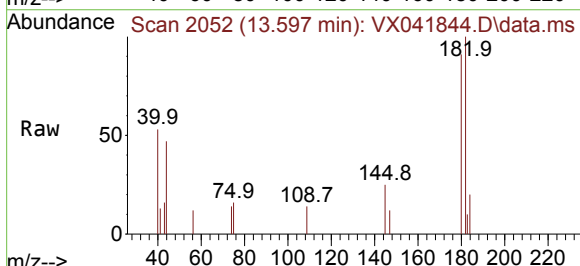

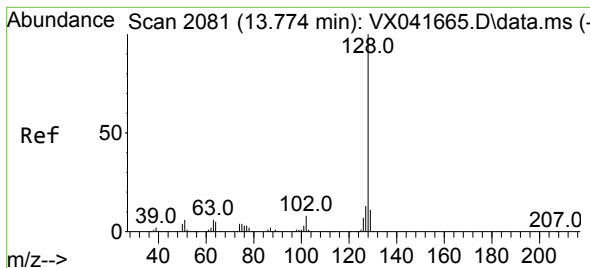

#95

Naphthalene

Concen: 0.369 ug/l

RT: 13.780 min Scan# 2081

Delta R.T. 0.006 min

Lab File: VX041844.D





Acq: 13 Jun 2024 11:25

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion:128	Resp:	3038
Ion Ratio	Lower	Upper
128	100	
127	15.2	10.3 15.5
129	10.0	8.8 13.2

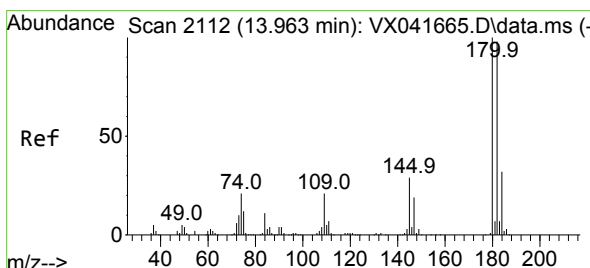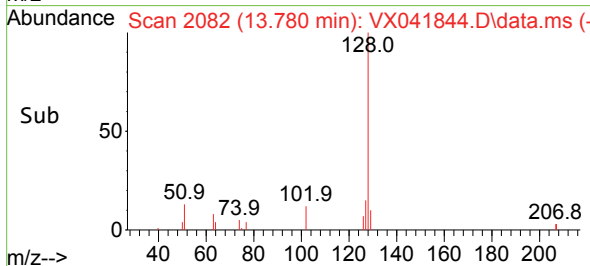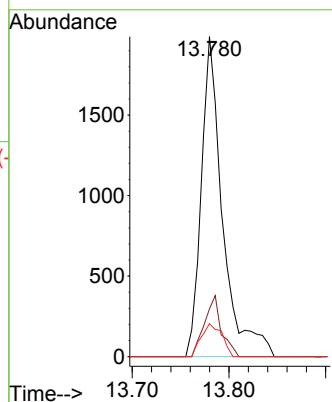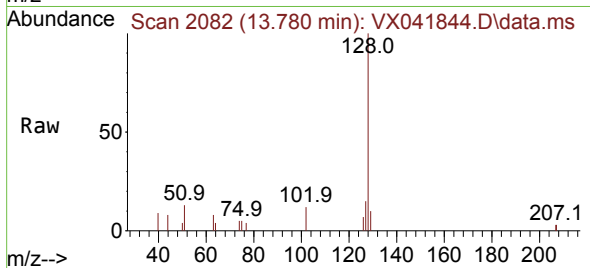

#96

1,2,3-Trichlorobenzene

Concen: 0.276 ug/l

RT: 13.963 min Scan# 2112

Delta R.T. -0.000 min

Lab File: VX041844.D

Acq: 13 Jun 2024 11:25

Tgt Ion:180	Resp:	794
Ion Ratio	Lower	Upper
180	100	
182	97.2	46.9 140.6
145	24.2	17.8 53.5

