

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061324\
 Data File : VX041860.D
 Acq On : 13 Jun 2024 17:38
 Operator : JC/MD
 Sample : PB161467ZHE#15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB161467ZHE#15

Quant Time: Jun 14 01:50:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 30 07:36:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	154303	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	240217	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	242599	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	115894	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	77661	41.037	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	82.080%
35) Dibromofluoromethane	5.385	113	73958	44.530	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	89.060%
50) Toluene-d8	8.647	98	288810	49.767	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.540%
62) 4-Bromofluorobenzene	11.079	95	107650	50.260	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	100.520%
Target Compounds						
					Qvalue	
16) Acetone	2.392	43	88203	104.612	ug/l	# 89
18) Methyl Acetate	2.709	43	7395	4.092	ug/l	97
20) Methylene Chloride	2.782	84	9693	5.723	ug/l	90
25) 2-Butanone	4.580	43	21759	18.500	ug/l	92
43) Isopropyl Acetate	6.348	43	120212	31.372	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061324\
Data File : VX041860.D
Acq On : 13 Jun 2024 17:38
Operator : JC/MD
Sample : PB161467ZHE#15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB161467ZHE#15

Quant Time: Jun 14 01:50:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
Quant Title : SW846 8260
QLast Update : Thu May 30 07:36:24 2024
Response via : Initial Calibration




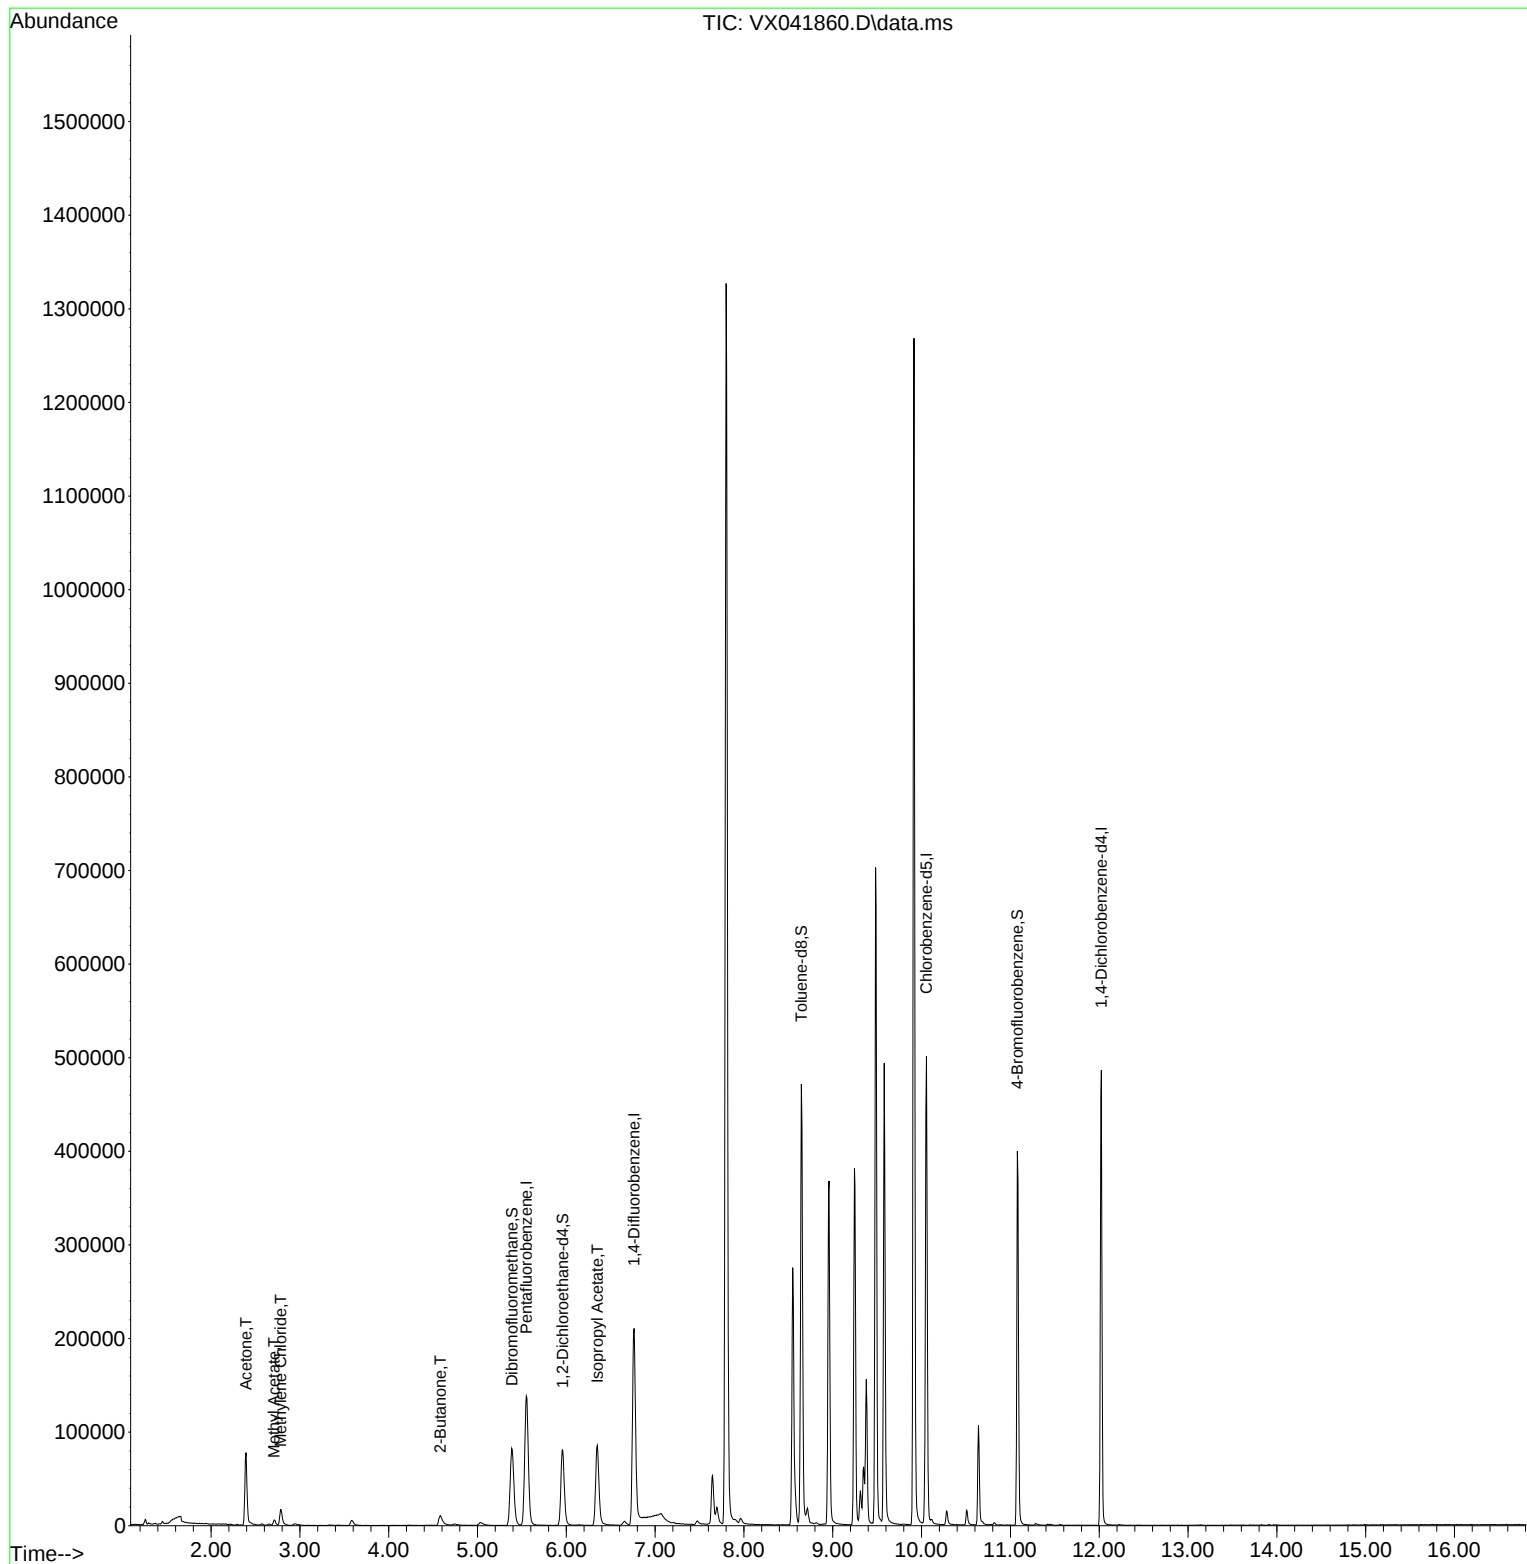


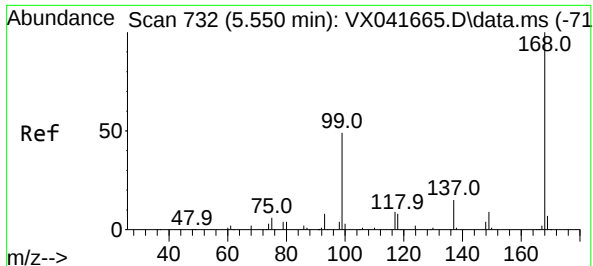

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX041860.D
Acq: 13 Jun 2024 17:38




Instrument :
MSVOA_X
ClientSampleId :
PB161467ZHE#15


Tgt Ion:168 Resp: 154303
Ion Ratio Lower Upper
168 100
99 45.1 56.6 85.0#

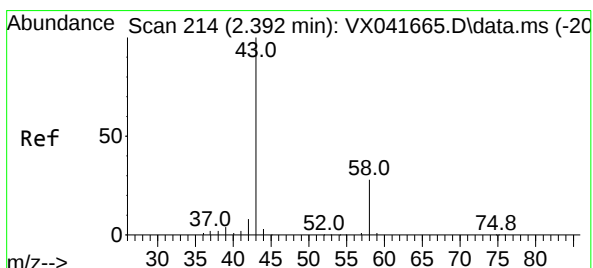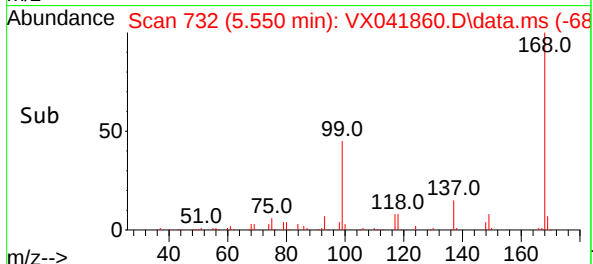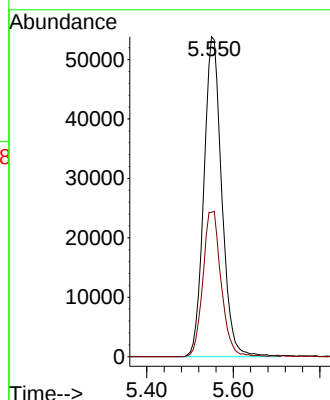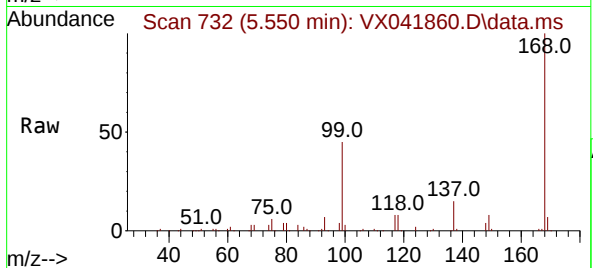

#16
Acetone
Concen: 104.612 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX041860.D
Acq: 13 Jun 2024 17:38

Tgt Ion: 43 Resp: 88203
Ion Ratio Lower Upper
43 100
58 33.3 21.9 32.9#


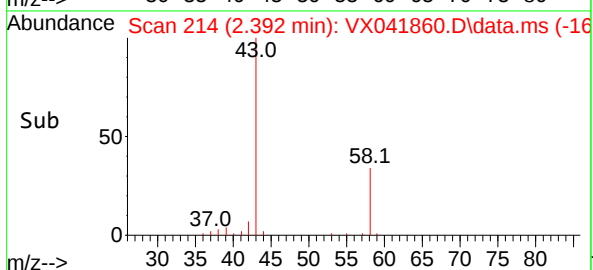
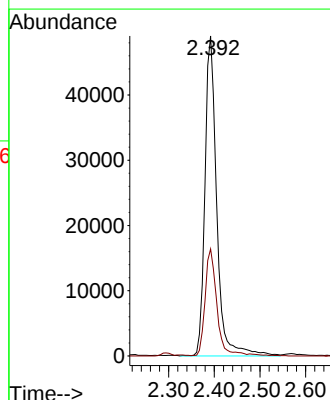
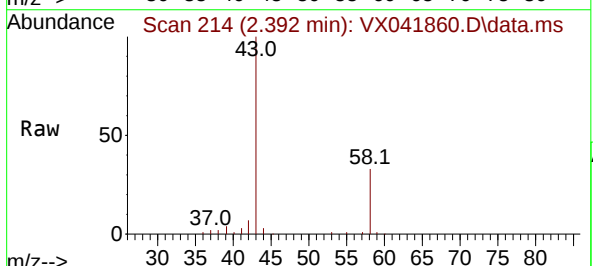




#18
Methyl Acetate
Concen: 4.092 ug/l
RT: 2.709 min Scan# 20
Delta R.T. 0.000 min
Lab File: VX041860.D
Acq: 13 Jun 2024 17:38




Instrument :
MSVOA_X
ClientSampleId :
PB161467ZHE#15


Tgt Ion: 43 Resp: 7395
Ion Ratio Lower Upper
43 100
74 23.9 17.8 26.8

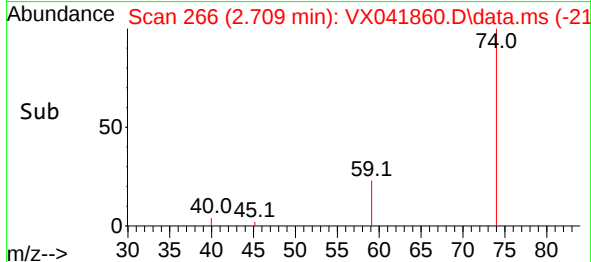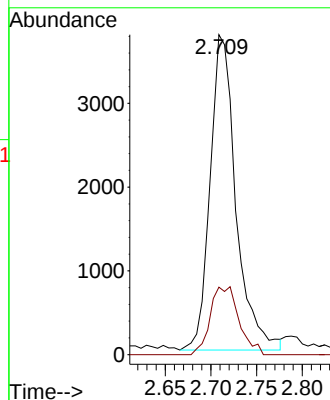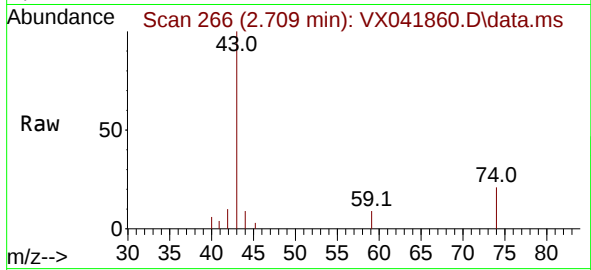

#20
Methylene Chloride
Concen: 5.723 ug/l
RT: 2.782 min Scan# 278
Delta R.T. -0.006 min
Lab File: VX041860.D
Acq: 13 Jun 2024 17:38

Tgt Ion: 84 Resp: 9693
Ion Ratio Lower Upper
84 100
49 114.3 103.6 155.4
51 35.9 33.8 50.6
86 65.2 49.4 74.0


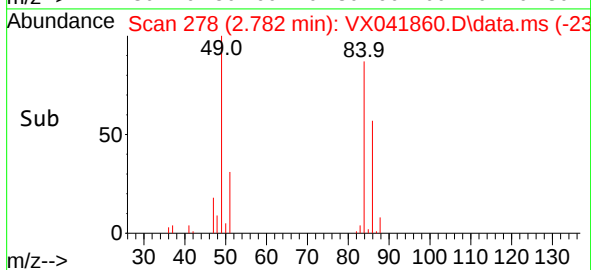
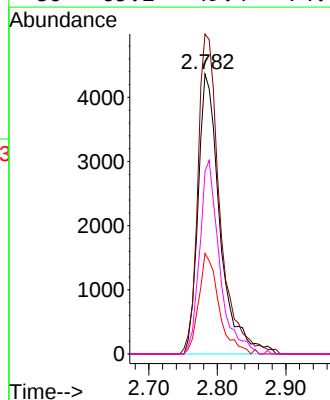
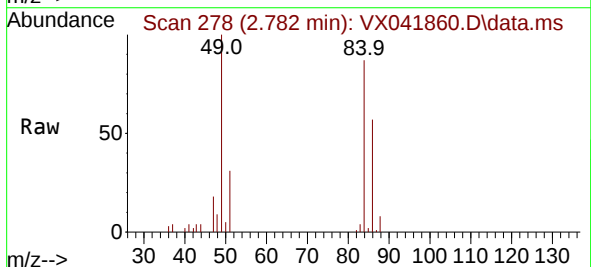




#25
2-Butanone
Concen: 18.500 ug/l
RT: 4.580 min Scan# 51
Delta R.T. 0.012 min
Lab File: VX041860.D
Acq: 13 Jun 2024 17:38




Instrument :
MSVOA_X
ClientSampleId :
PB161467ZHE#15


Tgt Ion: 43 Resp: 21759
Ion Ratio Lower Upper
43 100
72 28.1 19.4 29.2

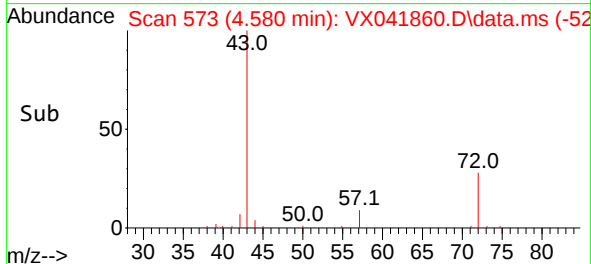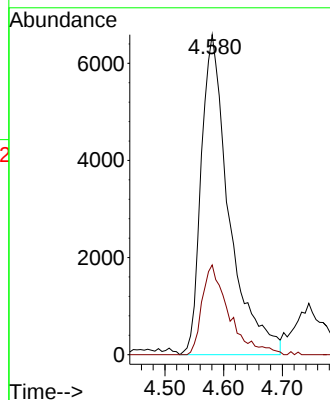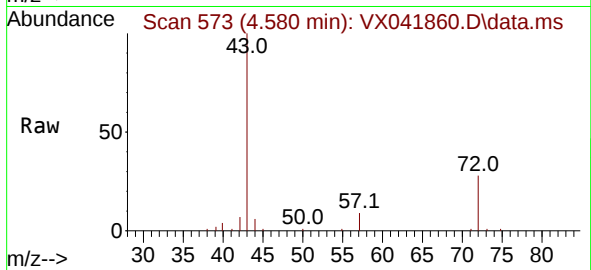

#33
1,2-Dichloroethane-d4
Concen: 41.037 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.006 min
Lab File: VX041860.D
Acq: 13 Jun 2024 17:38

Tgt Ion: 65 Resp: 77661
Ion Ratio Lower Upper
65 100
67 54.6 0.0 100.2



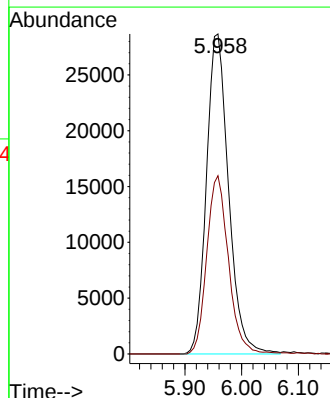
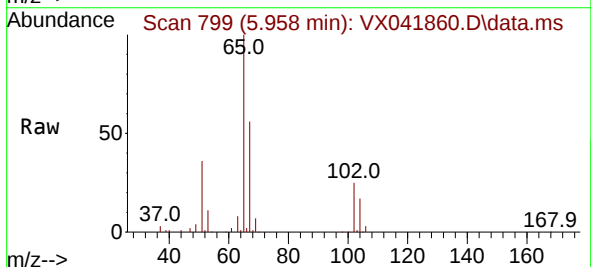


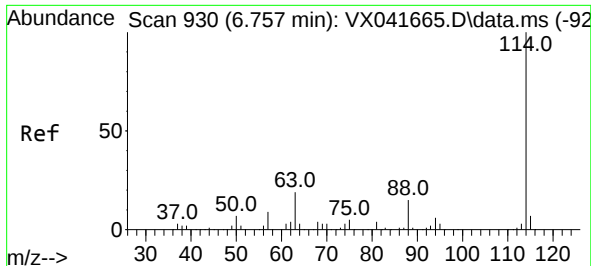

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX041860.D
Acq: 13 Jun 2024 17:38




Instrument :
MSVOA_X
ClientSampleId :
PB161467ZHE#15


Tgt Ion:114 Resp: 240217
Ion Ratio Lower Upper
114 100
63 17.7 0.0 45.0
88 15.0 0.0 36.6

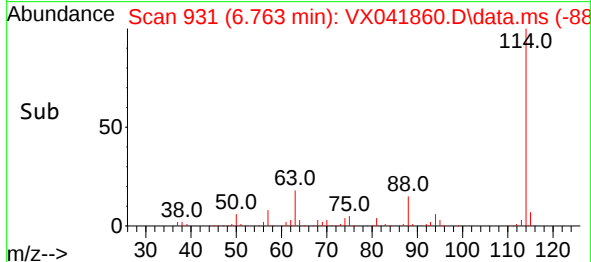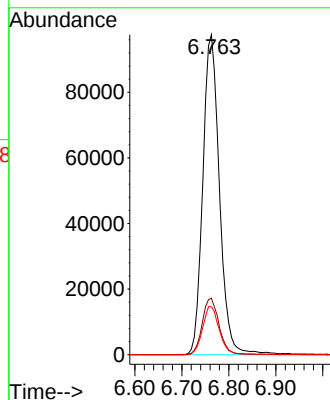

#35
Dibromofluoromethane
Concen: 44.530 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX041860.D
Acq: 13 Jun 2024 17:38

Tgt Ion:113 Resp: 73958
Ion Ratio Lower Upper
113 100
111 101.8 82.9 124.3
192 26.1 13.3 19.9#


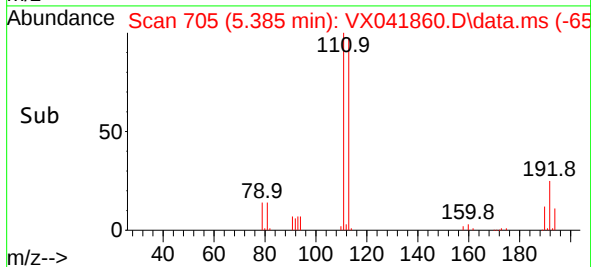
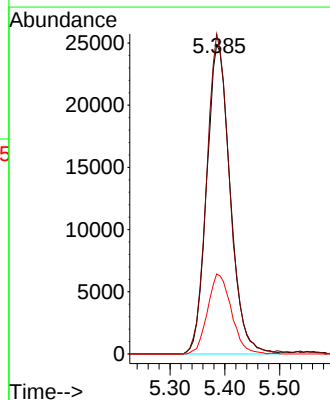
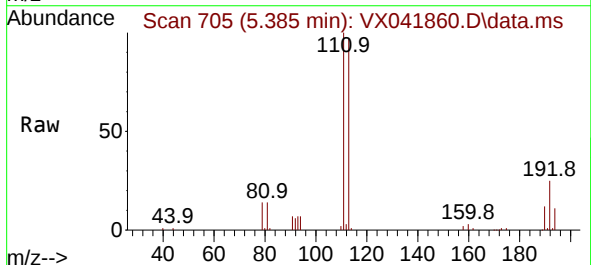




#43
Isopropyl Acetate
Concen: 31.372 ug/l
RT: 6.348 min Scan# 80
Delta R.T. 0.006 min
Lab File: VX041860.D
Acq: 13 Jun 2024 17:38




Instrument :
MSVOA_X
ClientSampleId :
PB161467ZHE#15


Tgt Ion: 43 Resp: 120212
Ion Ratio Lower Upper
43 100
61 21.1 15.2 22.8
87 14.3 9.8 14.6

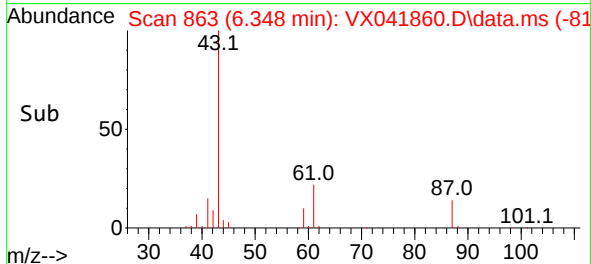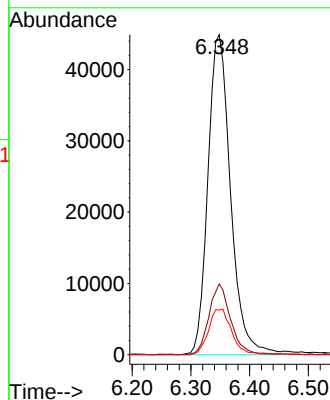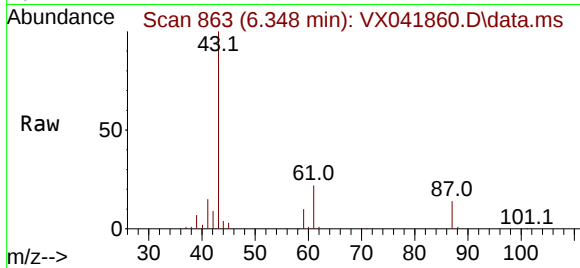

#50
Toluene-d8
Concen: 49.767 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX041860.D
Acq: 13 Jun 2024 17:38

Tgt Ion: 98 Resp: 288810
Ion Ratio Lower Upper
98 100
100 66.9 53.1 79.7



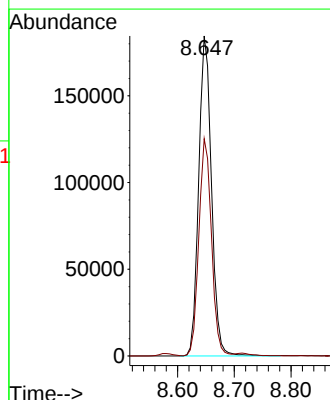
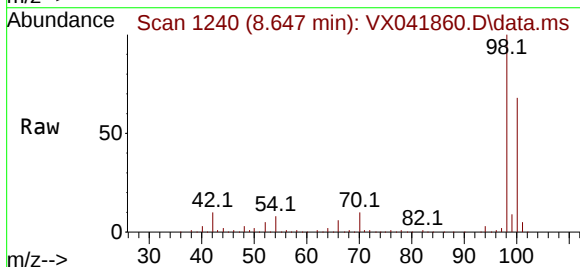




#62
4-Bromofluorobenzene
Concen: 50.260 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX041860.D
Acq: 13 Jun 2024 17:38




Instrument :
MSVOA_X
ClientSampleId :
PB161467ZHE#15


Tgt Ion: 95 Resp: 107650
Ion Ratio Lower Upper
95 100
174 97.8 0.0 135.6
176 95.5 0.0 131.0

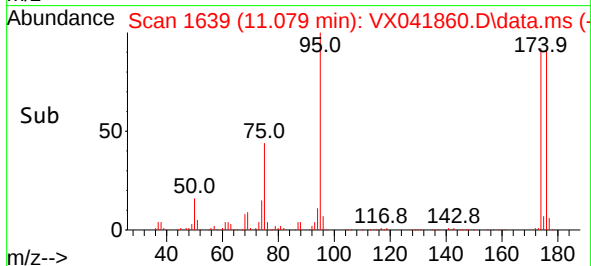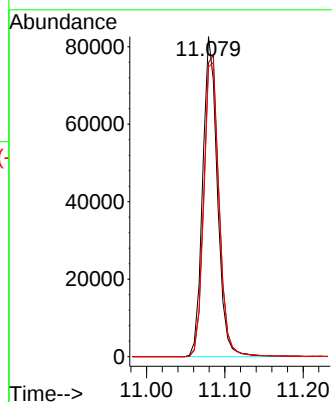

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX041860.D
Acq: 13 Jun 2024 17:38

Tgt Ion: 117 Resp: 242599
Ion Ratio Lower Upper
117 100
82 51.4 46.2 69.4
119 32.3 25.5 38.3

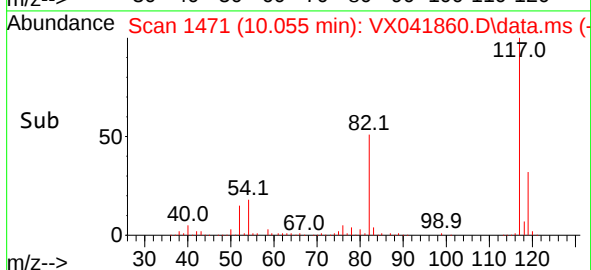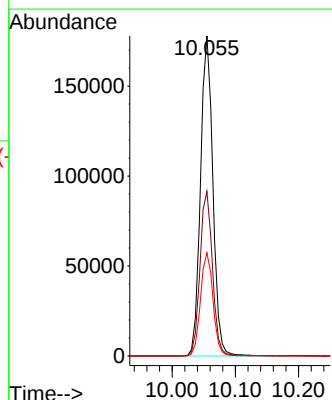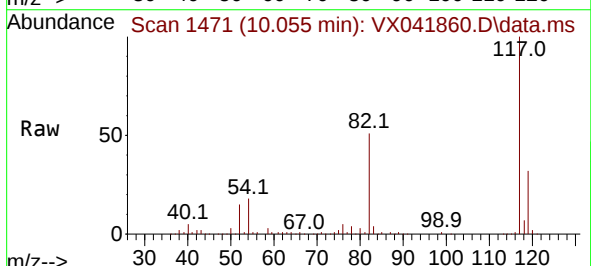



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX041860.D


Acq: 13 Jun 2024 17:38

Instrument :

MSVOA_X

ClientSampleId :

PB161467ZHE#15

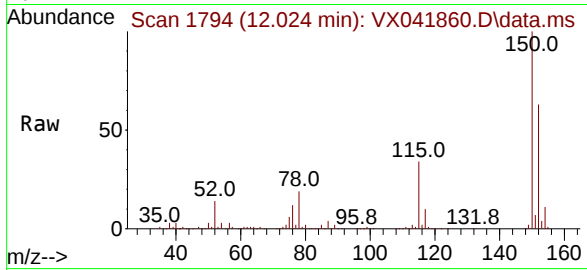

Tgt Ion:152 Resp: 115894

Ion Ratio Lower Upper

152 100

115 54.1 43.3 129.9

150 157.7 0.0 345.0

