
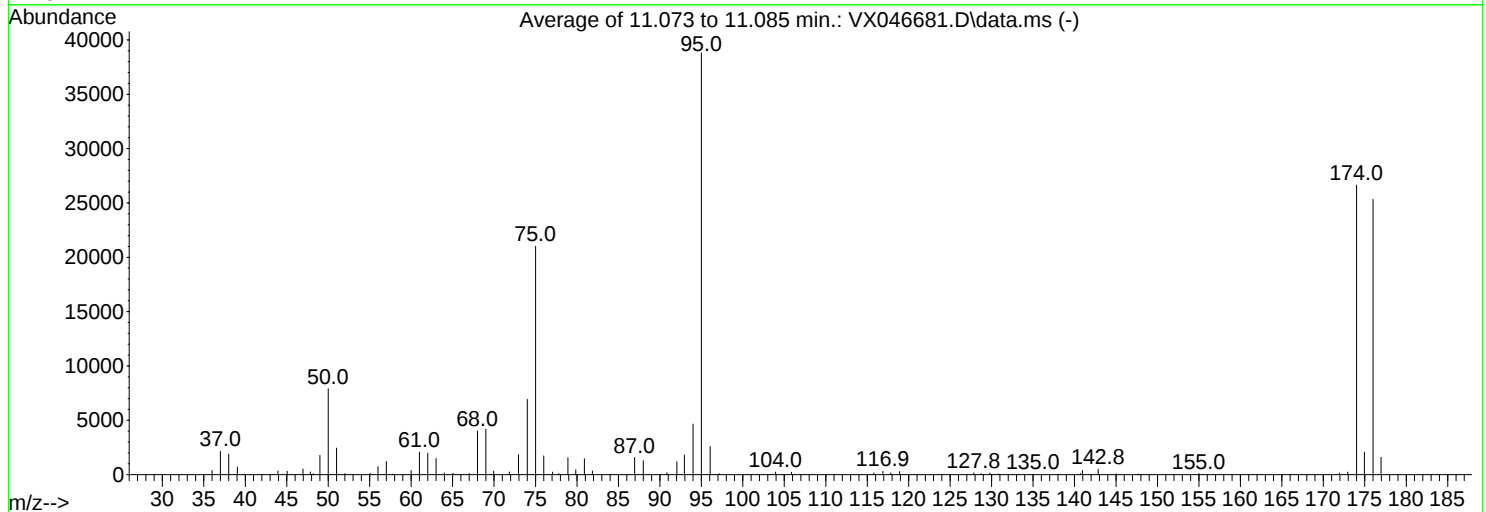


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061325\
Data File : VX046681.D
Acq On : 13 Jun 2025 11:58
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X061025W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Jun 11 06:20:28 2025

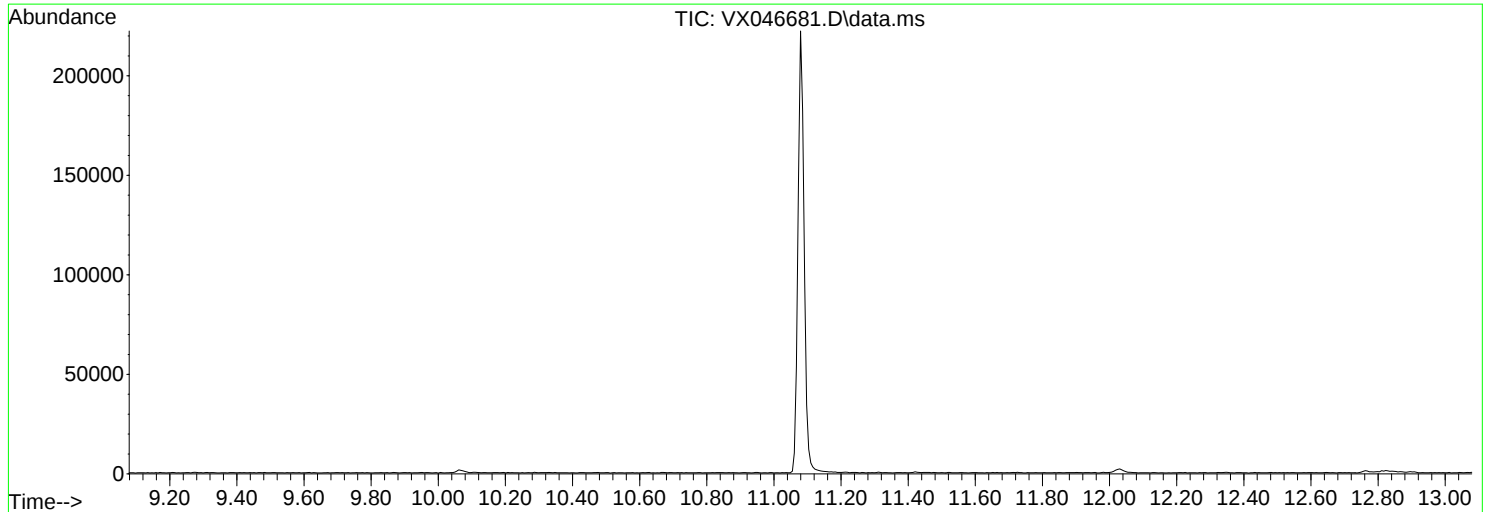

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	7907	PASS
75	95	30	60	54.1	21016	PASS
95	95	100	100	100.0	38811	PASS
96	95	5	9	6.7	2597	PASS
173	174	0.00	2	0.9	231	PASS
174	95	50	100	68.7	26645	PASS
175	174	5	9	7.8	2080	PASS
176	174	95	101	95.1	25331	PASS
177	176	5	9	6.3	1601	PASS