

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061421\
 Data File : VX022690.D
 Acq On : 14 Jun 2021 13:29
 Operator : JC/MD
 Sample : M2688-01DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jun 15 06:10:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 10 12:20:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	61628	50.00	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.769	114	124110	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	107971	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	41715	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	51795	46.73	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	93.46%
35) Dibromofluoromethane	5.397	113	37057	46.80	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	93.60%
50) Toluene-d8	8.653	98	152467	48.84	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.68%
62) 4-Bromofluorobenzene	11.085	95	51072	43.26	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	86.52%

Target Compounds				Qvalue		
3) Chloromethane	1.300	50	177	0.20	ug/l	# 86
5) Bromomethane	1.611	94	110	0.24	ug/l	92
10) Methyl Iodide	2.465	142	228	0.27	ug/l	# 42
11) Tert butyl alcohol	2.971	59	61	0.24	ug/l	# 73
13) Acrolein	2.221	56	83	0.77	ug/l	# 1
14) Allyl chloride	2.721	41	1294	0.89	ug/l	# 25
15) Acrylonitrile	3.105	53	724	1.44	ug/l	# 31
16) Acetone	2.386	43	3273	6.59	ug/l	92
18) Methyl Acetate	2.782	43	7317	4.90	ug/l	# 47
20) Methylene Chloride	2.800	84	676	0.43	ug/l	# 90
25) 2-Butanone	4.574	43	2604	3.24	ug/l	# 88
26) 2,2-Dichloropropane	4.318	77	447	0.35	ug/l	# 52
31) Cyclohexane	5.477	56	52052	38.93	ug/l	98
36) 1,1-Dichloropropene	5.556	75	6256	5.06	ug/l	# 48
37) Ethyl Acetate	4.574	43	2604	1.66	ug/l	# 64
38) Carbon Tetrachloride	5.562	117	7294	6.90	ug/l	# 17
39) Methylcyclohexane	7.385	83	13252	10.27	ug/l	95
40) Benzene	6.050	78	32481	8.83	ug/l	95
48) Methyl methacrylate	7.659	41	1085	0.91	ug/l	# 57
51) 4-Methyl-2-Pentanone	8.586	43	569	0.36	ug/l	# 58
52) Toluene	8.720	92	109953	48.02	ug/l	100
53) t-1,3-Dichloropropene	8.720	75	1262	4.02	ug/l	# 1
55) 1,1,2-Trichloroethane	9.110	97	640	0.68	ug/l	# 15
56) Ethyl methacrylate	9.104	69	221	2.42	ug/l	# 1
67) Ethyl Benzene	10.195	91	183376	44.27	ug/l	99
68) m/p-Xylenes	10.305	106	214096	142.68	ug/l	96
69) o-Xylene	10.646	106	106898	73.53	ug/l	96
70) Styrene	10.646	104	5031	3.27	ug/l	# 1
73) Isopropylbenzene	10.969	105	9717	2.84	ug/l	95
76) 1,2,3-Trichloropropane	11.378	75	1014	0.92	ug/l	# 1
78) n-propylbenzene	11.305	91	22590	5.46	ug/l	94
79) 2-Chlorotoluene	11.384	91	13806	5.51	ug/l	# 41
80) 1,3,5-Trimethylbenzene	11.457	105	30709	10.76	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.085	75	28954	65.63	ug/l	# 12
82) 4-Chlorotoluene	11.457	91	3416	1.19	ug/l	# 45
83) tert-Butylbenzene	11.756	119	14403	5.37	ug/l	# 49

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061421\
Data File : VX022690.D
Acq On : 14 Jun 2021 13:29
Operator : JC/MD
Sample : M2688-01DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jun 15 06:10:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 10 12:20:00 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
84) 1,2,4-Trimethylbenzene	11.756	105	123236	42.58	ug/l	99
85) sec-Butylbenzene	11.756	105	123236	35.21	ug/l #	57
86) p-Isopropyltoluene	11.975	119	2205	0.76	ug/l	98
89) n-Butylbenzene	12.317	91	2301	0.83	ug/l #	9
90) Hexachloroethane	12.616	117	796	5.21	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	12.926	75	21	4.01	ug/l #	1
95) Naphthalene	13.780	128	28817	9.36	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061421\
Data File : VX022690.D
Acq On : 14 Jun 2021 13:29
Operator : JC/MD
Sample : M2688-01DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jun 15 06:10:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 10 12:20:00 2021
Response via : Initial Calibration




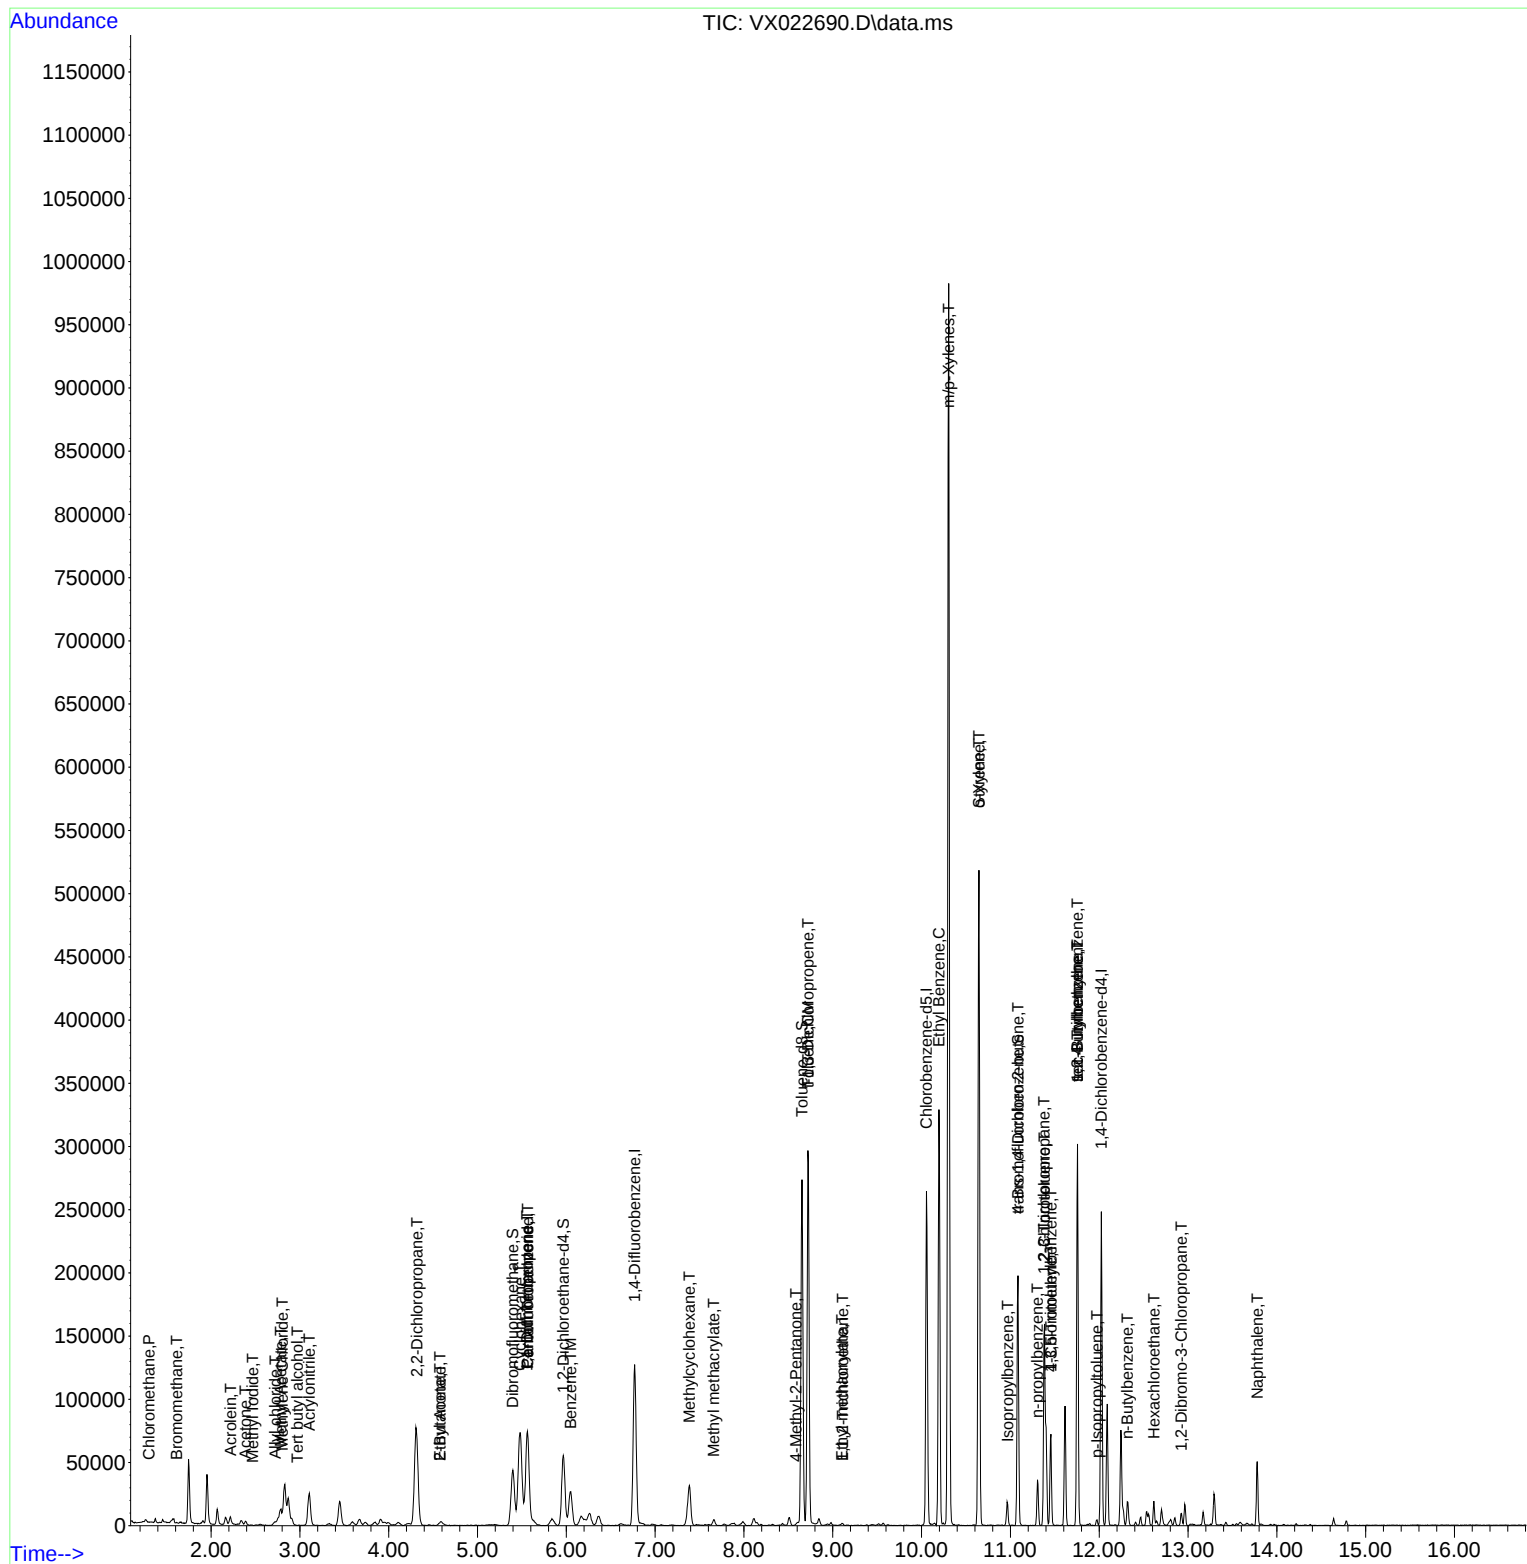




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 61628
Ion Ratio Lower Upper
168 100
99 70.2 45.8 68.6#

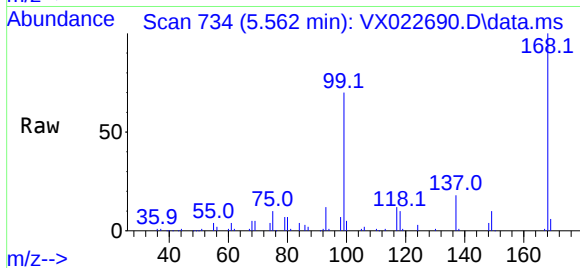

#3
Chloromethane
Concen: 0.20 ug/l
RT: 1.300 min Scan# 35
Delta R.T. 0.006 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 50 Resp: 177
Ion Ratio Lower Upper
50 100
52 41.2 26.4 39.6#




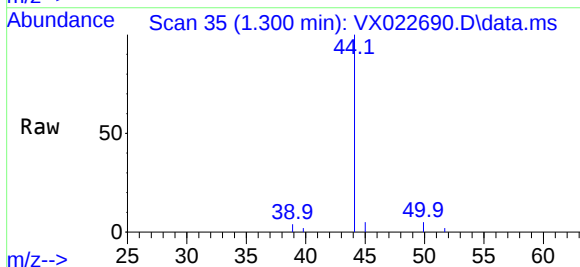


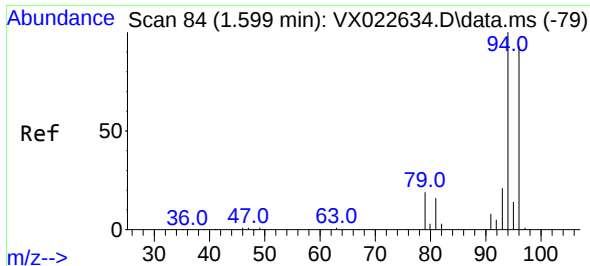

#5
Bromomethane
Concen: 0.24 ug/l
RT: 1.611 min Scan# 86
Delta R.T. 0.012 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 94 Resp: 110
Ion Ratio Lower Upper
94 100
96 103.5 76.4 114.6

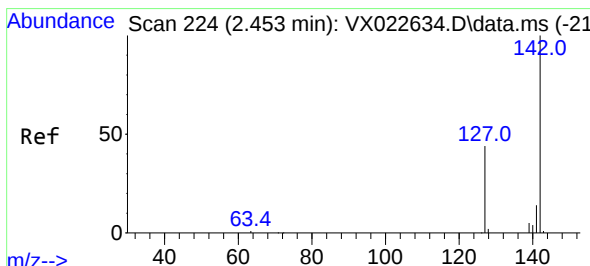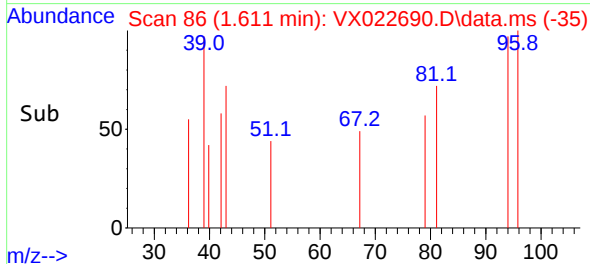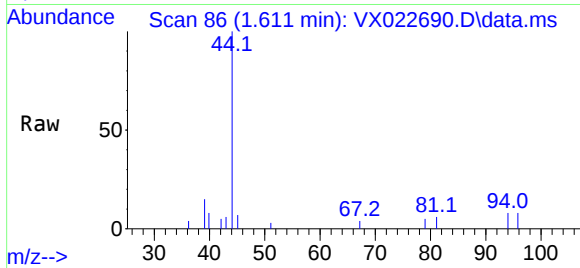

#10
Methyl Iodide
Concen: 0.27 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.012 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 142 Resp: 228
Ion Ratio Lower Upper
142 100
127 0.0 33.3 49.9#
141 0.0 11.4 17.0#

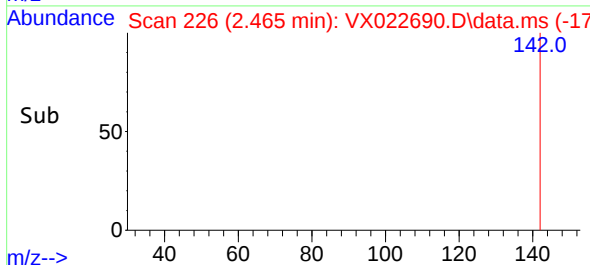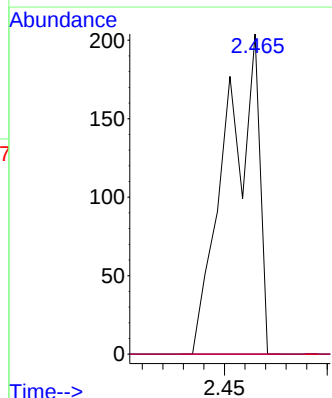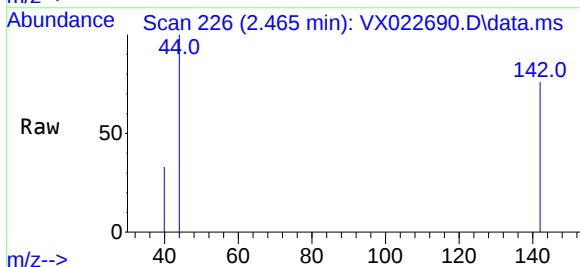







#11

Tert butyl alcohol
Concen: 0.24 ug/l
RT: 2.971 min Scan# 309
Delta R.T. -0.012 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Instrument :
MSVOA_X
ClientSampled :




Tgt Ion: 59 Resp: 61
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#




#13

Acrolein
Concen: 0.77 ug/l
RT: 2.221 min Scan# 186
Delta R.T. -0.018 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 56 Resp: 83
Ion Ratio Lower Upper
56 100
55 3604.8 56.4 84.6#









#14
 Allyl chloride
 Concen: 0.89 ug/l
 RT: 2.721 min Scan# 268
 Delta R.T. 0.055 min
 Lab File: VX022690.D
 Acq: 14 Jun 2021 13:29




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 41 Resp: 1294
 Ion Ratio Lower Upper
 41 100
 39 0.0 51.6 77.4#
 76 0.0 30.5 45.7#



#15
 Acrylonitrile
 Concen: 1.44 ug/l
 RT: 3.105 min Scan# 331
 Delta R.T. 0.030 min
 Lab File: VX022690.D
 Acq: 14 Jun 2021 13:29

Tgt Ion: 53 Resp: 724
 Ion Ratio Lower Upper
 53 100
 52 11.5 65.3 97.9#
 51 61.9 28.2 42.2#


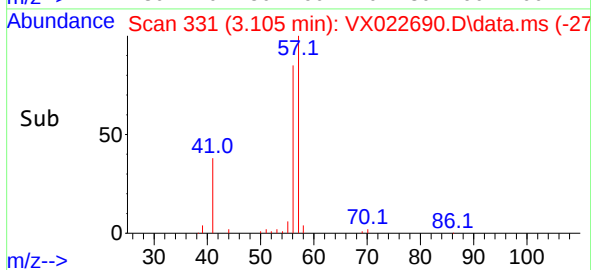






#16
Acetone
Concen: 6.59 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 3273
Ion Ratio Lower Upper
43 100
58 29.9 27.8 41.8



#18
Methyl Acetate
Concen: 4.90 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.073 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 43 Resp: 7317
Ion Ratio Lower Upper
43 100
74 0.0 21.9 32.9#

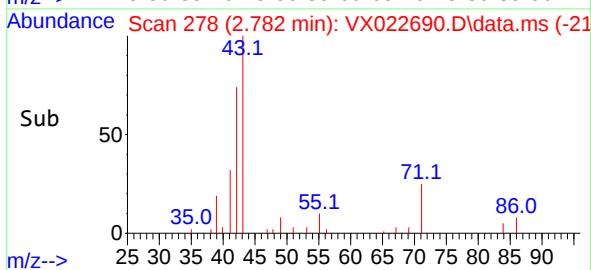







#20
Methylene Chloride
Concen: 0.43 ug/l
RT: 2.800 min Scan# 281
Delta R.T. 0.006 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 84 Resp: 676




Ion	Ratio	Lower	Upper
84	100		
49	123.7	88.6	132.8
51	26.2	27.0	40.6#
86	60.2	50.3	75.5

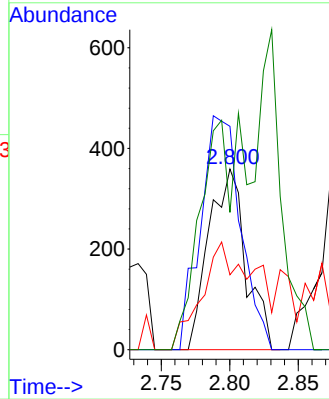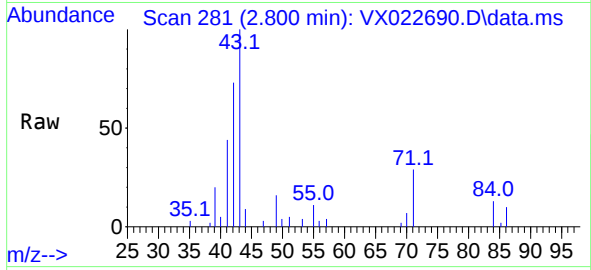


#25
2-Butanone
Concen: 3.24 ug/l
RT: 4.574 min Scan# 572
Delta R.T. 0.006 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 43 Resp: 2604

Ion	Ratio	Lower	Upper
43	100		
72	23.3	23.7	35.5#



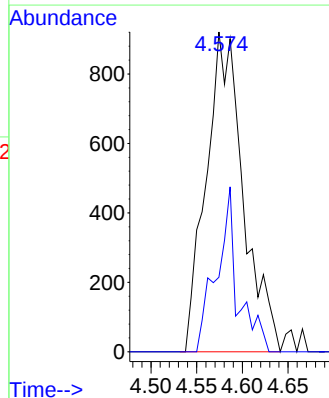





#26
2,2-Dichloropropane
Concen: 0.35 ug/l
RT: 4.318 min Scan# 530
Delta R.T. -0.171 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 77 Resp: 447
Ion Ratio Lower Upper
77 100
97 0.0 11.7 35.1#

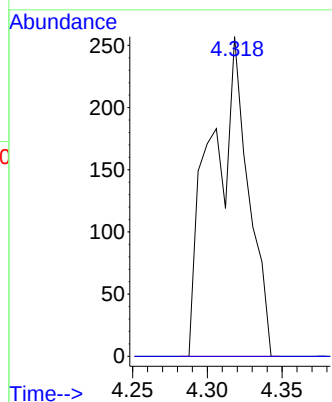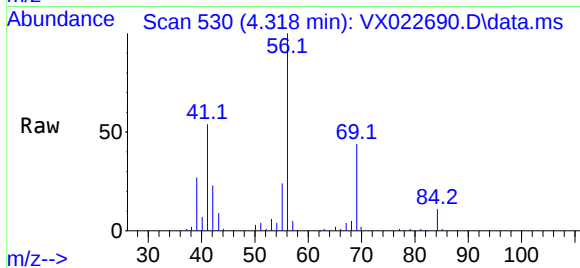

#31
Cyclohexane
Concen: 38.93 ug/l
RT: 5.477 min Scan# 720
Delta R.T. -0.000 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 56 Resp: 52052
Ion Ratio Lower Upper
56 100
69 28.8 25.3 37.9
84 89.5 71.4 107.0

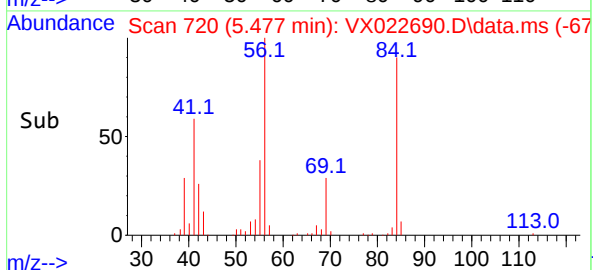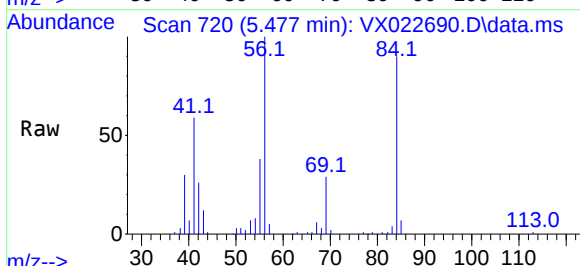







#33

1,2-Dichloroethane-d4
Concen: 46.73 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Instrument :
MSVOA_X
ClientSampled :




Tgt Ion: 65 Resp: 51795
Ion Ratio Lower Upper
65 100
67 52.5 0.0 105.4




#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 114 Resp: 124110
Ion Ratio Lower Upper
114 100
63 21.7 0.0 40.8
88 15.7 0.0 32.8



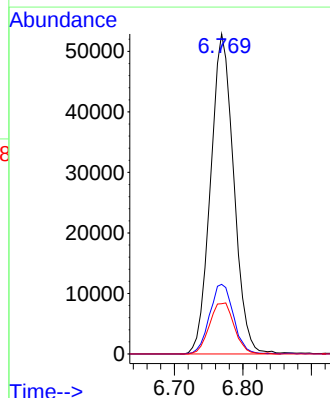





#35
Dibromofluoromethane
Concen: 46.80 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.006 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:113 Resp: 37057
Ion Ratio Lower Upper
113 100
111 105.6 81.9 122.9
192 15.3 16.7 25.1#



#36
1,1-Dichloropropene
Concen: 5.06 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.146 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 75 Resp: 6256
Ion Ratio Lower Upper
75 100
110 7.9 18.1 54.4#
77 0.0 25.3 37.9#



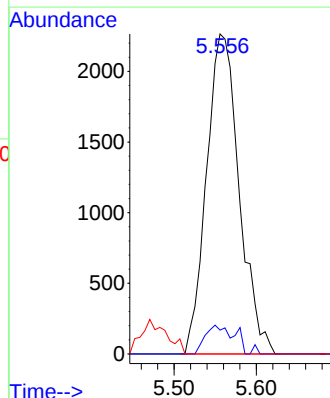





#37
Ethyl Acetate
Concen: 1.66 ug/l
RT: 4.574 min Scan# 572
Delta R.T. -0.153 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 2604
Ion Ratio Lower Upper
43 100
61 0.0 12.8 19.2#
70 0.0 10.5 15.7#

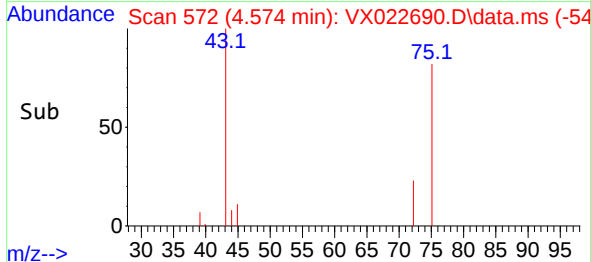

#38
Carbon Tetrachloride
Concen: 6.90 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.116 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 117 Resp: 7294
Ion Ratio Lower Upper
117 100
119 6.2 76.2 114.2#
121 0.0 24.8 37.2#

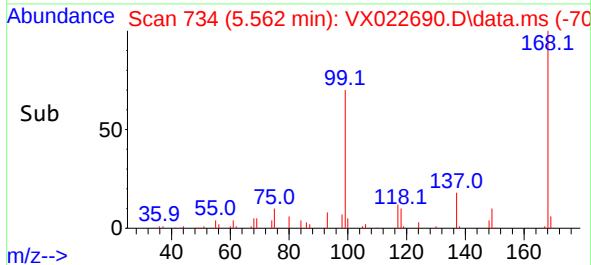



#39

Methylcyclohexane

Concen: 10.27 ug/l

RT: 7.385 min Scan# 1033

Delta R.T. -0.000 min

Lab File: VX022690.D

Acq: 14 Jun 2021 13:29





Tgt Ion: 83 Resp: 13252

Ion Ratio Lower Upper

83 100

55 78.9 58.9 88.3

98 49.1 38.1 57.1



#40

Benzene

Concen: 8.83 ug/l

RT: 6.050 min Scan# 814

Delta R.T. -0.000 min

Lab File: VX022690.D




Acq: 14 Jun 2021 13:29


Tgt Ion: 78 Resp: 32481

Ion Ratio Lower Upper

78 100

77 21.1 18.9 28.3



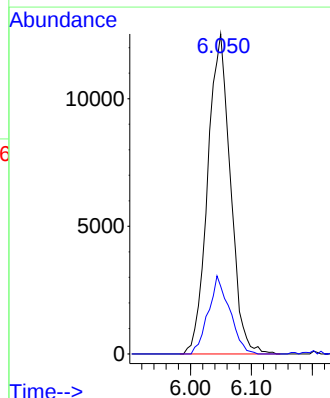





#48
Methyl methacrylate
Concen: 0.91 ug/l
RT: 7.659 min Scan# 1078
Delta R.T. -0.037 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 41 Resp: 1085
Ion Ratio Lower Upper
41 100
69 133.4 76.0 114.0#
39 92.1 44.6 67.0#

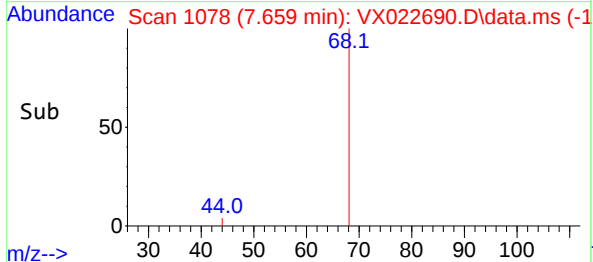

#50
Toluene-d8
Concen: 48.84 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 98 Resp: 152467
Ion Ratio Lower Upper
98 100
100 65.7 51.9 77.9


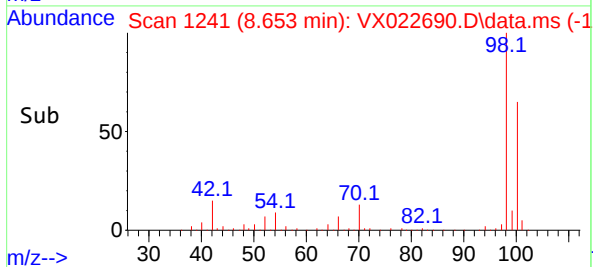

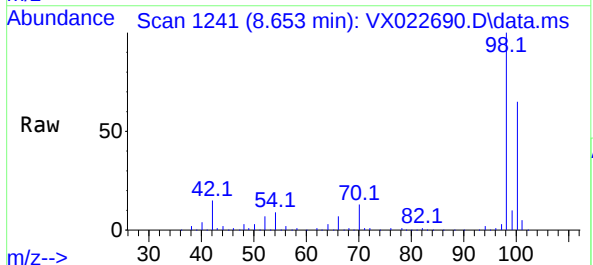




#51
4-Methyl-2-Pentanone
Concen: 0.36 ug/l
RT: 8.586 min Scan# 1230
Delta R.T. 0.006 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 569
Ion Ratio Lower Upper
43 100
58 17.0 35.4 53.0#

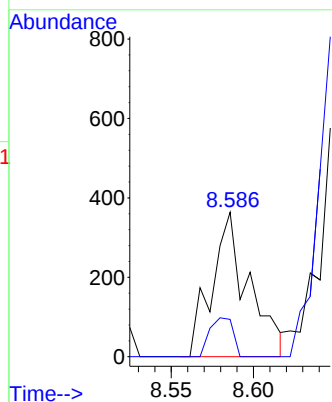

#52
Toluene
Concen: 48.02 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 92 Resp: 109953
Ion Ratio Lower Upper
92 100
91 172.1 137.1 205.7


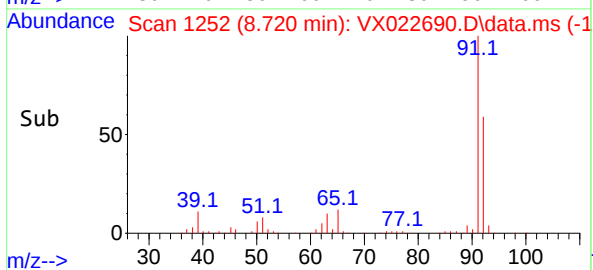
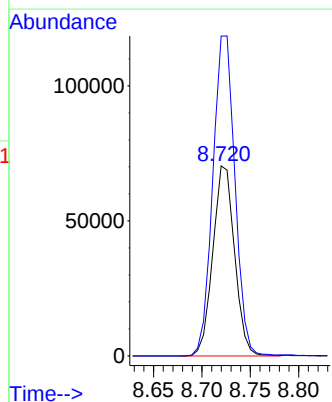





#53
t-1,3-Dichloropropene
Concen: 4.02 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.262 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 75 Resp: 1262
Ion Ratio Lower Upper
75 100
77 161.2 24.9 37.3#



#55
1,1,2-Trichloroethane
Concen: 0.68 ug/l
RT: 9.110 min Scan# 1316
Delta R.T. -0.049 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 97 Resp: 640
Ion Ratio Lower Upper
97 100
83 0.0 69.3 103.9#
85 0.0 44.3 66.5#
99 0.0 50.3 75.5#



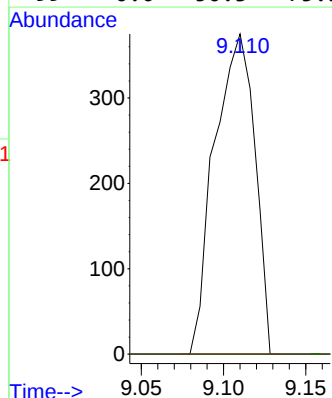
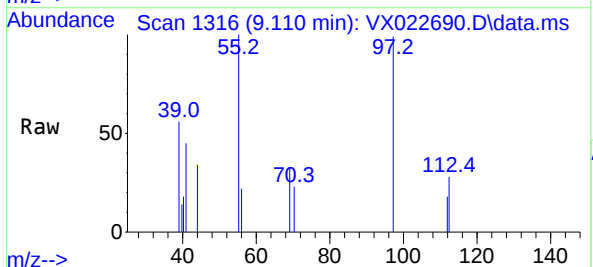




#56
Ethyl methacrylate
Concen: 2.42 ug/l
RT: 9.104 min Scan# 1315
Delta R.T. -0.018 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 69 Resp: 221
Ion Ratio Lower Upper
69 100
41 176.5 46.8 70.2#
39 95.0 24.7 37.1#

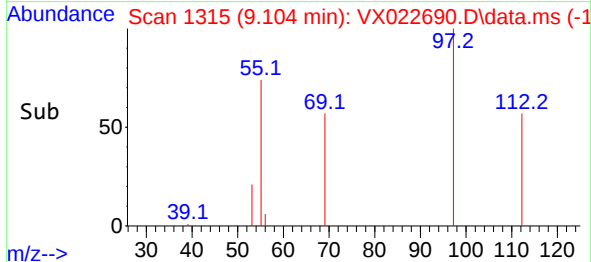

#62
4-Bromofluorobenzene
Concen: 43.26 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 95 Resp: 51072
Ion Ratio Lower Upper
95 100
174 65.2 0.0 154.6
176 62.5 0.0 155.8


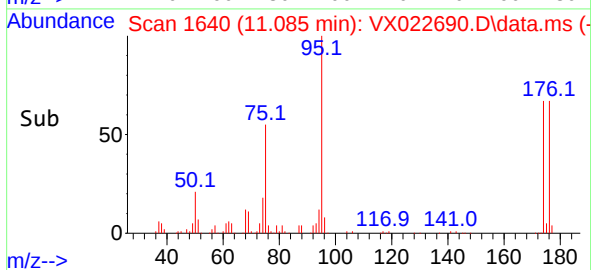






#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:117 Resp: 107971
Ion Ratio Lower Upper
117 100
82 62.1 47.4 71.2
119 33.1 26.6 39.8

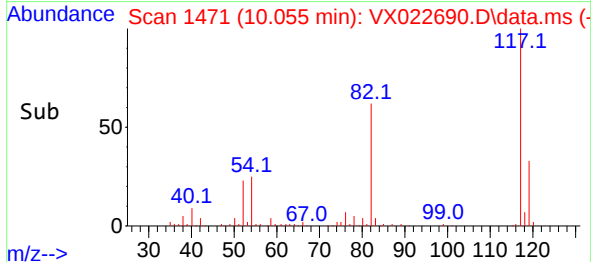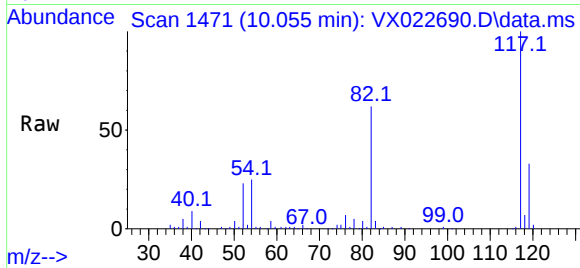

#67
Ethyl Benzene
Concen: 44.27 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29





Tgt Ion: 91 Resp: 183376
Ion Ratio Lower Upper
91 100
106 30.4 24.6 37.0

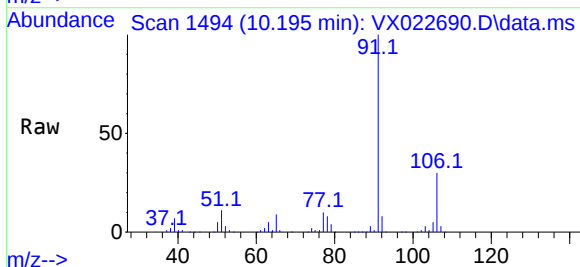






#68
m/p-Xylenes
Concen: 142.68 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29


Tgt Ion:106 Resp: 214096
Ion Ratio Lower Upper
106 100
91 209.5 162.8 244.2

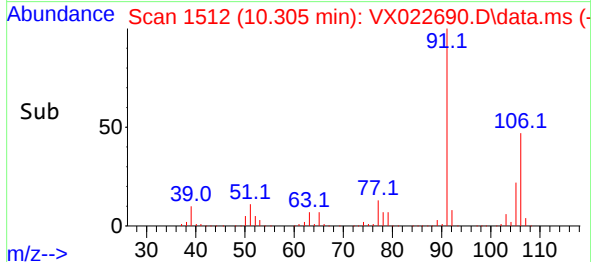

#69
o-Xylene
Concen: 73.53 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion:106 Resp: 106898
Ion Ratio Lower Upper
106 100
91 221.8 108.1 324.2




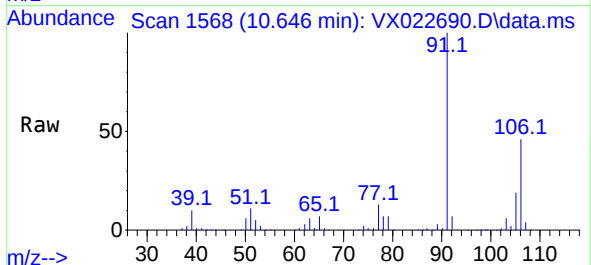




#70
Styrene
Concen: 3.27 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.013 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:104 Resp: 5031
Ion Ratio Lower Upper
104 100
78 347.9 40.0 60.0#
103 287.9 43.4 65.0#

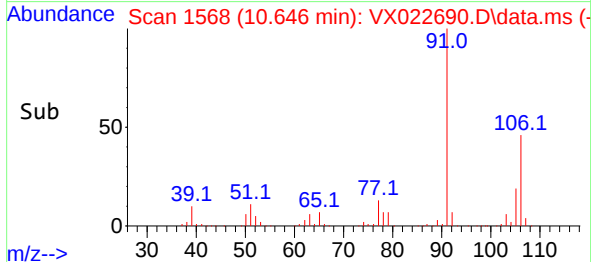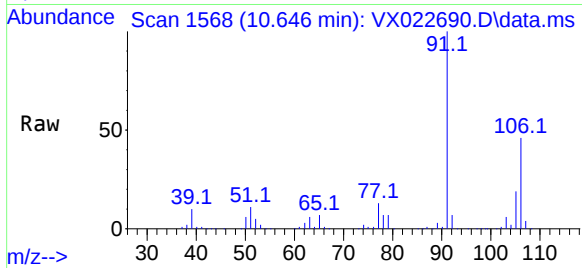

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion:152 Resp: 41715
Ion Ratio Lower Upper
152 100
115 69.7 41.1 123.3
150 162.6 0.0 349.0




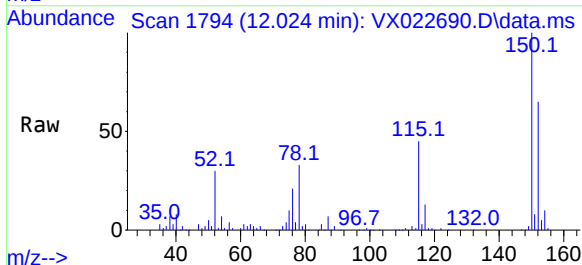




#73
Isopropylbenzene
Concen: 2.84 ug/l
RT: 10.969 min Scan# 1621
Delta R.T. 0.006 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:105 Resp: 9717
Ion Ratio Lower Upper
105 100
120 23.9 13.2 39.6

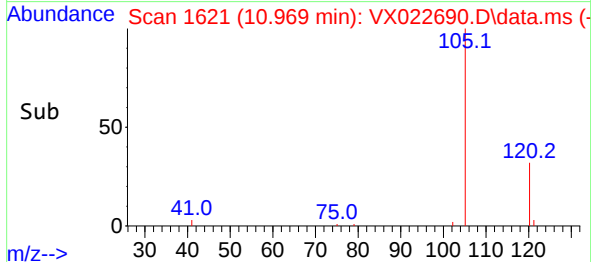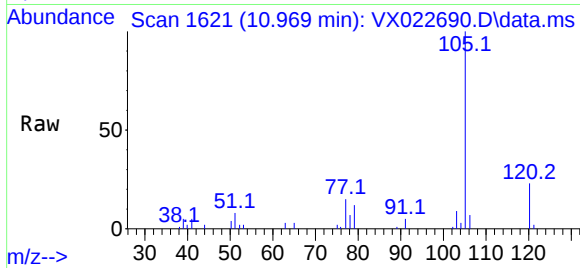

#76
1,2,3-Trichloropropane
Concen: 0.92 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.134 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 75 Resp: 1014
Ion Ratio Lower Upper
75 100
77 1331.4 19.1 57.5#




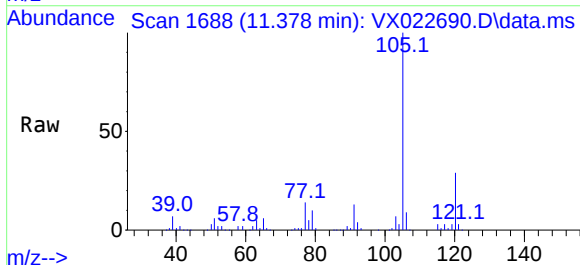




#78
n-propylbenzene
Concen: 5.46 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 91 Resp: 22590
Ion Ratio Lower Upper
91 100
120 20.1 11.5 34.5

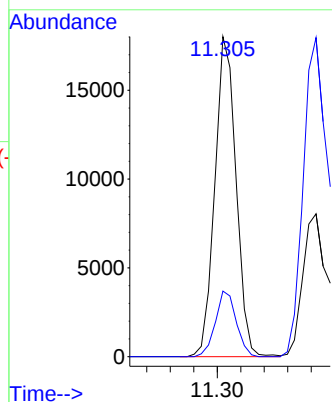

#79
2-Chlorotoluene
Concen: 5.51 ug/l
RT: 11.384 min Scan# 1689
Delta R.T. 0.018 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 91 Resp: 13806
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#


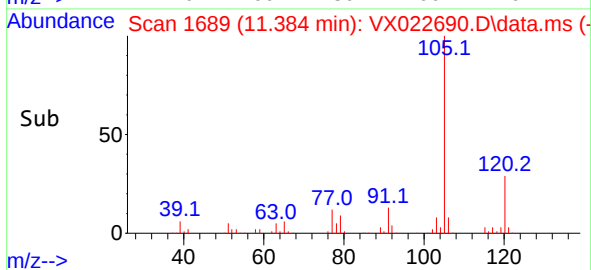
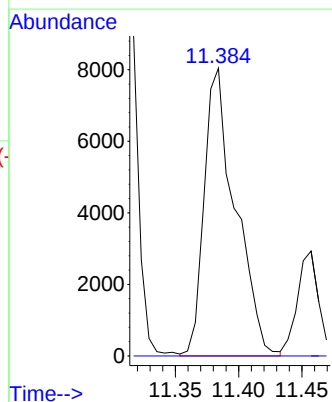





#80
1,3,5-Trimethylbenzene
Concen: 10.76 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:105 Resp: 30709
Ion Ratio Lower Upper
105 100
120 48.0 23.8 71.5

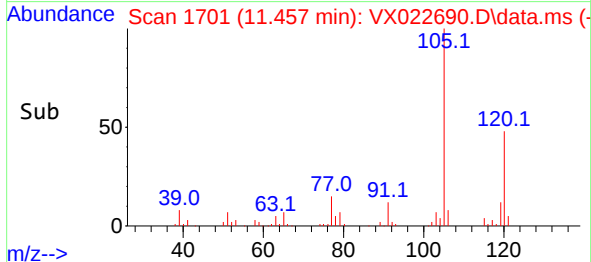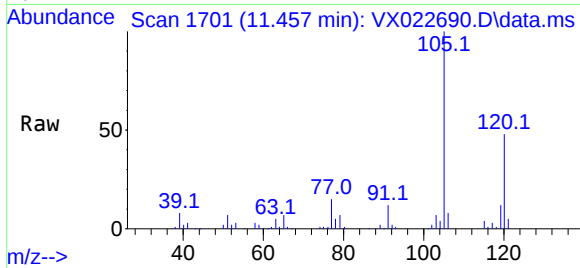

#81
trans-1,4-Dichloro-2-butene
Concen: 65.63 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 75 Resp: 28954
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#




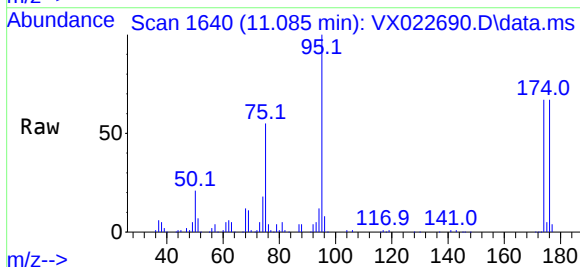




#82
4-Chlorotoluene
Concen: 1.19 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 91 Resp: 3416
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#

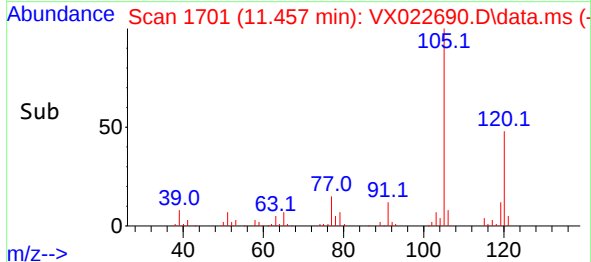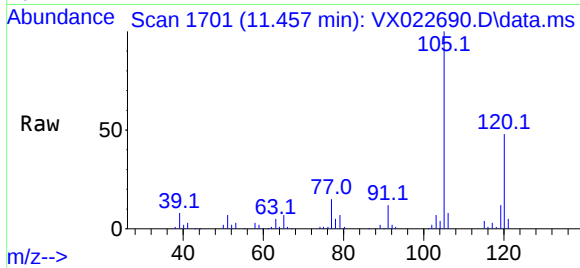

#83
tert-Butylbenzene
Concen: 5.37 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.037 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 119 Resp: 14403
Ion Ratio Lower Upper
119 100
91 94.5 27.9 83.7#
134 0.0 11.3 33.9#




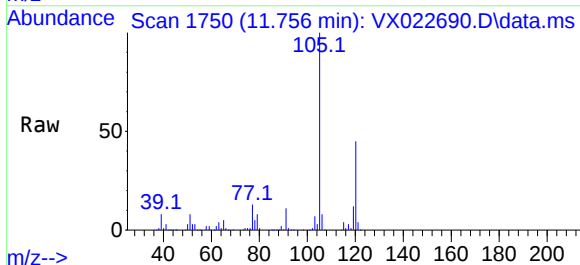




#84
1,2,4-Trimethylbenzene
Concen: 42.58 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:105 Resp: 123236
Ion Ratio Lower Upper
105 100
120 44.4 22.4 67.3

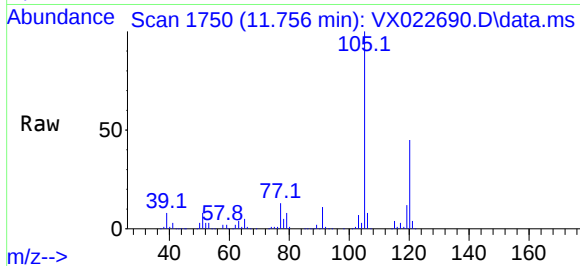

#85
sec-Butylbenzene
Concen: 35.21 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.140 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion:105 Resp: 123236
Ion Ratio Lower Upper
105 100
134 0.0 10.0 29.8#




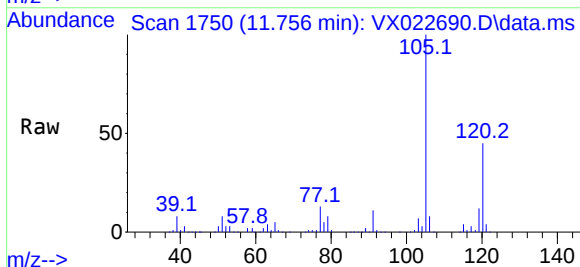




#86
p-Isopropyltoluene
Concen: 0.76 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. -0.037 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:119 Resp: 2205
Ion Ratio Lower Upper
119 100
134 25.8 12.9 38.7
91 25.4 11.7 35.0

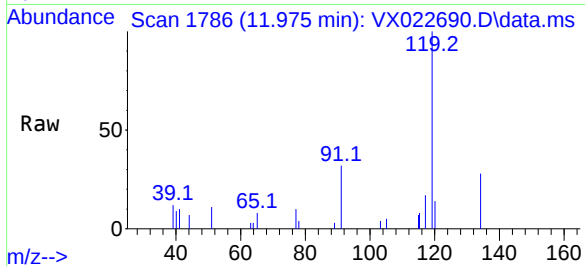

#89
n-Butylbenzene
Concen: 0.83 ug/l
RT: 12.317 min Scan# 1842
Delta R.T. -0.018 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 91 Resp: 2301
Ion Ratio Lower Upper
91 100
92 24.1 27.4 82.0#
134 124.2 13.2 39.5#



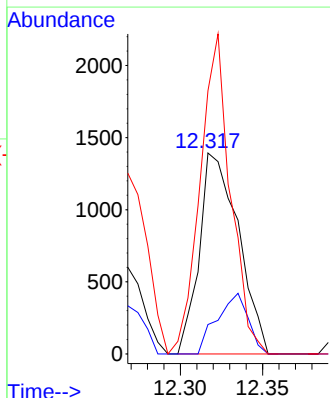
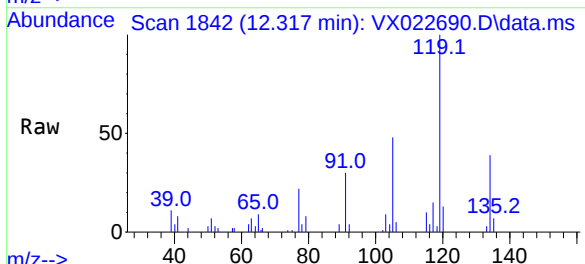




#90
Hexachloroethane
Concen: 5.21 ug/l
RT: 12.616 min Scan# 1891
Delta R.T. 0.074 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:117 Resp: 796
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

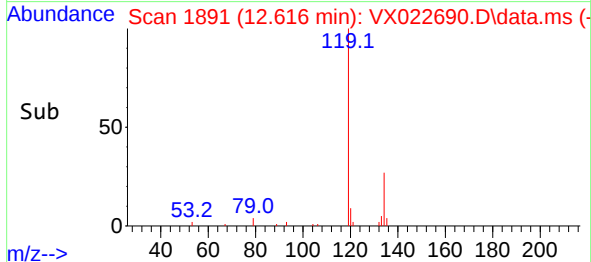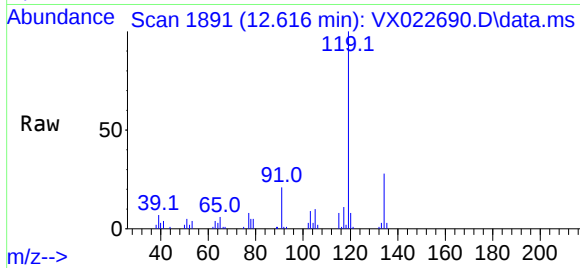

#92
1,2-Dibromo-3-Chloropropane
Concen: 4.01 ug/l
RT: 12.926 min Scan# 1942
Delta R.T. -0.019 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Tgt Ion: 75 Resp: 21
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#

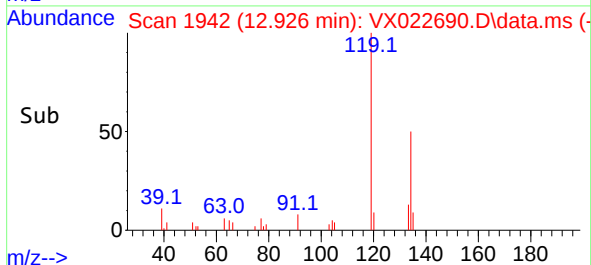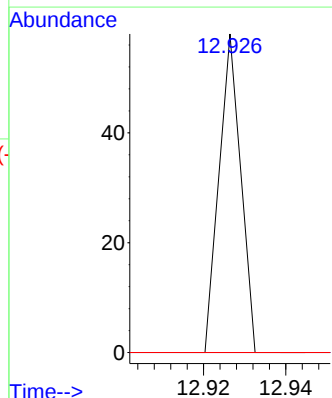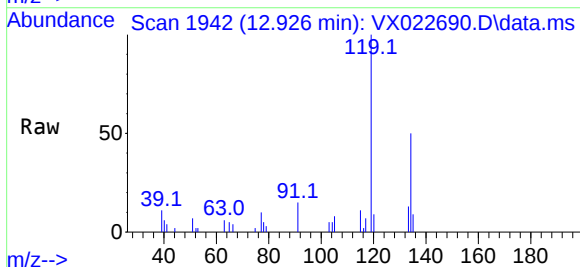



#95
Naphthalene
Concen: 9.36 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX022690.D
Acq: 14 Jun 2021 13:29

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:128	Resp:	28817
Ion Ratio	Lower	Upper
128	100	
127	13.3	10.3 15.5
129	11.5	8.8 13.2

