

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061421\
 Data File : VX022692.D
 Acq On : 14 Jun 2021 14:17
 Operator : JC/MD
 Sample : M2705-01DL 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PRODUCT02-NMW-PS-D3DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M

Title : SW846 8260

Signal : TIC: VX022692.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.569	71	79	82	rBV5	2839	5748	1.37%	0.233%
2	3.617	408	415	422	rBV	8254	17769	4.25%	0.720%
3	4.495	549	559	569	rBV2	36873	96516	23.07%	3.910%
4	5.391	695	706	720	rBV3	66540	197842	47.29%	8.015%
5	5.562	723	734	746	rBV	73594	208260	49.78%	8.437%
6	5.964	790	800	811	rBV2	55425	149753	35.80%	6.067%
7	6.769	921	932	945	rBV	130048	301729	72.13%	12.224%
8	7.135	983	992	1005	rVB	89798	189307	45.25%	7.670%
9	8.653	1234	1241	1249	rBV	275131	418329	100.00%	16.948%
10	10.055	1465	1471	1484	rBV	259159	351958	84.13%	14.259%
11	11.085	1634	1640	1648	rBV	197692	239651	57.29%	9.709%
12	12.024	1789	1794	1801	rBV	238301	285824	68.33%	11.580%
13	12.091	1801	1805	1812	rVB	4466	5609	1.34%	0.227%


Sum of corrected areas: 2468295

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061421\
Data File : VX022692.D
Acq On : 14 Jun 2021 14:17
Operator : JC/MD
Sample : M2705-01DL 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PRODUCT02-NMW-PS-D3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

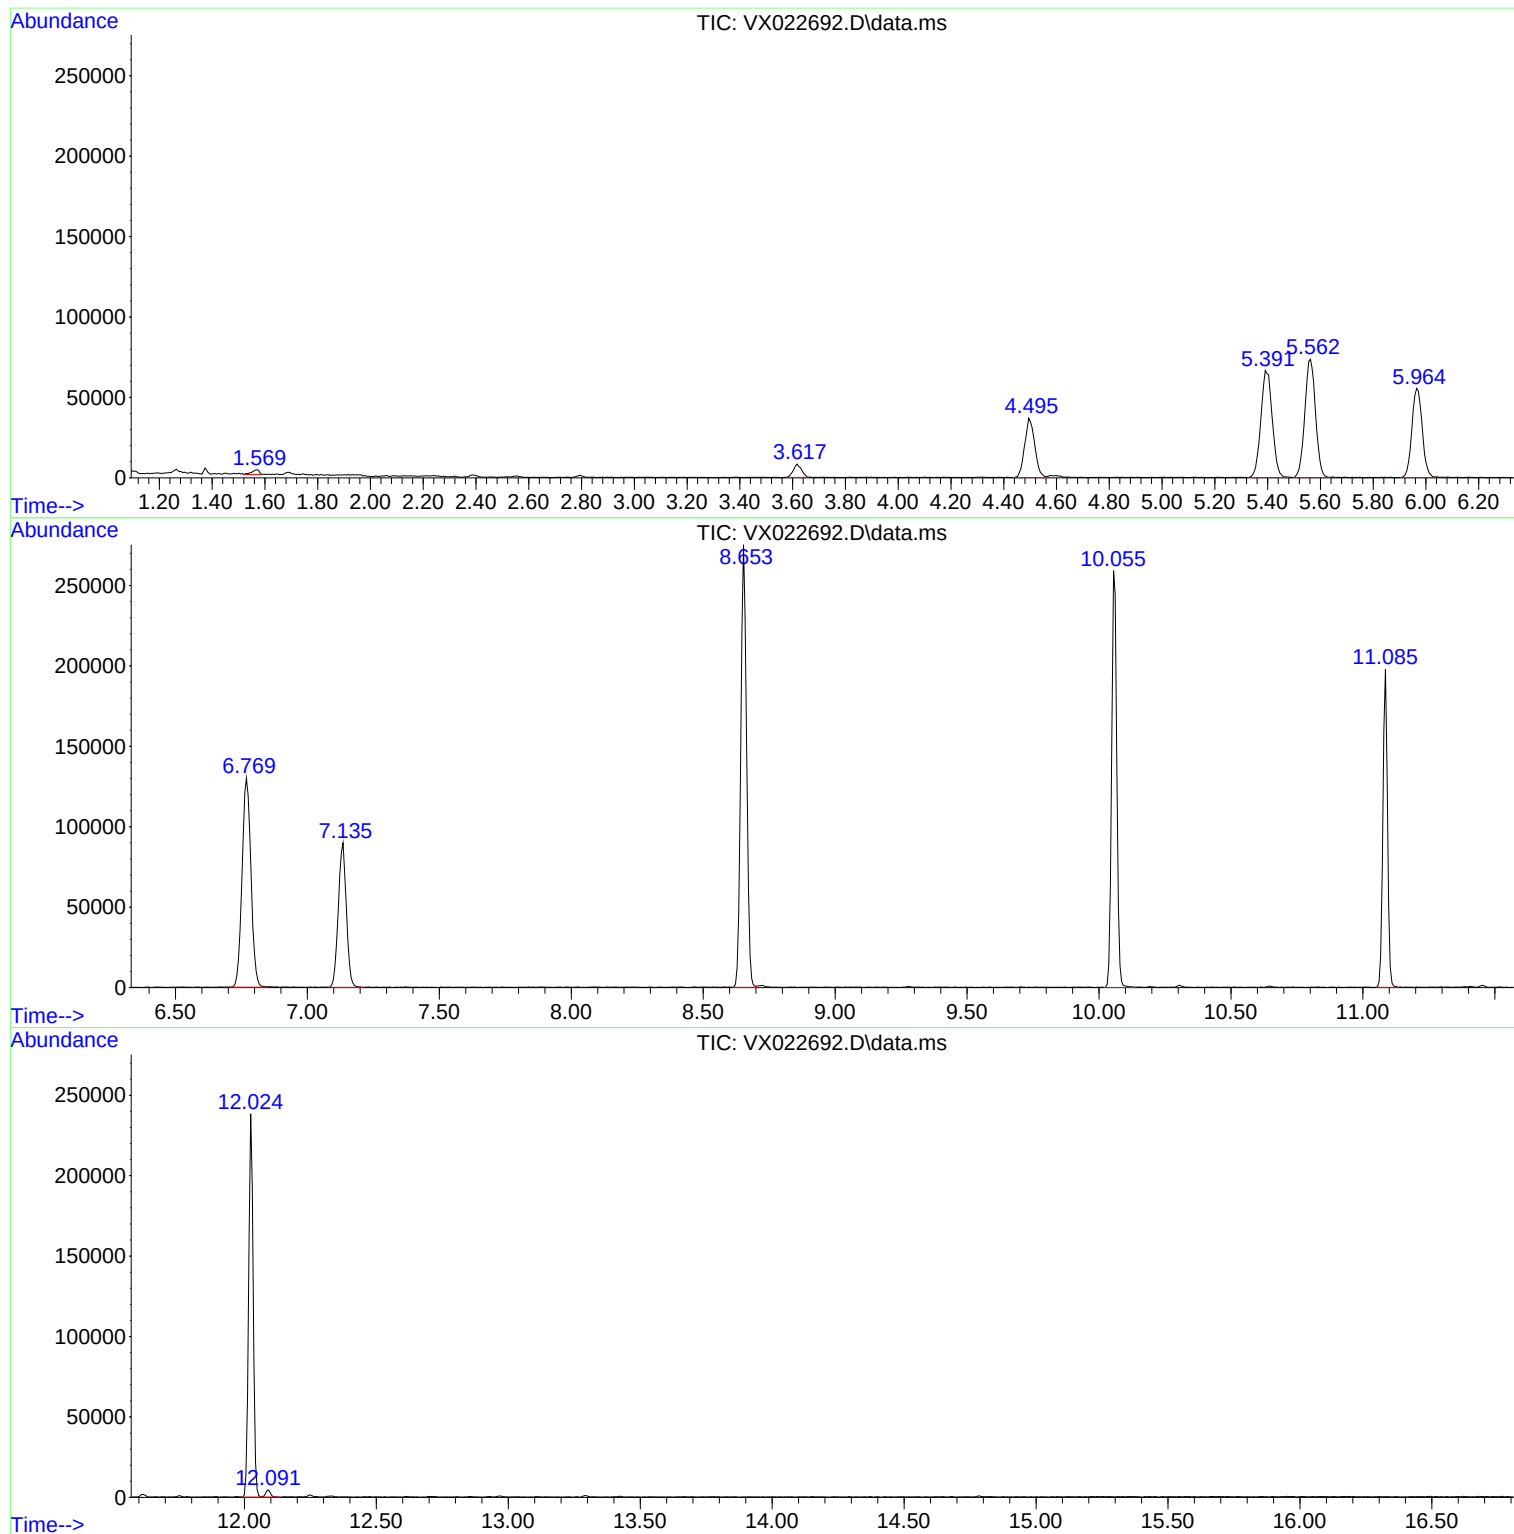

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061421\
Data File : VX022692.D
Acq On : 14 Jun 2021 14:17
Operator : JC/MD
Sample : M2705-01DL 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PRODUCT02-NMW-PS-D3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061421\
Data File : VX022692.D
Acq On : 14 Jun 2021 14:17
Operator : JC/MD
Sample : M2705-01DL 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PRODUCT02-NMW-PS-D3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------