

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029458.D
 Acq On : 14 Jun 2022 12:34
 Operator : JC/MD
 Sample : VX0614WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK660

Quant Time: Jun 15 05:43:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 15 05:41:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	377920	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	341453	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	167210	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	126129	43.105	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.220%
7) Chloroethane-d5	1.666	69	83323	45.821	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.640%
11) 1,1-Dichloroethene-d2	2.306	63	178414	33.842	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.680%
21) 2-Butanone-d5	4.458	46	187172	84.367	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	84.370%
24) Chloroform-d	5.056	84	235747	42.198	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.400%
26) 1,2-Dichloroethane-d4	5.958	65	151714	42.002	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.000%
32) Benzene-d6	5.976	84	498191	46.710	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.420%
36) 1,2-Dichloropropane-d6	7.312	67	144201	46.161	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.320%
41) Toluene-d8	8.653	98	453224	45.074	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.140%
43) trans-1,3-Dichloroprop...	8.952	79	64280	41.730	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.460%
47) 2-Hexanone-d5	9.384	63	146111	86.475	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	86.480%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	201222	43.930	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.860%
66) 1,2-Dichlorobenzene-d4	12.323	152	159361	45.841	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.680%
Target Compounds						
44) trans-1,3-Dichloropropene	8.952	75	2839	0.696	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029458.D
Acq On : 14 Jun 2022 12:34
Operator : JC/MD
Sample : VX0614WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK660

Quant Time: Jun 15 05:43:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 15 05:41:21 2022
Response via : Initial Calibration

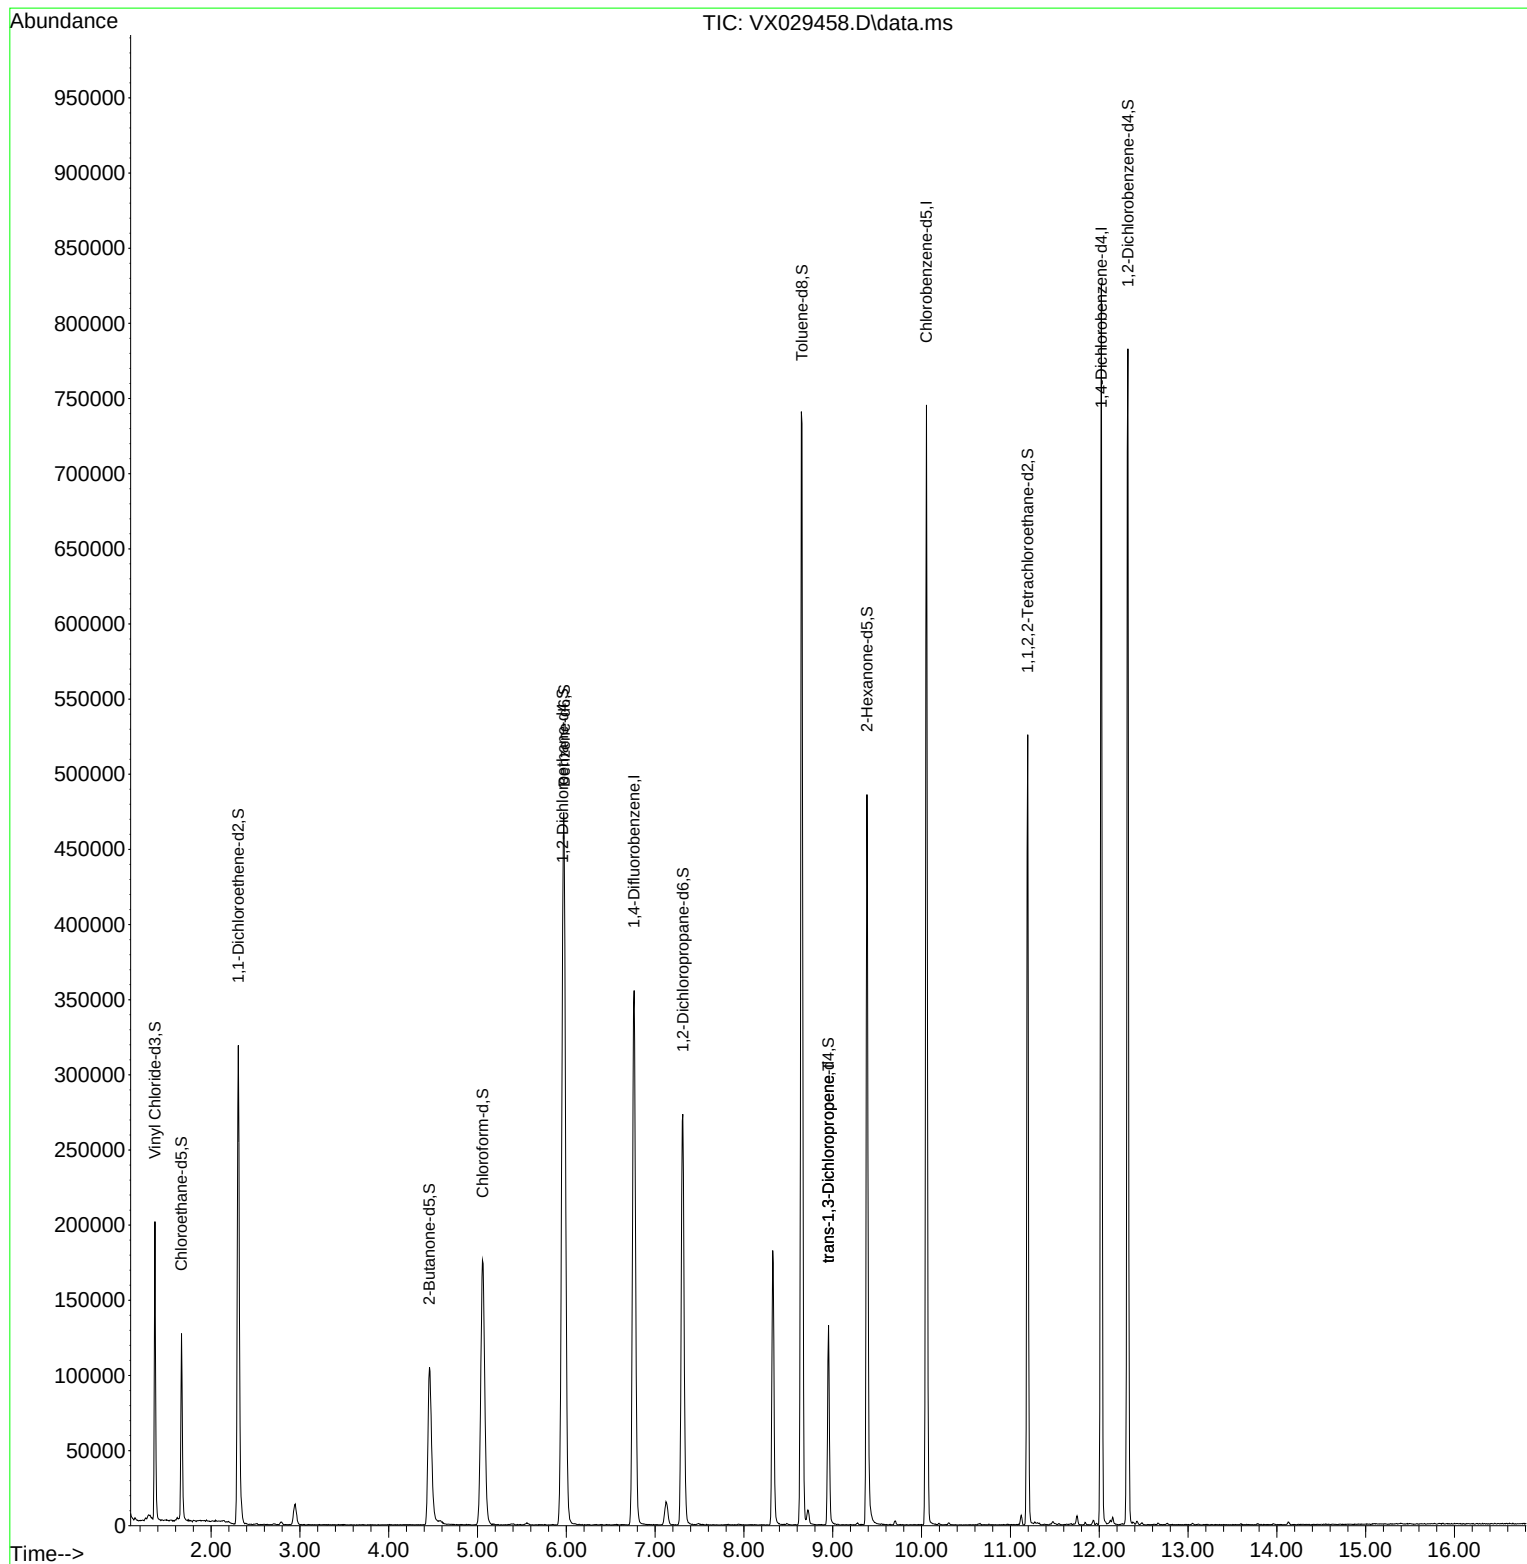

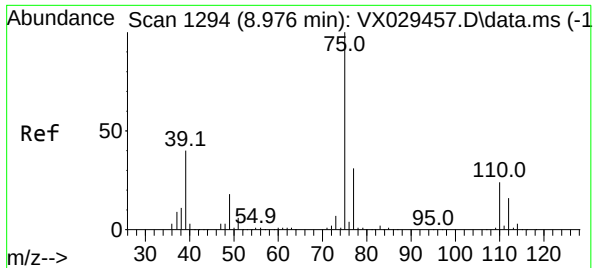

#44
trans-1,3-Dichloropropene
Concen: 0.696 ug/L
RT: 8.952 min Scan# 11
Delta R.T. -0.024 min
Lab File: VX029458.D
Acq: 14 Jun 2022 12:34

Instrument :
MSVOA_X
ClientSampleId :
VBLK660

Tgt Ion: 75 Resp: 2839
Ion Ratio Lower Upper
75 100
77 33.2 22.3 41.3

