

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029467.D
 Acq On : 14 Jun 2022 16:07
 Operator : JC/MD
 Sample : N3254-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Quant Time: Jun 15 05:46:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 15 05:41:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	282793	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	256334	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	118485	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	82815	37.823	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.640%
7) Chloroethane-d5	1.666	69	72639	53.383	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	106.760%
11) 1,1-Dichloroethene-d2	2.306	63	121906	30.902	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.800%
21) 2-Butanone-d5	4.464	46	200999	121.076	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	121.080%
24) Chloroform-d	5.062	84	201174	48.122	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.240%
26) 1,2-Dichloroethane-d4	5.964	65	145623	53.878	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.760%
32) Benzene-d6	5.976	84	400795	50.057	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.120%
36) 1,2-Dichloropropane-d6	7.311	67	127287	54.277	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	108.560%
41) Toluene-d8	8.652	98	350013	46.368	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.740%
43) trans-1,3-Dichloroprop...	8.951	79	55263	47.790	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.580%
47) 2-Hexanone-d5	9.390	63	154033	121.436	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	121.440%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	194440	56.545	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	113.080%
66) 1,2-Dichlorobenzene-d4	12.323	152	124551	50.562	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.120%
Target Compounds						
					Qvalue	
37) 1,2-Dichloropropane	7.311	63	14448	7.070	ug/L	# 85
44) trans-1,3-Dichloropropene	8.951	75	2749	0.897	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029467.D
Acq On : 14 Jun 2022 16:07
Operator : JC/MD
Sample : N3254-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Time: Jun 15 05:46:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM061322WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 15 05:41:21 2022
Response via : Initial Calibration

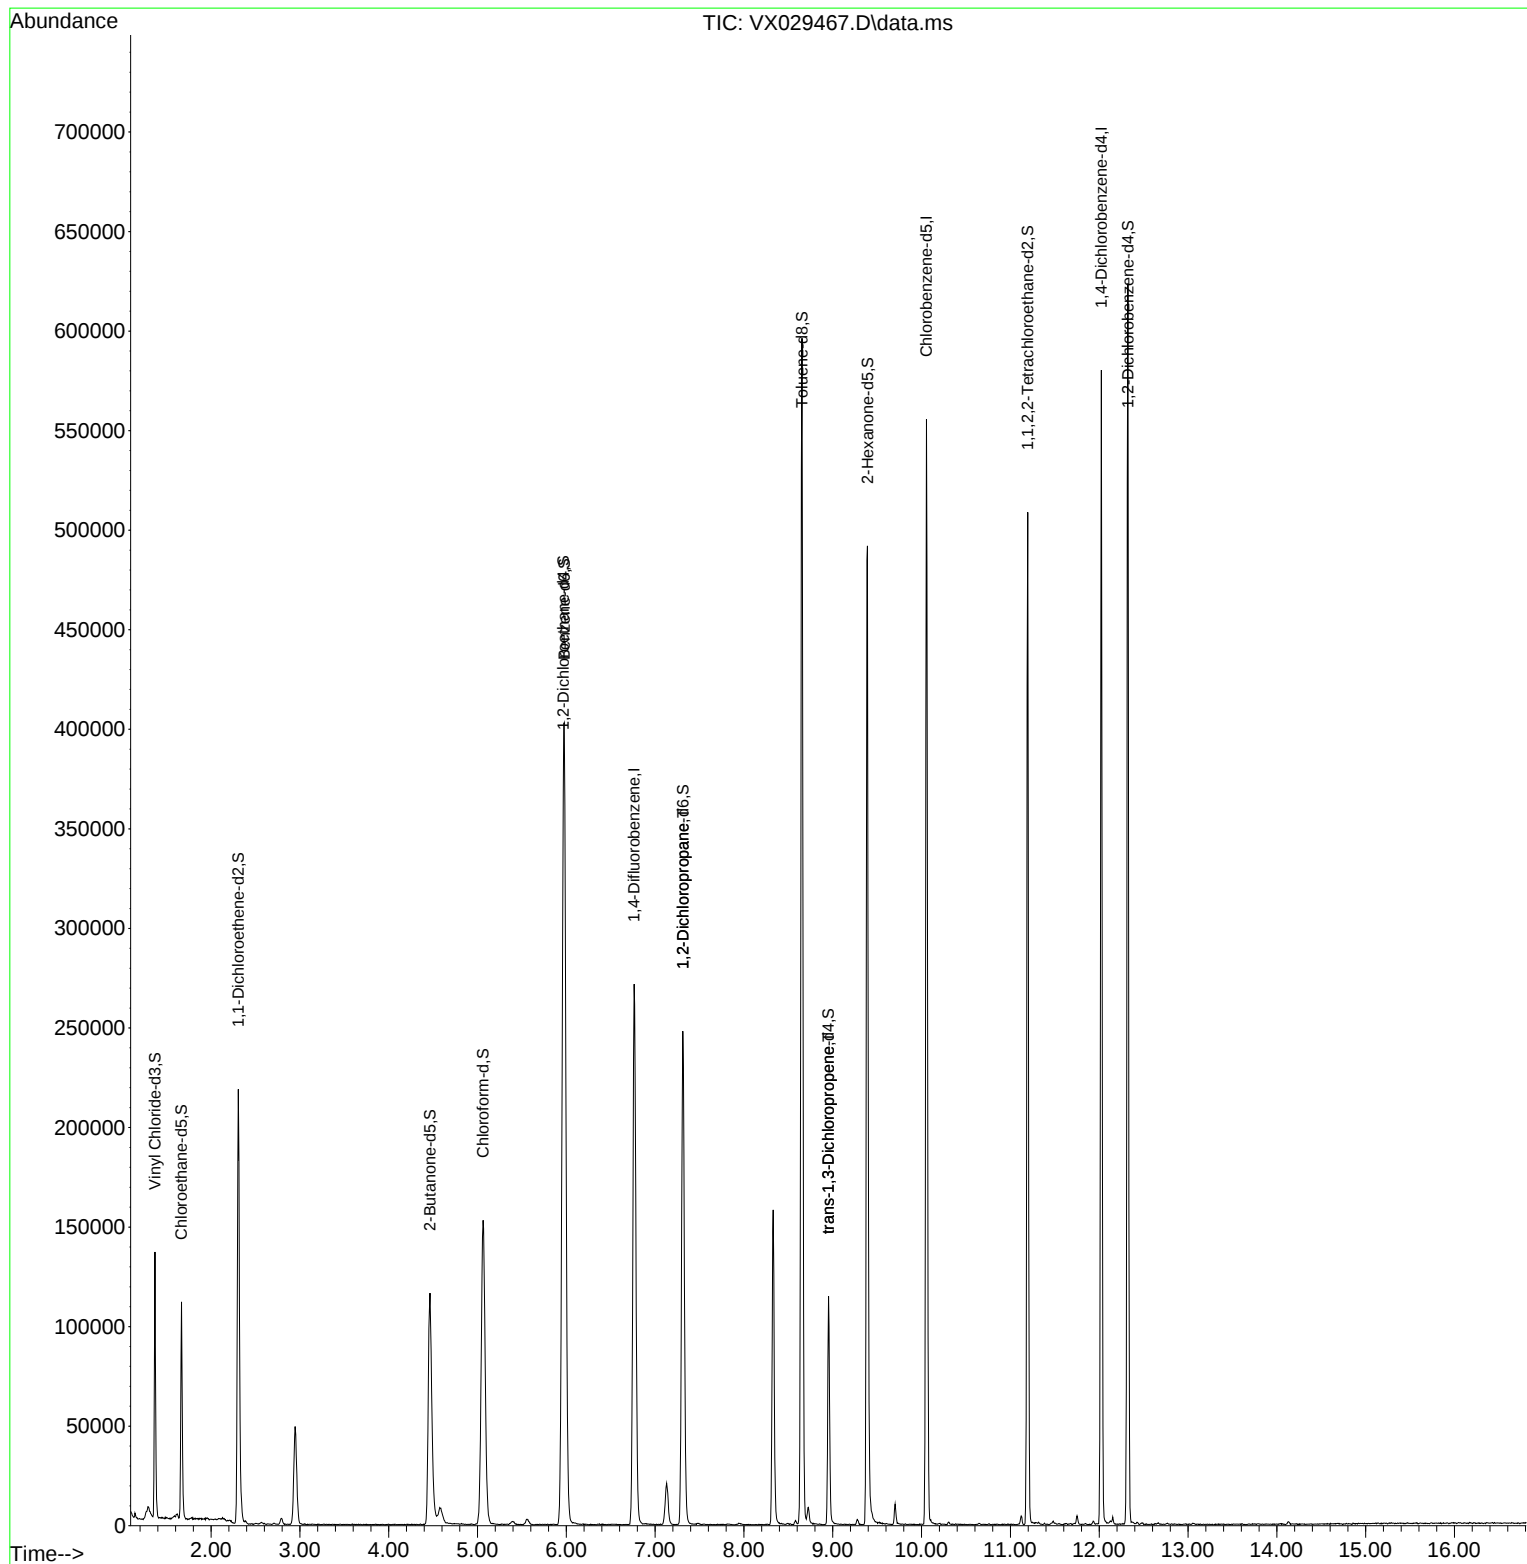

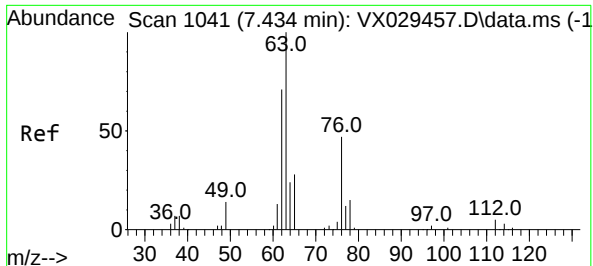

#37

1,2-Dichloropropane

Concen: 7.070 ug/L

RT: 7.311 min Scan# 10

Delta R.T. -0.122 min

Lab File: VX029467.D

Acq: 14 Jun 2022 16:07

Instrument :

MSVOA_X

ClientSampleId :





VHBLK001

Tgt Ion: 63 Resp: 14448

Ion Ratio Lower Upper

63 100

112 0.0 3.8 5.8#

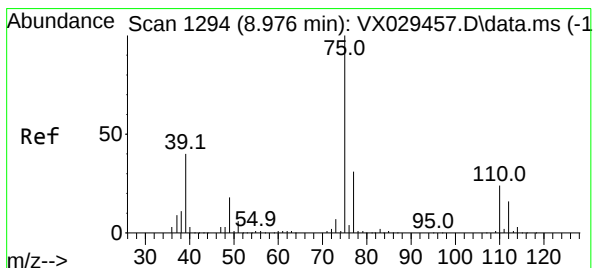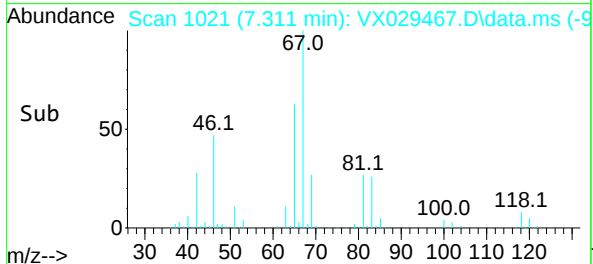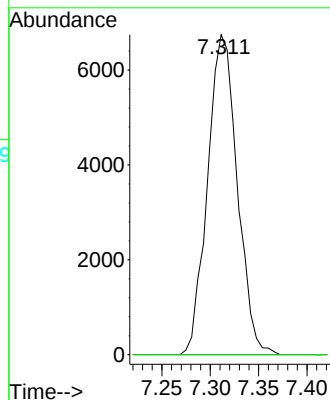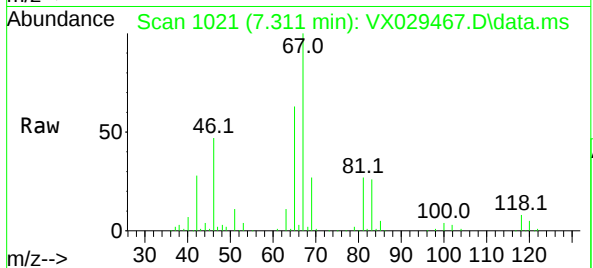

#44

trans-1,3-Dichloropropene

Concen: 0.897 ug/L

RT: 8.951 min Scan# 1290

Delta R.T. -0.025 min

Lab File: VX029467.D

Acq: 14 Jun 2022 16:07

Tgt Ion: 75 Resp: 2749

Ion Ratio Lower Upper

75 100

77 31.4 22.3 41.3

