

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029472.D
 Acq On : 14 Jun 2022 18:04
 Operator : JC/MD
 Sample : N3311-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0E07

Quant Time: Jun 15 05:48:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 15 05:41:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	352514	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	311096	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	150840	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	117663	43.110	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	86.220%	
7) Chloroethane-d5	1.666	69	90816	53.541	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	107.080%	
11) 1,1-Dichloroethene-d2	2.306	63	167851	34.133	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	68.260%	
21) 2-Butanone-d5	4.458	46	201099	97.178	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	97.180%	
24) Chloroform-d	5.062	84	233008	44.713	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	89.420%	
26) 1,2-Dichloroethane-d4	5.964	65	150559	44.687	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	89.380%	
32) Benzene-d6	5.976	84	479316	49.326	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.660%	
36) 1,2-Dichloropropane-d6	7.312	67	142169	49.951	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	99.900%	
41) Toluene-d8	8.653	98	431695	47.122	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	94.240%	
43) trans-1,3-Dichloroprop...	8.952	79	59941	42.711	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	85.420%	
47) 2-Hexanone-d5	9.384	63	153242	99.546	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	99.550%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	203842	48.844	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	97.680%	
66) 1,2-Dichlorobenzene-d4	12.323	152	150153	47.880	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	95.760%	
Target Compounds						
44) trans-1,3-Dichloropropene	8.952	75	2898	0.779	ug/L	Qvalue # 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029472.D
Acq On : 14 Jun 2022 18:04
Operator : JC/MD
Sample : N3311-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0E07

Quant Time: Jun 15 05:48:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 15 05:41:21 2022
Response via : Initial Calibration

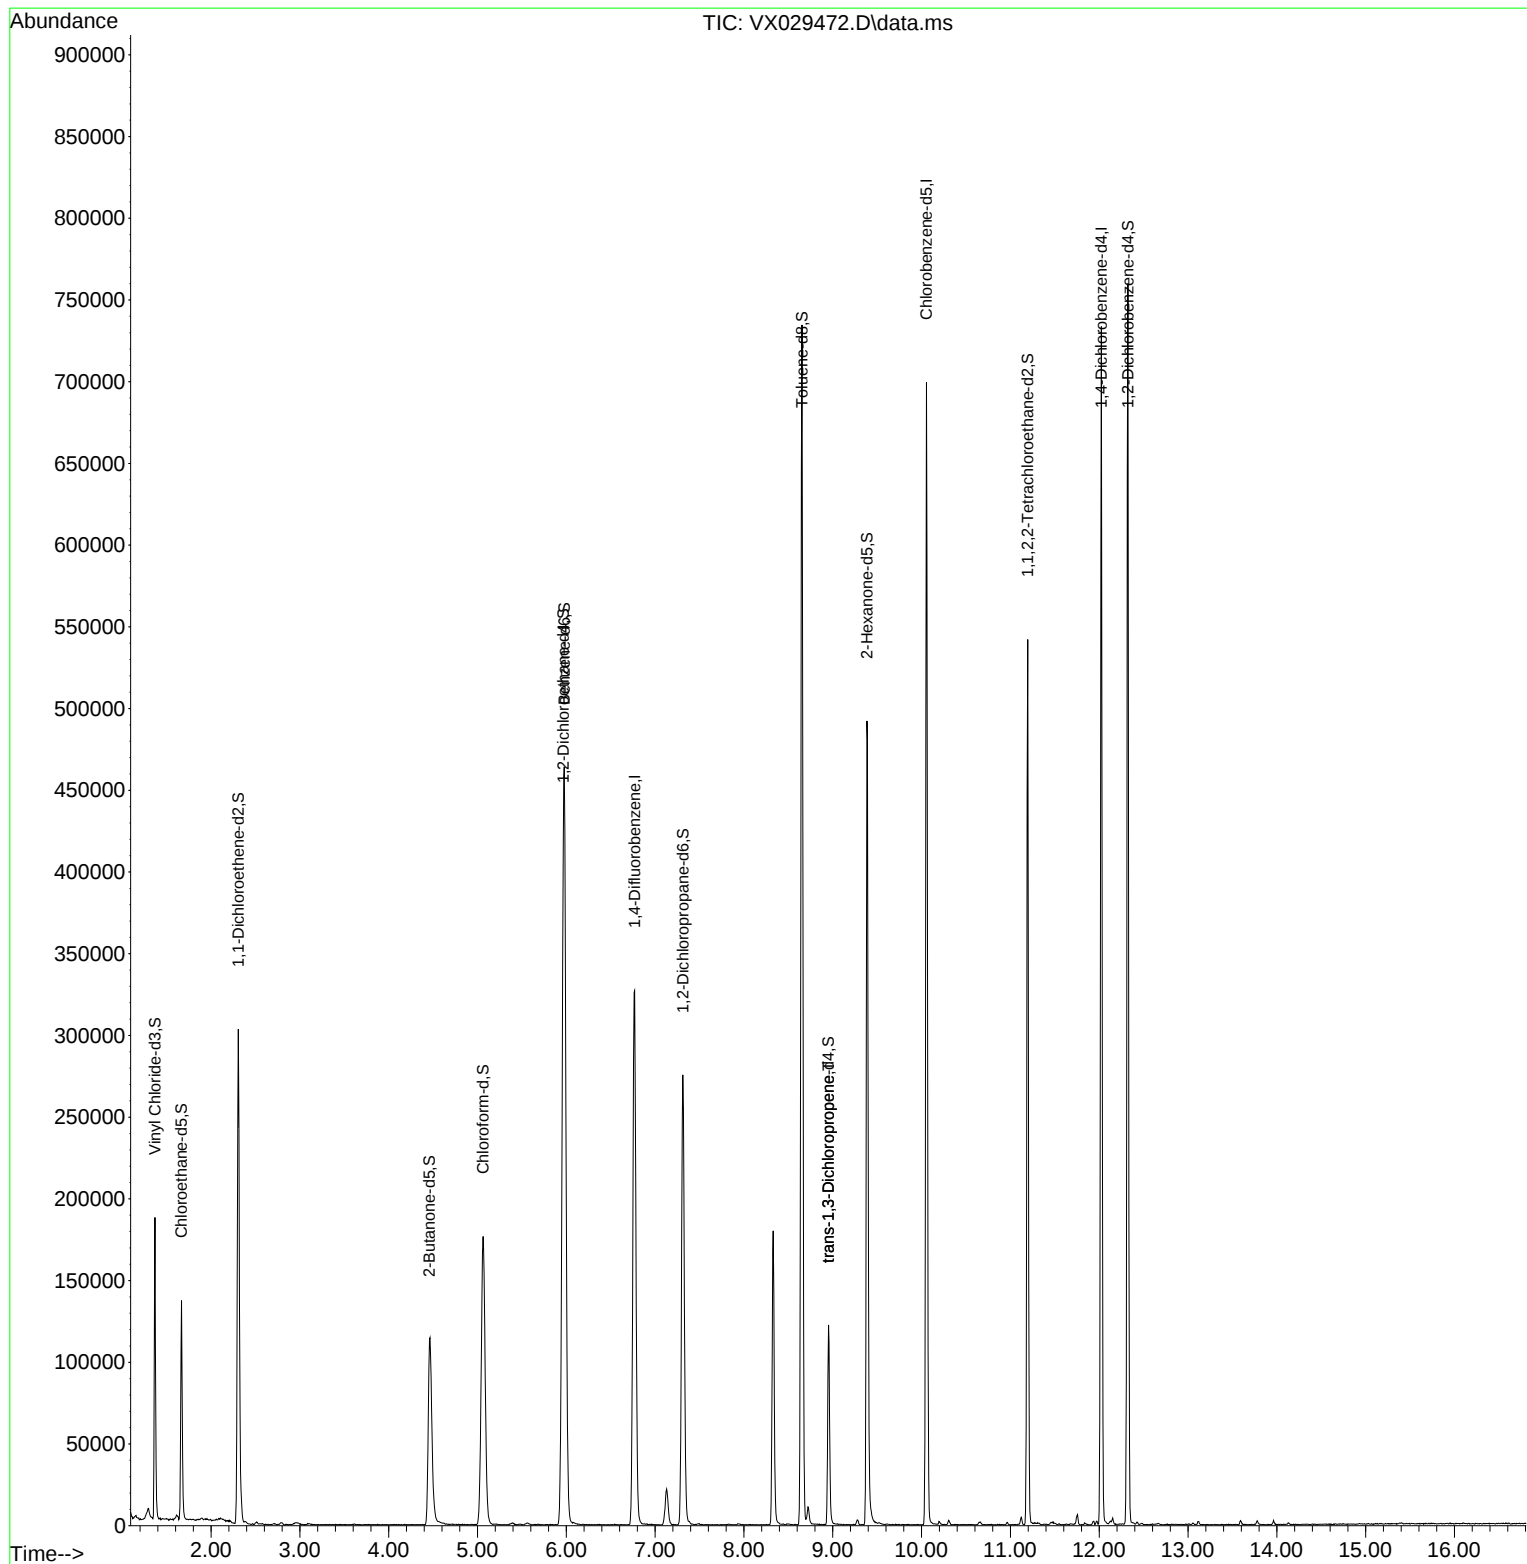

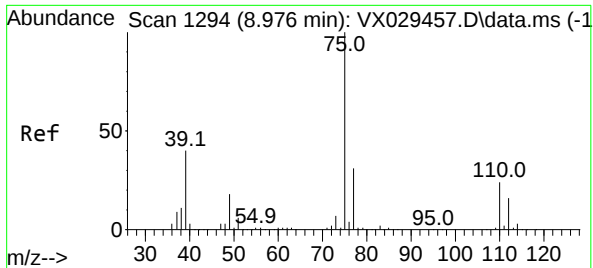

#44
trans-1,3-Dichloropropene
Concen: 0.779 ug/L
RT: 8.952 min Scan# 11
Delta R.T. -0.024 min
Lab File: VX029472.D
Acq: 14 Jun 2022 18:04

Instrument :
MSVOA_X
ClientSampleId :
C0E07

Tgt Ion: 75 Resp: 2898
Ion Ratio Lower Upper
75 100
77 41.5 22.3 41.3#

