

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029486.D
 Acq On : 14 Jun 2022 23:29
 Operator : JC/MD
 Sample : N3313-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Quant Time: Jun 15 07:16:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 15 07:14:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	337083	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	304304	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	143347	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	115186	44.134	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.260%
7) Chloroethane-d5	1.666	69	89137	54.957	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	109.920%
11) 1,1-Dichloroethene-d2	2.306	63	166662	35.443	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.880%
21) 2-Butanone-d5	4.458	46	195001	98.545	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.540%
24) Chloroform-d	5.068	84	227566	45.668	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.340%
26) 1,2-Dichloroethane-d4	5.958	65	147556	45.800	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.600%
32) Benzene-d6	5.976	84	474765	49.948	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.900%
36) 1,2-Dichloropropane-d6	7.311	67	139371	50.061	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.120%
41) Toluene-d8	8.653	98	431172	48.115	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.240%
43) trans-1,3-Dichloroprop...	8.951	79	56667	41.279	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.560%
47) 2-Hexanone-d5	9.384	63	148999	98.950	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	98.950%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	198424	48.607	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.220%
66) 1,2-Dichlorobenzene-d4	12.323	152	150484	50.494	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.980%
Target Compounds						
61) 1,2,3-Trichloropropane	12.024	75	17633	5.881	ug/L	Qvalue # 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029486.D
Acq On : 14 Jun 2022 23:29
Operator : JC/MD
Sample : N3313-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Time: Jun 15 07:16:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 15 07:14:08 2022
Response via : Initial Calibration

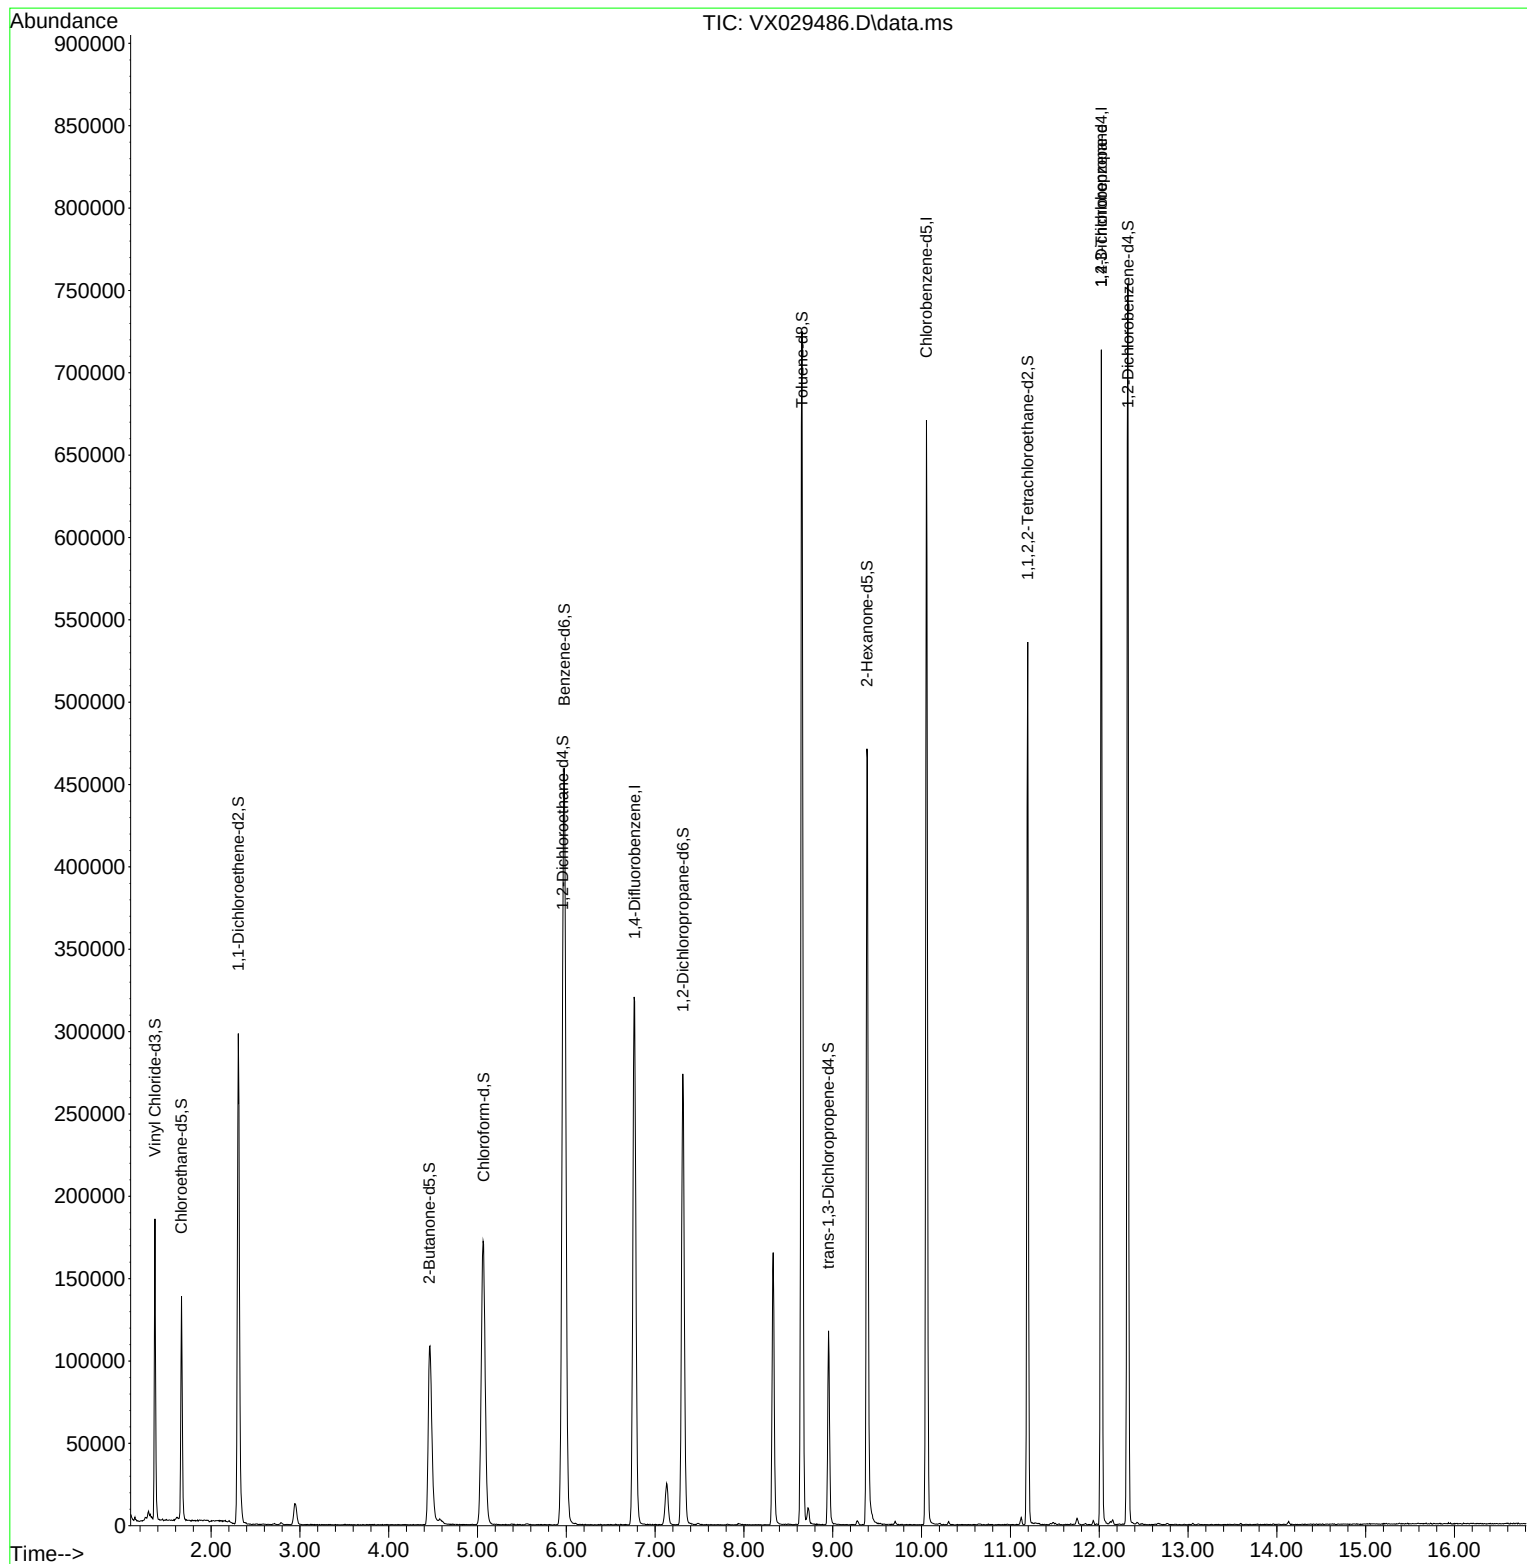

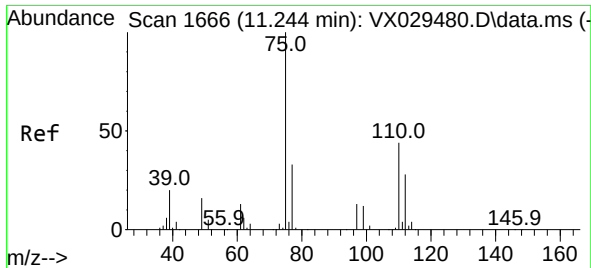

#61
 1,2,3-Trichloropropane
 Concen: 5.881 ug/L
 RT: 12.024 min Scan# 11
 Delta R.T. 0.781 min
 Lab File: VX029486.D
 Acq: 14 Jun 2022 23:29

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Tgt Ion: 75 Resp: 17633
 Ion Ratio Lower Upper
 75 100
 77 32.2 25.8 38.6
 110 3.1 33.4 50.0#

