

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029495.D
 Acq On : 15 Jun 2022 02:59
 Operator : JC/MD
 Sample : N3226-16ME
 Misc : 5.75g/5mL/100uL/5.03mL/MSVOA_X/MEOH
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW4N6ME

Quant Time: Jun 15 07:18:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 15 07:14:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	323761	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	285651	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	135192	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	62813	25.058	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	50.120%#		
7) Chloroethane-d5	1.666	69	26740	17.165	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	34.320%#		
11) 1,1-Dichloroethene-d2	2.282	63	88034	19.492	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	38.980%#		
21) 2-Butanone-d5	4.501	46	145763	76.693	ug/L	0.04
Spiked Amount 100.000	Range 40 - 130		Recovery =	76.690%		
24) Chloroform-d	5.068	84	150403	31.425	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	62.840%#		
26) 1,2-Dichloroethane-d4	5.958	65	105291	34.026	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	68.060%#		
32) Benzene-d6	5.970	84	295216	33.087	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	66.180%#		
36) 1,2-Dichloropropane-d6	7.311	67	95914	36.702	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	73.400%		
41) Toluene-d8	8.652	98	251432	29.890	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	59.780%#		
43) trans-1,3-Dichloroprop...	8.957	79	31071	24.112	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	48.220%#		
47) 2-Hexanone-d5	9.402	63	105592	74.703	ug/L	0.01
Spiked Amount 100.000	Range 45 - 130		Recovery =	74.700%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	134864	35.194	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	70.380%		
66) 1,2-Dichlorobenzene-d4	12.323	152	97439	34.667	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	69.340%#		
Target Compounds						Qvalue
15) Methyl Acetate	2.727	43	5490	2.185	ug/L #	88
35) Methylcyclohexane	7.378	83	2655	0.639	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029495.D
Acq On : 15 Jun 2022 02:59
Operator : JC/MD
Sample : N3226-16ME
Misc : 5.75g/5mL/100uL/5.03mL/MSVOA_X/MEOH
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW4N6ME

Quant Time: Jun 15 07:18:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 15 07:14:08 2022
Response via : Initial Calibration




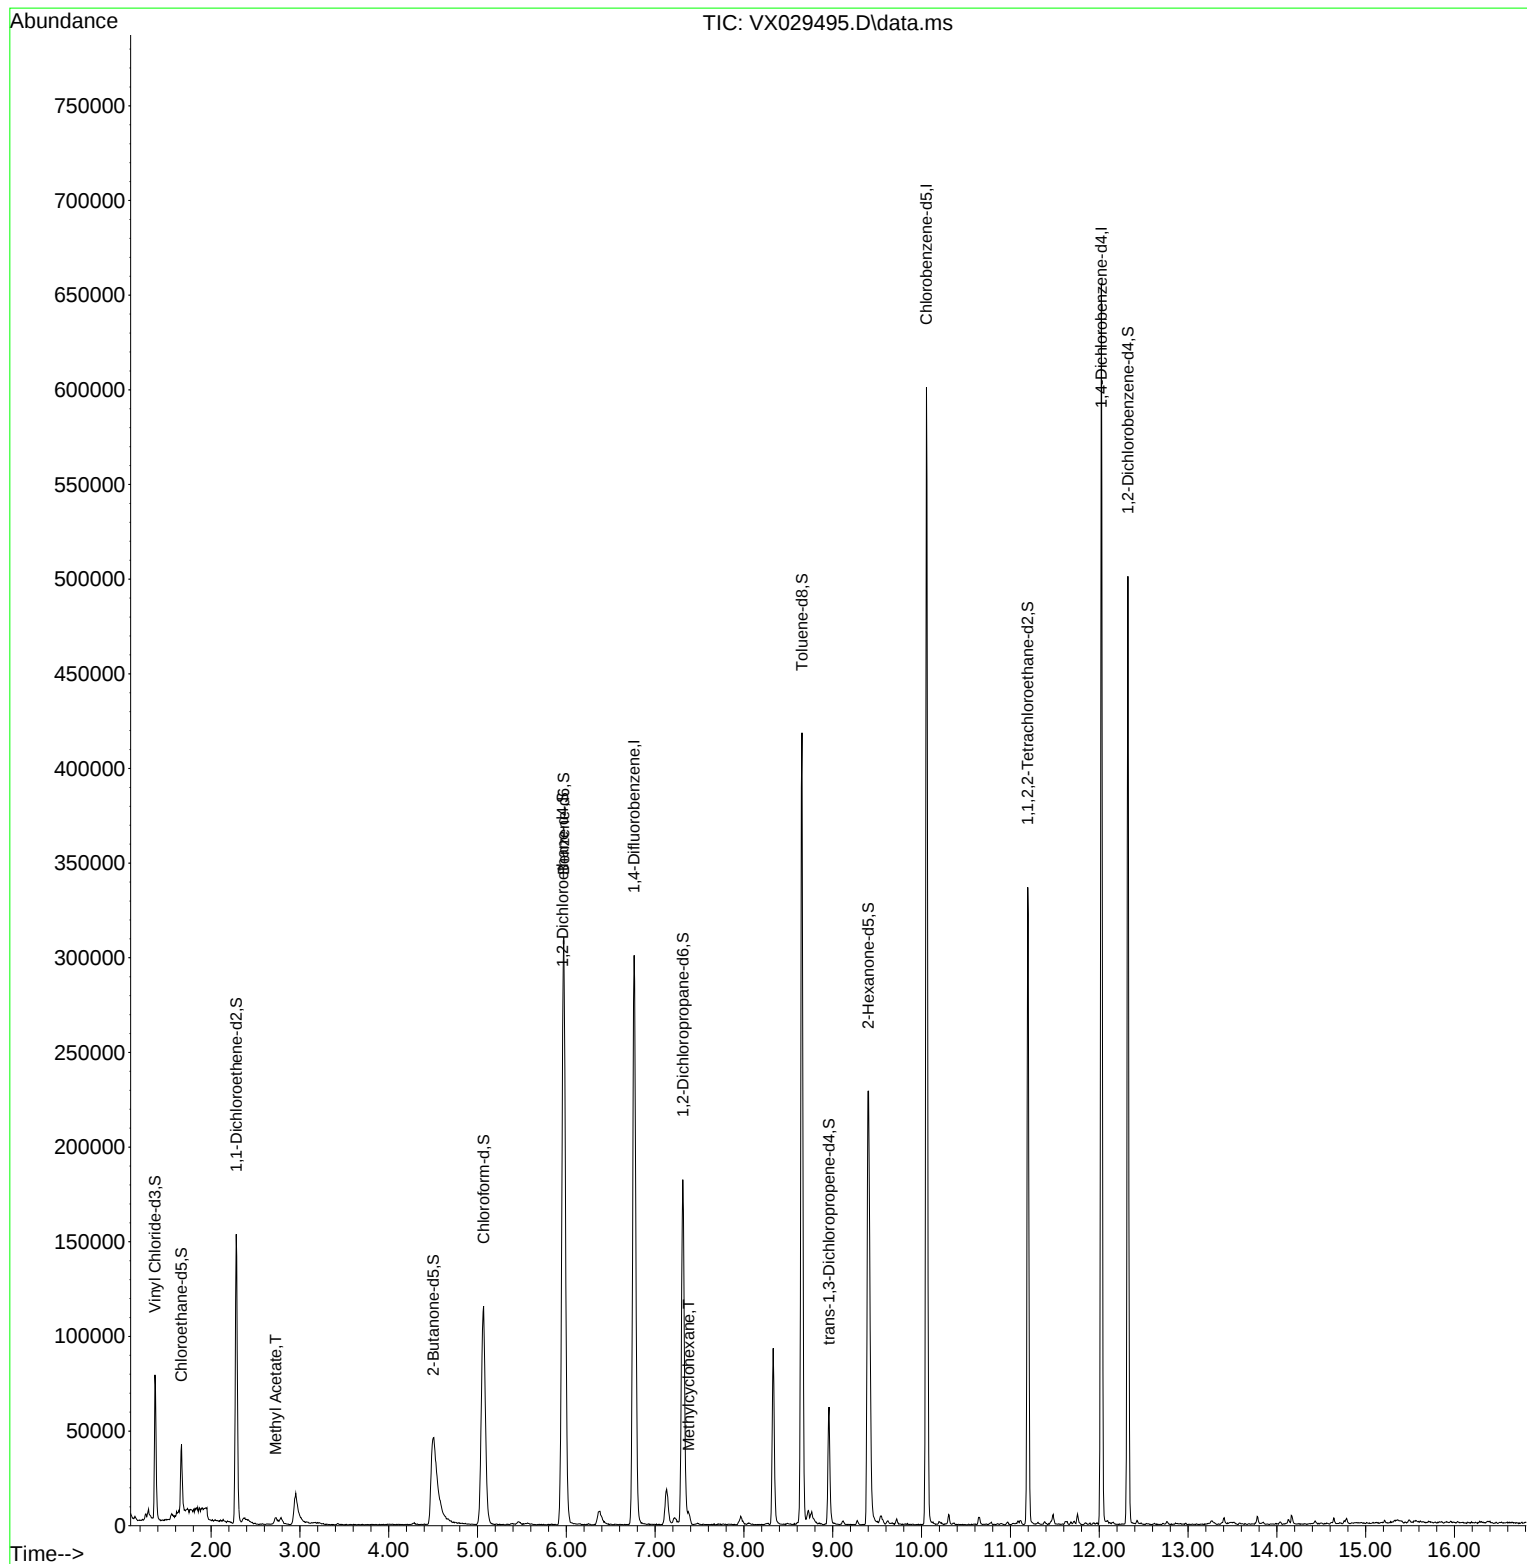


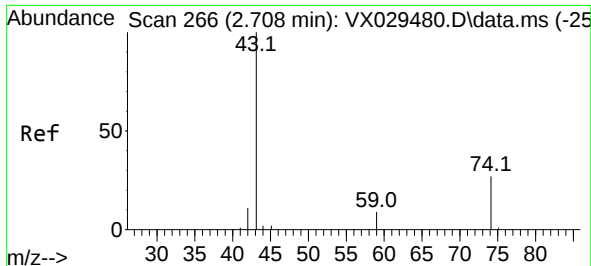

#15
Methyl Acetate
Concen: 2.185 ug/L
RT: 2.727 min Scan# 21
Delta R.T. 0.018 min
Lab File: VX029495.D
Acq: 15 Jun 2022 02:59

Instrument :
MSVOA_X
ClientSampleId :
EW4N6ME

Tgt Ion: 43 Resp: 5490
Ion Ratio Lower Upper
43 100
74 17.2 18.2 27.4#

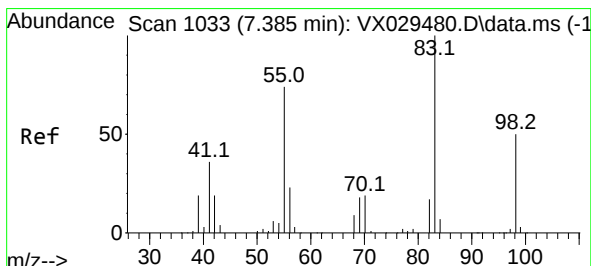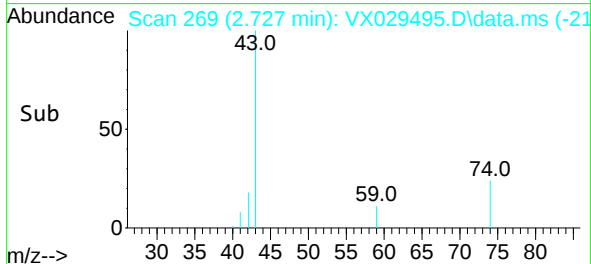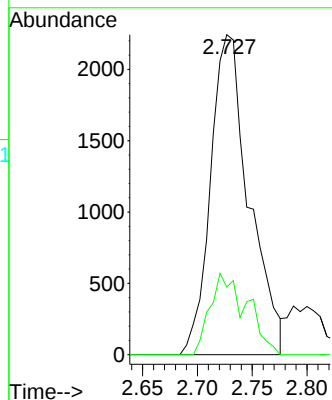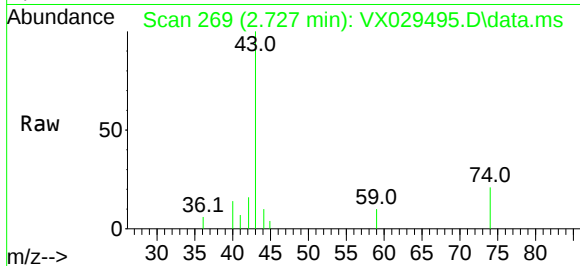

#35
Methylcyclohexane
Concen: 0.639 ug/L
RT: 7.378 min Scan# 1032
Delta R.T. -0.006 min
Lab File: VX029495.D
Acq: 15 Jun 2022 02:59

Tgt Ion: 83 Resp: 2655
Ion Ratio Lower Upper
83 100
55 77.9 60.6 90.8
98 50.9 39.8 59.8

