

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029498.D
 Acq On : 15 Jun 2022 04:08
 Operator : JC/MD
 Sample : N3292-01ME
 Misc : 6.24g/5mL/100uL/5.06mL/MSVOA_X/MEOH
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW4P2ME

Quant Time: Jun 15 07:19:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 15 07:14:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	362157	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	320416	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	154476	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	77430	27.614	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	55.220%#
7) Chloroethane-d5	1.666	69	35255	20.231	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	40.460%#
11) 1,1-Dichloroethene-d2	2.282	63	112335	22.235	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	44.480%#
21) 2-Butanone-d5	4.495	46	184716	86.884	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.880%
24) Chloroform-d	5.062	84	193893	36.217	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	72.440%
26) 1,2-Dichloroethane-d4	5.964	65	134461	38.846	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.700%
32) Benzene-d6	5.970	84	382880	38.256	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	76.520%
36) 1,2-Dichloropropane-d6	7.312	67	121586	41.477	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	82.960%
41) Toluene-d8	8.653	98	324940	34.437	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	68.880%#
43) trans-1,3-Dichloroprop...	8.952	79	40029	27.693	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	55.380%#
47) 2-Hexanone-d5	9.397	63	139406	87.924	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	87.920%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	177344	41.259	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	82.520%
66) 1,2-Dichlorobenzene-d4	12.323	152	126530	39.398	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	78.800%#
Target Compounds						Qvalue
15) Methyl Acetate	2.727	43	4804	1.709	ug/L	97
37) 1,2-Dichloropropane	7.312	63	14033	5.494	ug/L	# 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029498.D
Acq On : 15 Jun 2022 04:08
Operator : JC/MD
Sample : N3292-01ME
Misc : 6.24g/5mL/100uL/5.06mL/MSVOA_X/MEOH
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW4P2ME

Quant Time: Jun 15 07:19:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 15 07:14:08 2022
Response via : Initial Calibration




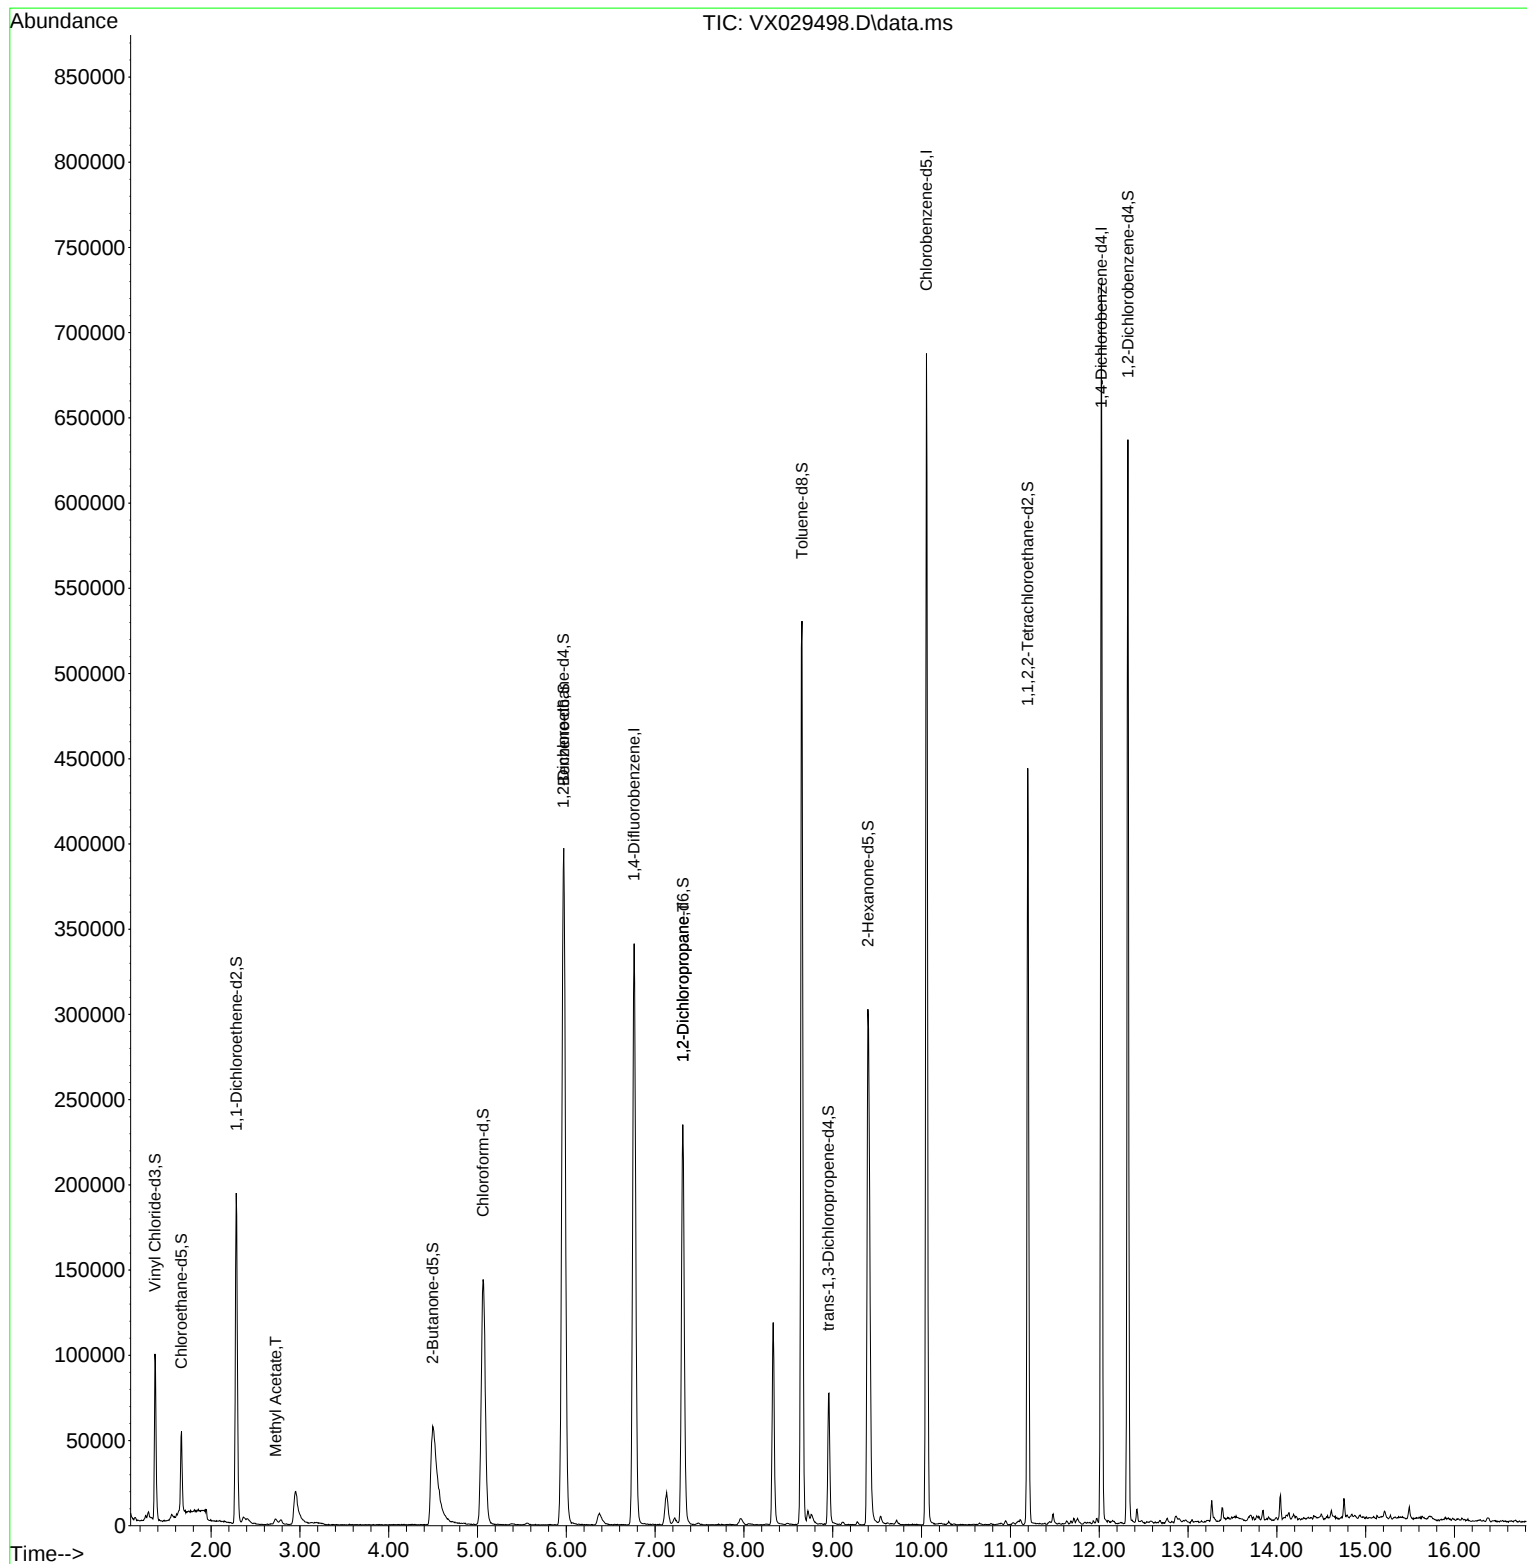


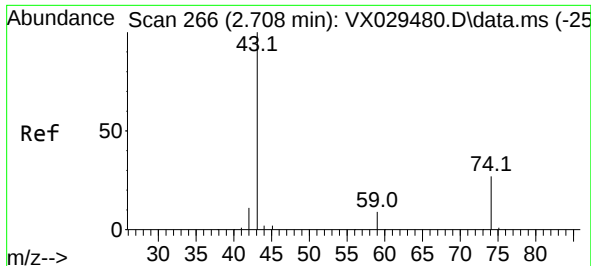

#15
Methyl Acetate
Concen: 1.709 ug/L
RT: 2.727 min Scan# 21
Delta R.T. 0.019 min
Lab File: VX029498.D
Acq: 15 Jun 2022 04:08

Instrument :
MSVOA_X
ClientSampleId :
EW4P2ME

Tgt Ion: 43 Resp: 4804
Ion Ratio Lower Upper
43 100
74 24.4 18.2 27.4

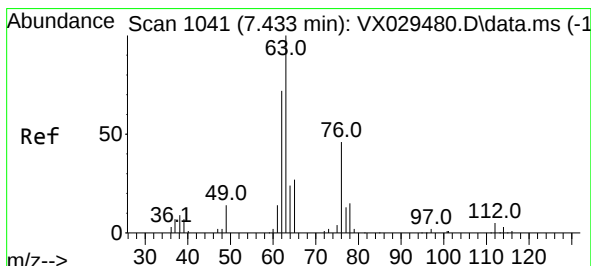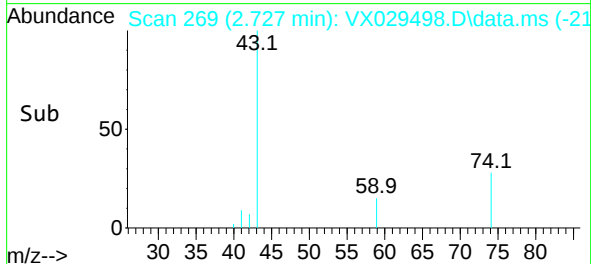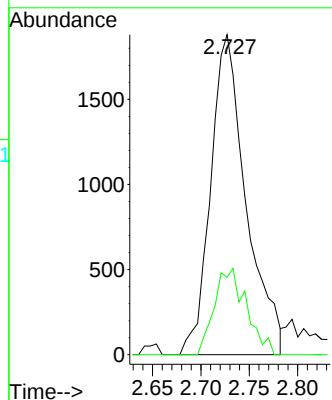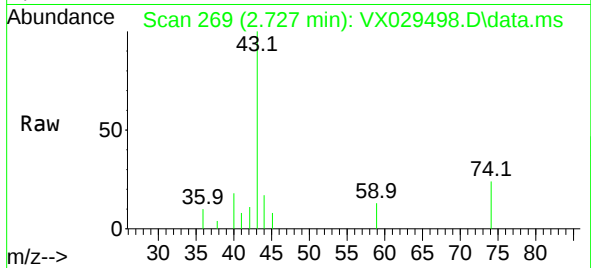

#37
1,2-Dichloropropane
Concen: 5.494 ug/L
RT: 7.312 min Scan# 1021
Delta R.T. -0.122 min
Lab File: VX029498.D
Acq: 15 Jun 2022 04:08

Tgt Ion: 63 Resp: 14033
Ion Ratio Lower Upper
63 100
112 0.0 3.8 5.8#

