

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029499.D
 Acq On : 15 Jun 2022 04:31
 Operator : JC/MD
 Sample : N3292-03ME
 Misc : 7.16g/5mL/100uL/5.07mL/MSVOA_X/MEOH
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW4P4ME

Quant Time: Jun 15 07:19:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 15 07:14:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	364903	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	310653	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	141739	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	64314	22.764	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	45.520%#
7) Chloroethane-d5	1.666	69	28750	16.374	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	32.740%#
11) 1,1-Dichloroethene-d2	2.282	63	90129	17.706	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	35.420%#
21) 2-Butanone-d5	4.507	46	156279	72.955	ug/L	0.04
Spiked Amount	100.000	Range	40 - 130	Recovery	=	72.960%
24) Chloroform-d	5.068	84	165287	30.641	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	61.280%#
26) 1,2-Dichloroethane-d4	5.964	65	114148	32.729	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	65.460%#
32) Benzene-d6	5.971	84	321421	33.124	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	66.240%#
36) 1,2-Dichloropropane-d6	7.312	67	104312	36.703	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	73.400%
41) Toluene-d8	8.653	98	266888	29.174	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	58.340%#
43) trans-1,3-Dichloroprop...	8.952	79	32091	22.899	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	45.800%#
47) 2-Hexanone-d5	9.403	63	116560	75.825	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	75.830%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	149299	35.826	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	71.660%
66) 1,2-Dichlorobenzene-d4	12.323	152	103340	35.069	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	70.140%#
Target Compounds						Qvalue
37) 1,2-Dichloropropane	7.306	63	11373	4.592	ug/L	# 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029499.D
Acq On : 15 Jun 2022 04:31
Operator : JC/MD
Sample : N3292-03ME
Misc : 7.16g/5mL/100uL/5.07mL/MSVOA_X/MEOH
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW4P4ME

Quant Time: Jun 15 07:19:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 15 07:14:08 2022
Response via : Initial Calibration

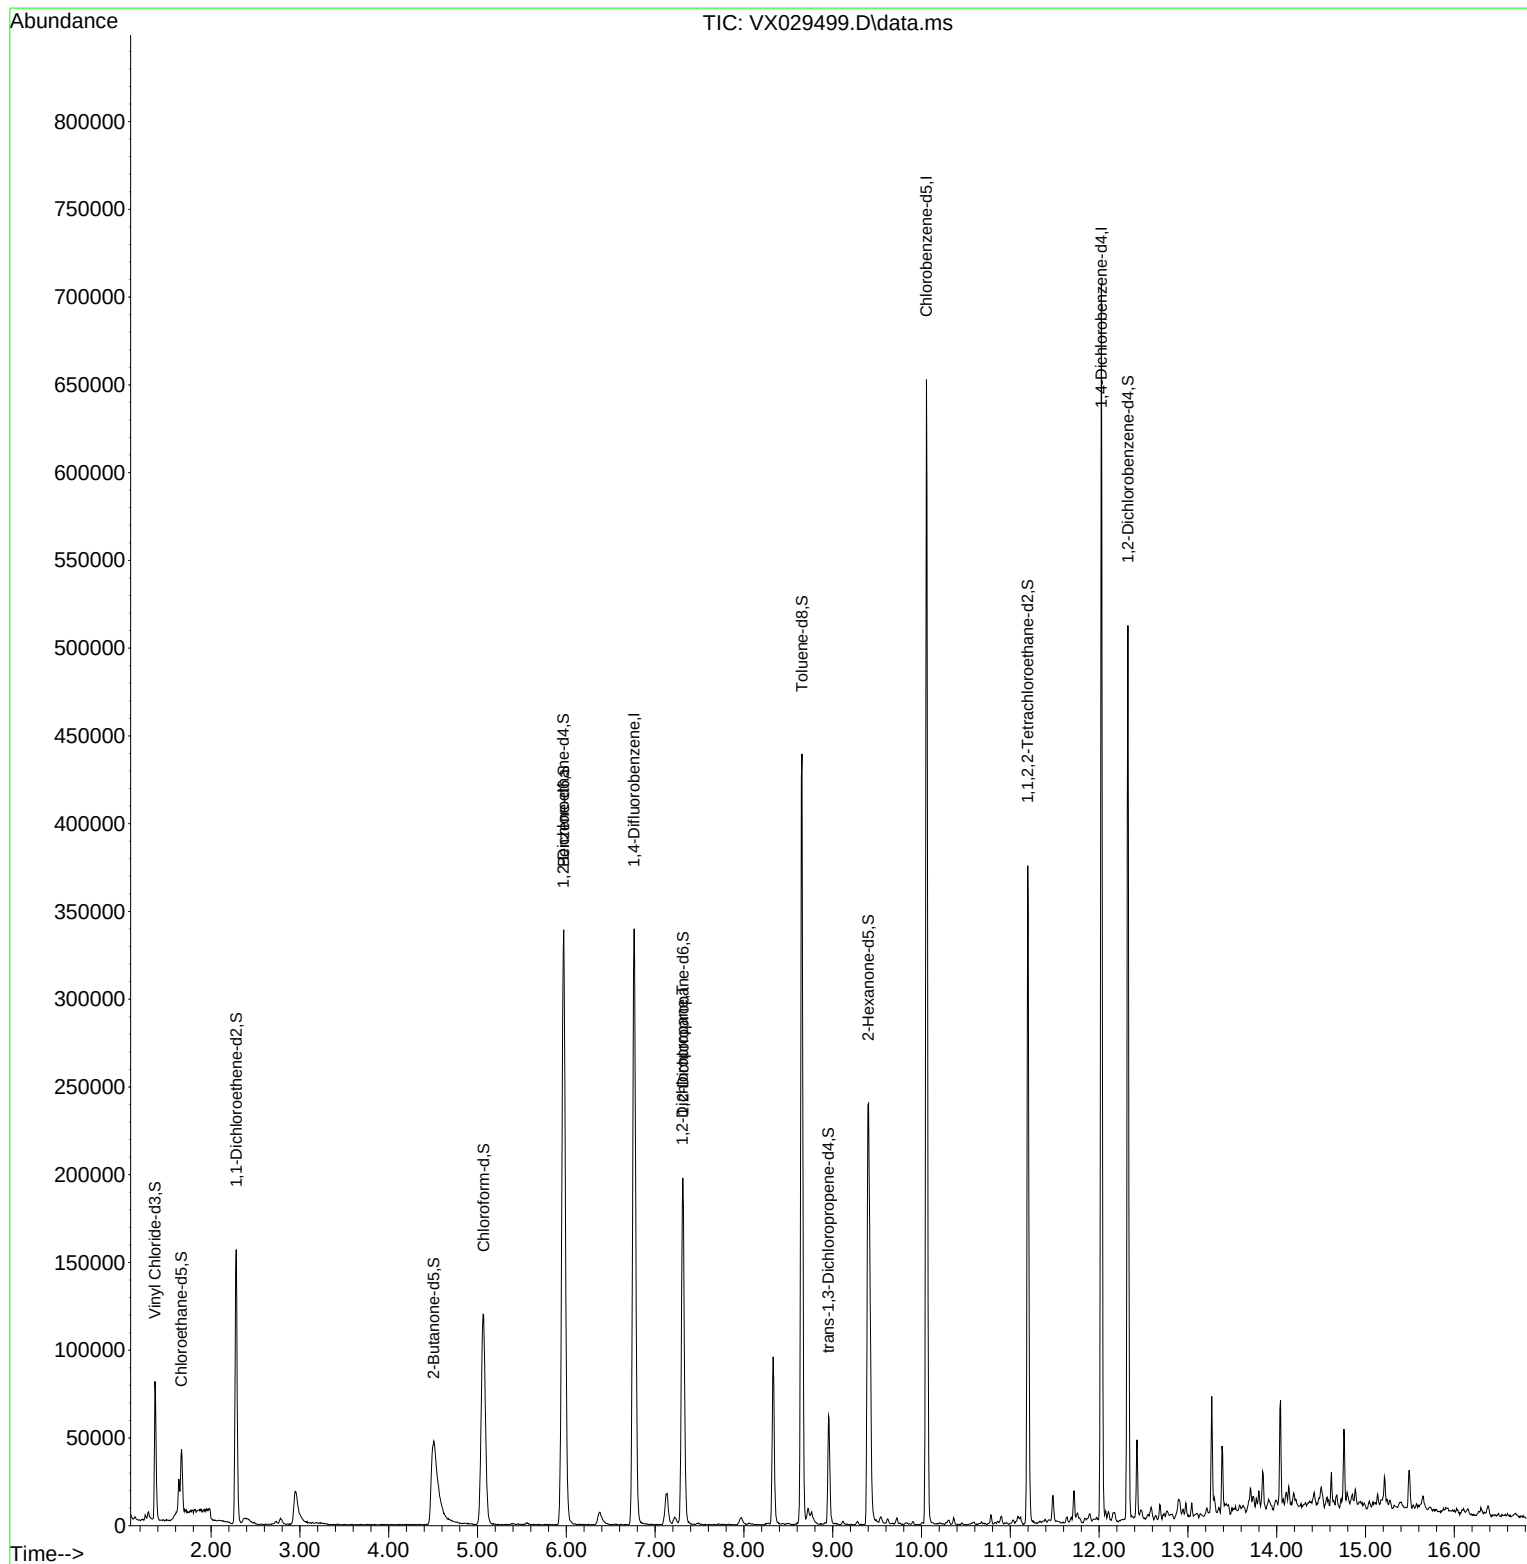

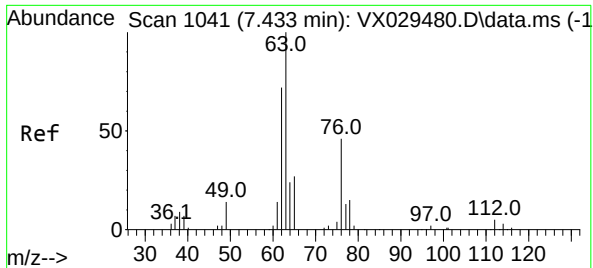

#37
 1,2-Dichloropropane
 Concen: 4.592 ug/L
 RT: 7.306 min Scan# 10
 Delta R.T. -0.128 min
 Lab File: VX029499.D
 Acq: 15 Jun 2022 04:31

Instrument :
 MSVOA_X
 ClientSampleId :
 EW4P4ME

Tgt Ion: 63 Resp: 11373
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.8 5.8#

