

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029473.D
 Acq On : 14 Jun 2022 18:27
 Operator : JC/MD
 Sample : N3311-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Quant Time: Jun 15 05:48:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 15 05:41:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	348239	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	312965	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	148515	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	111962	41.525	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.040%
7) Chloroethane-d5	1.666	69	87802	52.400	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	104.800%
11) 1,1-Dichloroethene-d2	2.306	63	160637	33.067	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.140%
21) 2-Butanone-d5	4.458	46	194719	95.250	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.250%
24) Chloroform-d	5.062	84	222657	43.251	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.500%
26) 1,2-Dichloroethane-d4	5.958	65	143108	42.997	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.000%
32) Benzene-d6	5.976	84	460952	47.153	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.300%
36) 1,2-Dichloropropane-d6	7.311	67	137401	47.988	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.980%
41) Toluene-d8	8.653	98	420571	45.634	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.260%
43) trans-1,3-Dichloroprop...	8.951	79	57944	41.041	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.080%
47) 2-Hexanone-d5	9.384	63	147145	95.015	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.010%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	193741	46.146	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.300%
66) 1,2-Dichlorobenzene-d4	12.323	152	144803	46.897	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.800%
Target Compounds					Qvalue	
13) Acetone	2.392	43	3698	2.714	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029473.D
Acq On : 14 Jun 2022 18:27
Operator : JC/MD
Sample : N3311-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Time: Jun 15 05:48:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 15 05:41:21 2022
Response via : Initial Calibration

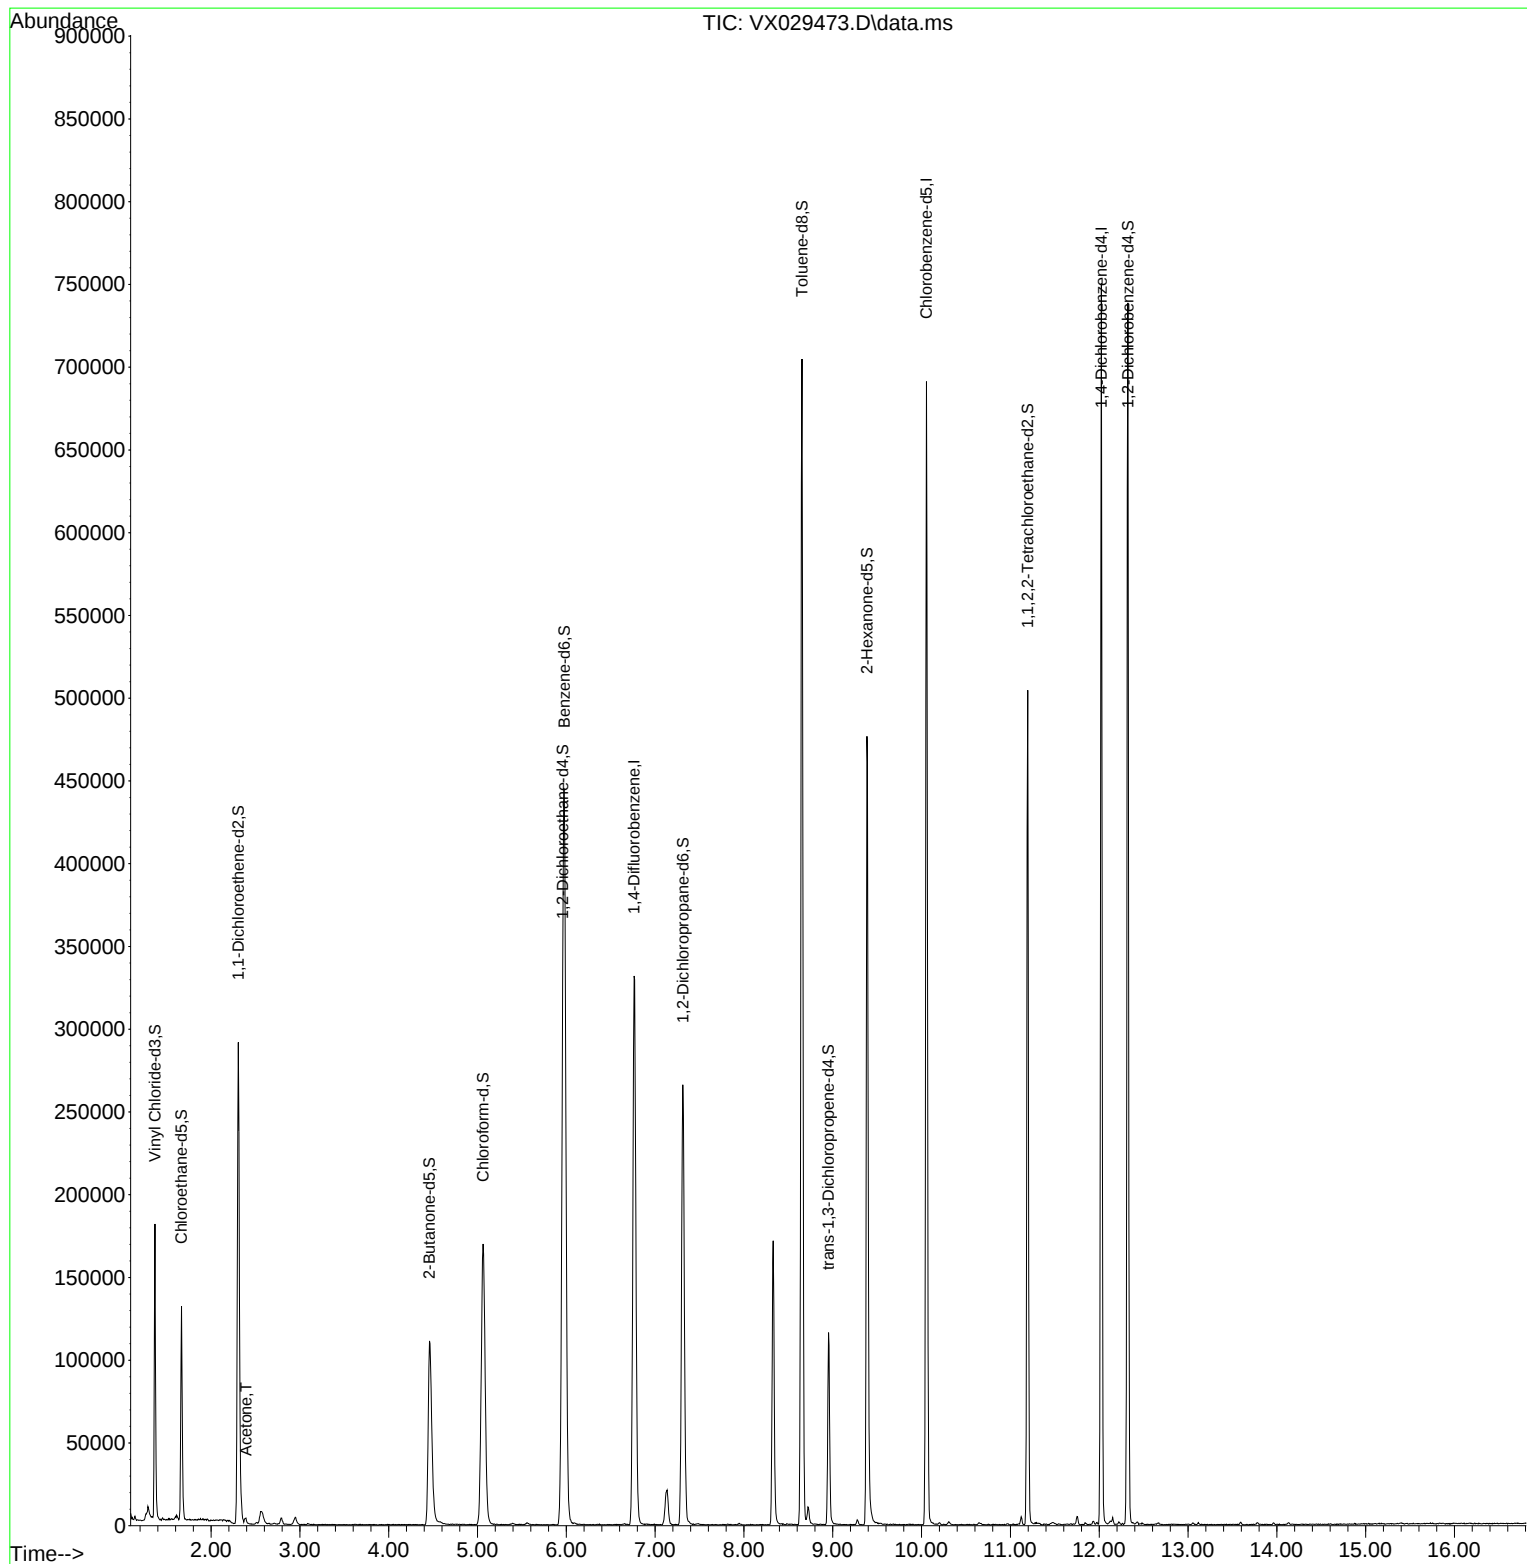

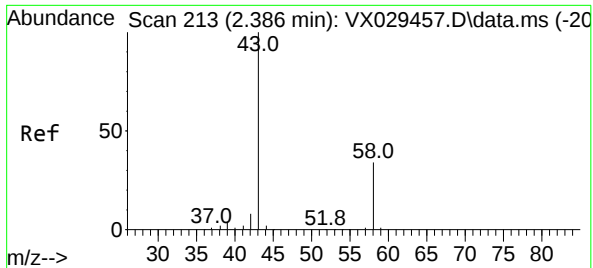

#13
 Acetone
 Concen: 2.714 ug/L
 RT: 2.392 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VX029473.D
 Acq: 14 Jun 2022 18:27

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Tgt Ion: 43 Resp: 3698
 Ion Ratio Lower Upper
 43 100
 58 38.6 0.0 61.4

