

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029458.D
 Acq On : 14 Jun 2022 12:34
 Operator : JC/MD
 Sample : VX0614WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK660

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029458.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	198412	197956	14.05%	1.829%
2	1.666	91	95	106	rVB	124511	150301	10.66%	1.388%
3	2.306	194	200	212	rBV	318313	506189	35.92%	4.676%
4	2.483	226	229	230	rBV2	309	293	0.02%	0.003%
5	2.703	262	265	271	rVB3	669	1301	0.09%	0.012%
6	2.794	275	280	284	rVB4	1871	3426	0.24%	0.032%
7	2.837	284	287	290	rBV3	281	351	0.02%	0.003%
8	2.947	296	305	314	rVV	13823	32138	2.28%	0.297%
9	3.038	318	320	324	rVB3	407	535	0.04%	0.005%
10	3.099	327	330	333	rBV2	300	405	0.03%	0.004%
11	3.318	364	366	368	rBV	398	315	0.02%	0.003%
12	3.495	394	395	401	rVB2	432	586	0.04%	0.005%
13	3.666	420	423	426	rBV2	336	401	0.03%	0.004%
14	3.763	437	439	441	rBV	330	253	0.02%	0.002%
15	3.885	456	459	462	rBV2	265	337	0.02%	0.003%
16	4.129	496	499	502	rVB3	229	314	0.02%	0.003%
17	4.160	502	504	506	rBV2	276	251	0.02%	0.002%
18	4.306	526	528	529	rBV	272	278	0.02%	0.003%
19	4.458	544	553	569	rBV	104695	305488	21.68%	2.822%
20	5.056	639	651	668	rVV	176110	549016	38.96%	5.072%
21	5.233	679	680	683	rVB3	421	254	0.02%	0.002%
22	5.342	697	698	700	rBV2	315	274	0.02%	0.003%
23	5.446	713	715	716	rBV2	444	303	0.02%	0.003%
24	5.556	724	733	741	rBV4	1585	4038	0.29%	0.037%
25	5.653	746	749	753	rBV2	258	502	0.04%	0.005%
26	5.757	764	766	770	rVB2	405	354	0.03%	0.003%
27	5.970	787	801	820	rBV2	474171	1409309	100.00%	13.018%
28	6.178	833	835	838	rVB2	365	252	0.02%	0.002%
29	6.239	843	845	846	rBV	267	257	0.02%	0.002%
30	6.318	854	858	859	rBV	305	302	0.02%	0.003%
31	6.452	875	880	882	rBV2	453	568	0.04%	0.005%
32	6.568	889	899	900	rBV3	519	1215	0.09%	0.011%
33	6.763	922	931	948	rBV	355527	854428	60.63%	7.893%
34	6.927	956	958	962	rBV3	249	413	0.03%	0.004%
35	7.123	980	990	1000	rBV4	15370	39046	2.77%	0.361%
36	7.312	1012	1021	1037	rVV	273258	610854	43.34%	5.643%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029458.D
 Acq On : 14 Jun 2022 12:34
 Operator : JC/MD
 Sample : VX0614WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK660

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.488	1045	1050	1053	rBV3	767	1307	0.09%	0.012%
38	7.531	1056	1057	1060	rVB	403	318	0.02%	0.003%
39	7.653	1074	1077	1079	rBV2	317	401	0.03%	0.004%
40	7.793	1098	1100	1102	rBV2	268	267	0.02%	0.002%
41	7.940	1120	1124	1127	rVV2	595	887	0.06%	0.008%
42	8.324	1181	1187	1203	rVV	182579	309448	21.96%	2.859%
43	8.452	1206	1208	1209	rVV2	512	331	0.02%	0.003%
44	8.482	1211	1213	1219	rVB3	866	1219	0.09%	0.011%
45	8.647	1231	1240	1248	rBV	740746	1188480	84.33%	10.979%
46	8.720	1249	1252	1264	rVB	9773	17820	1.26%	0.165%
47	8.952	1284	1290	1301	rBV	132639	192022	13.63%	1.774%
48	9.281	1340	1344	1349	rVB3	1458	2056	0.15%	0.019%
49	9.384	1356	1361	1384	rVV	485544	697048	49.46%	6.439%
50	9.647	1401	1404	1406	rVB3	347	283	0.02%	0.003%
51	9.701	1409	1413	1420	rVB3	2605	3762	0.27%	0.035%
52	9.793	1424	1428	1431	rVB2	296	451	0.03%	0.004%
53	9.823	1431	1433	1438	rVB2	251	392	0.03%	0.004%
54	10.055	1465	1471	1483	rBV	745147	993662	70.51%	9.179%
55	10.195	1491	1494	1500	rVB3	993	1320	0.09%	0.012%
56	10.305	1508	1512	1518	rBV2	1369	2260	0.16%	0.021%
57	10.378	1522	1524	1531	rVV2	178	303	0.02%	0.003%
58	10.659	1564	1570	1573	rVV3	980	1661	0.12%	0.015%
59	10.756	1584	1586	1591	rVB3	599	829	0.06%	0.008%
60	10.805	1591	1594	1597	rBV3	309	522	0.04%	0.005%
61	10.963	1618	1620	1623	rVB3	445	419	0.03%	0.004%
62	11.091	1639	1641	1642	rBV2	424	263	0.02%	0.002%
63	11.122	1642	1646	1652	rVB2	6458	8368	0.59%	0.077%
64	11.195	1652	1658	1669	rBV	525823	666446	47.29%	6.156%
65	11.274	1669	1671	1674	rBV3	1148	1186	0.08%	0.011%
66	11.384	1687	1689	1690	rBV2	404	314	0.02%	0.003%
67	11.451	1696	1700	1701	rBV2	641	736	0.05%	0.007%
68	11.482	1701	1705	1708	rVV4	1720	2598	0.18%	0.024%
69	11.543	1713	1715	1719	rVB3	757	1039	0.07%	0.010%
70	11.713	1741	1743	1744	rBV	554	396	0.03%	0.004%
71	11.750	1745	1749	1756	rVB3	6013	8034	0.57%	0.074%
72	11.841	1759	1764	1769	rBV	1743	2062	0.15%	0.019%
73	11.933	1772	1779	1782	rVB3	3110	4348	0.31%	0.040%
74	11.969	1782	1785	1788	rVB4	931	1030	0.07%	0.010%
75	12.024	1789	1794	1804	rVV	825616	1011567	71.78%	9.344%
76	12.128	1808	1811	1813	rVV4	2636	3549	0.25%	0.033%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029458.D
 Acq On : 14 Jun 2022 12:34
 Operator : JC/MD
 Sample : VX0614WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK660

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.152	1813	1815	1820	rVB2	4687	5130	0.36%	0.047%
78	12.231	1825	1828	1829	rBV2	270	261	0.02%	0.002%
79	12.323	1836	1843	1851	rBV	782082	997220	70.76%	9.212%
80	12.427	1856	1860	1865	rVV3	2290	3217	0.23%	0.030%
81	12.481	1865	1869	1877	rVB3	1569	2692	0.19%	0.025%
82	12.548	1877	1880	1883	rBV	428	614	0.04%	0.006%
83	12.664	1896	1899	1903	rVB4	1043	1275	0.09%	0.012%
84	12.768	1912	1916	1920	rBV2	986	1376	0.10%	0.013%
85	13.048	1960	1962	1966	rVB4	986	1230	0.09%	0.011%
86	13.268	1996	1998	2004	rVB2	348	559	0.04%	0.005%
87	13.310	2004	2005	2008	rBV2	295	312	0.02%	0.003%
88	13.597	2049	2052	2055	rVB3	815	907	0.06%	0.008%
89	13.658	2060	2062	2064	rBV2	325	331	0.02%	0.003%
90	13.780	2079	2082	2087	rVV3	751	1084	0.08%	0.010%
91	13.823	2087	2089	2093	rVB	409	332	0.02%	0.003%
92	13.853	2093	2094	2096	rBV2	383	299	0.02%	0.003%
93	13.957	2109	2111	2118	rVB4	674	1021	0.07%	0.009%
94	14.134	2134	2140	2144	rVB3	1937	3147	0.22%	0.029%
95	14.182	2144	2148	2149	rBV2	332	380	0.03%	0.004%
96	14.402	2182	2184	2185	rBV	299	287	0.02%	0.003%
97	14.707	2230	2234	2238	rBV3	331	533	0.04%	0.005%
98	15.078	2294	2295	2297	rBV2	511	491	0.03%	0.005%
99	16.097	2461	2462	2466	rVB2	567	486	0.03%	0.004%
100	16.657	2552	2554	2557	rVB4	600	409	0.03%	0.004%




Sum of corrected areas: 10825500

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029458.D
Acq On : 14 Jun 2022 12:34
Operator : JC/MD
Sample : VX0614WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK660

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

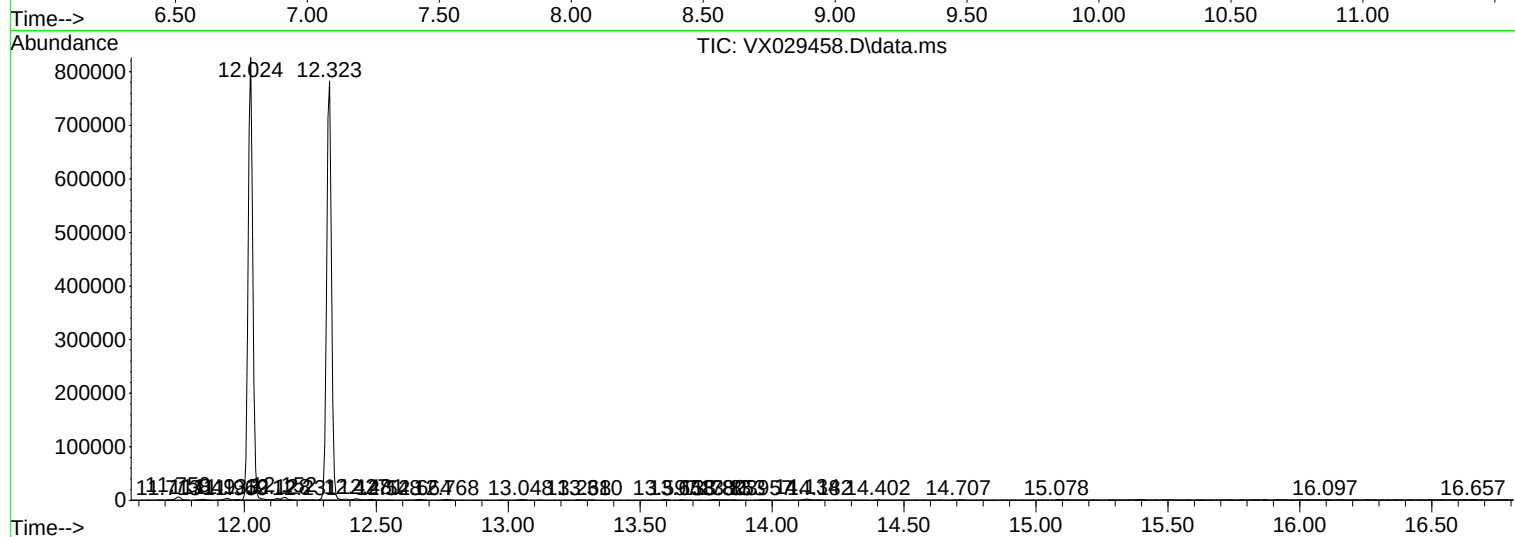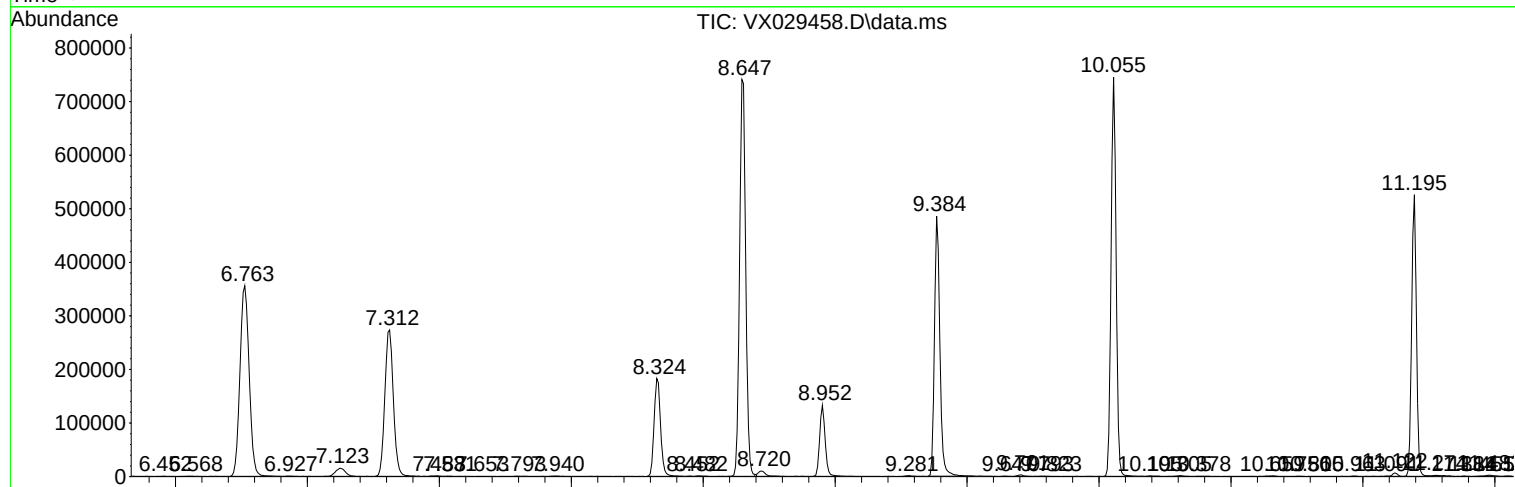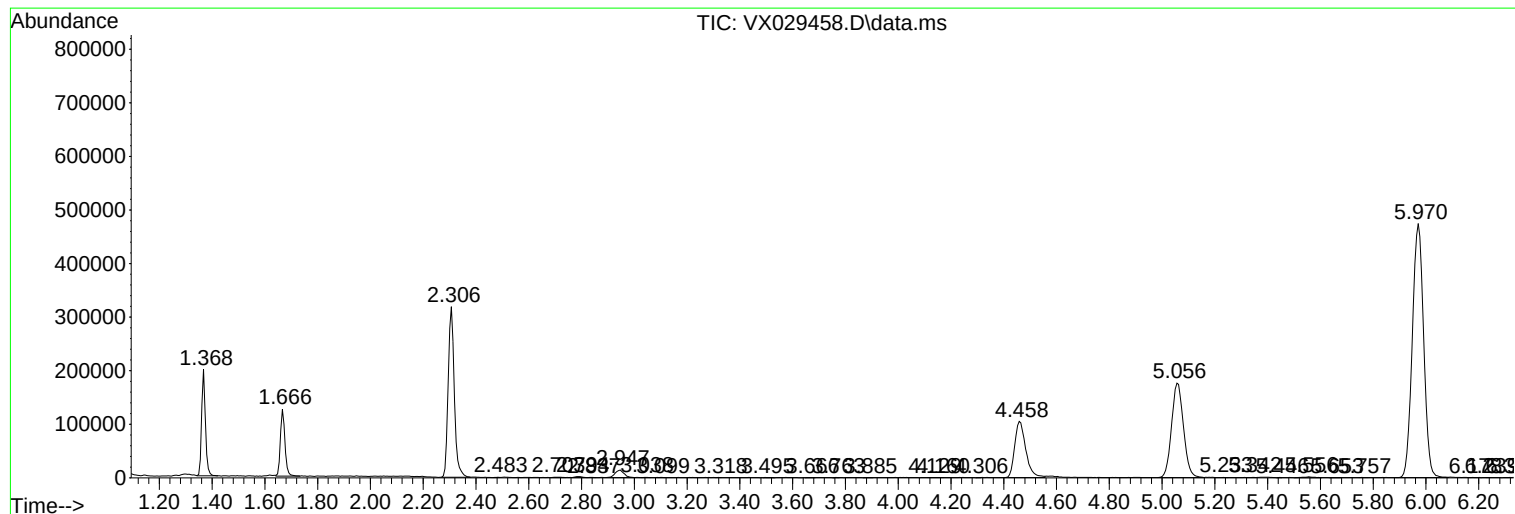

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029458.D
Acq On : 14 Jun 2022 12:34
Operator : JC/MD
Sample : VX0614WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK660

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029458.D
Acq On : 14 Jun 2022 12:34
Operator : JC/MD
Sample : VX0614WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK660

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc