

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029459.D
 Acq On : 14 Jun 2022 13:01
 Operator : JC/MD
 Sample : N3255-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029459.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	56	rVB	191229	191396	13.62%	1.780%
2	1.666	91	95	104	rVB	123863	141735	10.09%	1.318%
3	2.306	194	200	212	rVB	310077	489539	34.84%	4.553%
4	2.483	227	229	230	rBV	454	338	0.02%	0.003%
5	2.715	260	267	271	rBV3	741	1636	0.12%	0.015%
6	2.794	275	280	285	rVV2	2169	3719	0.26%	0.035%
7	2.946	297	305	317	rVB	17187	41056	2.92%	0.382%
8	3.032	317	319	324	rBV	303	361	0.03%	0.003%
9	3.166	338	341	345	rBV	284	396	0.03%	0.004%
10	3.257	354	356	358	rVB	447	339	0.02%	0.003%
11	3.471	389	391	393	rBV	387	333	0.02%	0.003%
12	3.617	411	415	416	rBV2	281	280	0.02%	0.003%
13	3.684	423	426	430	rBV2	272	388	0.03%	0.004%
14	3.739	433	435	437	rVB	428	332	0.02%	0.003%
15	4.147	500	502	504	rVB2	356	334	0.02%	0.003%
16	4.458	542	553	566	rBV	108316	316593	22.53%	2.945%
17	4.842	614	616	619	rBV2	291	280	0.02%	0.003%
18	5.062	640	652	668	rVV	173537	549964	39.15%	5.115%
19	5.281	685	688	691	rVB2	437	508	0.04%	0.005%
20	5.562	726	734	736	rBV3	1367	2925	0.21%	0.027%
21	5.970	788	801	818	rBV2	478700	1404919	100.00%	13.067%
22	6.238	843	845	850	rVB3	621	551	0.04%	0.005%
23	6.763	920	931	943	rBV	347299	814640	57.98%	7.577%
24	7.025	973	974	978	rVB3	357	387	0.03%	0.004%
25	7.129	978	991	1002	rBV4	14569	37602	2.68%	0.350%
26	7.311	1012	1021	1037	rVV	277974	617059	43.92%	5.739%
27	7.439	1040	1042	1046	rVV2	417	548	0.04%	0.005%
28	7.488	1046	1050	1053	rVV2	1182	1610	0.11%	0.015%
29	7.610	1066	1070	1074	rBV2	295	453	0.03%	0.004%
30	7.689	1081	1083	1087	rVB2	352	363	0.03%	0.003%
31	7.811	1100	1103	1106	rBV3	360	510	0.04%	0.005%
32	7.939	1122	1124	1128	rVB3	628	564	0.04%	0.005%
33	8.061	1142	1144	1148	rBV2	195	262	0.02%	0.002%
34	8.323	1180	1187	1203	rVV	184670	313450	22.31%	2.915%
35	8.537	1220	1222	1225	rVB2	392	318	0.02%	0.003%
36	8.586	1225	1230	1232	rBV3	632	827	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029459.D
 Acq On : 14 Jun 2022 13:01
 Operator : JC/MD
 Sample : N3255-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	8.653	1234	1241	1248	rVV	737645	1180333	84.01%	10.978%
38	8.720	1248	1252	1260	rVB	11598	19370	1.38%	0.180%
39	8.951	1284	1290	1300	rBV	129976	196217	13.97%	1.825%
40	9.165	1323	1325	1328	rVB3	347	341	0.02%	0.003%
41	9.207	1328	1332	1333	rVB2	258	317	0.02%	0.003%
42	9.275	1340	1343	1350	rVV4	1492	1984	0.14%	0.018%
43	9.384	1356	1361	1374	rBV	509020	725717	51.66%	6.750%
44	9.701	1409	1413	1421	rVB4	3356	4429	0.32%	0.041%
45	9.762	1421	1423	1426	rBV2	314	319	0.02%	0.003%
46	9.860	1435	1439	1441	rVB2	414	524	0.04%	0.005%
47	10.055	1465	1471	1488	rVV	734359	960687	68.38%	8.935%
48	10.195	1492	1494	1498	rVB2	814	929	0.07%	0.009%
49	10.305	1507	1512	1517	rVB4	1352	2149	0.15%	0.020%
50	10.396	1525	1527	1531	rBV2	275	356	0.03%	0.003%
51	10.494	1542	1543	1546	rVB	413	262	0.02%	0.002%
52	10.536	1546	1550	1553	rBV2	395	514	0.04%	0.005%
53	10.561	1553	1554	1557	rBV2	327	296	0.02%	0.003%
54	10.646	1566	1568	1572	rVV2	628	798	0.06%	0.007%
55	10.799	1591	1593	1598	rVB2	368	522	0.04%	0.005%
56	10.841	1598	1600	1602	rVB	463	264	0.02%	0.002%
57	10.957	1617	1619	1620	rBV2	309	269	0.02%	0.003%
58	11.030	1629	1631	1633	rBV2	404	426	0.03%	0.004%
59	11.122	1642	1646	1650	rVB2	6562	8098	0.58%	0.075%
60	11.195	1652	1658	1667	rBV	534374	687208	48.91%	6.392%
61	11.378	1686	1688	1689	rBV	512	344	0.02%	0.003%
62	11.396	1689	1691	1694	rVB2	628	595	0.04%	0.006%
63	11.457	1696	1701	1702	rBV3	558	740	0.05%	0.007%
64	11.475	1702	1704	1714	rVB5	2252	3870	0.28%	0.036%
65	11.549	1714	1716	1722	rVB3	745	1124	0.08%	0.010%
66	11.622	1726	1728	1731	rBV3	300	337	0.02%	0.003%
67	11.713	1741	1743	1745	rBV3	554	743	0.05%	0.007%
68	11.750	1745	1749	1753	rVV3	6188	7357	0.52%	0.068%
69	11.841	1761	1764	1768	rBV3	1268	1482	0.11%	0.014%
70	11.939	1775	1780	1783	rVB2	3061	4071	0.29%	0.038%
71	11.969	1783	1785	1788	rBV2	1012	1071	0.08%	0.010%
72	12.024	1789	1794	1805	rVV	783800	973163	69.27%	9.051%
73	12.152	1812	1815	1820	rVB3	4712	5717	0.41%	0.053%
74	12.231	1826	1828	1830	rBV2	424	288	0.02%	0.003%
75	12.323	1835	1843	1850	rBV	791956	1001658	71.30%	9.317%
76	12.426	1857	1860	1864	rVB3	2132	2628	0.19%	0.024%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029459.D
 Acq On : 14 Jun 2022 13:01
 Operator : JC/MD
 Sample : N3255-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.481	1864	1869	1874	rVB4	1047	2130	0.15%	0.020%
78	12.530	1874	1877	1878	rBV2	388	394	0.03%	0.004%
79	12.591	1882	1887	1889	rBV3	356	650	0.05%	0.006%
80	12.664	1896	1899	1903	rVB3	936	1110	0.08%	0.010%
81	12.762	1910	1915	1920	rBV4	1005	1757	0.13%	0.016%
82	12.817	1922	1924	1926	rVB2	487	348	0.02%	0.003%
83	12.859	1929	1931	1933	rBV2	596	566	0.04%	0.005%
84	12.963	1945	1948	1950	rBV2	429	425	0.03%	0.004%
85	13.048	1959	1962	1967	rVB4	648	1213	0.09%	0.011%
86	13.121	1971	1974	1975	rBV2	428	490	0.03%	0.005%
87	13.225	1988	1991	1995	rBV2	215	458	0.03%	0.004%
88	13.591	2049	2051	2055	rVB	654	550	0.04%	0.005%
89	13.633	2055	2058	2062	rBV3	421	470	0.03%	0.004%
90	13.780	2078	2082	2086	rBV3	657	1144	0.08%	0.011%
91	13.859	2093	2095	2096	rBV2	324	312	0.02%	0.003%
92	14.127	2135	2139	2144	rVB	1490	2217	0.16%	0.021%
93	14.304	2164	2168	2169	rBV2	336	389	0.03%	0.004%
94	14.505	2199	2201	2204	rBV3	339	409	0.03%	0.004%
95	14.743	2238	2240	2242	rBV2	430	515	0.04%	0.005%
96	14.932	2269	2271	2272	rBV	451	310	0.02%	0.003%
97	15.109	2298	2300	2303	rBV2	447	396	0.03%	0.004%
98	15.145	2305	2306	2308	rVB	494	273	0.02%	0.003%
99	15.347	2337	2339	2341	rBV3	592	553	0.04%	0.005%
100	15.694	2394	2396	2397	rBV2	506	329	0.02%	0.003%



Sum of corrected areas: 10751440

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029459.D
Acq On : 14 Jun 2022 13:01
Operator : JC/MD
Sample : N3255-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

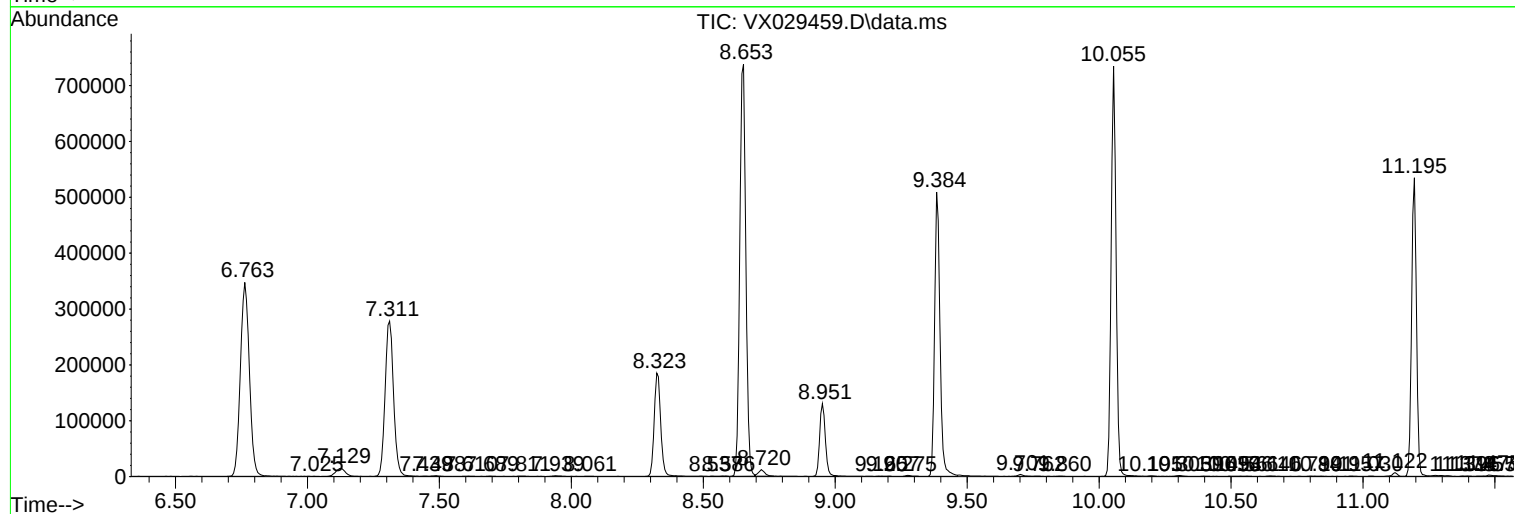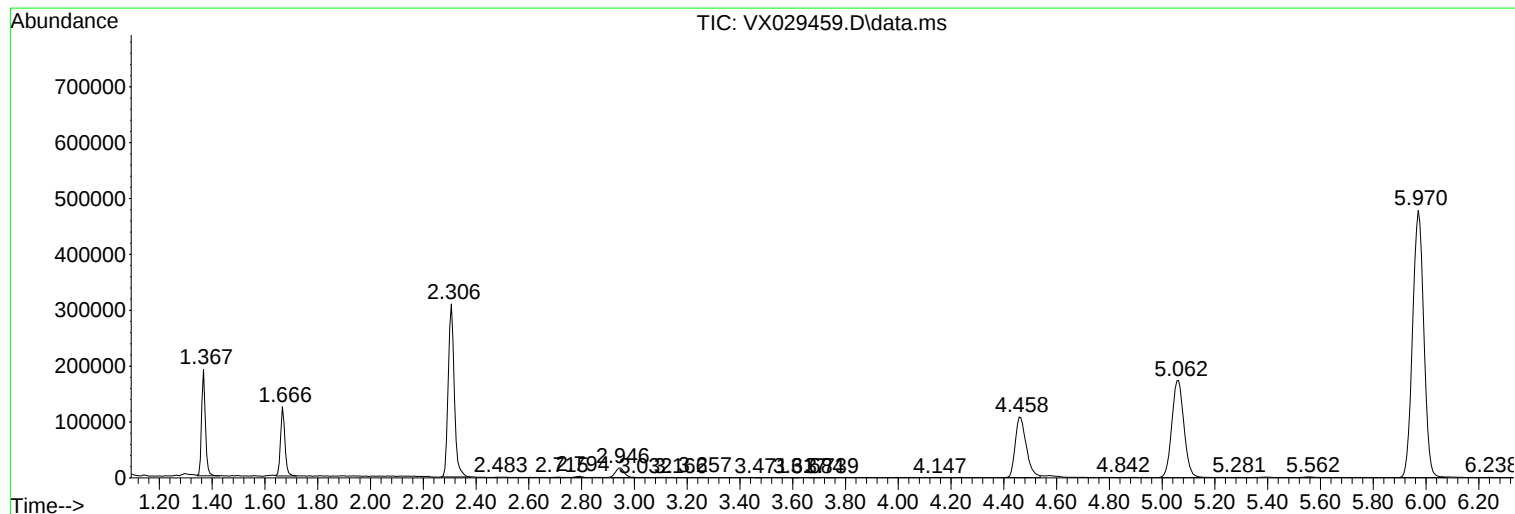

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029459.D
Acq On : 14 Jun 2022 13:01
Operator : JC/MD
Sample : N3255-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029459.D
Acq On : 14 Jun 2022 13:01
Operator : JC/MD
Sample : N3255-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc