

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029460.D
 Acq On : 14 Jun 2022 13:24
 Operator : JC/MD
 Sample : N3248-14 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB	175129	188217	14.35%	1.873%
2	1.660	90	94	108	rVB	86569	111072	8.47%	1.105%
3	2.300	193	199	213	rBV	298646	464541	35.41%	4.622%
4	2.630	251	253	254	rBV2	551	521	0.04%	0.005%
5	2.788	275	279	285	rBB2	1378	2295	0.17%	0.023%
6	2.947	296	305	317	rBV	38145	99758	7.60%	0.993%
7	3.087	326	328	332	rVB3	574	526	0.04%	0.005%
8	3.123	332	334	340	rVB3	440	548	0.04%	0.005%
9	3.434	383	385	389	rBV2	366	485	0.04%	0.005%
10	3.562	404	406	407	rBV	323	295	0.02%	0.003%
11	3.611	407	414	421	rVB2	8085	18099	1.38%	0.180%
12	3.763	434	439	442	rBV2	402	769	0.06%	0.008%
13	3.885	456	459	461	rBV3	255	255	0.02%	0.003%
14	3.928	464	466	469	rVV	354	291	0.02%	0.003%
15	4.001	476	478	481	rBV2	430	523	0.04%	0.005%
16	4.074	488	490	491	rBV	413	305	0.02%	0.003%
17	4.471	545	555	572	rBV	90364	296269	22.58%	2.948%
18	4.891	623	624	627	rVB2	437	320	0.02%	0.003%
19	4.916	627	628	630	rBV2	415	343	0.03%	0.003%
20	5.062	640	652	671	rBV	164512	514867	39.24%	5.123%
21	5.202	673	675	679	rBV3	405	402	0.03%	0.004%
22	5.385	696	705	718	rVB5	8415	24829	1.89%	0.247%
23	5.562	726	734	740	rVB3	2011	4689	0.36%	0.047%
24	5.970	787	801	815	rBV2	453155	1312005	100.00%	13.054%
25	6.348	859	863	871	rBV4	1951	4515	0.34%	0.045%
26	6.543	891	895	896	rBV2	438	618	0.05%	0.006%
27	6.763	921	931	944	rBV	301977	708248	53.98%	7.047%
28	6.915	953	956	959	rBV2	514	561	0.04%	0.006%
29	7.129	981	991	1000	rBV3	23641	56353	4.30%	0.561%
30	7.202	1001	1003	1004	rBV	527	412	0.03%	0.004%
31	7.312	1012	1021	1040	rBV	263522	572927	43.67%	5.700%
32	7.470	1046	1047	1049	rBV2	766	706	0.05%	0.007%
33	7.793	1096	1100	1102	rBV	392	423	0.03%	0.004%
34	7.818	1102	1104	1106	rBV3	467	508	0.04%	0.005%
35	7.952	1121	1126	1128	rBV5	1009	1767	0.13%	0.018%
36	8.257	1174	1176	1178	rVB2	324	253	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029460.D
 Acq On : 14 Jun 2022 13:24
 Operator : JC/MD
 Sample : N3248-14 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	8.330	1181	1188	1200	rBV	166428	280223	21.36%	2.788%
38	8.592	1226	1231	1233	rBV3	795	1271	0.10%	0.013%
39	8.653	1234	1241	1249	rBV	708668	1105701	84.28%	11.001%
40	8.720	1249	1252	1258	rVB	8038	12819	0.98%	0.128%
41	8.952	1285	1290	1300	rVV	114082	172701	13.16%	1.718%
42	9.275	1338	1343	1351	rBV2	19167	29046	2.21%	0.289%
43	9.391	1357	1362	1376	rBV	380928	617853	47.09%	6.147%
44	9.610	1396	1398	1406	rBB6	568	986	0.08%	0.010%
45	9.769	1423	1424	1427	rBV2	332	323	0.02%	0.003%
46	9.829	1430	1434	1435	rBV2	248	358	0.03%	0.004%
47	9.939	1449	1452	1455	rBV	291	377	0.03%	0.004%
48	10.055	1465	1471	1480	rBV	612607	823160	62.74%	8.190%
49	10.195	1490	1494	1502	rVB	2804	3913	0.30%	0.039%
50	10.275	1505	1507	1509	rVV2	383	379	0.03%	0.004%
51	10.305	1509	1512	1524	rVB3	2898	4478	0.34%	0.045%
52	10.646	1564	1568	1572	rBV3	1164	1778	0.14%	0.018%
53	10.756	1584	1586	1587	rVV	553	388	0.03%	0.004%
54	10.774	1587	1589	1596	rVB3	889	1286	0.10%	0.013%
55	10.866	1598	1604	1606	rVV4	515	706	0.05%	0.007%
56	10.963	1617	1620	1625	rVB3	1355	1842	0.14%	0.018%
57	11.006	1625	1627	1628	rBV	417	267	0.02%	0.003%
58	11.091	1638	1641	1642	rBV2	842	833	0.06%	0.008%
59	11.122	1642	1646	1650	rVB2	6329	8528	0.65%	0.085%
60	11.195	1652	1658	1666	rBV	479862	598520	45.62%	5.955%
61	11.305	1673	1676	1683	rVB3	5517	8112	0.62%	0.081%
62	11.378	1685	1688	1696	rBV3	2459	4809	0.37%	0.048%
63	11.451	1696	1700	1708	rBV	26357	36155	2.76%	0.360%
64	11.549	1713	1716	1721	rVB3	854	959	0.07%	0.010%
65	11.616	1722	1727	1734	rBV	23315	31444	2.40%	0.313%
66	11.713	1741	1743	1744	rBV	929	623	0.05%	0.006%
67	11.756	1745	1750	1755	rVB	69172	89606	6.83%	0.892%
68	11.847	1761	1765	1767	rBV2	979	1447	0.11%	0.014%
69	11.933	1775	1779	1783	rBV2	2825	3656	0.28%	0.036%
70	11.969	1783	1785	1788	rVB2	4465	4600	0.35%	0.046%
71	12.024	1789	1794	1800	rVV	650518	797261	60.77%	7.932%
72	12.091	1801	1805	1808	rVV	19435	24610	1.88%	0.245%
73	12.152	1812	1815	1817	rVB	4098	4036	0.31%	0.040%
74	12.250	1826	1831	1833	rBV	10551	16001	1.22%	0.159%
75	12.323	1837	1843	1850	rVB	711136	892446	68.02%	8.879%
76	12.427	1858	1860	1863	rVB3	1909	1556	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029460.D
 Acq On : 14 Jun 2022 13:24
 Operator : JC/MD
 Sample : N3248-14 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.463	1863	1866	1873	rVB2	4954	7317	0.56%	0.073%
78	12.536	1873	1878	1879	rBV2	5501	6554	0.50%	0.065%
79	12.616	1887	1891	1895	rBV	7656	9307	0.71%	0.093%
80	12.701	1902	1905	1913	rVB6	3317	6792	0.52%	0.068%
81	12.762	1913	1915	1919	rVB2	916	1001	0.08%	0.010%
82	12.798	1919	1921	1923	rBV2	792	629	0.05%	0.006%
83	12.853	1926	1930	1935	rVB3	2490	3345	0.25%	0.033%
84	12.920	1937	1941	1944	rBV2	3608	4208	0.32%	0.042%
85	12.963	1945	1948	1953	rVB2	6180	7643	0.58%	0.076%
86	13.018	1956	1957	1959	rBV2	562	432	0.03%	0.004%
87	13.055	1961	1963	1967	rVB4	1473	1103	0.08%	0.011%
88	13.164	1979	1981	1987	rBV4	947	1134	0.09%	0.011%
89	13.256	1992	1996	1997	rBV	723	542	0.04%	0.005%
90	13.286	1997	2001	2008	rVB2	6909	9570	0.73%	0.095%
91	13.365	2012	2014	2019	rVB2	489	489	0.04%	0.005%
92	13.426	2019	2024	2027	rBV3	2403	2708	0.21%	0.027%
93	13.542	2041	2043	2045	rBV	332	379	0.03%	0.004%
94	13.591	2047	2051	2057	rVB3	1313	1501	0.11%	0.015%
95	13.780	2077	2082	2087	rBV2	4922	6699	0.51%	0.067%
96	13.957	2109	2111	2112	rBV2	579	356	0.03%	0.004%
97	14.134	2137	2140	2144	rVB2	1924	2260	0.17%	0.022%
98	14.298	2166	2167	2170	rBV2	298	367	0.03%	0.004%
99	15.389	2344	2346	2350	rVV2	1309	1765	0.13%	0.018%
100	16.389	2508	2510	2511	rVB	555	288	0.02%	0.003%



Sum of corrected areas: 10050961

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029460.D
Acq On : 14 Jun 2022 13:24
Operator : JC/MD
Sample : N3248-14 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

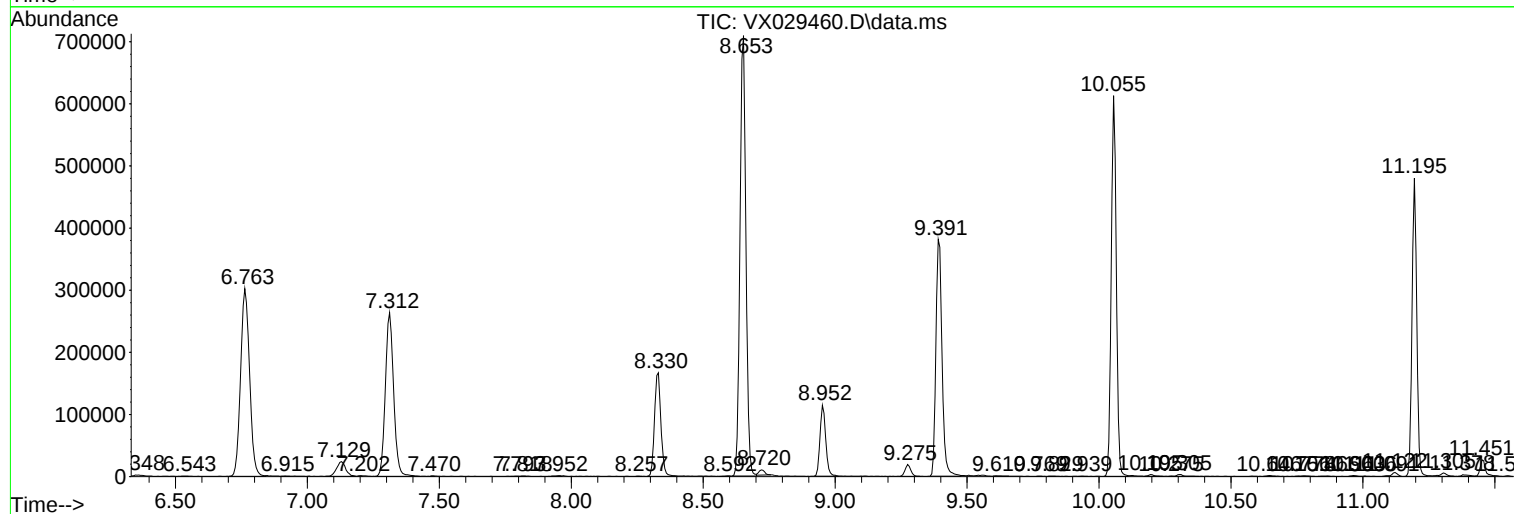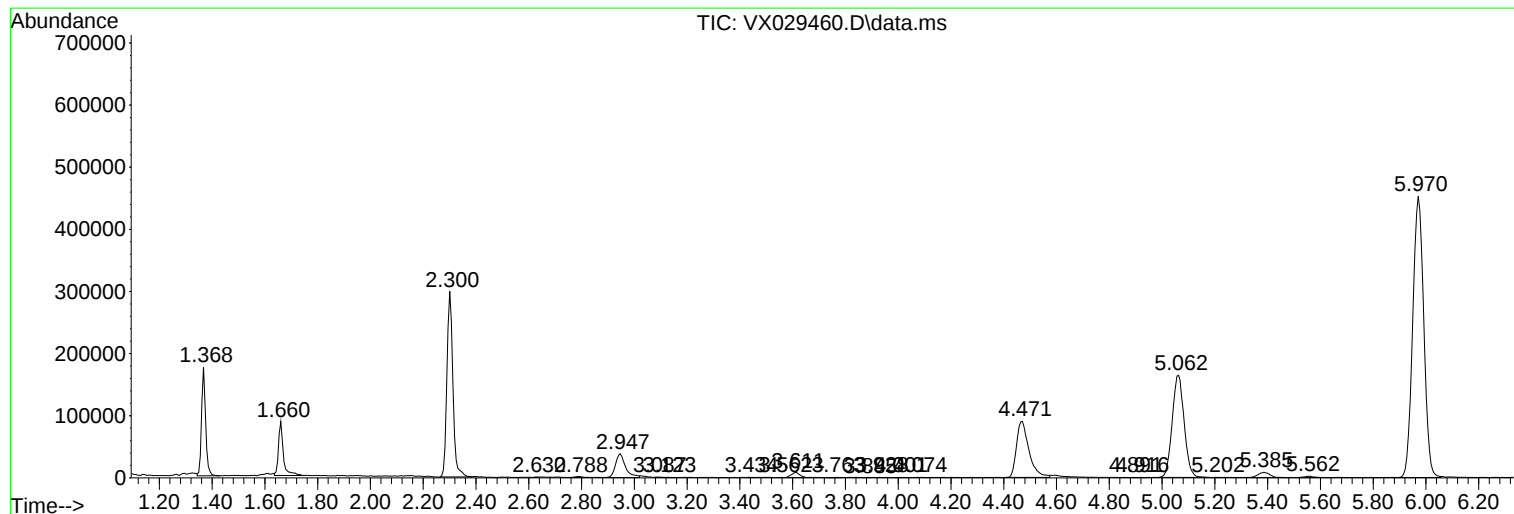

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029460.D
Acq On : 14 Jun 2022 13:24
Operator : JC/MD
Sample : N3248-14 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029460.D
Acq On : 14 Jun 2022 13:24
Operator : JC/MD
Sample : N3248-14 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc