

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029462.D
 Acq On : 14 Jun 2022 14:10
 Operator : JC/MD
 Sample : N3248-19DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029462.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB	197713	199321	13.95%	1.774%
2	1.666	91	95	105	rVB	144093	169006	11.82%	1.504%
3	2.307	194	200	212	rBV	317567	505011	35.33%	4.494%
4	2.666	257	259	260	rBV	352	236	0.02%	0.002%
5	2.788	275	279	284	rVB2	1630	2357	0.16%	0.021%
6	2.947	296	305	318	rVB2	30217	73199	5.12%	0.651%
7	3.099	325	330	334	rVB4	1001	1747	0.12%	0.016%
8	3.184	342	344	348	rVB2	316	441	0.03%	0.004%
9	3.245	348	354	356	rBV2	406	727	0.05%	0.006%
10	3.611	406	414	425	rVB	19956	47386	3.32%	0.422%
11	3.770	438	440	444	rBV2	260	292	0.02%	0.003%
12	3.831	447	450	451	rBV2	317	292	0.02%	0.003%
13	3.971	471	473	476	rVB2	304	240	0.02%	0.002%
14	4.007	476	479	484	rBV2	257	452	0.03%	0.004%
15	4.105	491	495	498	rVB3	262	373	0.03%	0.003%
16	4.135	498	500	502	rBV3	332	257	0.02%	0.002%
17	4.306	526	528	531	rBV2	280	303	0.02%	0.003%
18	4.465	544	554	569	rBV2	127795	463243	32.41%	4.122%
19	4.873	620	621	623	rBV2	454	451	0.03%	0.004%
20	5.062	639	652	671	rBV	180031	565287	39.55%	5.031%
21	5.391	693	706	719	rBV2	49778	156635	10.96%	1.394%
22	5.562	726	734	736	rBV3	2686	4713	0.33%	0.042%
23	5.806	771	774	776	rBV3	213	237	0.02%	0.002%
24	5.879	784	786	789	rBV	295	268	0.02%	0.002%
25	5.971	789	801	823	rBV2	480067	1429300	100.00%	12.720%
26	6.361	863	865	869	rVV2	420	395	0.03%	0.004%
27	6.507	886	889	890	rBV2	259	227	0.02%	0.002%
28	6.647	911	912	919	rVB2	212	349	0.02%	0.003%
29	6.763	921	931	944	rBV	347002	827897	57.92%	7.368%
30	7.068	979	981	983	rBV2	307	276	0.02%	0.002%
31	7.129	983	991	1003	rBV5	22723	55352	3.87%	0.493%
32	7.312	1009	1021	1037	rBV	284303	622947	43.58%	5.544%
33	7.568	1062	1063	1065	rBV	405	306	0.02%	0.003%
34	7.653	1074	1077	1079	rBV2	266	346	0.02%	0.003%
35	7.696	1082	1084	1086	rVB	444	325	0.02%	0.003%
36	7.726	1088	1089	1093	rBV2	268	329	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029462.D
 Acq On : 14 Jun 2022 14:10
 Operator : JC/MD
 Sample : N3248-19DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.799	1098	1101	1102	rBV2	365	446	0.03%	0.004%
38	7.909	1115	1119	1121	rBV2	326	394	0.03%	0.004%
39	7.940	1121	1124	1127	rVV4	821	1123	0.08%	0.010%
40	7.988	1130	1132	1135	rVB2	350	340	0.02%	0.003%
41	8.031	1138	1139	1142	rBV	344	225	0.02%	0.002%
42	8.214	1165	1169	1170	rBV	377	371	0.03%	0.003%
43	8.330	1181	1188	1201	rVV	181027	307064	21.48%	2.733%
44	8.653	1234	1241	1249	rBV	757127	1196114	83.69%	10.644%
45	8.726	1249	1253	1261	rVB	11075	17894	1.25%	0.159%
46	8.952	1284	1290	1302	rBV	130026	191606	13.41%	1.705%
47	9.275	1339	1343	1348	rBV2	6964	10405	0.73%	0.093%
48	9.385	1356	1361	1377	rBV	499850	738485	51.67%	6.572%
49	9.635	1400	1402	1404	rVB3	330	238	0.02%	0.002%
50	9.769	1422	1424	1426	rVB	573	301	0.02%	0.003%
51	10.055	1465	1471	1482	rBV	735440	969492	67.83%	8.628%
52	10.269	1505	1506	1508	rBV2	462	291	0.02%	0.003%
53	10.305	1508	1512	1519	rVV2	1335	2411	0.17%	0.021%
54	10.366	1521	1522	1524	rVB	394	224	0.02%	0.002%
55	10.543	1548	1551	1552	rBV	350	285	0.02%	0.003%
56	10.653	1565	1569	1576	rBV5	896	1601	0.11%	0.014%
57	10.744	1582	1584	1590	rVV3	373	608	0.04%	0.005%
58	10.872	1603	1605	1608	rVB	561	424	0.03%	0.004%
59	10.933	1613	1615	1617	rVB	394	290	0.02%	0.003%
60	10.964	1617	1620	1624	rBV2	532	760	0.05%	0.007%
61	11.122	1641	1646	1652	rBV	6136	8067	0.56%	0.072%
62	11.195	1652	1658	1669	rBV	532317	686353	48.02%	6.108%
63	11.384	1687	1689	1692	rBV	529	688	0.05%	0.006%
64	11.409	1692	1693	1695	rVV	427	311	0.02%	0.003%
65	11.482	1699	1705	1713	rVV4	1980	4802	0.34%	0.043%
66	11.543	1713	1715	1719	rVB3	757	799	0.06%	0.007%
67	11.628	1728	1729	1731	rBV2	336	292	0.02%	0.003%
68	11.707	1741	1742	1745	rBV2	516	584	0.04%	0.005%
69	11.750	1745	1749	1753	rVB2	5454	6463	0.45%	0.058%
70	11.841	1761	1764	1767	rVB3	1336	1697	0.12%	0.015%
71	11.933	1776	1779	1783	rBV4	2854	3546	0.25%	0.032%
72	11.969	1783	1785	1788	rVB2	925	820	0.06%	0.007%
73	12.024	1789	1794	1804	rVB	796962	944658	66.09%	8.407%
74	12.323	1835	1843	1850	rBV	780083	987164	69.07%	8.785%
75	12.427	1857	1860	1864	rVB3	2293	2585	0.18%	0.023%
76	12.475	1866	1868	1874	rVB3	1242	1862	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029462.D
 Acq On : 14 Jun 2022 14:10
 Operator : JC/MD
 Sample : N3248-19DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.530	1874	1877	1878	rBV	514	418	0.03%	0.004%
78	12.658	1896	1898	1903	rVB3	958	1101	0.08%	0.010%
79	12.762	1913	1915	1919	rVB2	677	739	0.05%	0.007%
80	12.799	1919	1921	1922	rBV2	427	279	0.02%	0.002%
81	12.853	1928	1930	1933	rVB2	357	434	0.03%	0.004%
82	12.921	1938	1941	1944	rVV	433	422	0.03%	0.004%
83	12.969	1947	1949	1955	rVV3	917	1046	0.07%	0.009%
84	13.018	1955	1957	1959	rVV	464	353	0.02%	0.003%
85	13.055	1959	1963	1967	rVB3	895	1395	0.10%	0.012%
86	13.152	1976	1979	1980	rVB	350	277	0.02%	0.002%
87	13.268	1994	1998	2000	rBV2	244	320	0.02%	0.003%
88	13.780	2079	2082	2085	rBV2	533	729	0.05%	0.006%
89	13.878	2096	2098	2100	rVB2	328	262	0.02%	0.002%
90	14.018	2118	2121	2124	rVB3	499	563	0.04%	0.005%
91	14.054	2125	2127	2128	rBV2	306	254	0.02%	0.002%
92	14.134	2136	2140	2146	rVB	1875	2615	0.18%	0.023%
93	14.182	2146	2148	2151	rVB	432	260	0.02%	0.002%
94	14.371	2177	2179	2180	rBV2	326	238	0.02%	0.002%
95	14.426	2185	2188	2192	rBV4	323	495	0.03%	0.004%
96	14.609	2216	2218	2219	rBV2	439	302	0.02%	0.003%
97	14.908	2265	2267	2269	rBV	416	345	0.02%	0.003%
98	14.951	2272	2274	2278	rBV3	569	777	0.05%	0.007%
99	15.085	2294	2296	2297	rVB2	529	271	0.02%	0.002%
100	16.524	2529	2532	2533	rBV2	521	524	0.04%	0.005%


Sum of corrected areas: 11237025

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029462.D
Acq On : 14 Jun 2022 14:10
Operator : JC/MD
Sample : N3248-19DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

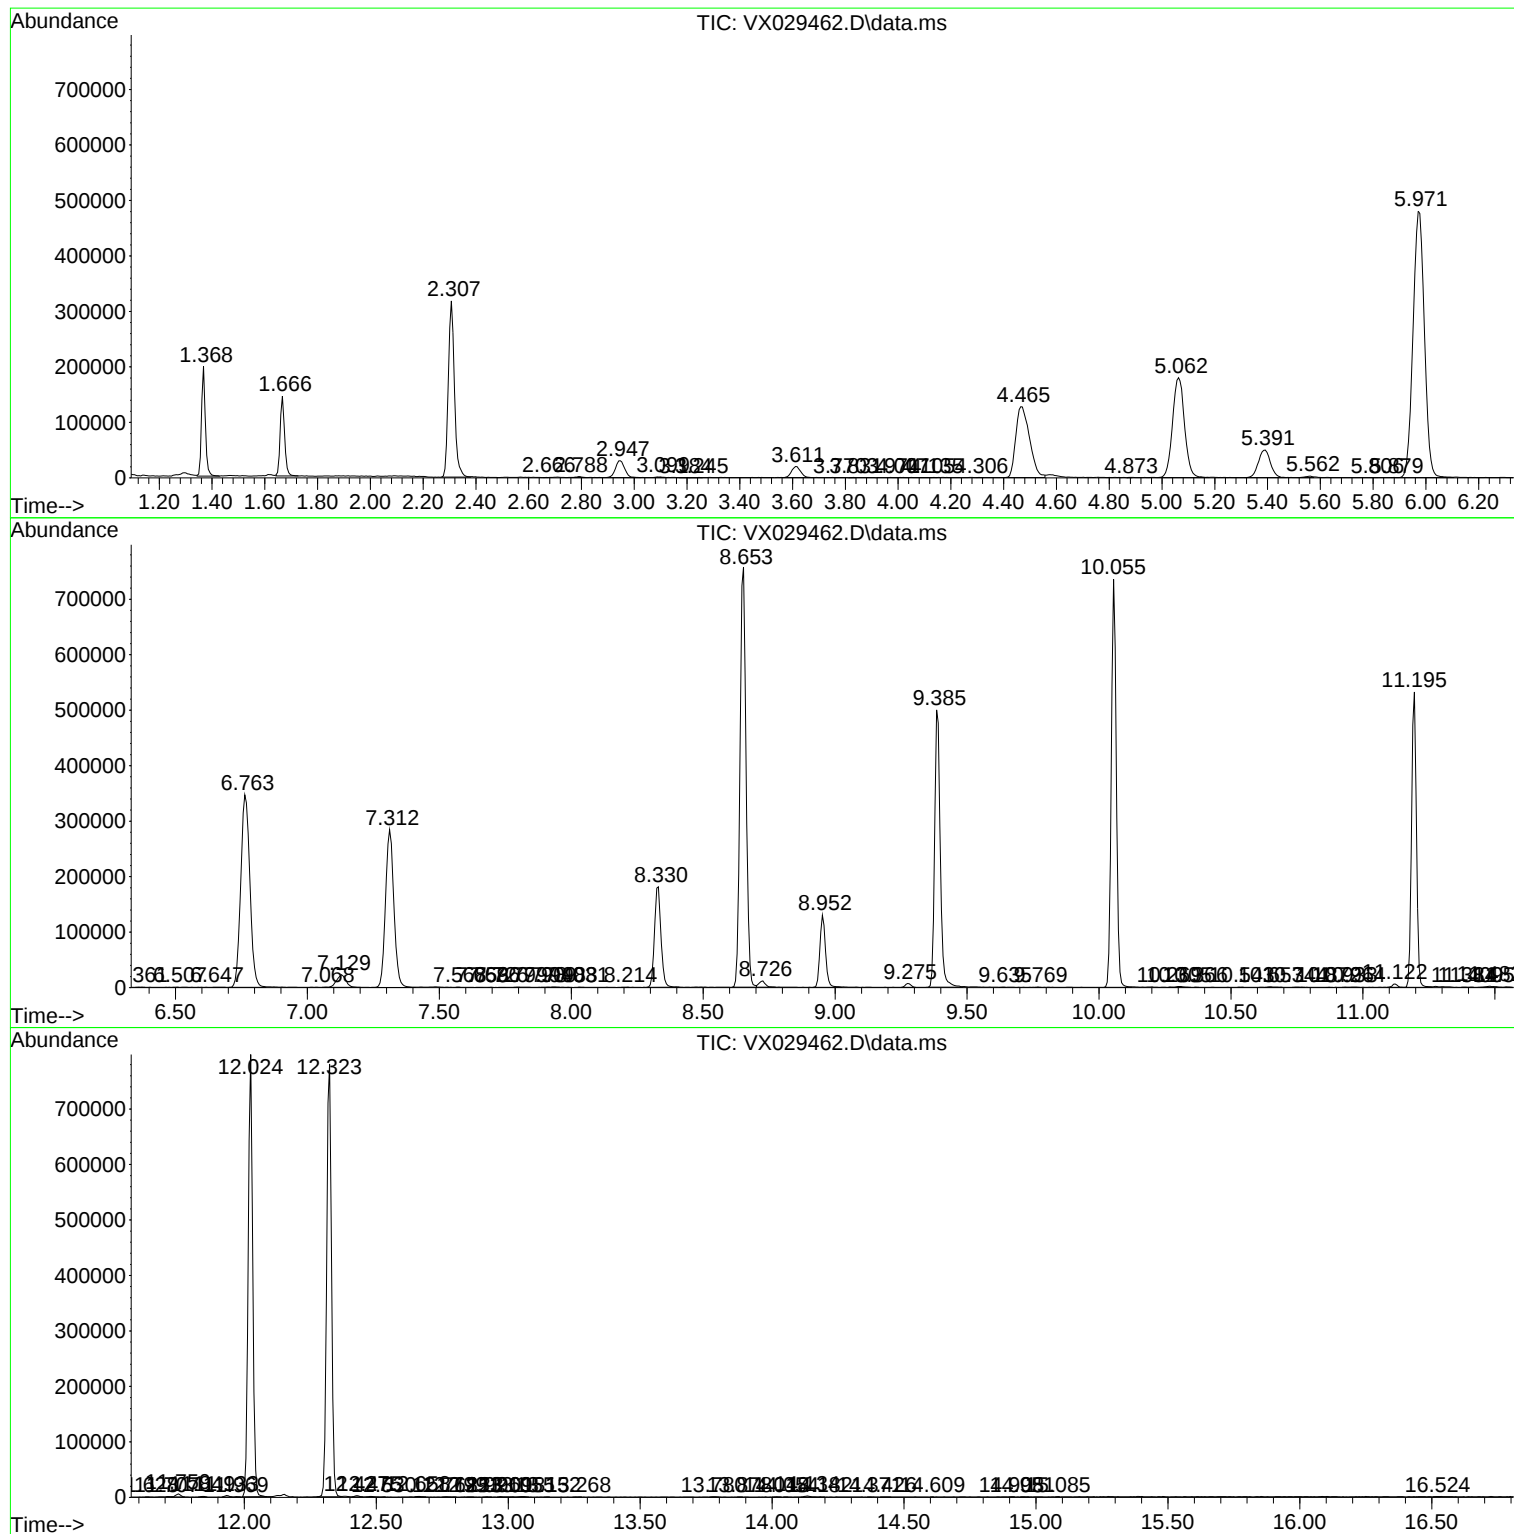

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029462.D
Acq On : 14 Jun 2022 14:10
Operator : JC/MD
Sample : N3248-19DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029462.D
Acq On : 14 Jun 2022 14:10
Operator : JC/MD
Sample : N3248-19DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------