

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029463.D
 Acq On : 14 Jun 2022 14:34
 Operator : JC/MD
 Sample : N3248-20 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029463.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB	191911	197348	14.05%	1.748%
2	1.666	91	95	106	rVB	130598	158094	11.26%	1.400%
3	2.307	194	200	211	rBV	311815	499337	35.56%	4.423%
4	2.703	263	265	266	rBV	840	655	0.05%	0.006%
5	2.782	274	278	286	rBV5	1440	2796	0.20%	0.025%
6	2.947	297	305	316	rBV	41154	97363	6.93%	0.862%
7	3.099	325	330	338	rVB4	1814	3979	0.28%	0.035%
8	3.184	342	344	346	rVB2	412	365	0.03%	0.003%
9	3.227	349	351	353	rBV2	277	292	0.02%	0.003%
10	3.611	407	414	424	rBV	10841	25854	1.84%	0.229%
11	3.751	433	437	439	rBV2	287	419	0.03%	0.004%
12	3.831	447	450	453	rBV3	279	348	0.02%	0.003%
13	3.910	461	463	467	rVB2	243	356	0.03%	0.003%
14	3.959	467	471	472	rBV2	231	285	0.02%	0.003%
15	4.184	505	508	510	rBV2	299	407	0.03%	0.004%
16	4.477	545	556	568	rBV2	158269	601405	42.83%	5.327%
17	5.062	640	652	670	rBV	179328	555333	39.55%	4.919%
18	5.239	678	681	683	rBV3	387	574	0.04%	0.005%
19	5.385	694	705	717	rBV	57397	178462	12.71%	1.581%
20	5.556	727	733	743	rVB4	1835	4616	0.33%	0.041%
21	5.970	785	801	818	rBV2	482129	1404230	100.00%	12.437%
22	6.178	833	835	837	rBV	371	273	0.02%	0.002%
23	6.257	846	848	850	rBV	281	313	0.02%	0.003%
24	6.281	850	852	854	rVV2	394	314	0.02%	0.003%
25	6.537	889	894	895	rBV3	456	716	0.05%	0.006%
26	6.702	918	921	922	rBV2	282	331	0.02%	0.003%
27	6.763	922	931	946	rBV	344347	825339	58.78%	7.310%
28	7.129	983	991	1001	rVV5	23085	55079	3.92%	0.488%
29	7.214	1003	1005	1007	rVB	433	376	0.03%	0.003%
30	7.312	1012	1021	1035	rBV	283923	608968	43.37%	5.394%
31	7.556	1059	1061	1063	rBV	290	282	0.02%	0.002%
32	7.617	1069	1071	1074	rBV	363	284	0.02%	0.003%
33	7.653	1074	1077	1078	rBV2	291	262	0.02%	0.002%
34	7.751	1091	1093	1096	rBV3	228	293	0.02%	0.003%
35	7.799	1099	1101	1102	rBV	477	324	0.02%	0.003%
36	7.818	1102	1104	1106	rBV	397	259	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029463.D
 Acq On : 14 Jun 2022 14:34
 Operator : JC/MD
 Sample : N3248-20 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.934	1119	1123	1125	rBV3	600	803	0.06%	0.007%
38	8.324	1181	1187	1202	rVV	177808	303012	21.58%	2.684%
39	8.580	1226	1229	1234	rBV4	647	889	0.06%	0.008%
40	8.653	1234	1241	1249	rBV	745926	1178780	83.94%	10.440%
41	8.726	1249	1253	1259	rVB	12954	19740	1.41%	0.175%
42	8.952	1284	1290	1302	rBV	130194	192622	13.72%	1.706%
43	9.153	1321	1323	1326	rBV2	345	328	0.02%	0.003%
44	9.183	1326	1328	1330	rVB	345	263	0.02%	0.002%
45	9.275	1339	1343	1350	rVB4	5892	9015	0.64%	0.080%
46	9.385	1356	1361	1380	rBV	492722	721516	51.38%	6.390%
47	9.872	1439	1441	1442	rBV	336	259	0.02%	0.002%
48	9.921	1445	1449	1450	rBV2	226	267	0.02%	0.002%
49	9.982	1456	1459	1461	rVB3	303	335	0.02%	0.003%
50	10.055	1465	1471	1487	rVV	725867	962119	68.52%	8.521%
51	10.201	1491	1495	1502	rVB4	1564	2676	0.19%	0.024%
52	10.299	1507	1511	1518	rVV3	3976	6166	0.44%	0.055%
53	10.360	1519	1521	1523	rVB2	330	286	0.02%	0.003%
54	10.598	1558	1560	1562	rVV3	615	411	0.03%	0.004%
55	10.646	1564	1568	1573	rVB2	3063	4130	0.29%	0.037%
56	10.689	1573	1575	1577	rBV	278	294	0.02%	0.003%
57	10.963	1617	1620	1628	rBV2	399	831	0.06%	0.007%
58	11.037	1628	1632	1636	rVB3	488	660	0.05%	0.006%
59	11.122	1641	1646	1650	rVB3	5698	7472	0.53%	0.066%
60	11.195	1652	1658	1669	rBV	524774	673284	47.95%	5.963%
61	11.384	1685	1689	1691	rBV2	2973	3880	0.28%	0.034%
62	11.457	1696	1701	1703	rBV	2759	3958	0.28%	0.035%
63	11.549	1714	1716	1719	rVB2	828	780	0.06%	0.007%
64	11.616	1724	1727	1732	rVV2	2287	2981	0.21%	0.026%
65	11.677	1736	1737	1741	rVB4	657	716	0.05%	0.006%
66	11.713	1741	1743	1745	rBV2	975	984	0.07%	0.009%
67	11.750	1745	1749	1756	rVB2	11952	15670	1.12%	0.139%
68	11.841	1760	1764	1769	rVB4	1232	1698	0.12%	0.015%
69	11.902	1769	1774	1775	rBV	494	809	0.06%	0.007%
70	11.933	1775	1779	1783	rBV3	2579	3536	0.25%	0.031%
71	12.024	1788	1794	1802	rBV	783512	943397	67.18%	8.356%
72	12.085	1802	1804	1808	rVV	4698	6145	0.44%	0.054%
73	12.152	1812	1815	1819	rVB2	4497	5482	0.39%	0.049%
74	12.323	1837	1843	1852	rVB	762216	968518	68.97%	8.578%
75	12.427	1858	1860	1864	rVB2	1985	2069	0.15%	0.018%
76	12.469	1864	1867	1868	rBV2	790	791	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029463.D
 Acq On : 14 Jun 2022 14:34
 Operator : JC/MD
 Sample : N3248-20 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYY9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.542	1875	1879	1885	rBV4	1103	1927	0.14%	0.017%
78	12.610	1888	1890	1895	rVB2	545	1024	0.07%	0.009%
79	12.658	1895	1898	1903	rBV4	1282	1712	0.12%	0.015%
80	12.799	1919	1921	1922	rBV	454	323	0.02%	0.003%
81	12.847	1928	1929	1932	rBV3	356	336	0.02%	0.003%
82	12.927	1939	1942	1943	rBV2	366	408	0.03%	0.004%
83	12.969	1947	1949	1953	rVB2	1023	881	0.06%	0.008%
84	13.048	1958	1962	1968	rBV3	1178	2020	0.14%	0.018%
85	13.146	1976	1978	1982	rBV2	249	371	0.03%	0.003%
86	13.335	2007	2009	2013	rVB2	401	414	0.03%	0.004%
87	13.384	2013	2017	2018	rBV2	298	313	0.02%	0.003%
88	13.475	2030	2032	2034	rBV2	308	281	0.02%	0.002%
89	13.561	2045	2046	2049	rBV	277	290	0.02%	0.003%
90	13.664	2061	2063	2064	rBV2	358	272	0.02%	0.002%
91	13.780	2081	2082	2086	rVB	747	667	0.05%	0.006%
92	13.914	2102	2104	2108	rBV2	213	275	0.02%	0.002%
93	13.957	2109	2111	2114	rVB2	406	308	0.02%	0.003%
94	14.000	2116	2118	2120	rBV2	380	328	0.02%	0.003%
95	14.067	2127	2129	2132	rBV2	281	332	0.02%	0.003%
96	14.128	2136	2139	2146	rVB2	1846	2576	0.18%	0.023%
97	14.682	2228	2230	2231	rBV2	361	284	0.02%	0.003%
98	14.847	2255	2257	2259	rBV2	555	594	0.04%	0.005%
99	15.255	2322	2324	2327	rVB2	745	514	0.04%	0.005%
100	15.804	2412	2414	2418	rBV2	489	582	0.04%	0.005%




Sum of corrected areas: 11290535

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029463.D
Acq On : 14 Jun 2022 14:34
Operator : JC/MD
Sample : N3248-20 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

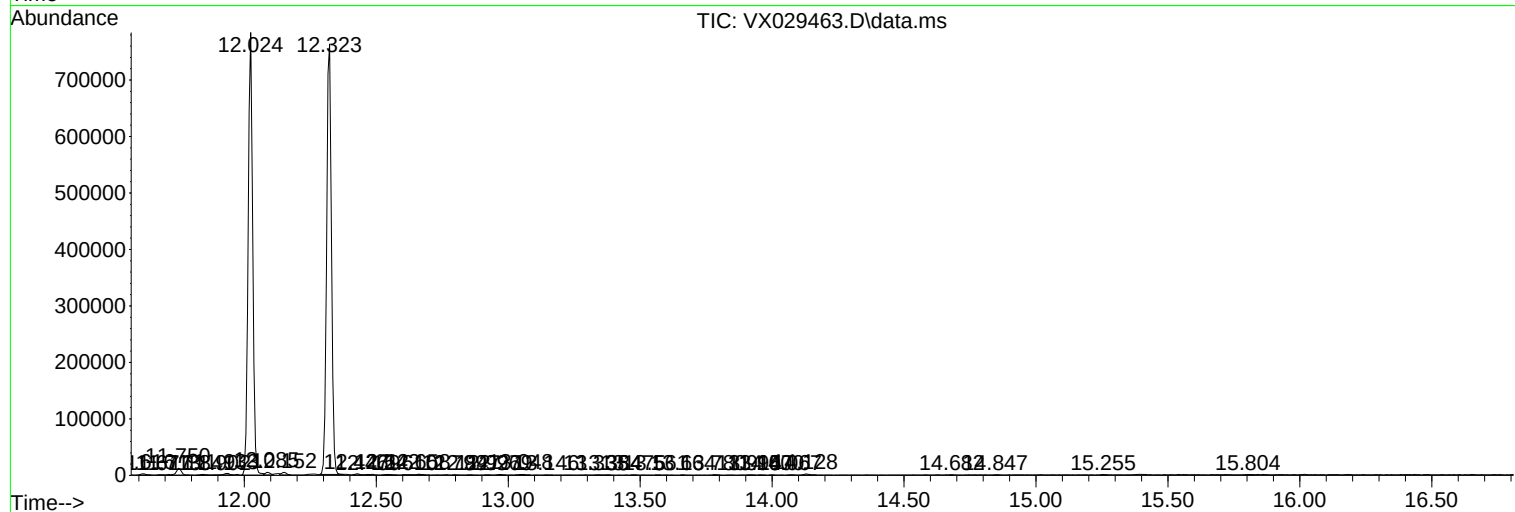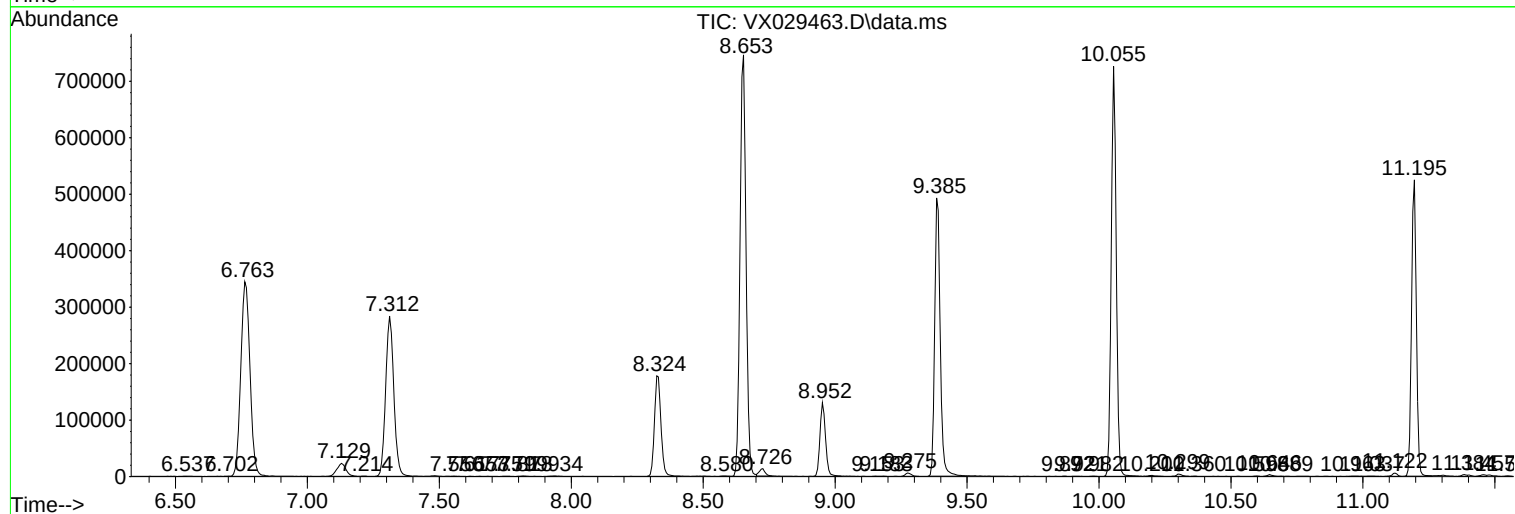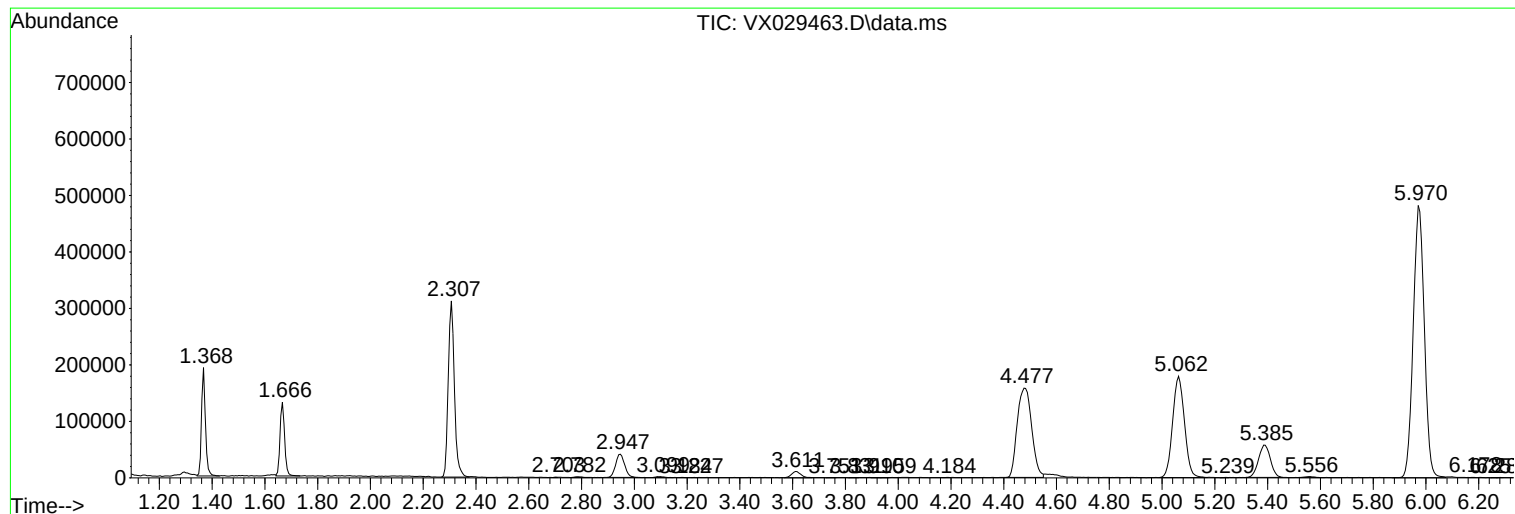

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029463.D
Acq On : 14 Jun 2022 14:34
Operator : JC/MD
Sample : N3248-20 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029463.D
Acq On : 14 Jun 2022 14:34
Operator : JC/MD
Sample : N3248-20 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYY9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc