

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029464.D
 Acq On : 14 Jun 2022 14:57
 Operator : JC/MD
 Sample : N3248-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

Signal : TIC: VX029464.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	135455	134841	12.63%	1.565%
2	1.666	90	95	102	rVB	102816	122694	11.50%	1.424%
3	2.307	194	200	210	rBV	216715	350254	32.82%	4.066%
4	2.544	238	239	240	rBV	495	264	0.02%	0.003%
5	2.709	262	266	271	rBV3	1088	1901	0.18%	0.022%
6	2.788	275	279	284	rBV4	998	1785	0.17%	0.021%
7	2.898	295	297	299	rBV2	322	243	0.02%	0.003%
8	2.934	299	303	304	rBV3	616	673	0.06%	0.008%
9	3.093	320	329	338	rBV2	13621	27171	2.55%	0.315%
10	3.203	346	347	350	rVB2	310	265	0.02%	0.003%
11	3.282	357	360	361	rBV2	219	238	0.02%	0.003%
12	3.343	368	370	375	rBV	280	328	0.03%	0.004%
13	3.410	378	381	382	rBV2	271	239	0.02%	0.003%
14	3.611	406	414	423	rBV	18763	43479	4.07%	0.505%
15	3.910	461	463	464	rBV2	295	281	0.03%	0.003%
16	3.989	474	476	477	rBV	370	296	0.03%	0.003%
17	4.007	477	479	482	rVV2	310	289	0.03%	0.003%
18	4.196	506	510	513	rBV2	362	554	0.05%	0.006%
19	4.270	520	522	525	rBV	308	260	0.02%	0.003%
20	4.306	526	528	530	rVB	423	322	0.03%	0.004%
21	4.471	545	555	578	rBV2	114002	431091	40.39%	5.005%
22	4.642	582	583	587	rVB3	540	339	0.03%	0.004%
23	5.062	638	652	669	rBV	134505	424221	39.75%	4.925%
24	5.269	683	686	687	rBV2	293	306	0.03%	0.004%
25	5.385	693	705	715	rBV	35720	110796	10.38%	1.286%
26	5.562	728	734	740	rVB2	1520	3498	0.33%	0.041%
27	5.727	758	761	763	rBV2	415	344	0.03%	0.004%
28	5.824	775	777	778	rBV	333	242	0.02%	0.003%
29	5.971	788	801	815	rBV2	359695	1067336	100.00%	12.392%
30	6.208	837	840	841	rBV	329	303	0.03%	0.004%
31	6.355	862	864	869	rBV3	493	707	0.07%	0.008%
32	6.452	878	880	881	rBV2	477	319	0.03%	0.004%
33	6.763	922	931	946	rBV	251317	597232	55.96%	6.934%
34	6.970	964	965	967	rBV	288	274	0.03%	0.003%
35	7.025	971	974	975	rBV	310	317	0.03%	0.004%
36	7.129	983	991	1003	rBV	88976	201479	18.88%	2.339%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029464.D
 Acq On : 14 Jun 2022 14:57
 Operator : JC/MD
 Sample : N3248-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	7.312	1011	1021	1035	rBV	220620	474044	44.41%	5.504%
38	7.482	1045	1049	1051	rBV3	571	757	0.07%	0.009%
39	7.690	1081	1083	1086	rBV2	401	377	0.04%	0.004%
40	7.812	1100	1103	1105	rVV2	326	441	0.04%	0.005%
41	7.830	1105	1106	1108	rVB2	578	323	0.03%	0.004%
42	7.940	1117	1124	1131	rVB3	774	1653	0.15%	0.019%
43	8.049	1139	1142	1144	rBV3	315	341	0.03%	0.004%
44	8.232	1170	1172	1175	rVB2	345	283	0.03%	0.003%
45	8.330	1179	1188	1197	rBV	139763	232141	21.75%	2.695%
46	8.458	1207	1209	1211	rBV2	293	324	0.03%	0.004%
47	8.525	1218	1220	1223	rVB2	373	347	0.03%	0.004%
48	8.580	1227	1229	1232	rVV2	410	428	0.04%	0.005%
49	8.653	1234	1241	1248	rVV	543835	863690	80.92%	10.027%
50	8.720	1249	1252	1265	rVB2	8138	14305	1.34%	0.166%
51	8.952	1283	1290	1301	rBV	107538	162701	15.24%	1.889%
52	9.196	1329	1330	1333	rBV2	277	230	0.02%	0.003%
53	9.226	1333	1335	1337	rBV2	202	236	0.02%	0.003%
54	9.275	1337	1343	1352	rVB	69099	97215	9.11%	1.129%
55	9.385	1356	1361	1376	rBV	425533	623699	58.44%	7.241%
56	9.750	1419	1421	1422	rBV	451	307	0.03%	0.004%
57	10.055	1465	1471	1487	rVV	533522	696693	65.27%	8.089%
58	10.238	1498	1501	1505	rBV2	361	574	0.05%	0.007%
59	10.305	1508	1512	1517	rBV2	1821	3041	0.28%	0.035%
60	10.403	1524	1528	1531	rBV	322	442	0.04%	0.005%
61	10.610	1558	1562	1565	rBV3	230	460	0.04%	0.005%
62	10.756	1584	1586	1589	rBV2	288	268	0.03%	0.003%
63	10.787	1589	1591	1595	rVB2	357	571	0.05%	0.007%
64	10.823	1595	1597	1598	rBV	262	287	0.03%	0.003%
65	10.970	1620	1621	1623	rVB	562	276	0.03%	0.003%
66	11.085	1637	1640	1643	rBV5	627	969	0.09%	0.011%
67	11.116	1643	1645	1649	rVB2	3747	4648	0.44%	0.054%
68	11.195	1652	1658	1666	rBV	431248	547372	51.28%	6.355%
69	11.384	1686	1689	1690	rBV	444	415	0.04%	0.005%
70	11.451	1698	1700	1702	rBV3	708	654	0.06%	0.008%
71	11.482	1702	1705	1708	rVB3	1405	1728	0.16%	0.020%
72	11.549	1714	1716	1718	rVB2	455	284	0.03%	0.003%
73	11.616	1725	1727	1728	rBV	379	228	0.02%	0.003%
74	11.689	1734	1739	1741	rBV2	452	778	0.07%	0.009%
75	11.720	1741	1744	1745	rVV2	596	685	0.06%	0.008%
76	11.750	1745	1749	1754	rVB3	3962	5395	0.51%	0.063%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029464.D
 Acq On : 14 Jun 2022 14:57
 Operator : JC/MD
 Sample : N3248-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EXYX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	11.841	1762	1764	1767	rVB2	938	861	0.08%	0.010%
78	11.933	1776	1779	1783	rBV4	1779	2695	0.25%	0.031%
79	11.976	1783	1786	1789	rBV2	648	761	0.07%	0.009%
80	12.024	1789	1794	1806	rBV	538740	643308	60.27%	7.469%
81	12.122	1807	1810	1811	rBV3	918	1012	0.09%	0.012%
82	12.219	1824	1826	1827	rBV2	505	449	0.04%	0.005%
83	12.323	1837	1843	1851	rBV	544066	688875	64.54%	7.998%
84	12.427	1858	1860	1864	rVB2	1749	1662	0.16%	0.019%
85	12.530	1875	1877	1881	rBV2	319	285	0.03%	0.003%
86	12.664	1897	1899	1902	rVB2	676	609	0.06%	0.007%
87	12.896	1934	1937	1939	rBV	497	448	0.04%	0.005%
88	13.116	1971	1973	1976	rBV2	502	421	0.04%	0.005%
89	13.585	2048	2050	2051	rBV	462	353	0.03%	0.004%
90	13.737	2073	2075	2077	rVB	380	256	0.02%	0.003%
91	13.786	2081	2083	2088	rVB2	758	806	0.08%	0.009%
92	13.847	2091	2093	2095	rBV3	339	393	0.04%	0.005%
93	13.914	2101	2104	2107	rBV3	292	505	0.05%	0.006%
94	14.000	2116	2118	2121	rVB	306	232	0.02%	0.003%
95	14.134	2136	2140	2145	rVB3	1449	2144	0.20%	0.025%
96	14.579	2209	2213	2214	rBV	395	578	0.05%	0.007%
97	15.012	2282	2284	2285	rBV2	436	277	0.03%	0.003%
98	16.280	2491	2492	2495	rBV2	396	459	0.04%	0.005%
99	16.389	2508	2510	2513	rBV3	623	692	0.06%	0.008%
100	16.591	2541	2543	2544	rBV	710	431	0.04%	0.005%


Sum of corrected areas: 8613303

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029464.D
Acq On : 14 Jun 2022 14:57
Operator : JC/MD
Sample : N3248-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

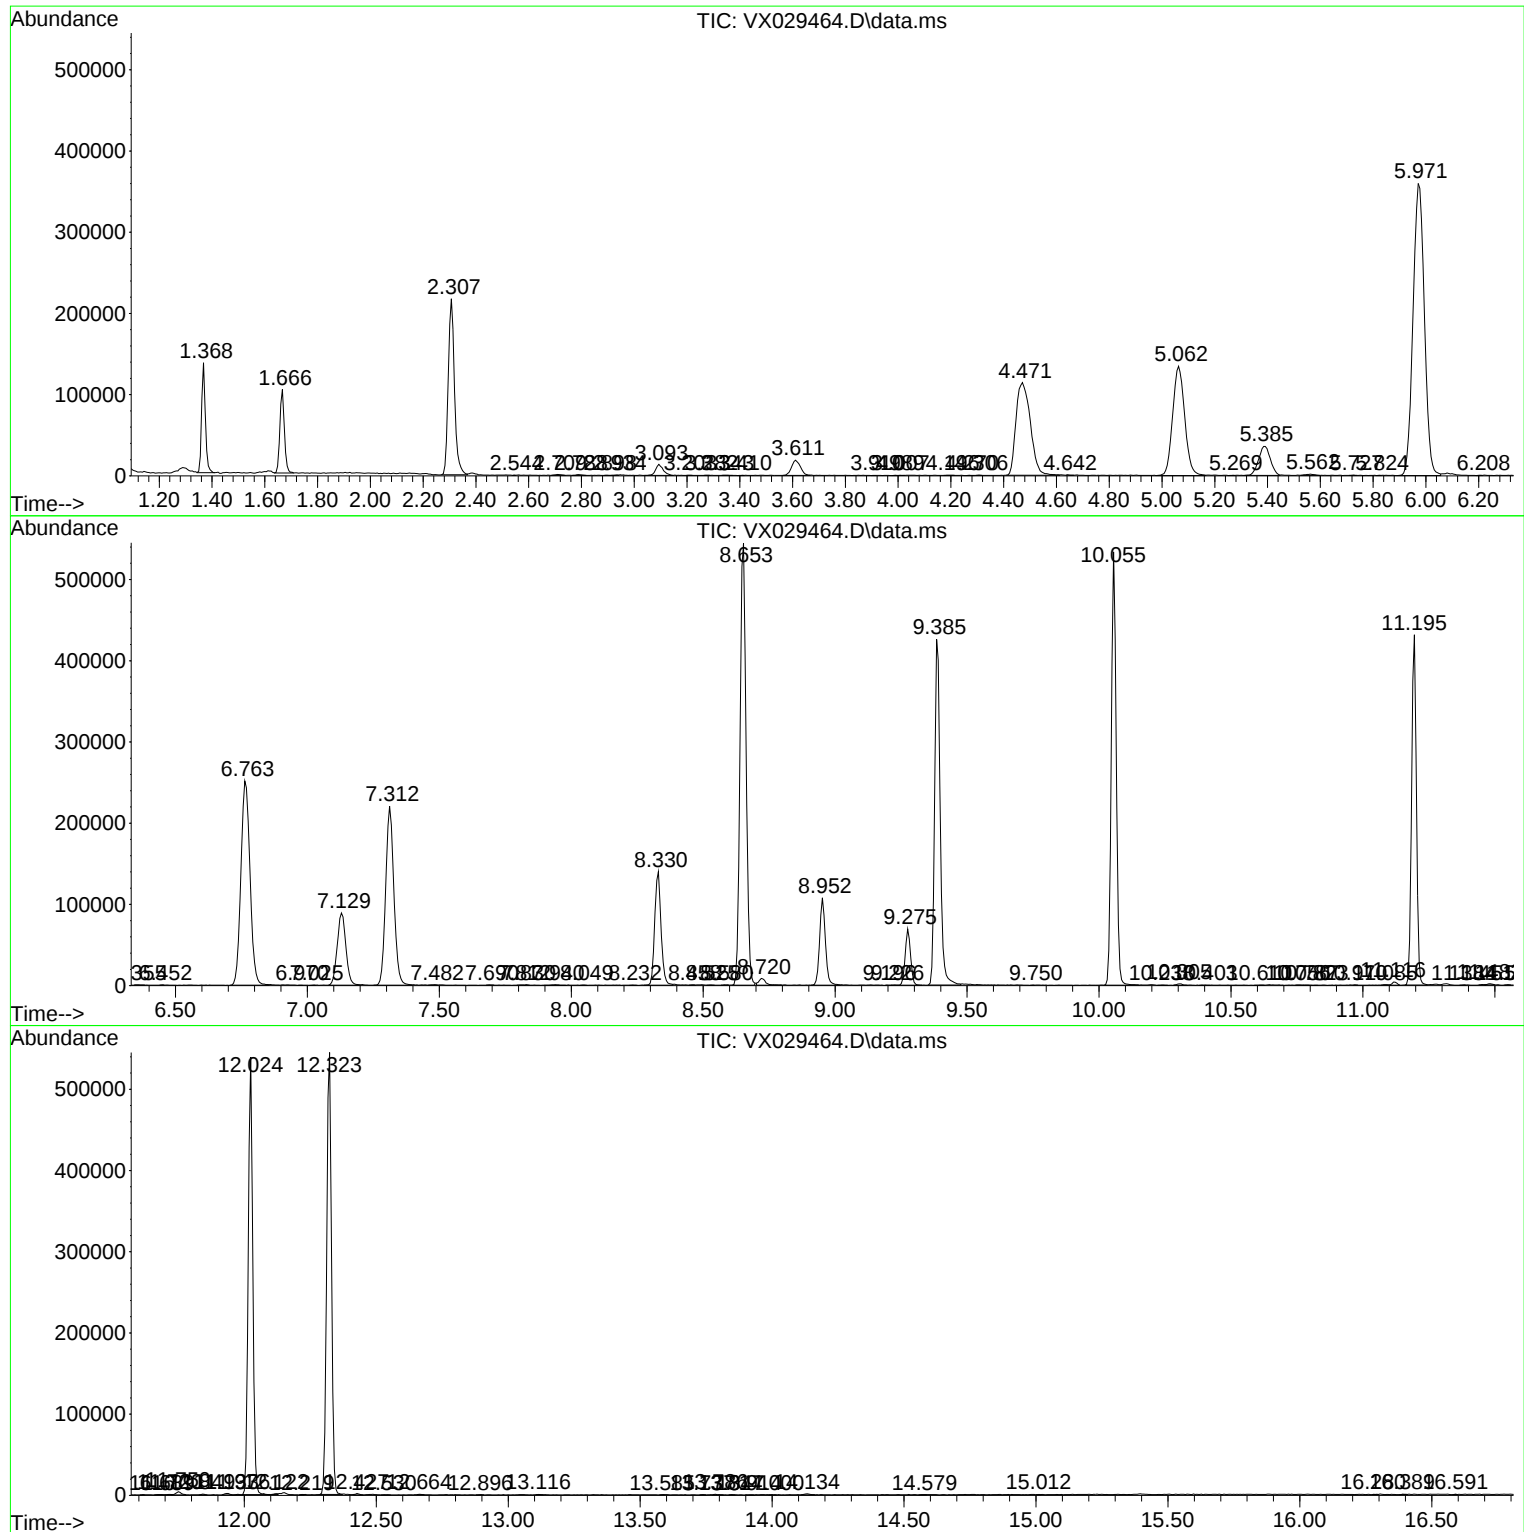

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029464.D
Acq On : 14 Jun 2022 14:57
Operator : JC/MD
Sample : N3248-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029464.D
Acq On : 14 Jun 2022 14:57
Operator : JC/MD
Sample : N3248-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EXYX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc