

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029466.D
 Acq On : 14 Jun 2022 15:44
 Operator : JC/MD
 Sample : N3254-04DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DF4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M

Title : VOC Analysis

Signal : TIC: VX029466.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	56	rVB	176918	190532	14.13%	1.741%
2	1.660	90	94	102	rVB	92848	107671	7.98%	0.984%
3	2.300	193	199	211	rBV	297139	498140	36.93%	4.552%
4	2.636	252	254	255	rVB2	551	282	0.02%	0.003%
5	2.703	263	265	266	rBV	476	320	0.02%	0.003%
6	2.794	274	280	285	rVB3	2257	4484	0.33%	0.041%
7	2.946	296	305	315	rBV	29934	71255	5.28%	0.651%
8	3.087	325	328	329	rBV2	499	463	0.03%	0.004%
9	3.172	339	342	344	rBV2	257	277	0.02%	0.003%
10	3.337	367	369	372	rBV3	261	332	0.02%	0.003%
11	3.392	376	378	380	rVB2	303	318	0.02%	0.003%
12	3.446	384	387	391	rBV4	352	494	0.04%	0.005%
13	3.550	401	404	407	rVB2	307	445	0.03%	0.004%
14	3.605	410	413	416	rBV4	577	1071	0.08%	0.010%
15	3.849	448	453	455	rVB	510	648	0.05%	0.006%
16	3.867	455	456	459	rBV2	430	437	0.03%	0.004%
17	3.928	464	466	469	rBV2	292	322	0.02%	0.003%
18	3.995	475	477	480	rVV	386	322	0.02%	0.003%
19	4.044	483	485	488	rVB2	255	330	0.02%	0.003%
20	4.087	491	492	496	rVB3	255	318	0.02%	0.003%
21	4.227	513	515	518	rBV2	332	388	0.03%	0.004%
22	4.275	521	523	528	rBV2	283	526	0.04%	0.005%
23	4.391	538	542	544	rVB	340	278	0.02%	0.003%
24	4.464	544	554	568	rBV2	112262	355692	26.37%	3.250%
25	4.721	594	596	598	rVB2	460	319	0.02%	0.003%
26	4.879	620	622	624	rVB	366	289	0.02%	0.003%
27	4.928	627	630	631	rBV	334	366	0.03%	0.003%
28	5.062	639	652	670	rBV2	172047	534375	39.62%	4.883%
29	5.385	696	705	716	rVB4	9017	28129	2.09%	0.257%
30	5.562	725	734	741	rBV3	3038	7308	0.54%	0.067%
31	5.970	789	801	817	rBV2	451626	1348713	100.00%	12.324%
32	6.239	843	845	847	rVB2	336	297	0.02%	0.003%
33	6.342	858	862	863	rBV3	735	879	0.07%	0.008%
34	6.360	863	865	872	rVV4	1224	2051	0.15%	0.019%
35	6.409	872	873	878	rVB	297	363	0.03%	0.003%
36	6.562	896	898	901	rVB	397	289	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029466.D
 Acq On : 14 Jun 2022 15:44
 Operator : JC/MD
 Sample : N3254-04DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DF4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

37	6.763	922	931	944	rBV	349714	827009	61.32%	7.557%
38	7.129	982	991	1012	rBV	263629	580579	43.05%	5.305%
39	7.312	1012	1021	1035	rBV	271503	586234	43.47%	5.357%
40	7.811	1096	1103	1109	rBV4	465	1398	0.10%	0.013%
41	7.879	1112	1114	1116	rVB2	428	339	0.03%	0.003%
42	7.909	1116	1119	1120	rBV2	288	292	0.02%	0.003%
43	7.952	1120	1126	1134	rVB6	978	2554	0.19%	0.023%
44	8.330	1181	1188	1197	rBV	173665	284598	21.10%	2.600%
45	8.586	1226	1230	1234	rVB4	470	804	0.06%	0.007%
46	8.653	1234	1241	1248	rBV	727911	1133072	84.01%	10.353%
47	8.726	1249	1253	1263	rVB	10393	19576	1.45%	0.179%
48	8.842	1270	1272	1274	rVB2	381	290	0.02%	0.003%
49	8.951	1285	1290	1301	rBV	120835	177615	13.17%	1.623%
50	9.281	1337	1344	1348	rBV5	2665	4136	0.31%	0.038%
51	9.390	1356	1362	1379	rBV	469766	691396	51.26%	6.317%
52	9.890	1443	1444	1448	rVB	364	296	0.02%	0.003%
53	10.055	1465	1471	1481	rBV	711201	948733	70.34%	8.669%
54	10.195	1491	1494	1500	rVB3	987	1419	0.11%	0.013%
55	10.305	1509	1512	1516	rVV2	1730	2302	0.17%	0.021%
56	10.445	1532	1535	1537	rBV2	347	433	0.03%	0.004%
57	10.488	1541	1542	1544	rBV2	391	286	0.02%	0.003%
58	10.610	1560	1562	1563	rBV2	335	269	0.02%	0.002%
59	10.646	1565	1568	1570	rVV3	805	797	0.06%	0.007%
60	10.756	1584	1586	1590	rVB	448	419	0.03%	0.004%
61	10.963	1618	1620	1627	rVB3	375	737	0.05%	0.007%
62	11.091	1637	1641	1642	rBV2	663	685	0.05%	0.006%
63	11.122	1642	1646	1652	rVB3	5226	6718	0.50%	0.061%
64	11.195	1652	1658	1667	rBV	499429	635070	47.09%	5.803%
65	11.384	1687	1689	1691	rBV2	536	463	0.03%	0.004%
66	11.482	1697	1705	1713	rBV4	2243	5106	0.38%	0.047%
67	11.549	1713	1716	1718	rVB3	571	643	0.05%	0.006%
68	11.622	1724	1728	1733	rBV4	750	1521	0.11%	0.014%
69	11.677	1733	1737	1741	rBV4	630	933	0.07%	0.009%
70	11.750	1745	1749	1757	rVB3	6406	9195	0.68%	0.084%
71	11.823	1759	1761	1762	rBV2	299	294	0.02%	0.003%
72	11.847	1762	1765	1767	rVB2	919	966	0.07%	0.009%
73	11.939	1775	1780	1783	rBV2	2604	3173	0.24%	0.029%
74	12.024	1789	1794	1803	rBV	770455	926598	68.70%	8.467%
75	12.152	1813	1815	1821	rVB	4168	4604	0.34%	0.042%
76	12.225	1825	1827	1828	rBV2	528	305	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
 Data File : VX029466.D
 Acq On : 14 Jun 2022 15:44
 Operator : JC/MD
 Sample : N3254-04DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0DF4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
 Title : VOC Analysis

77	12.323	1836	1843	1850	rBV	714571	903688	67.00%	8.257%
78	12.426	1858	1860	1864	rVB2	1760	2094	0.16%	0.019%
79	12.481	1864	1869	1873	rBV4	1132	1947	0.14%	0.018%
80	12.542	1877	1879	1881	rVB2	425	286	0.02%	0.003%
81	12.658	1896	1898	1904	rBV4	921	1273	0.09%	0.012%
82	12.756	1912	1914	1919	rBV3	345	560	0.04%	0.005%
83	12.865	1929	1932	1933	rBV3	269	309	0.02%	0.003%
84	13.054	1959	1963	1965	rBV4	894	1112	0.08%	0.010%
85	13.115	1970	1973	1976	rVB3	284	420	0.03%	0.004%
86	13.408	2019	2021	2023	rVB2	338	304	0.02%	0.003%
87	13.432	2023	2025	2027	rBV	346	376	0.03%	0.003%
88	13.536	2040	2042	2044	rBV	393	416	0.03%	0.004%
89	13.780	2080	2082	2087	rVB2	479	643	0.05%	0.006%
90	13.969	2111	2113	2115	rBV2	258	288	0.02%	0.003%
91	14.133	2136	2140	2145	rVB2	2111	3140	0.23%	0.029%
92	14.463	2192	2194	2195	rBV	370	365	0.03%	0.003%
93	14.493	2197	2199	2202	rBV	339	321	0.02%	0.003%
94	14.633	2220	2222	2225	rBV2	506	358	0.03%	0.003%
95	15.042	2286	2289	2291	rBV3	356	468	0.03%	0.004%
96	15.395	2343	2347	2351	rBV4	1660	2651	0.20%	0.024%
97	15.511	2363	2366	2367	rBV3	704	691	0.05%	0.006%
98	15.578	2373	2377	2378	rBV	612	781	0.06%	0.007%
99	16.225	2481	2483	2485	rBV3	646	443	0.03%	0.004%
100	16.627	2547	2549	2552	rBV2	636	677	0.05%	0.006%

Sum of corrected areas: 10944191




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029466.D
Acq On : 14 Jun 2022 15:44
Operator : JC/MD
Sample : N3254-04DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DF4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

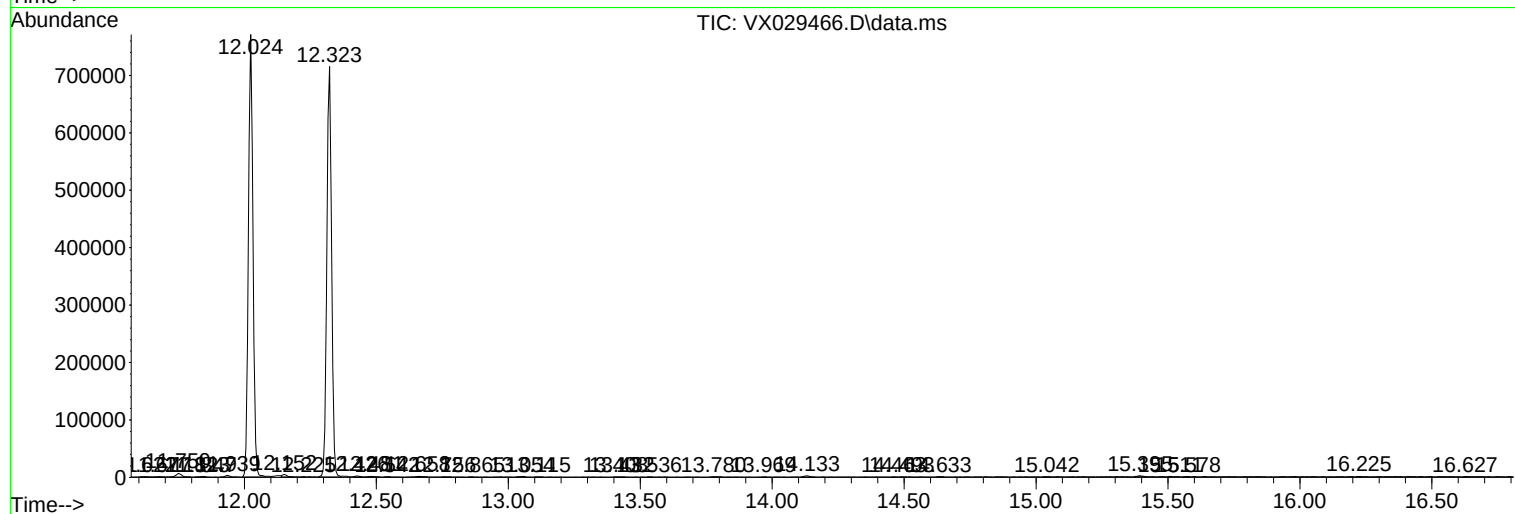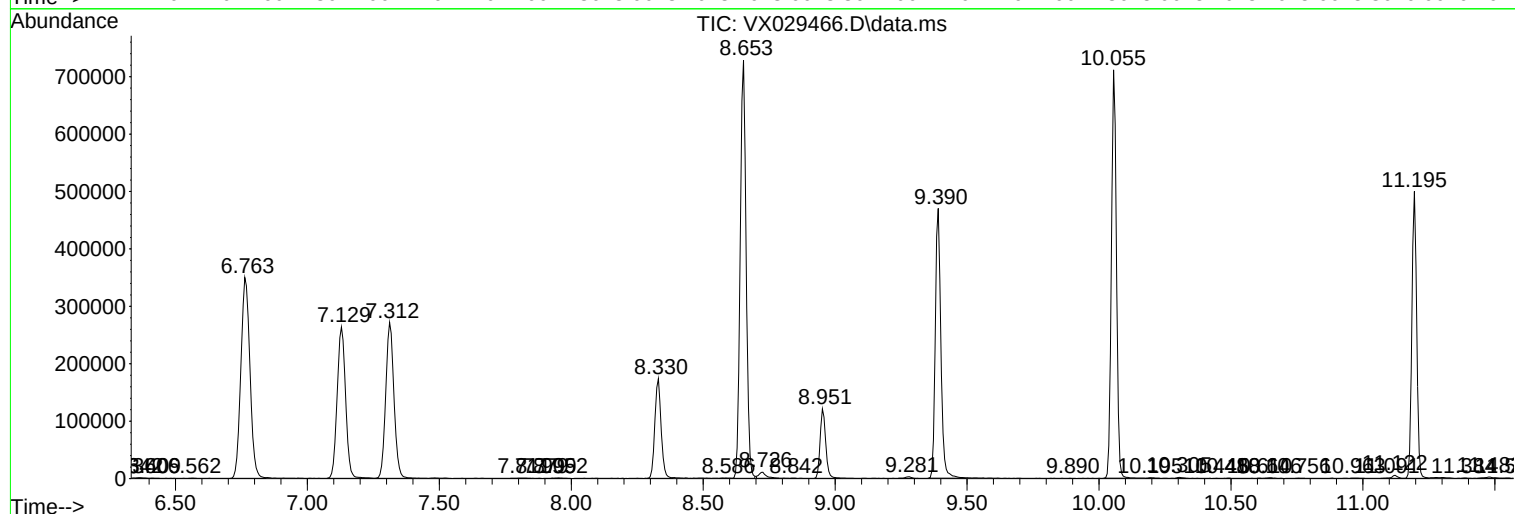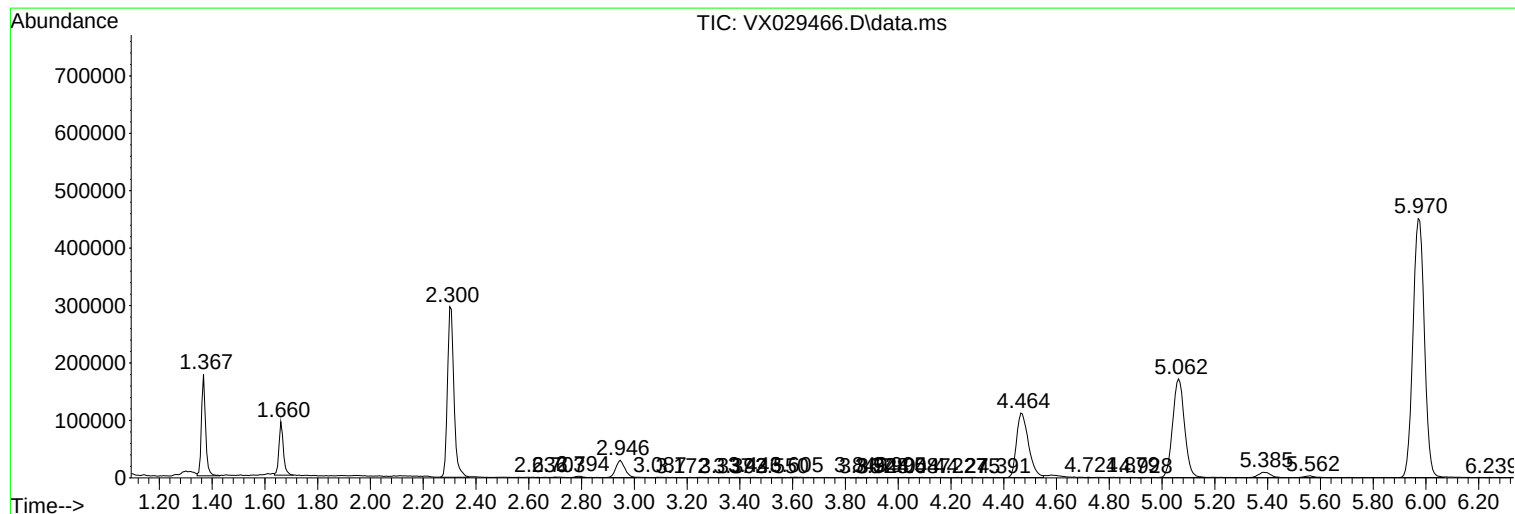

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029466.D
Acq On : 14 Jun 2022 15:44
Operator : JC/MD
Sample : N3254-04DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DF4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061422\
Data File : VX029466.D
Acq On : 14 Jun 2022 15:44
Operator : JC/MD
Sample : N3254-04DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0DF4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML061322WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc